

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110724\
 Data File : FB031148.D
 Signal(s) : FID2B.CH
 Acq On : 7 Nov 2024 20:44
 Operator : YP/AJ
 Sample : BSF1107S3
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF1107S3

Integration File: Calibration.e
 Quant Time: Nov 08 02:47:56 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB102824.M
 Quant Title :
 QLast Update : Mon Oct 28 12:19:57 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.794	547741	19.844 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.719	1147925	29.228 ng/ml
2) t 2,2,4-Trimethylpentane	7.424	1394182	29.767 ng/ml
3) t n-Heptane	7.754	429804	9.484 ng/ml
4) t Benzene	7.894	533257	9.976 ng/ml
6) t Toluene	10.622	1486860	29.775 ng/ml
7) t Ethylbenzene	13.059	457688	10.225 ng/ml
8) t m-Xylene	13.192	1030385	21.185 ng/ml
9) t O-Xylene	13.920	884268	19.399 ng/ml
10) t 1,2,4-Trimethylbenzene	16.196	859507	23.100 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110724\
Data File : FB031148.D
Signal(s) : FID2B.CH
Acq On : 7 Nov 2024 20:44
Operator : YP/AJ
Sample : BSF1107S3
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF1107S3

Integration File: Calibration.e
Quant Time: Nov 08 02:47:56 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB102824.M
Quant Title :
QLast Update : Mon Oct 28 12:19:57 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

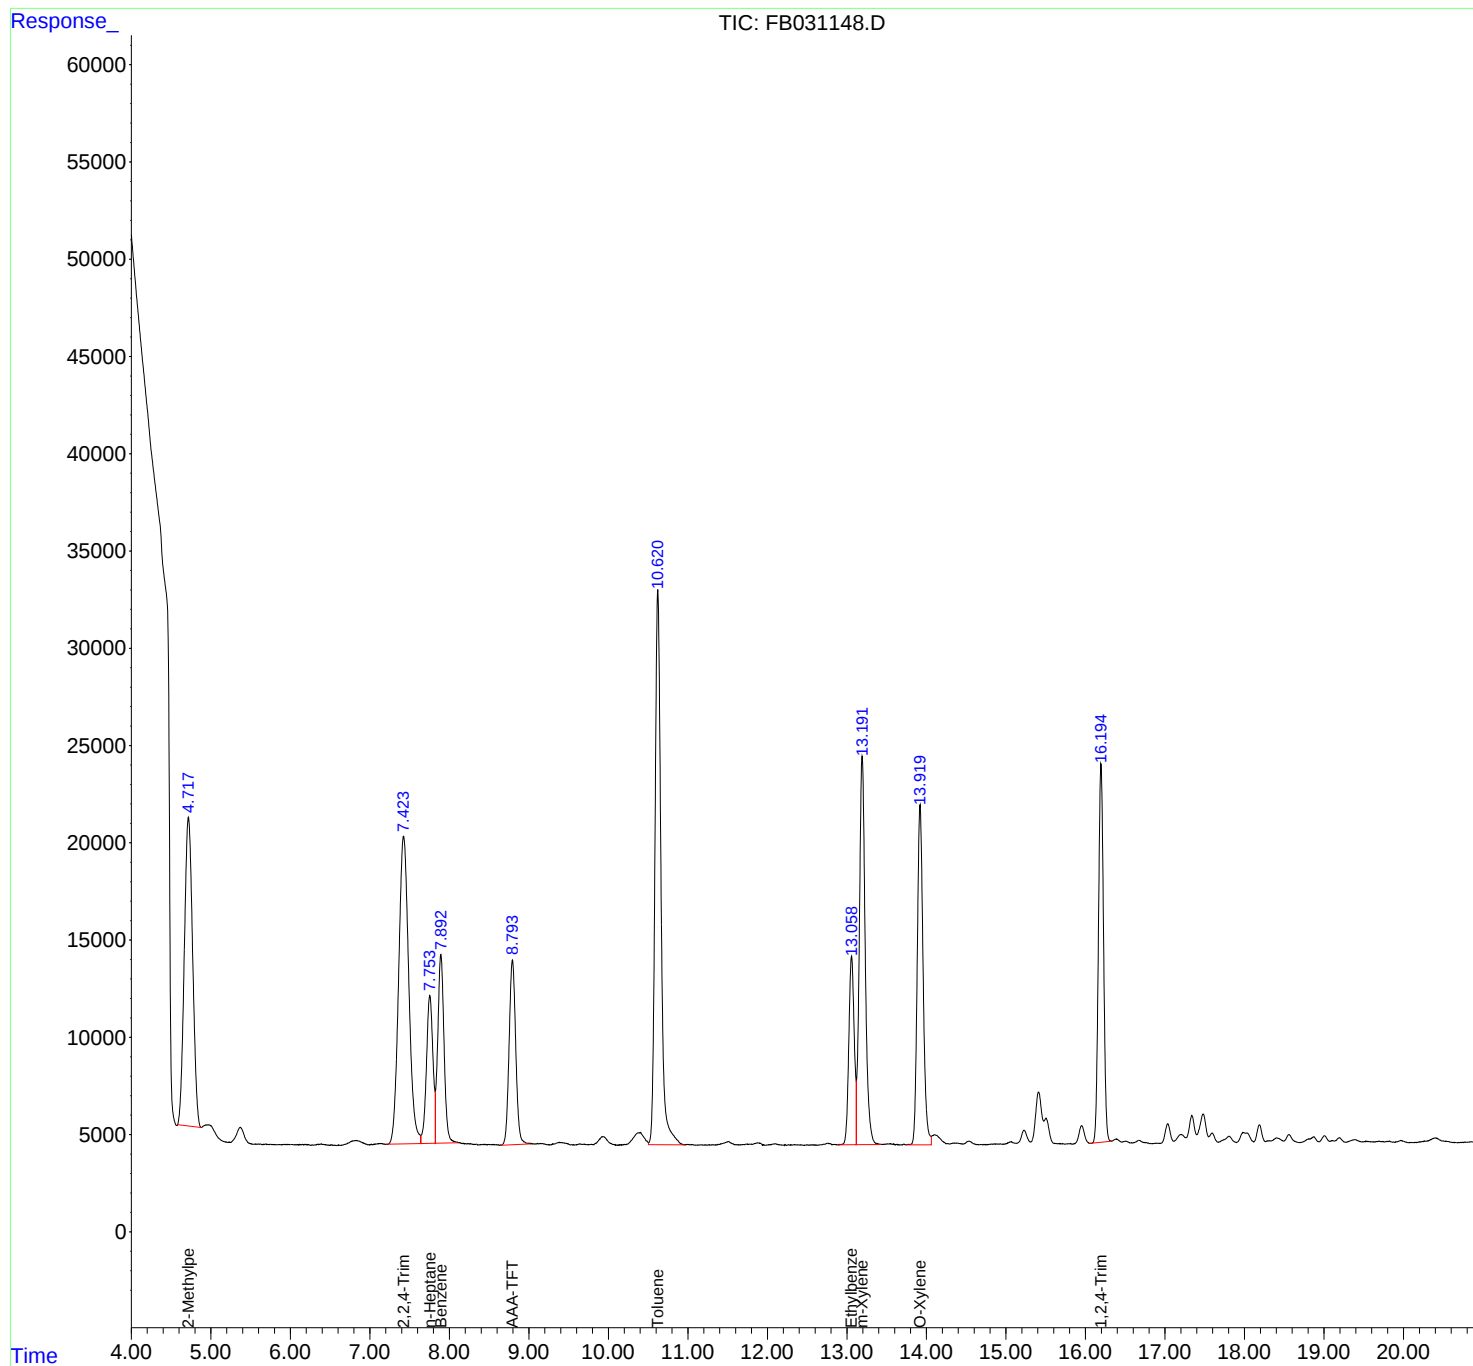


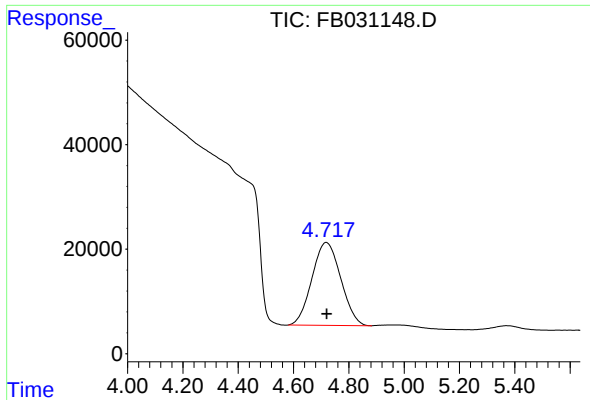

#1 2-Methylpentane


R.T.: 4.719 min
Delta R.T.: -0.001 min
Response: 1147925
Conc: 29.23 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1107S3

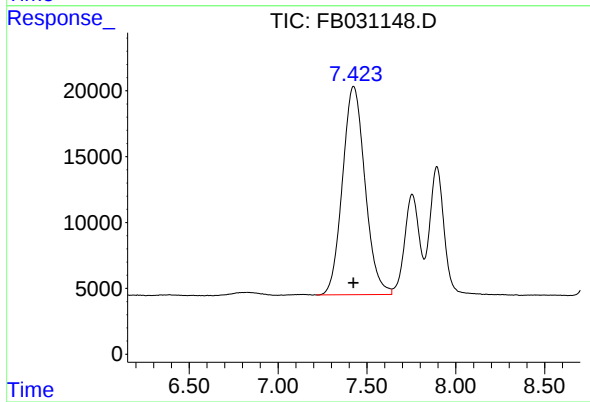


#2 2,2,4-Trimethylpentane

R.T.: 7.424 min
Delta R.T.: 0.000 min
Response: 1394182
Conc: 29.77 ng/ml

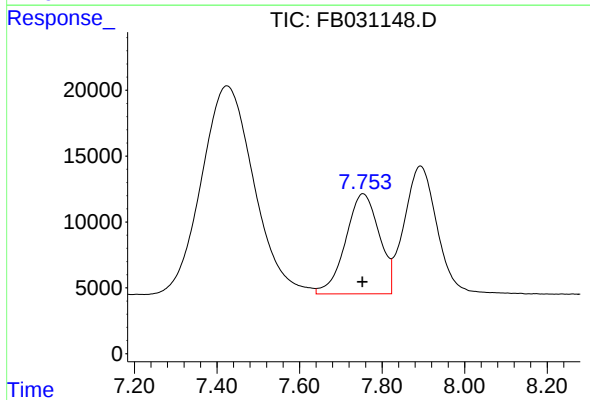


#3 n-Heptane

R.T.: 7.754 min
Delta R.T.: 0.002 min
Response: 429804
Conc: 9.48 ng/ml

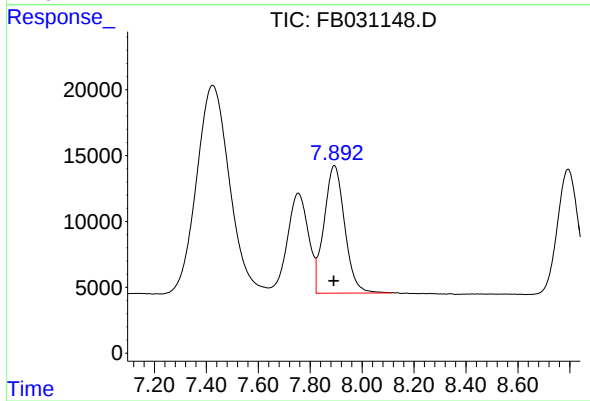

#4 Benzene


R.T.: 7.894 min
Delta R.T.: 0.002 min
Response: 533257
Conc: 9.98 ng/ml

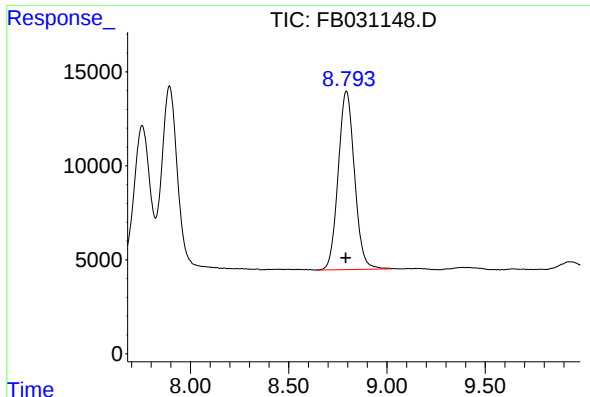

#5 AAA-TFT


R.T.: 8.794 min
Delta R.T.: 0.003 min
Response: 547741
Conc: 19.84 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1107S3

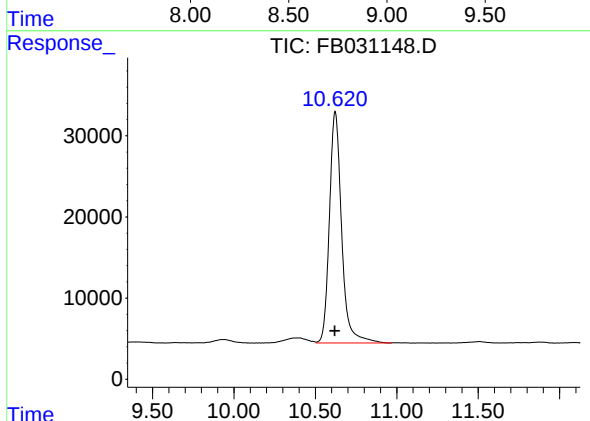


#6 Toluene

R.T.: 10.622 min
Delta R.T.: 0.003 min
Response: 1486860
Conc: 29.77 ng/ml

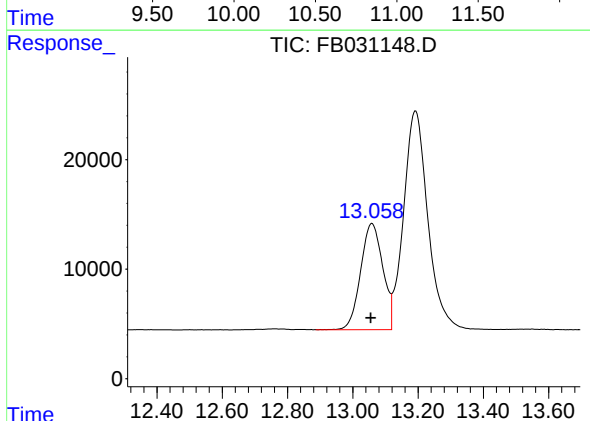


#7 Ethylbenzene

R.T.: 13.059 min
Delta R.T.: 0.004 min
Response: 457688
Conc: 10.22 ng/ml

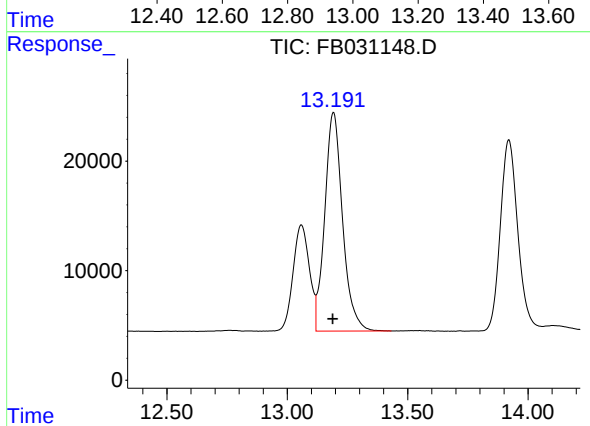

#8 m-Xylene


R.T.: 13.192 min
Delta R.T.: 0.004 min
Response: 1030385
Conc: 21.18 ng/ml

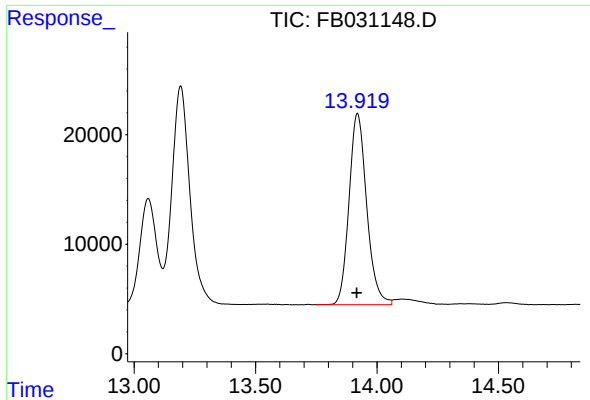

#9 O-Xylene

R.T.: 13.920 min
Delta R.T.: 0.004 min
Response: 884268
Conc: 19.40 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1107S3

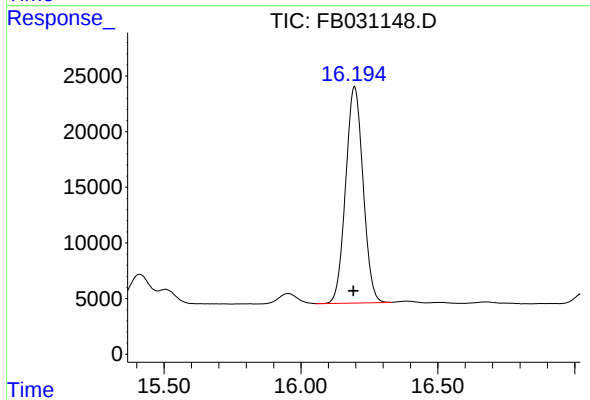

#10 1,2,4-Trimethylbenzene

R.T.: 16.196 min
Delta R.T.: 0.004 min
Response: 859507
Conc: 23.10 ng/ml