

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110724\
 Data File : FB031159.D
 Signal(s) : FID2B.CH
 Acq On : 8 Nov 2024 2:29
 Operator : YP/AJ
 Sample : BSF1107S4
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF1107S4

Integration File: Calibration.e
 Quant Time: Nov 08 02:48:58 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB102824.M
 Quant Title :
 QLast Update : Mon Oct 28 12:19:57 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.791	396002	14.346 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.716	1063279	27.073 ng/ml
2) t 2,2,4-Trimethylpentane	7.421	1308409	27.936 ng/ml
3) t n-Heptane	7.752	395141	8.719 ng/ml
4) t Benzene	7.891	474292	8.873 ng/ml
6) t Toluene	10.619	1334966	26.733 ng/ml
7) t Ethylbenzene	13.057	385691	8.616 ng/ml
8) t m-Xylene	13.190	825941	16.981 ng/ml
9) t O-Xylene	13.917	771163	16.918 ng/ml
10) t 1,2,4-Trimethylbenzene	16.194	611347	16.430 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110724\
Data File : FB031159.D
Signal(s) : FID2B.CH
Acq On : 8 Nov 2024 2:29
Operator : YP/AJ
Sample : BSF1107S4
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF1107S4

Integration File: Calibration.e
Quant Time: Nov 08 02:48:58 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB102824.M
Quant Title :
QLast Update : Mon Oct 28 12:19:57 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

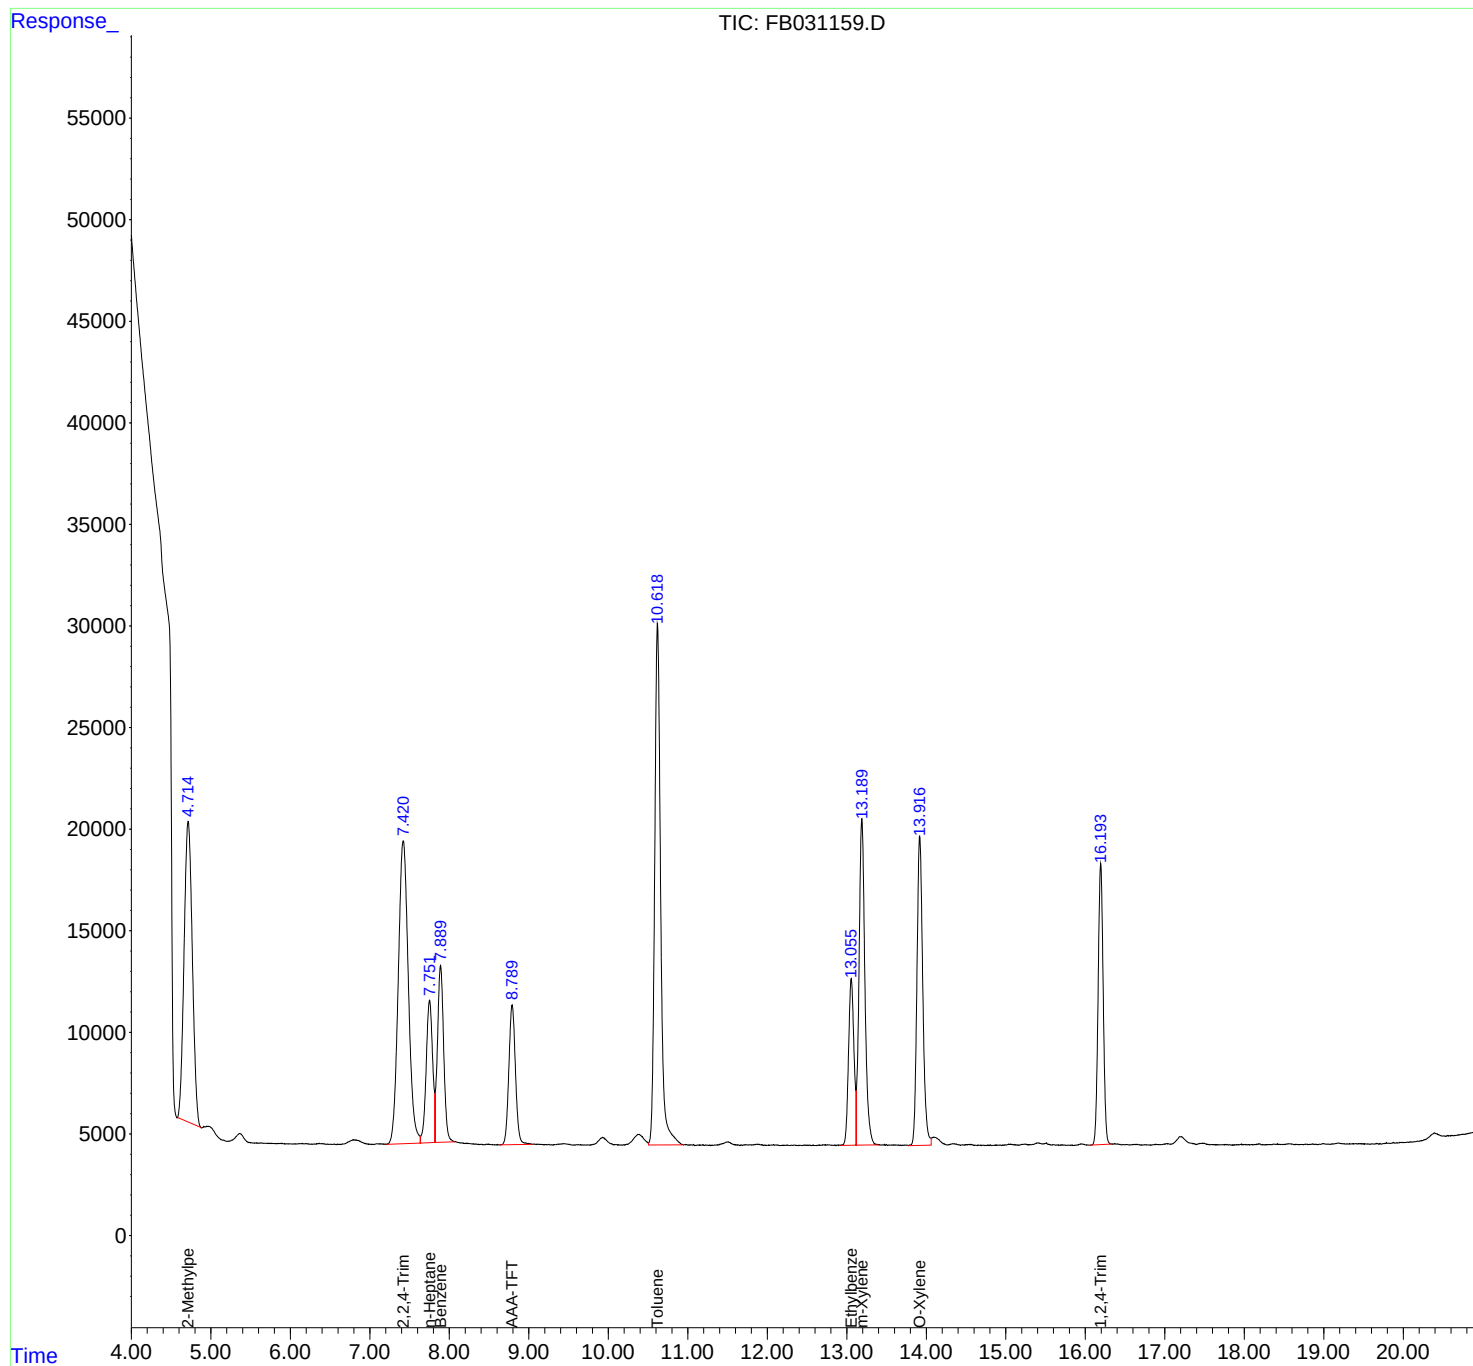


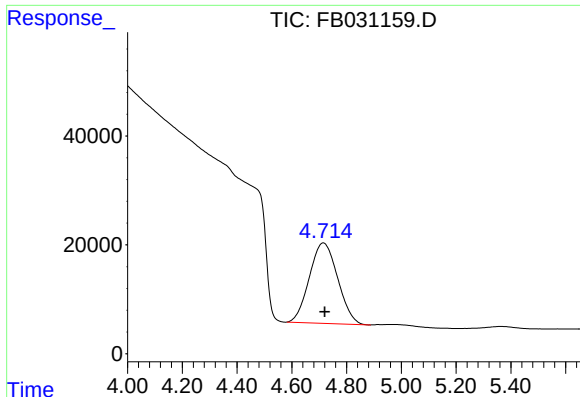

#1 2-Methylpentane


R.T.: 4.716 min
Delta R.T.: -0.004 min
Response: 1063279
Conc: 27.07 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1107S4

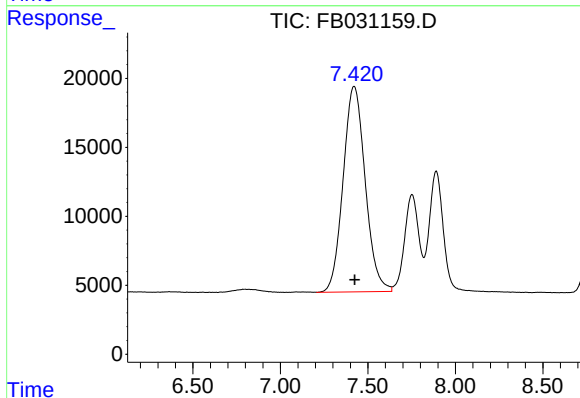


#2 2,2,4-Trimethylpentane

R.T.: 7.421 min
Delta R.T.: -0.003 min
Response: 1308409
Conc: 27.94 ng/ml

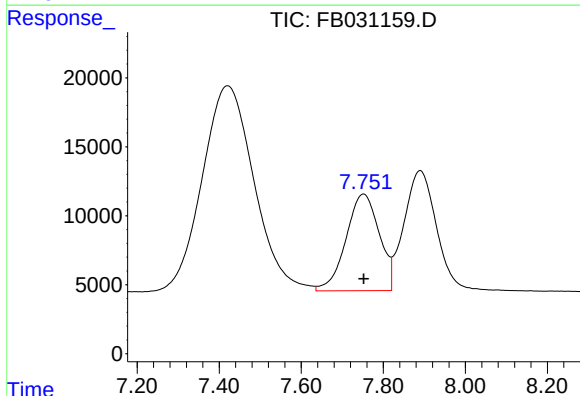


#3 n-Heptane

R.T.: 7.752 min
Delta R.T.: 0.000 min
Response: 395141
Conc: 8.72 ng/ml

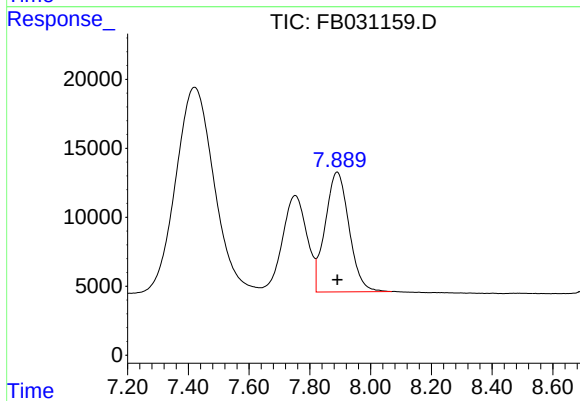

#4 Benzene


R.T.: 7.891 min
Delta R.T.: -0.001 min
Response: 474292
Conc: 8.87 ng/ml

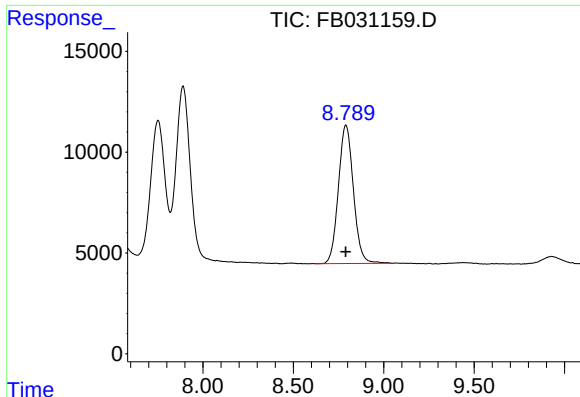

#5 AAA-TFT


R.T.: 8.791 min
Delta R.T.: 0.000 min
Response: 396002
Conc: 14.35 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1107S4

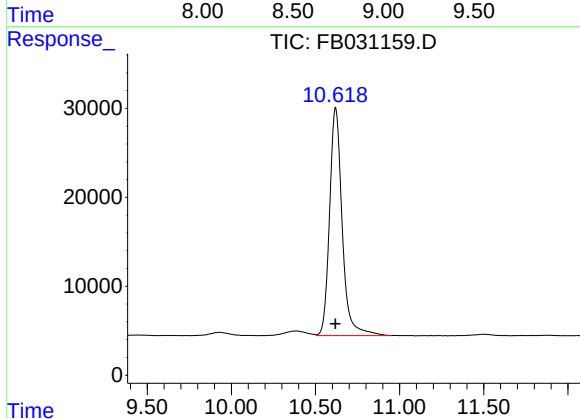


#6 Toluene

R.T.: 10.619 min
Delta R.T.: 0.000 min
Response: 1334966
Conc: 26.73 ng/ml

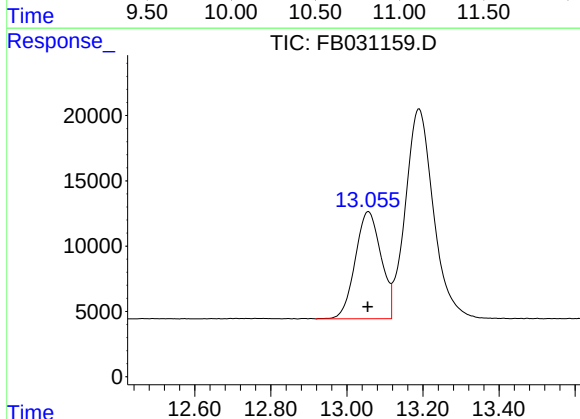


#7 Ethylbenzene

R.T.: 13.057 min
Delta R.T.: 0.002 min
Response: 385691
Conc: 8.62 ng/ml

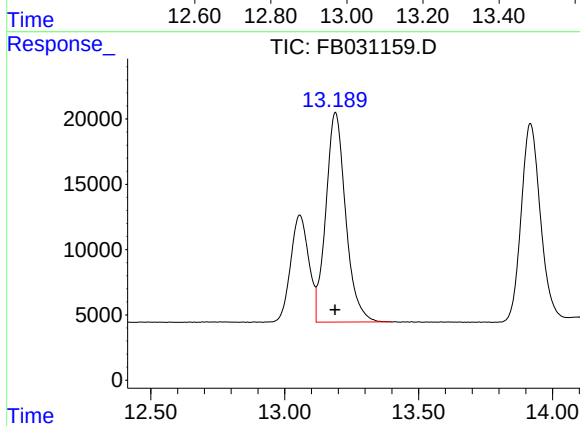

#8 m-Xylene


R.T.: 13.190 min
Delta R.T.: 0.002 min
Response: 825941
Conc: 16.98 ng/ml

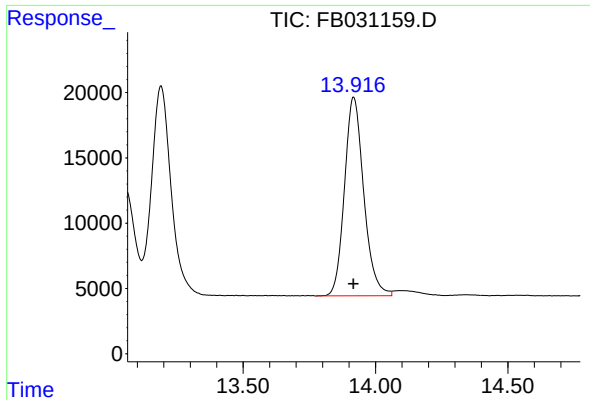

#9 O-Xylene

R.T.: 13.917 min
Delta R.T.: 0.000 min
Response: 771163
Conc: 16.92 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1107S4

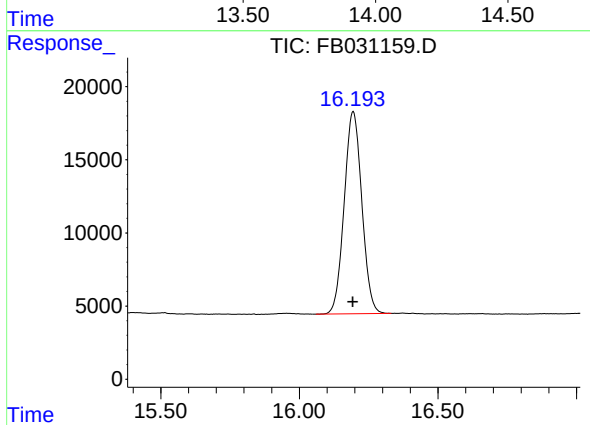

#10 1,2,4-Trimethylbenzene

R.T.: 16.194 min
Delta R.T.: 0.002 min
Response: 611347
Conc: 16.43 ng/ml