

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110819\
 Data File : FB022935.D
 Signal(s) : FID2B.CH
 Acq On : 8 Nov 2019 11:14
 Operator : DD/AJ
 Sample : K5742-09
 Misc : 5.03g/5.00ml DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 SB-37-(8-10)

Integration File: Calibration.e
 Quant Time: Nov 08 23:41:12 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB103119.M
 Quant Title :
 QLast Update : Thu Oct 31 14:57:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.796	432610	19.217 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.681	6237	0.194 ng/ml
2) t 2,2,4-Trimethylpentane	7.410	1438	0.041 ng/ml
3) t n-Heptane	7.755	10630	0.306 ng/ml
4) t Benzene	7.826	216	0.005 ng/ml
6) t Toluene	10.629	7869	0.183 ng/ml
7) t Ethylbenzene	13.063	9640	0.241 ng/ml
8) t m-Xylene	13.195	19745	0.523 ng/ml
9) t O-Xylene	13.930	1414	0.040 ng/ml
10) t 1,2,4-Trimethylbenzene	16.211	11746	0.414 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110819\
Data File : FB022935.D
Signal(s) : FID2B.CH
Acq On : 8 Nov 2019 11:14
Operator : DD/AJ
Sample : K5742-09
Misc : 5.03g/5.00ml DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
SB-37-(8-10)

Integration File: Calibration.e
Quant Time: Nov 08 23:41:12 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB103119.M
Quant Title :
QLast Update : Thu Oct 31 14:57:42 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

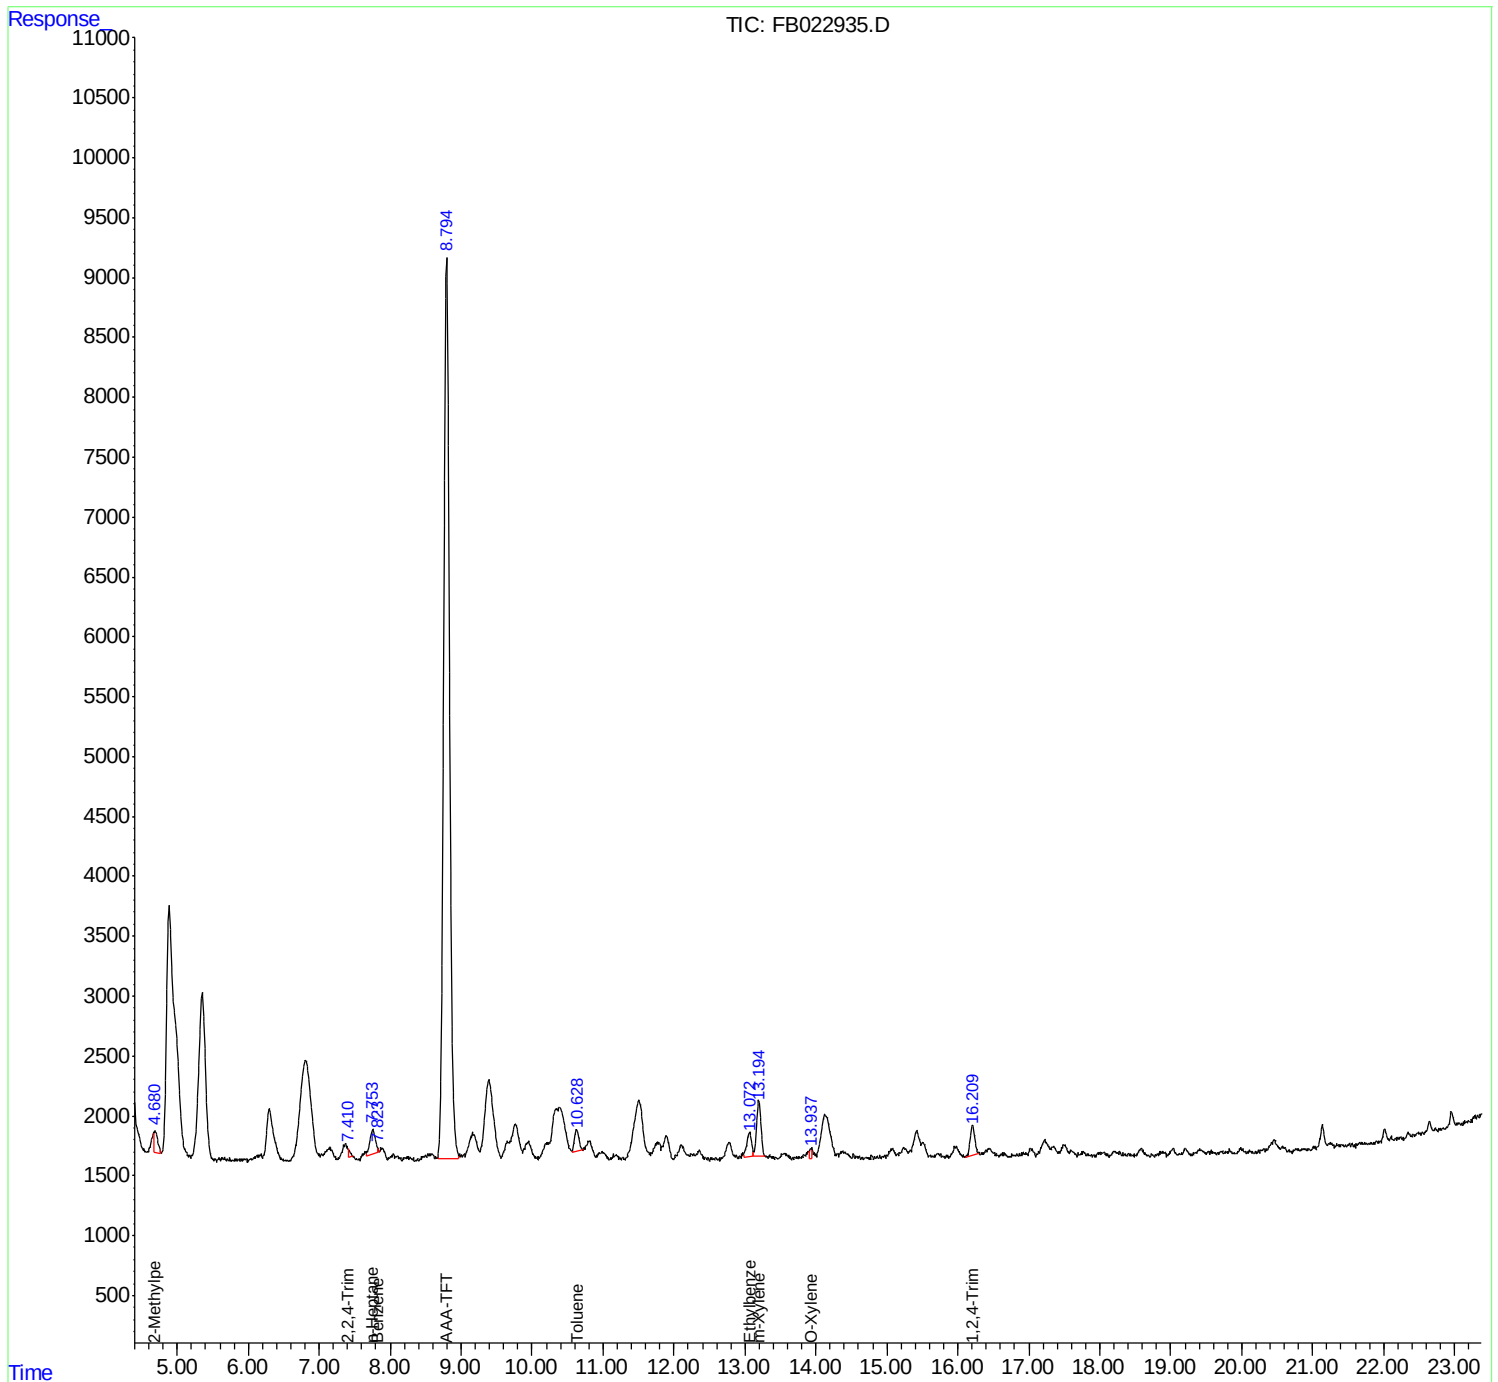


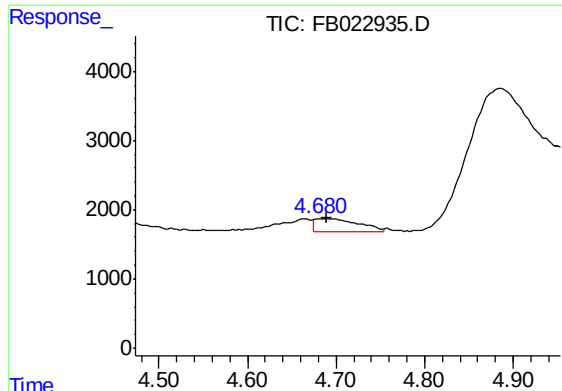

#1 2-Methylpentane


R.T.: 4.681 min
Delta R.T.: -0.008 min
Response: 6237
Conc: 0.19 ng/ml

Instrument :
FID_B
ClientSampleId :
SB-37-(8-10)

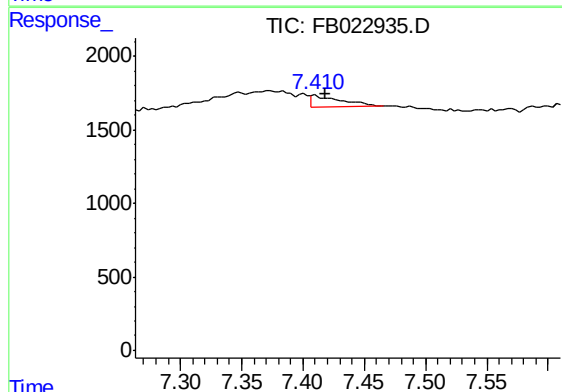


#2 2,2,4-Trimethylpentane

R.T.: 7.410 min
Delta R.T.: -0.008 min
Response: 1438
Conc: 0.04 ng/ml

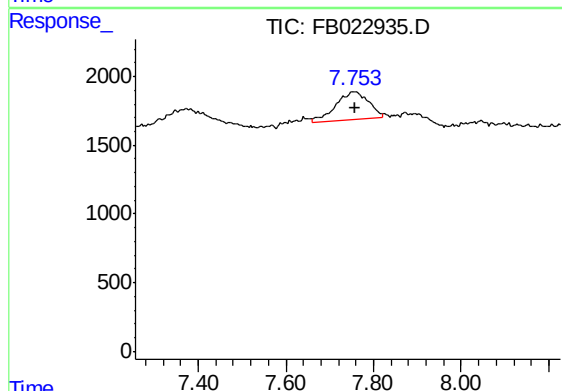


#3 n-Heptane

R.T.: 7.755 min
Delta R.T.: -0.003 min
Response: 10630
Conc: 0.31 ng/ml

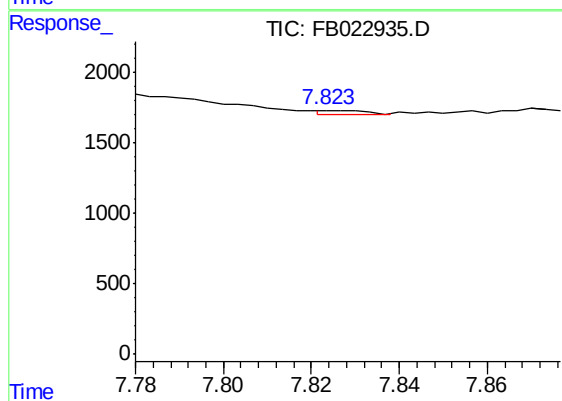

#4 Benzene


R.T.: 7.826 min
Delta R.T.: -0.067 min
Response: 216
Conc: 0.00 ng/ml

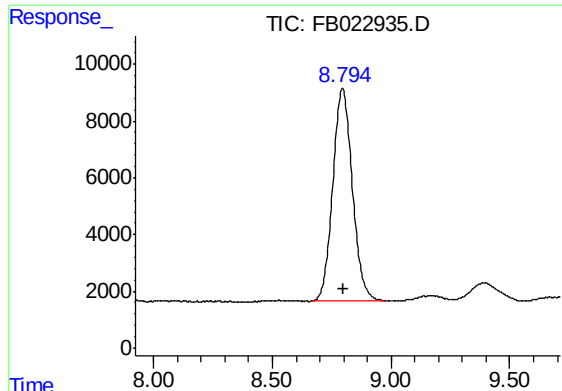

#5 AAA-TFT


R.T.: 8.796 min
Delta R.T.: -0.004 min
Response: 432610
Conc: 19.22 ng/ml

Instrument :
FID_B
ClientSampleId :
SB-37-(8-10)

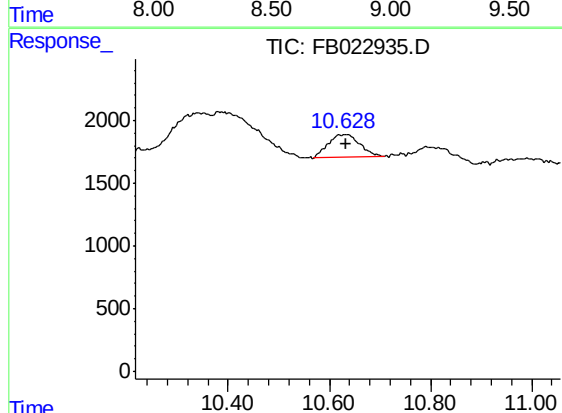


#6 Toluene

R.T.: 10.629 min
Delta R.T.: -0.002 min
Response: 7869
Conc: 0.18 ng/ml

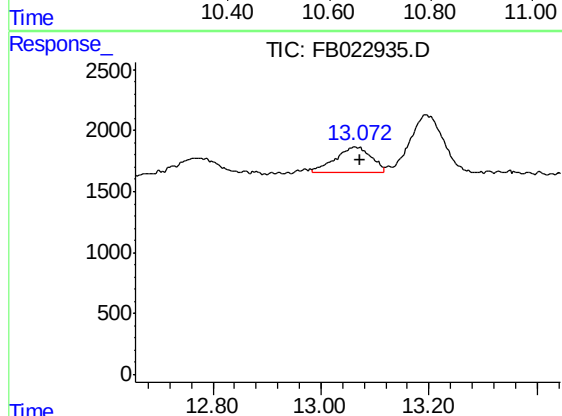


#7 Ethylbenzene

R.T.: 13.063 min
Delta R.T.: -0.009 min
Response: 9640
Conc: 0.24 ng/ml

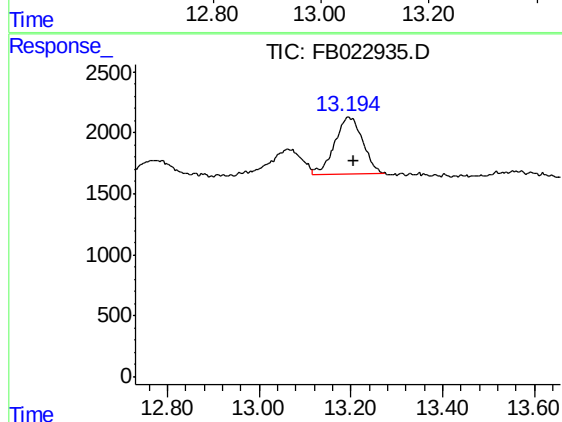

#8 m-Xylene


R.T.: 13.195 min
Delta R.T.: -0.010 min
Response: 19745
Conc: 0.52 ng/ml

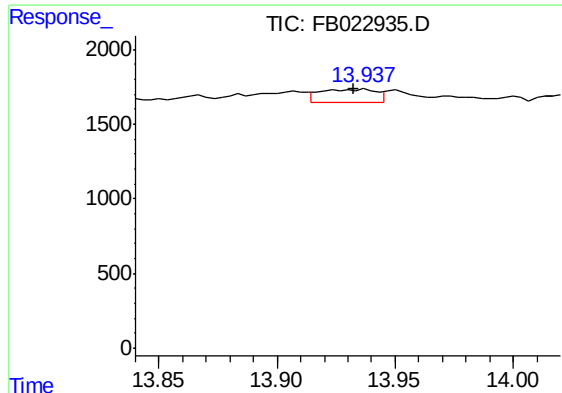

#9 O-Xylene

R.T.: 13.930 min
Delta R.T.: -0.002 min
Response: 1414
Conc: 0.04 ng/ml

Instrument :
FID_B
ClientSampleId :
SB-37-(8-10)

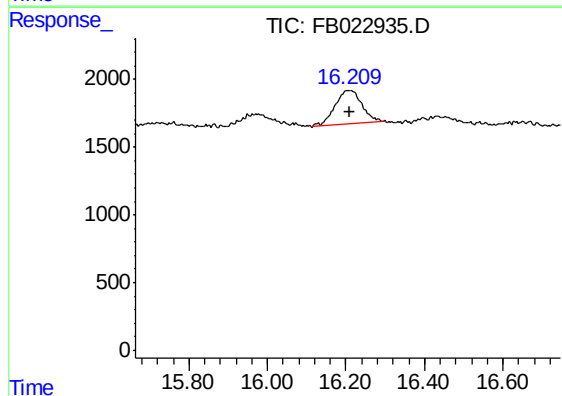

#10 1,2,4-Trimethylbenzene

R.T.: 16.211 min
Delta R.T.: 0.000 min
Response: 11746
Conc: 0.41 ng/ml