

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110819\
Data File : FB022937.D
Signal(s) : FID2B.CH
Acq On : 8 Nov 2019 12:14
Operator : DD/AJ
Sample : K5742-11
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
K5742-10MS

Integration File: Calibration.e
Quant Time: Nov 08 23:41:25 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB103119.M
Quant Title :
QLast Update : Thu Oct 31 14:57:42 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.796	377172	16.754 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.663	581	0.018 ng/ml
6) t Toluene	10.630	6591	0.153 ng/ml
7) t Ethylbenzene	13.072	3758	0.094 ng/ml
8) t m-Xylene	13.196	9596	0.254 ng/ml
10) t 1,2,4-Trimethylbenzene	16.209	7340	0.259 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110819\
Data File : FB022937.D
Signal(s) : FID2B.CH
Acq On : 8 Nov 2019 12:14
Operator : DD/AJ
Sample : K5742-11
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
K5742-10MS

Integration File: Calibration.e
Quant Time: Nov 08 23:41:25 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB103119.M
Quant Title :
QLast Update : Thu Oct 31 14:57:42 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

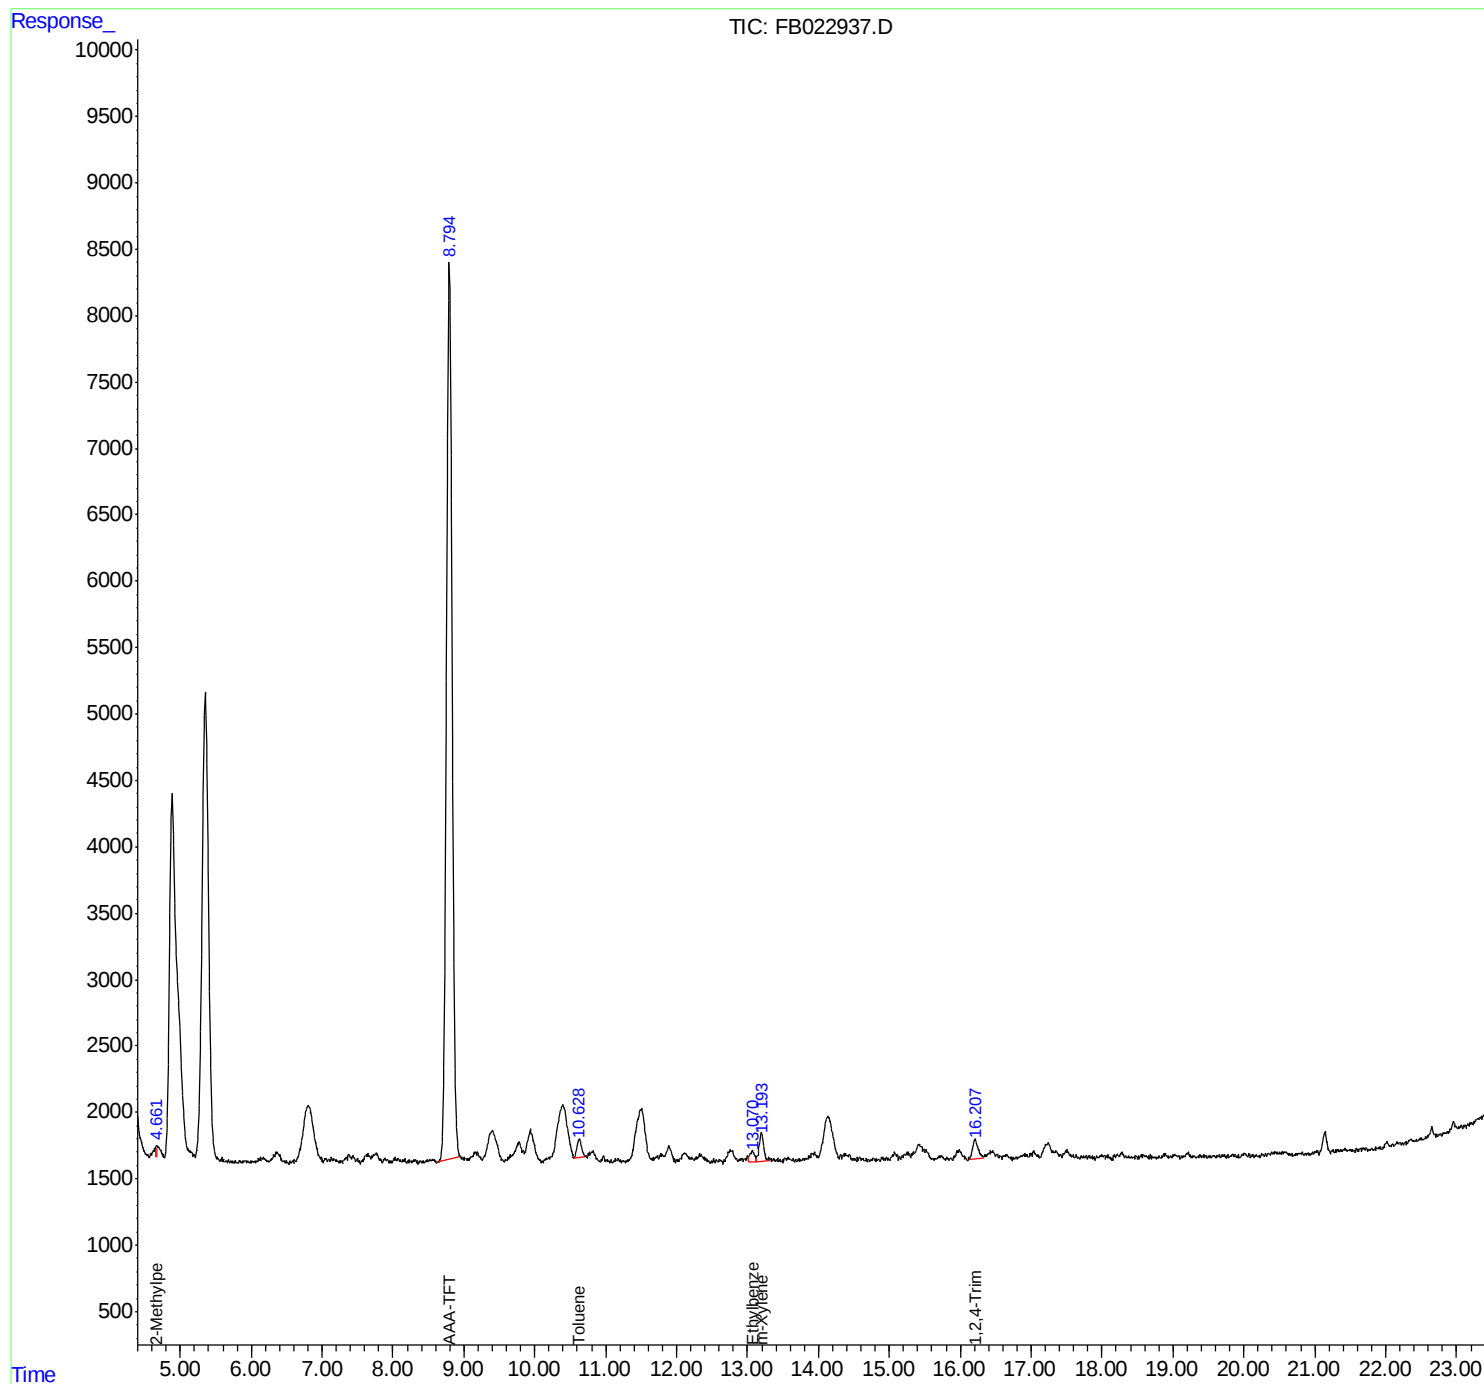


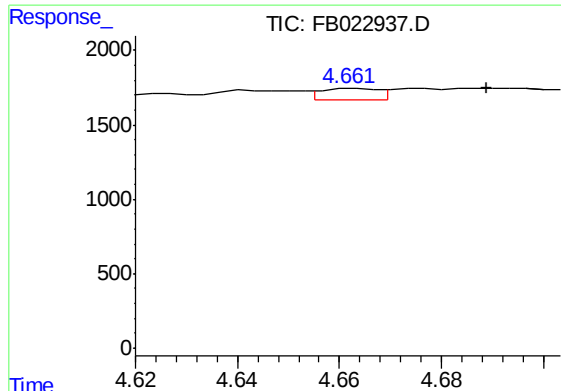

#1 2-Methylpentane


R.T.: 4.663 min
Delta R.T.: -0.026 min
Response: 581
Conc: 0.02 ng/ml

Instrument :
FID_B
ClientSampleId :
K5742-10MS

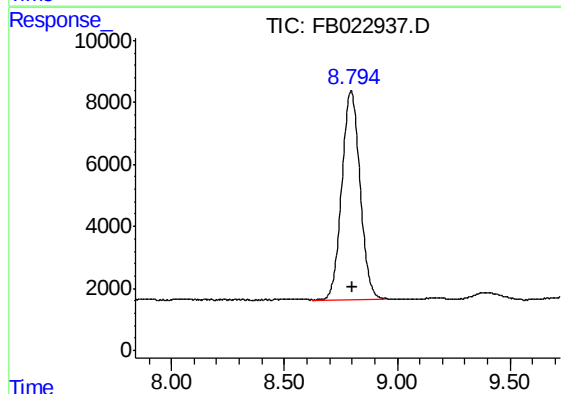


#5 AAA-TFT

R.T.: 8.796 min
Delta R.T.: -0.004 min
Response: 377172
Conc: 16.75 ng/ml

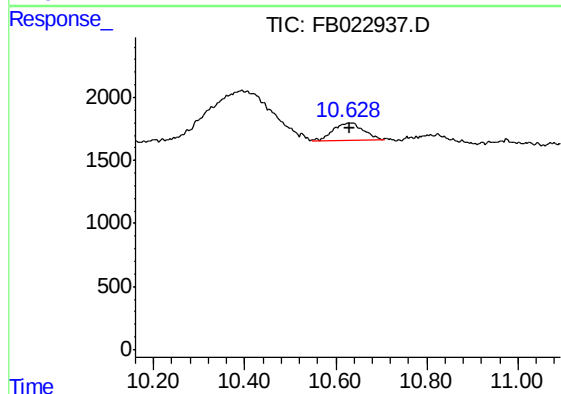


#6 Toluene

R.T.: 10.630 min
Delta R.T.: -0.002 min
Response: 6591
Conc: 0.15 ng/ml

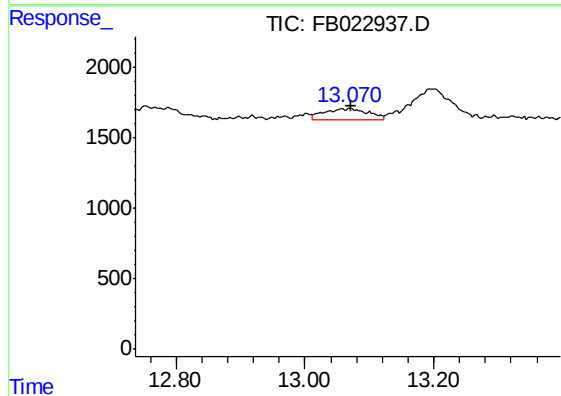

#7 Ethylbenzene


R.T.: 13.072 min
Delta R.T.: 0.000 min
Response: 3758
Conc: 0.09 ng/ml

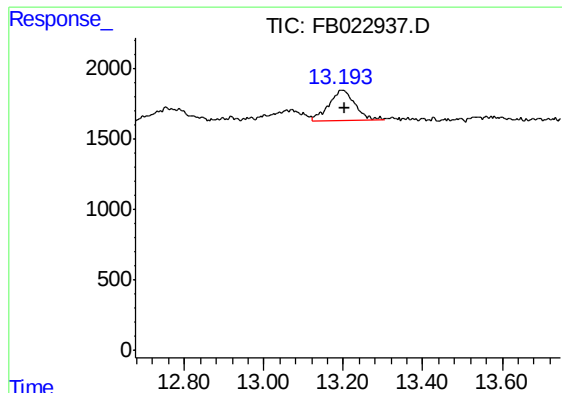

#8 m-Xylene

R.T.: 13.196 min
Delta R.T.: -0.009 min
Response: 9596
Conc: 0.25 ng/ml

Instrument :
FID_B
ClientSampleId :
K5742-10MS

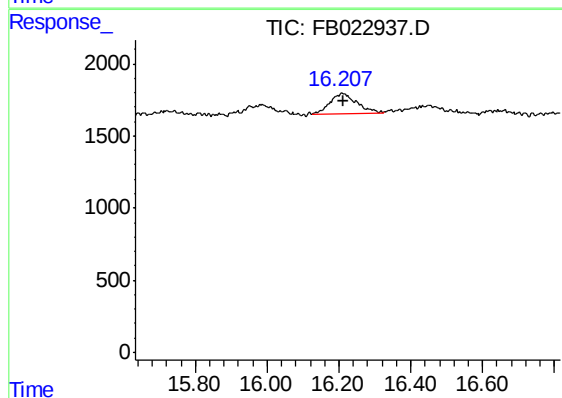

#10 1,2,4-Trimethylbenzene

R.T.: 16.209 min
Delta R.T.: -0.003 min
Response: 7340
Conc: 0.26 ng/ml