

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110819\
 Data File : FB022942.D
 Signal(s) : FID2B.CH
 Acq On : 8 Nov 2019 14:53
 Operator : DD/AJ
 Sample : K5742-13
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 (ERB)-EQUIPMENT-RINSATE-BLAN

Integration File: Calibration.e
 Quant Time: Nov 08 23:42:06 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB103119.M
 Quant Title :
 QLast Update : Thu Oct 31 14:57:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.794	409056	18.171 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.663	128	0.004 ng/ml
2) t 2,2,4-Trimethylpentane	7.408	358	0.010 ng/ml
6) t Toluene	10.631	6108	0.142 ng/ml
7) t Ethylbenzene	13.064	2226	0.056 ng/ml
8) t m-Xylene	13.200	7521	0.199 ng/ml
9) t o-Xylene	13.930	3334	0.094 ng/ml
10) t 1,2,4-Trimethylbenzene	16.206	6370	0.225 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110819\
Data File : FB022942.D
Signal(s) : FID2B.CH
Acq On : 8 Nov 2019 14:53
Operator : DD/AJ
Sample : K5742-13
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
(ERB)-EQUIPMENT-RINSATE-BLAN

Integration File: Calibration.e
Quant Time: Nov 08 23:42:06 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB103119.M
Quant Title :
QLast Update : Thu Oct 31 14:57:42 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

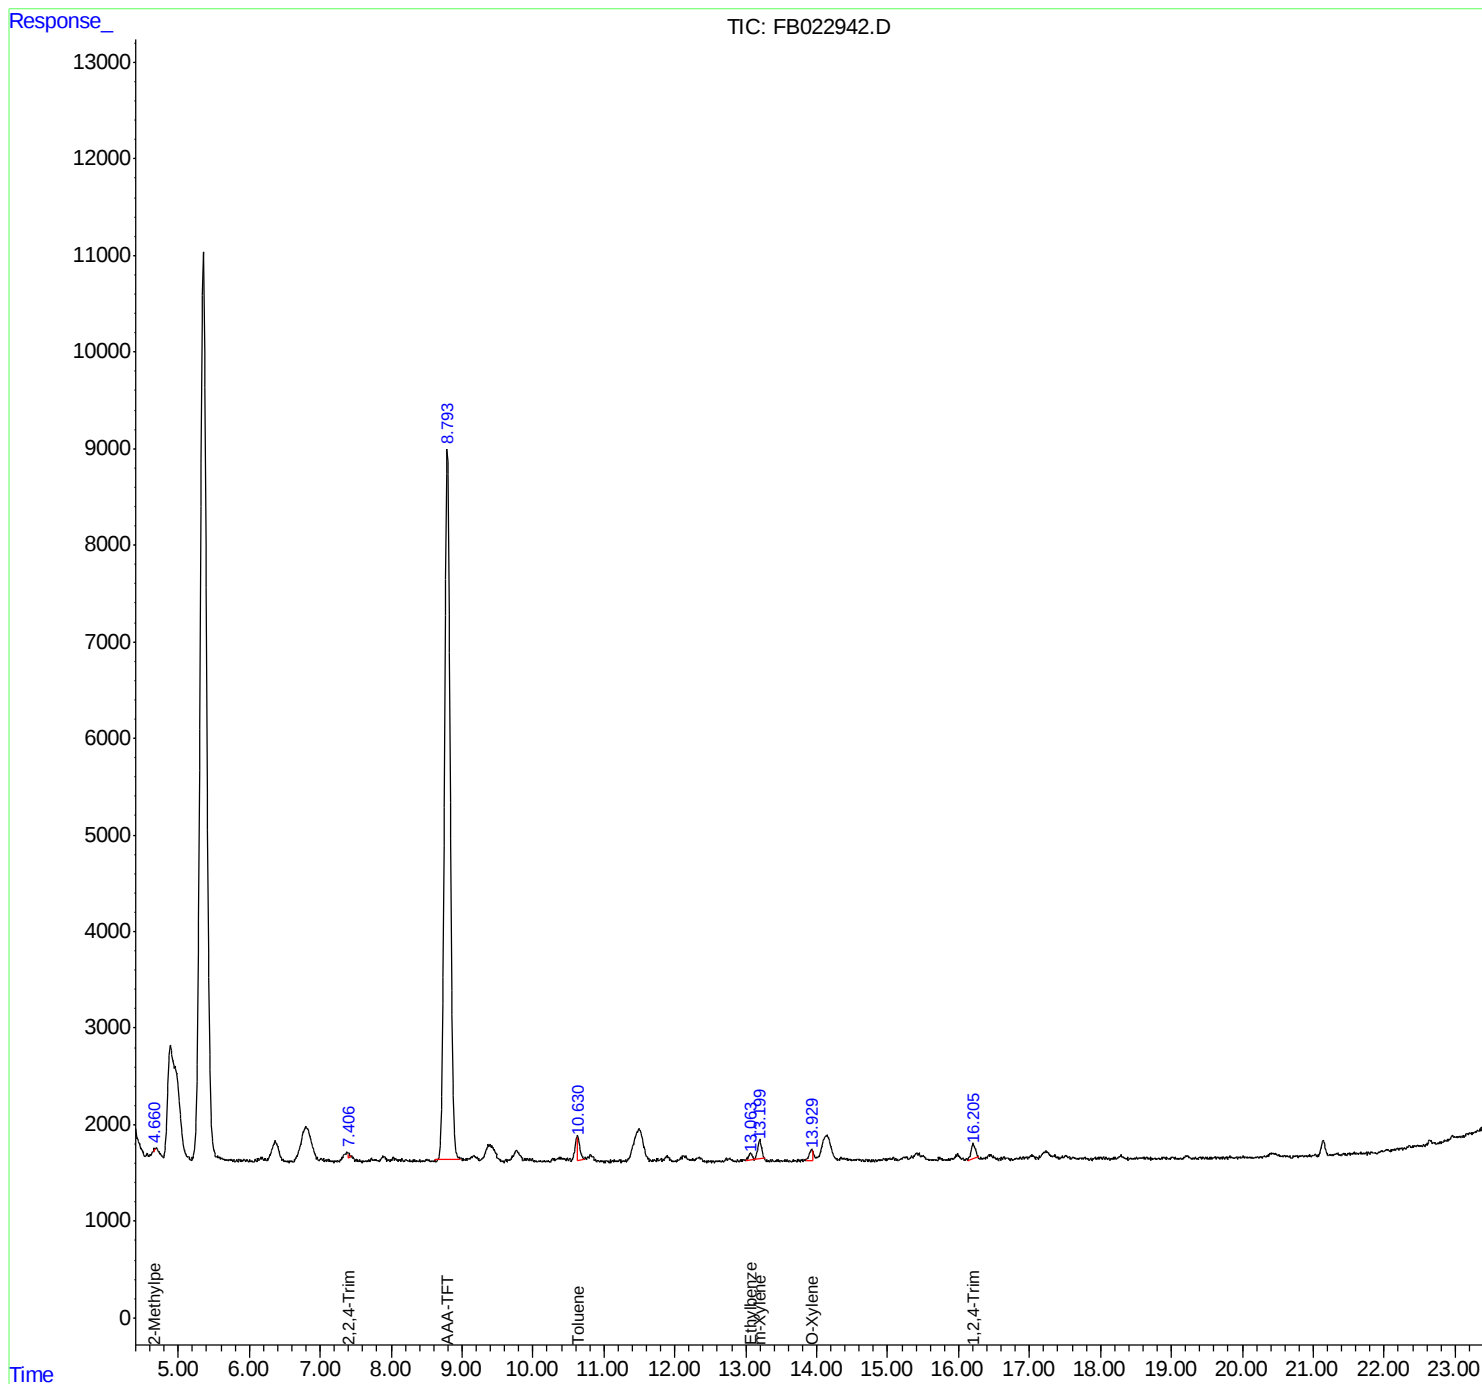


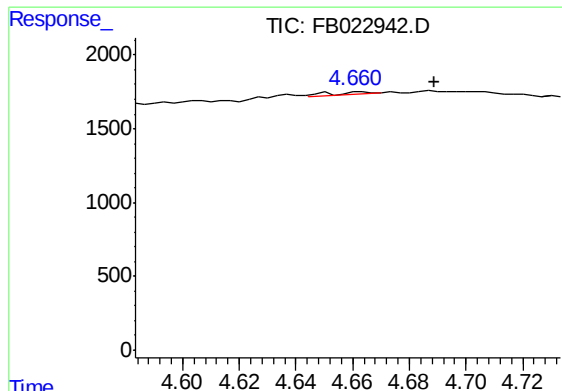

#1 2-Methylpentane


R.T.: 4.663 min
Delta R.T.: -0.026 min
Response: 128
Conc: 0.00 ng/ml

Instrument :
FID_B
ClientSampleId :
(ERB)-EQUIPMENT-RINSATE-BLAN

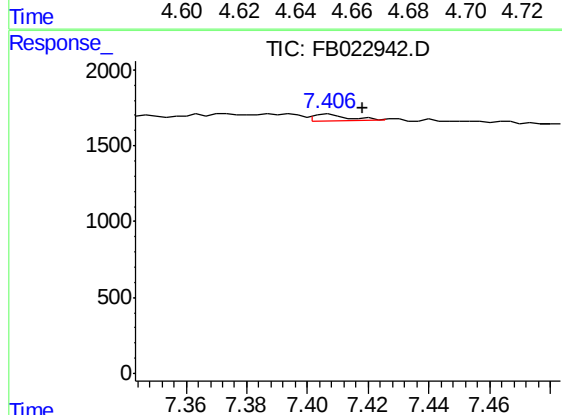


#2 2,2,4-Trimethylpentane

R.T.: 7.408 min
Delta R.T.: -0.010 min
Response: 358
Conc: 0.01 ng/ml

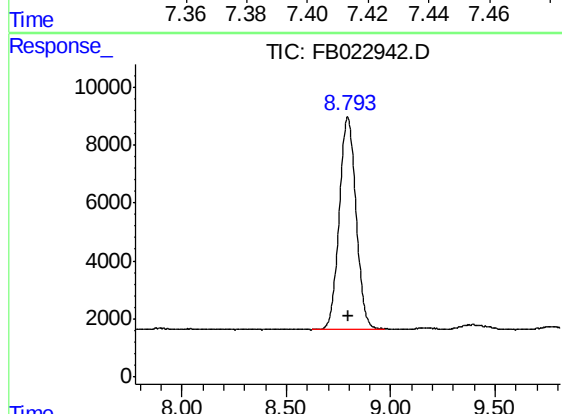


#5 AAA-TFT

R.T.: 8.794 min
Delta R.T.: -0.005 min
Response: 409056
Conc: 18.17 ng/ml

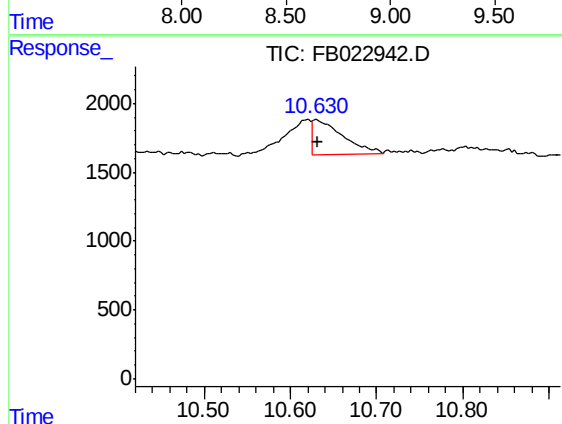

#6 Toluene


R.T.: 10.631 min
Delta R.T.: 0.000 min
Response: 6108
Conc: 0.14 ng/ml

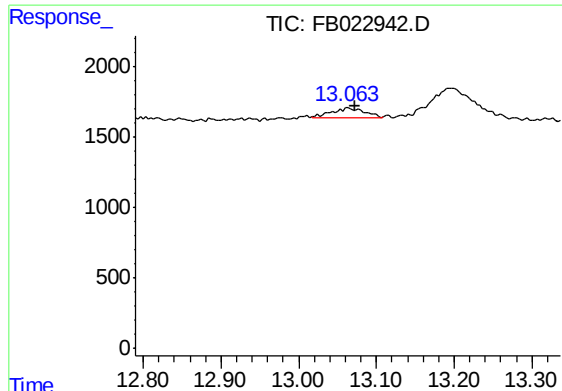

#7 Ethylbenzene


R.T.: 13.064 min
Delta R.T.: -0.007 min
Response: 2226
Conc: 0.06 ng/ml

Instrument :
FID_B
ClientSampleId :
(ERB)-EQUIPMENT-RINSATE-BLAN

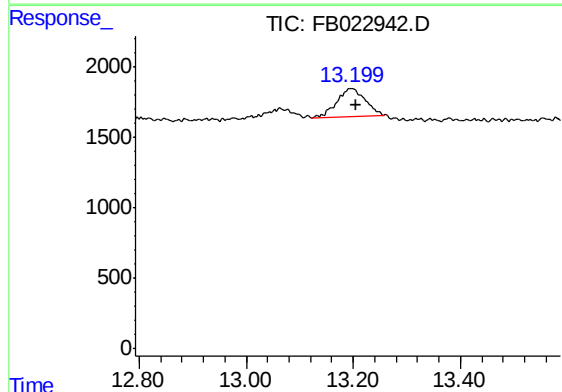


#8 m-Xylene

R.T.: 13.200 min
Delta R.T.: -0.005 min
Response: 7521
Conc: 0.20 ng/ml

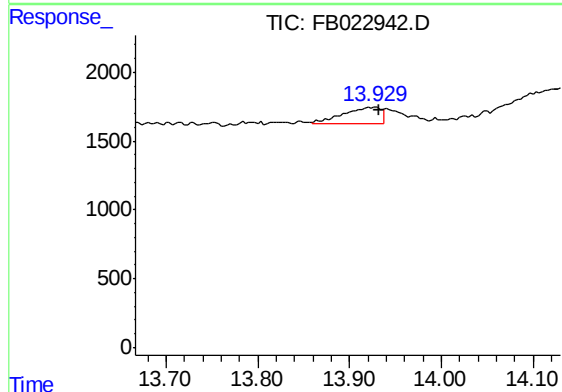

#9 o-Xylene

R.T.: 13.930 min
Delta R.T.: -0.003 min
Response: 3334
Conc: 0.09 ng/ml

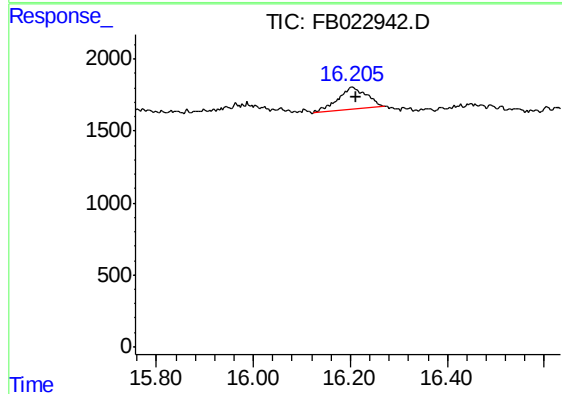

#10 1,2,4-Trimethylbenzene

R.T.: 16.206 min
Delta R.T.: -0.005 min
Response: 6370
Conc: 0.22 ng/ml