

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110819\
 Data File : FB022944.D
 Signal(s) : FID2B.CH
 Acq On : 8 Nov 2019 15:53
 Operator : DD/AJ
 Sample : K5742-10MSD
 Misc : 5.06g/5.00ml DI WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 SB-38-(2-4)MSD

Integration File: Calibration.e
 Quant Time: Nov 08 23:42:20 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB103119.M
 Quant Title :
 QLast Update : Thu Oct 31 14:57:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.794	424251	18.846 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.685	959793	29.837 ng/ml
2) t 2,2,4-Trimethylpentane	7.410	1090436	30.890 ng/ml
3) t n-Heptane	7.752	353147	10.152 ng/ml
4) t Benzene	7.886	427999	9.881 ng/ml
6) t Toluene	10.625	1254036	29.089 ng/ml
7) t Ethylbenzene	13.065	393260	9.851 ng/ml
8) t m-Xylene	13.199	743607	19.689 ng/ml
9) t O-Xylene	13.927	697955	19.583 ng/ml
10) t 1,2,4-Trimethylbenzene	16.206	576816	20.340 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110819\
Data File : FB022944.D
Signal(s) : FID2B.CH
Acq On : 8 Nov 2019 15:53
Operator : DD/AJ
Sample : K5742-10MSD
Misc : 5.06g/5.00ml DI WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
SB-38-(2-4)MSD

Integration File: Calibration.e
Quant Time: Nov 08 23:42:20 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB103119.M
Quant Title :
QLast Update : Thu Oct 31 14:57:42 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

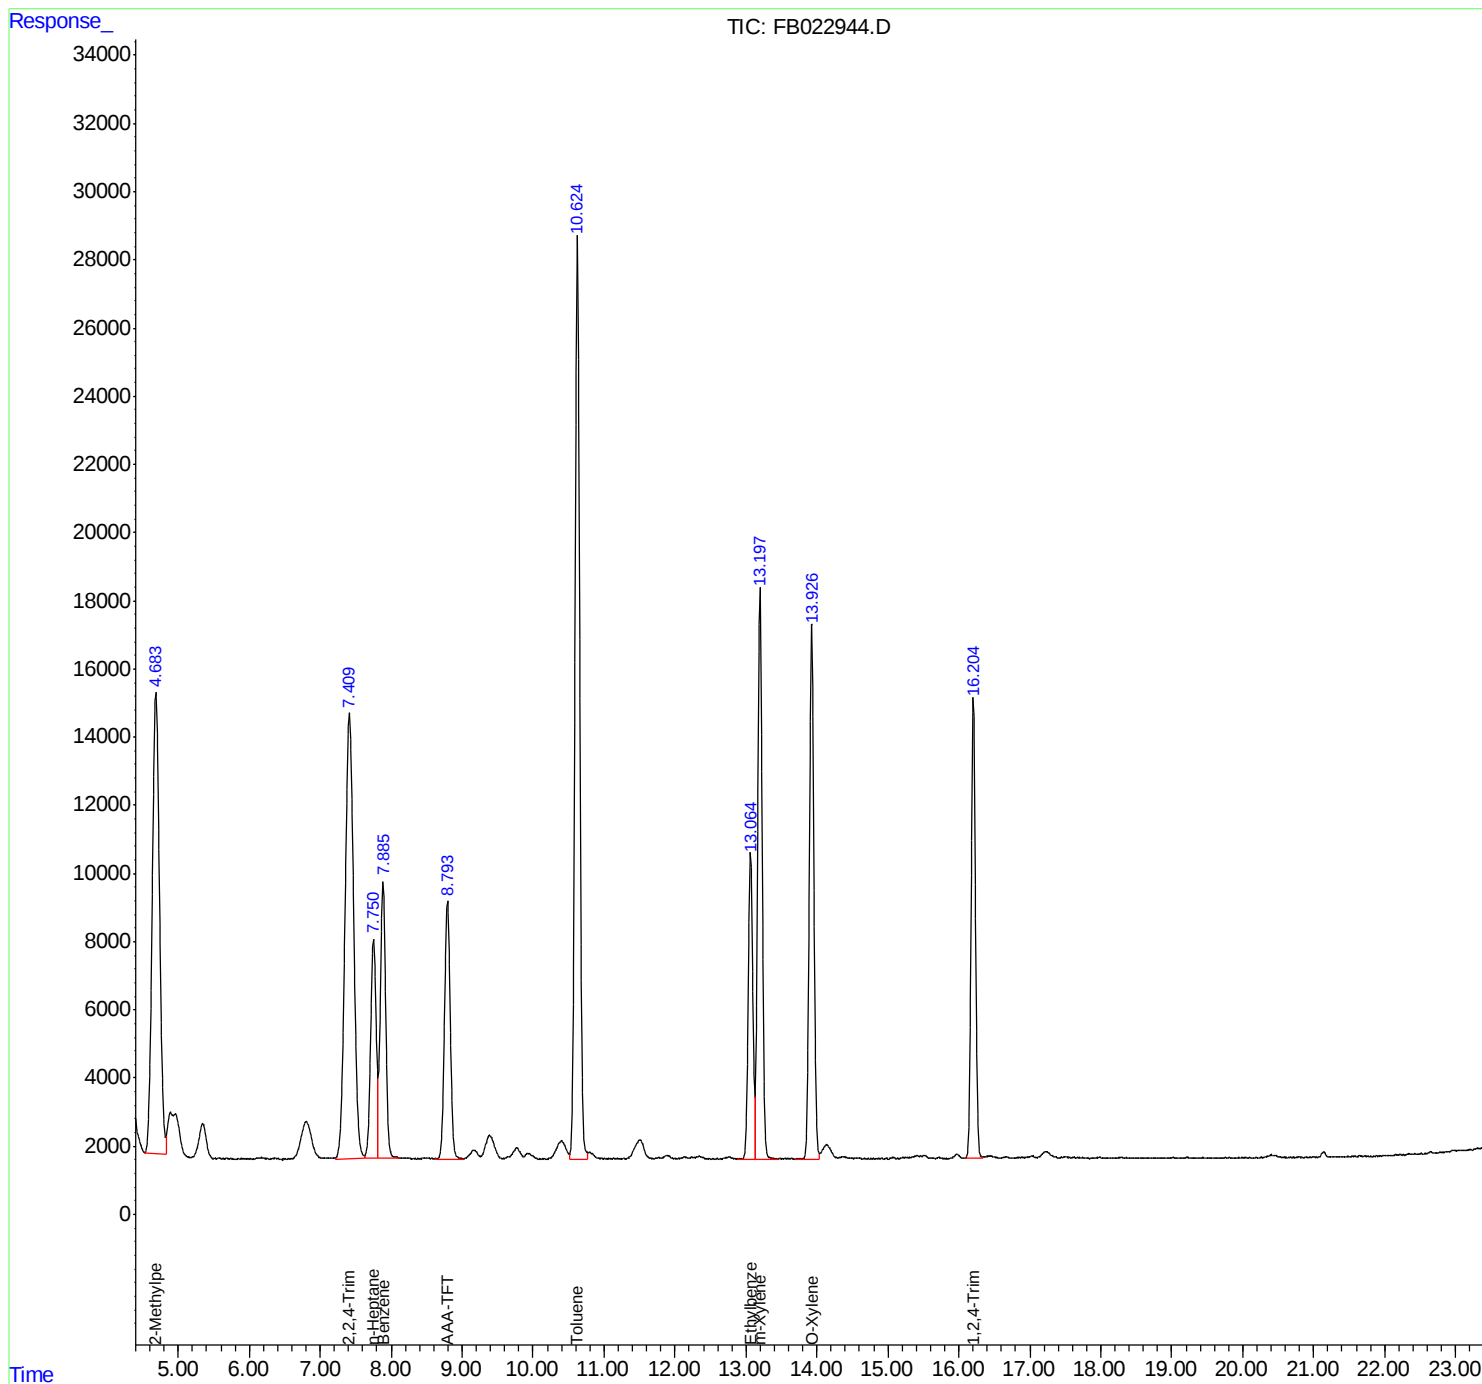


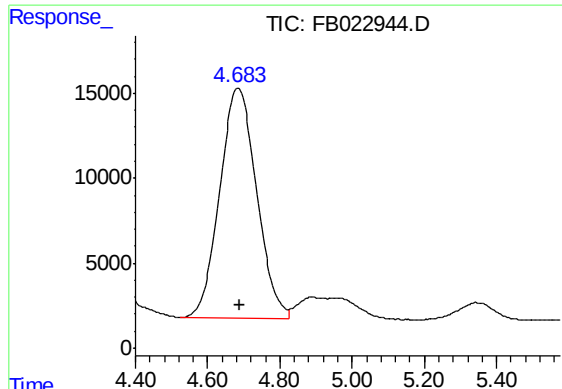

#1 2-Methylpentane


R.T.: 4.685 min
Delta R.T.: -0.004 min
Response: 959793
Conc: 29.84 ng/ml

Instrument :
FID_B
ClientSampleId :
SB-38-(2-4)MSD

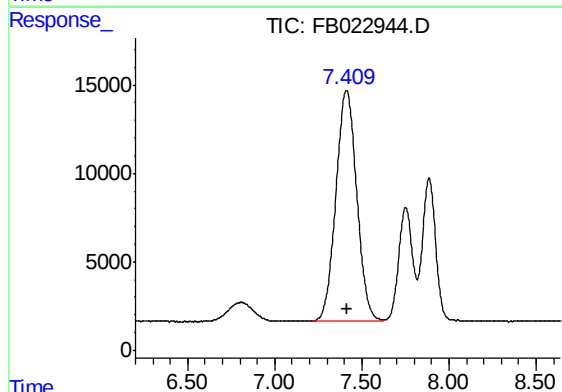


#2 2,2,4-Trimethylpentane

R.T.: 7.410 min
Delta R.T.: -0.008 min
Response: 1090436
Conc: 30.89 ng/ml

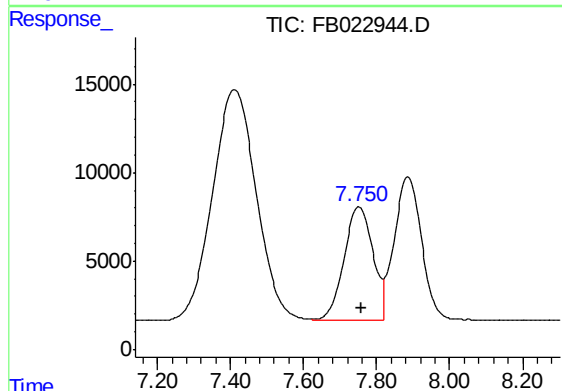


#3 n-Heptane

R.T.: 7.752 min
Delta R.T.: -0.007 min
Response: 353147
Conc: 10.15 ng/ml

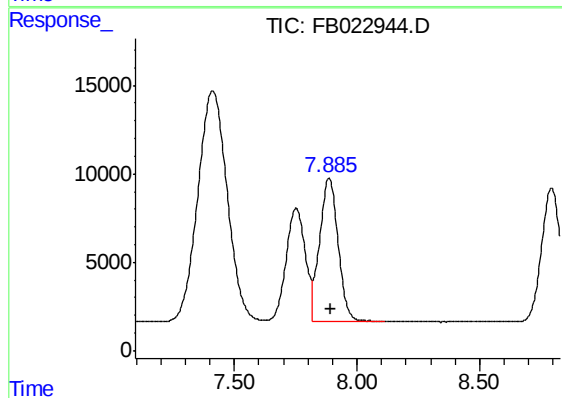

#4 Benzene


R.T.: 7.886 min
Delta R.T.: -0.007 min
Response: 427999
Conc: 9.88 ng/ml

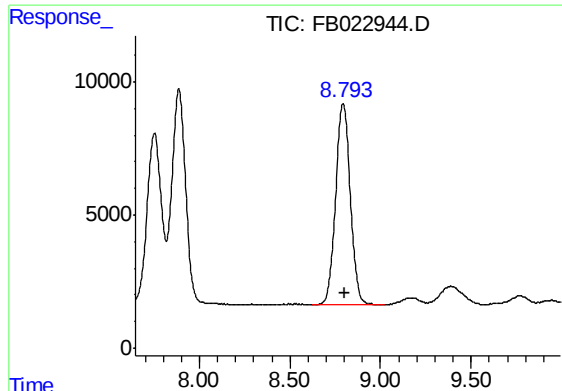

#5 AAA-TFT


R.T.: 8.794 min
Delta R.T.: -0.006 min
Response: 424251
Conc: 18.85 ng/ml

Instrument :
FID_B
ClientSampleId :
SB-38-(2-4)MSD

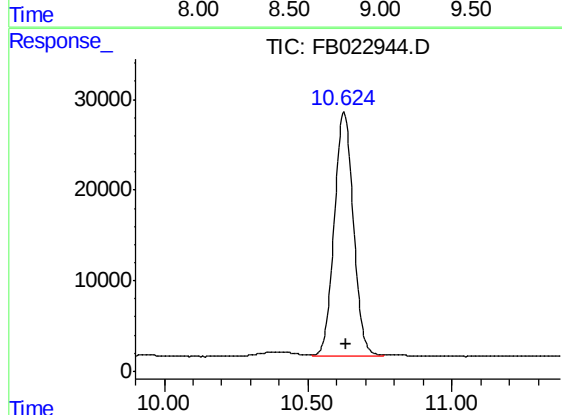


#6 Toluene

R.T.: 10.625 min
Delta R.T.: -0.007 min
Response: 1254036
Conc: 29.09 ng/ml

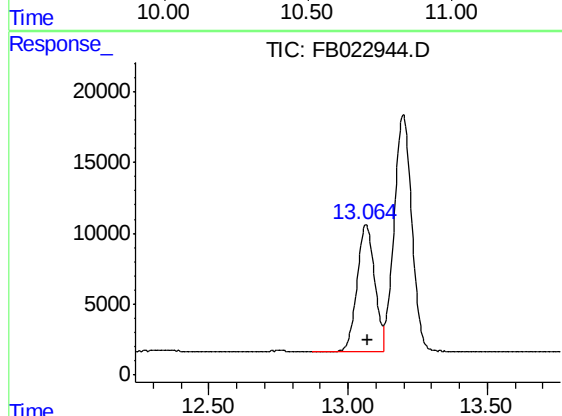


#7 Ethylbenzene

R.T.: 13.065 min
Delta R.T.: -0.006 min
Response: 393260
Conc: 9.85 ng/ml

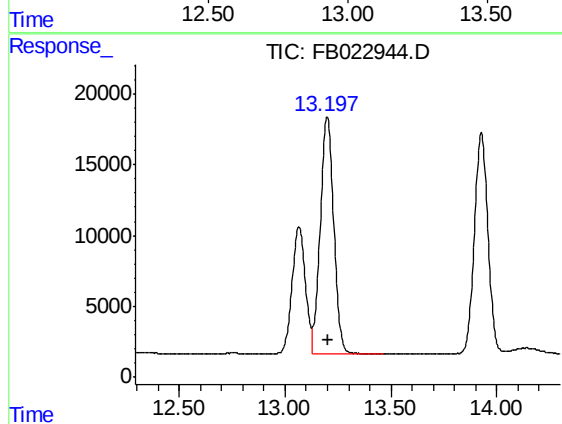

#8 m-Xylene


R.T.: 13.199 min
Delta R.T.: -0.006 min
Response: 743607
Conc: 19.69 ng/ml

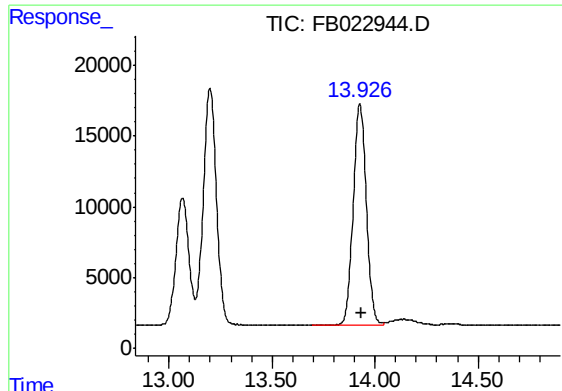

#9 O-Xylene

R.T.: 13.927 min
Delta R.T.: -0.006 min
Response: 697955
Conc: 19.58 ng/ml

Instrument :
FID_B
ClientSampleId :
SB-38-(2-4)MSD

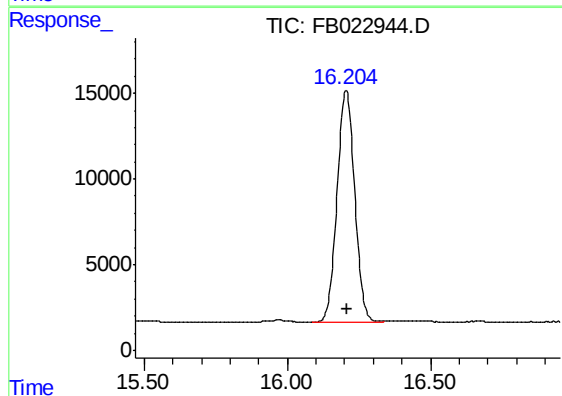

#10 1,2,4-Trimethylbenzene

R.T.: 16.206 min
Delta R.T.: -0.005 min
Response: 576816
Conc: 20.34 ng/ml