

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110819\
 Data File : FB022949.D
 Signal(s) : FID2B.CH
 Acq On : 8 Nov 2019 18:58
 Operator : DD/AJ
 Sample : K5742-07 50X
 Misc : 5.00g/5.00ml DI WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 SB-35-(6-8)

Integration File: Calibration.e
 Quant Time: Nov 08 23:42:57 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB103119.M
 Quant Title :
 QLast Update : Thu Oct 31 14:57:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.796	552448	24.540 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.691	5514	0.171 ng/ml
2) t 2,2,4-Trimethylpentane	7.427	5369	0.152 ng/ml
3) t n-Heptane	7.771	40294	1.158 ng/ml
7) t Ethylbenzene	13.020	999669	25.040 ng/ml
9) t O-Xylene	13.945	134847	3.784 ng/ml
10) t 1,2,4-Trimethylbenzene	16.207	542050	19.114 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110819\
Data File : FB022949.D
Signal(s) : FID2B.CH
Acq On : 8 Nov 2019 18:58
Operator : DD/AJ
Sample : K5742-07 50X
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
SB-35-(6-8)

Integration File: Calibration.e
Quant Time: Nov 08 23:42:57 2019
Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB103119.M
Quant Title :
QLast Update : Thu Oct 31 14:57:42 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

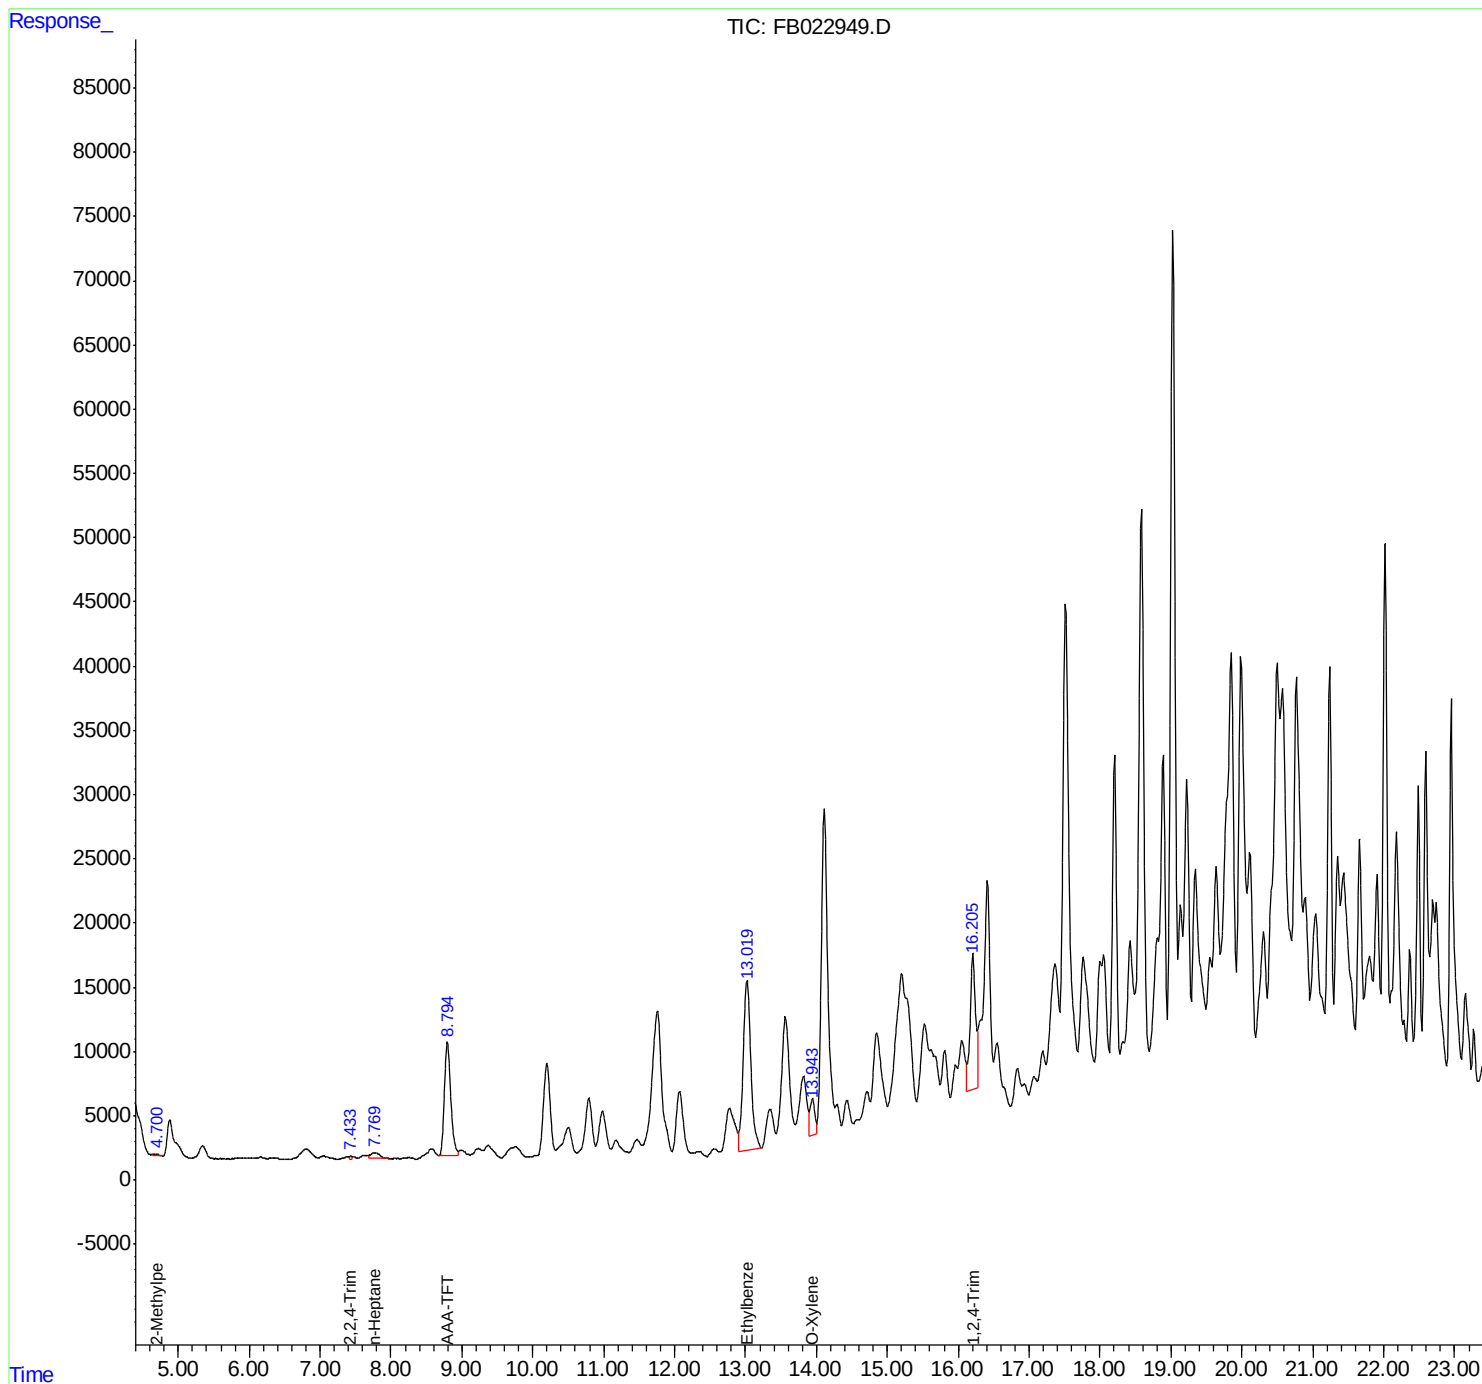


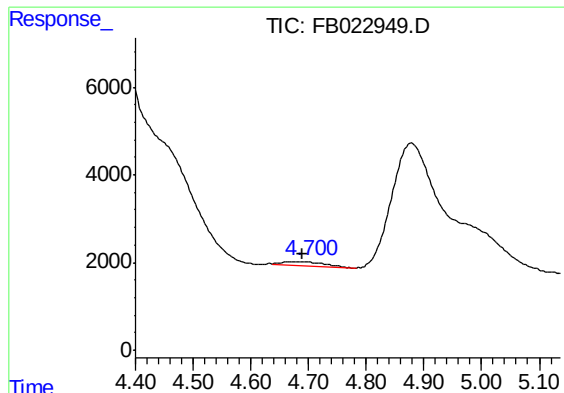

#1 2-Methylpentane


R.T.: 4.691 min
Delta R.T.: 0.002 min
Response: 5514
Conc: 0.17 ng/ml

Instrument :
FID_B
ClientSampleId :
SB-35-(6-8)

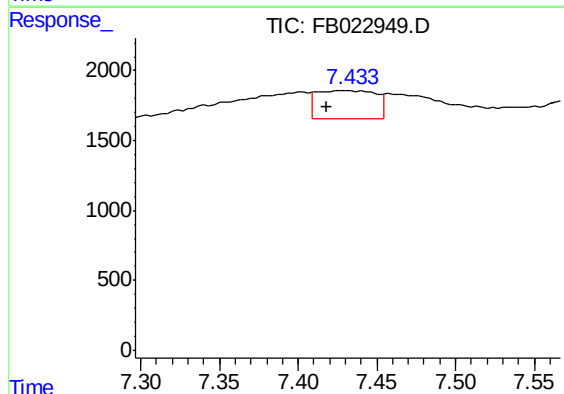


#2 2,2,4-Trimethylpentane

R.T.: 7.427 min
Delta R.T.: 0.009 min
Response: 5369
Conc: 0.15 ng/ml

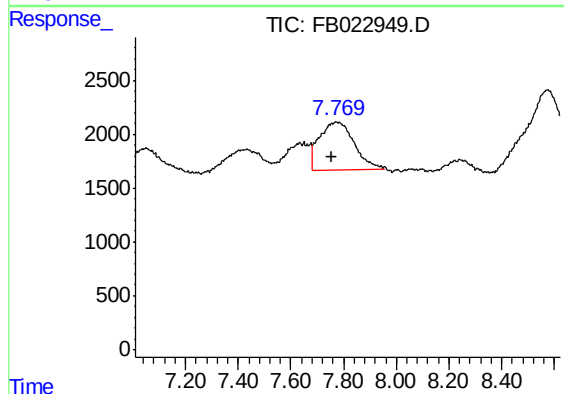


#3 n-Heptane

R.T.: 7.771 min
Delta R.T.: 0.012 min
Response: 40294
Conc: 1.16 ng/ml

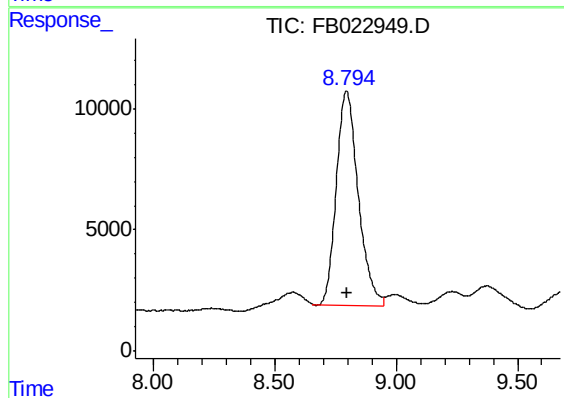

#5 AAA-TFT


R.T.: 8.796 min
Delta R.T.: -0.004 min
Response: 552448
Conc: 24.54 ng/ml

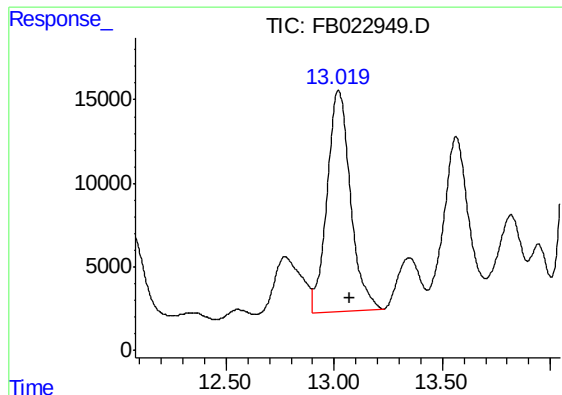

#7 Ethylbenzene


R.T.: 13.020 min
Delta R.T.: -0.052 min
Response: 999669
Conc: 25.04 ng/ml

Instrument :
FID_B
ClientSampleId :
SB-35-(6-8)

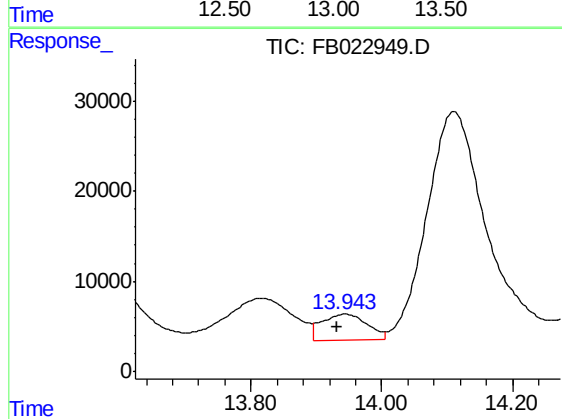

#9 O-Xylene

R.T.: 13.945 min
Delta R.T.: 0.013 min
Response: 134847
Conc: 3.78 ng/ml

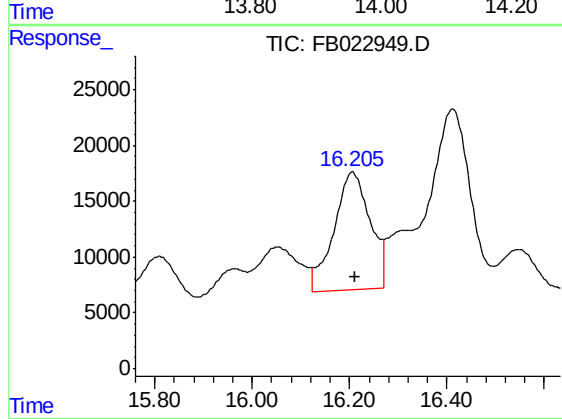

#10 1,2,4-Trimethylbenzene

R.T.: 16.207 min
Delta R.T.: -0.004 min
Response: 542050
Conc: 19.11 ng/ml