

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110819\
 Data File : FB022934.D
 Signal(s) : FID2B.CH
 Acq On : 8 Nov 2019 10:44
 Operator : DD/AJ
 Sample : BSF1108S1
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF1108S1

Integration File: Calibration.e
 Quant Time: Nov 08 23:41:06 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB103119.M
 Quant Title :
 QLast Update : Thu Oct 31 14:57:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.795	461808	20.514 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.687	974165	30.284 ng/ml
2) t 2,2,4-Trimethylpentane	7.414	1091256	30.913 ng/ml
3) t n-Heptane	7.754	351771	10.113 ng/ml
4) t Benzene	7.889	442983	10.227 ng/ml
6) t Toluene	10.627	1312097	30.436 ng/ml
7) t Ethylbenzene	13.067	411405	10.305 ng/ml
8) t m-Xylene	13.200	789532	20.905 ng/ml
9) t O-Xylene	13.928	738799	20.729 ng/ml
10) t 1,2,4-Trimethylbenzene	16.206	585012	20.629 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110819\
Data File : FB022934.D
Signal(s) : FID2B.CH
Acq On : 8 Nov 2019 10:44
Operator : DD/AJ
Sample : BSF1108S1
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF1108S1

Integration File: Calibration.e
Quant Time: Nov 08 23:41:06 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB103119.M
Quant Title :
QLast Update : Thu Oct 31 14:57:42 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

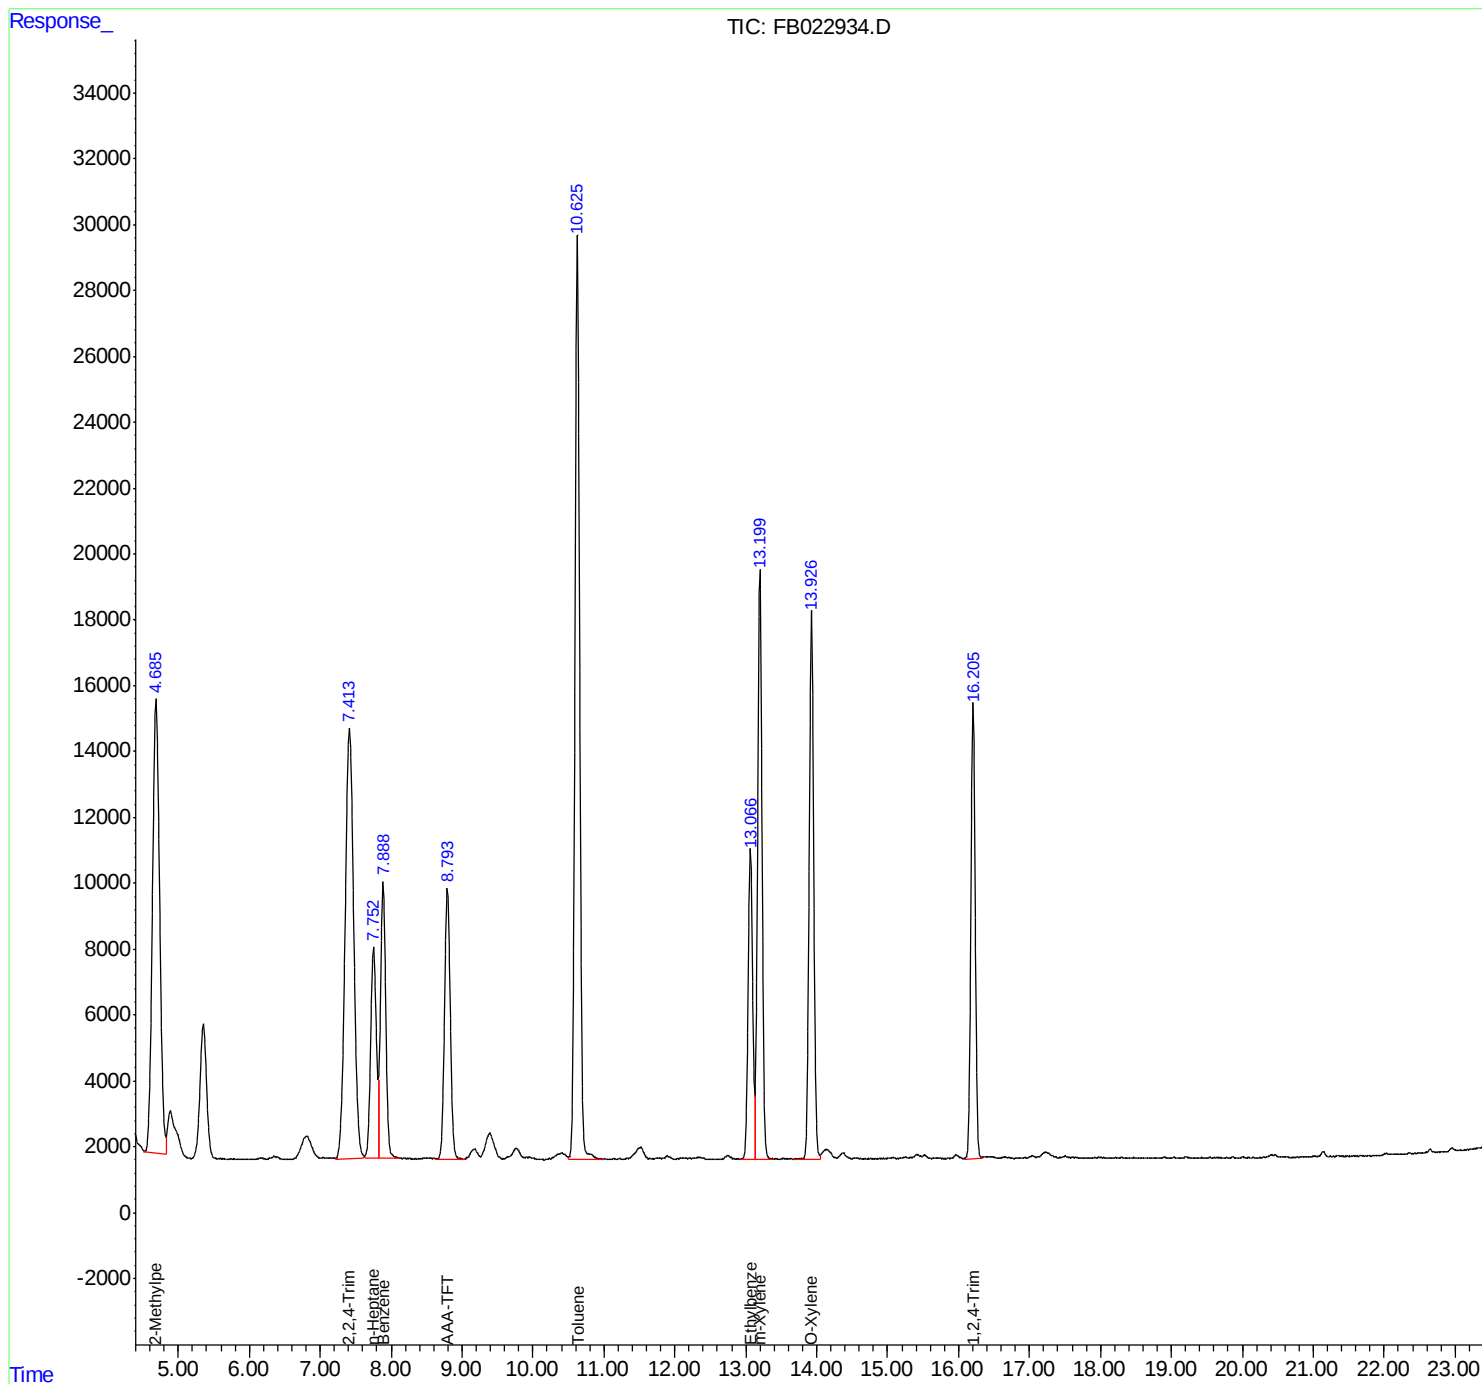


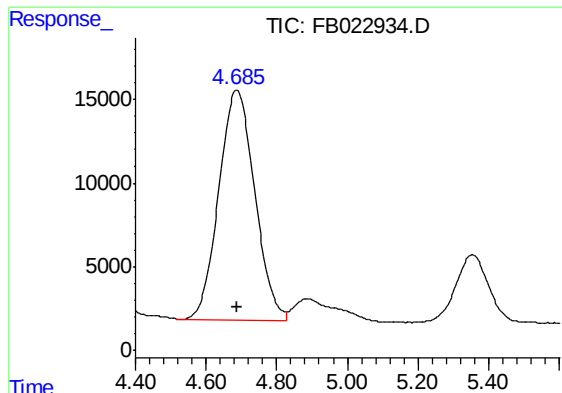

#1 2-Methylpentane


R.T.: 4.687 min
Delta R.T.: -0.002 min
Response: 974165
Conc: 30.28 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1108S1

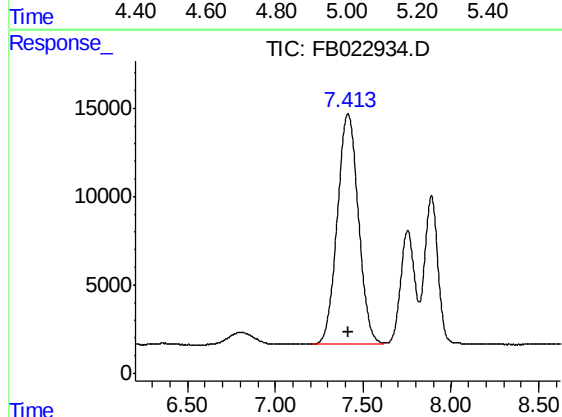


#2 2,2,4-Trimethylpentane

R.T.: 7.414 min
Delta R.T.: -0.004 min
Response: 1091256
Conc: 30.91 ng/ml

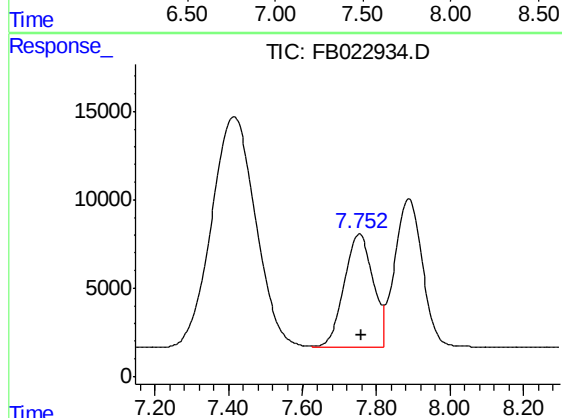


#3 n-Heptane

R.T.: 7.754 min
Delta R.T.: -0.004 min
Response: 351771
Conc: 10.11 ng/ml

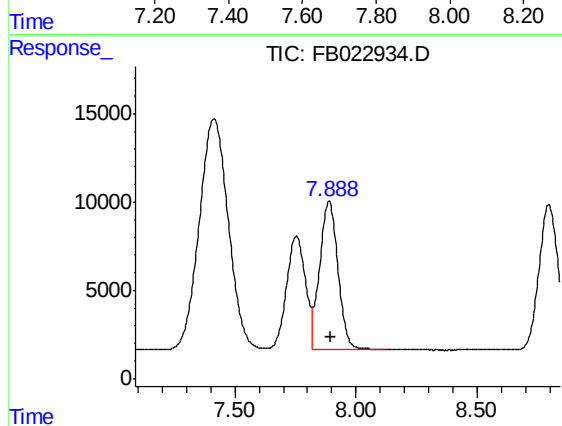

#4 Benzene


R.T.: 7.889 min
Delta R.T.: -0.004 min
Response: 442983
Conc: 10.23 ng/ml

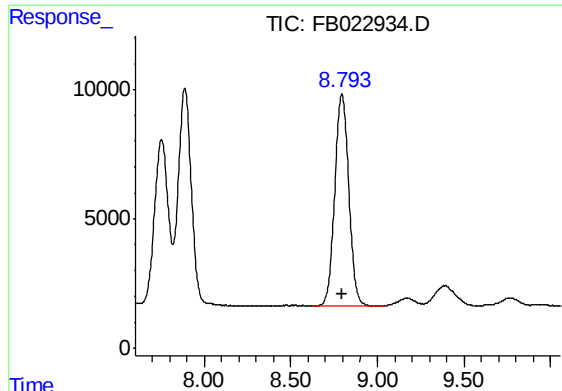

#5 AAA-TFT


R.T.: 8.795 min
Delta R.T.: -0.004 min
Response: 461808
Conc: 20.51 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1108S1

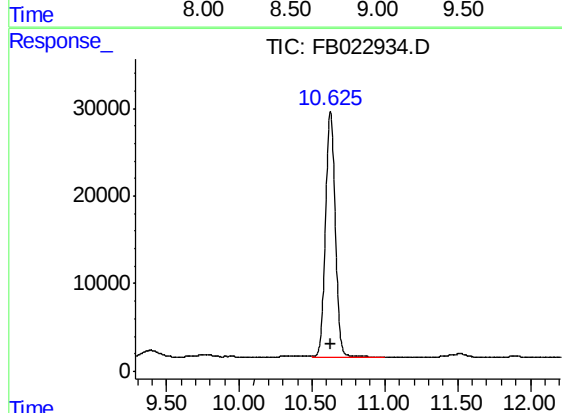


#6 Toluene

R.T.: 10.627 min
Delta R.T.: -0.005 min
Response: 1312097
Conc: 30.44 ng/ml

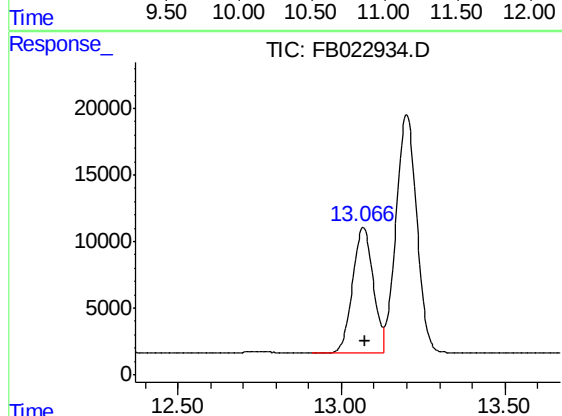


#7 Ethylbenzene

R.T.: 13.067 min
Delta R.T.: -0.005 min
Response: 411405
Conc: 10.31 ng/ml

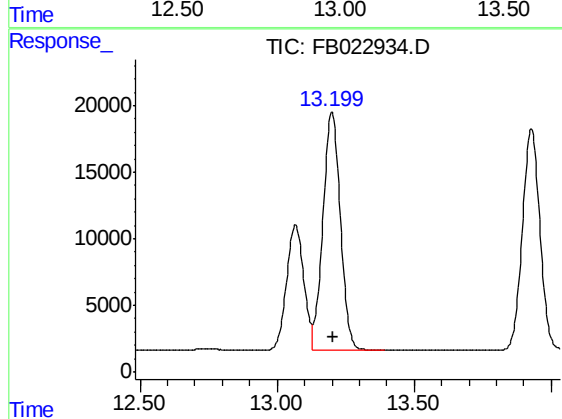

#8 m-Xylene


R.T.: 13.200 min
Delta R.T.: -0.005 min
Response: 789532
Conc: 20.91 ng/ml

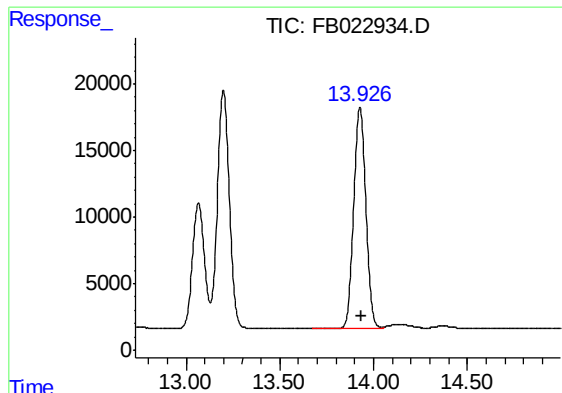

#9 O-Xylene

R.T.: 13.928 min
Delta R.T.: -0.005 min
Response: 738799
Conc: 20.73 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1108S1

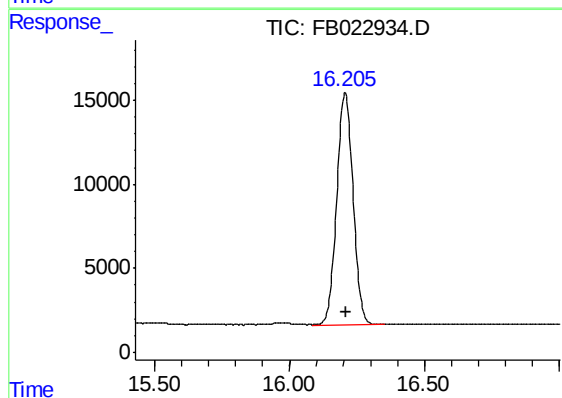

#10 1,2,4-Trimethylbenzene

R.T.: 16.206 min
Delta R.T.: -0.005 min
Response: 585012
Conc: 20.63 ng/ml