

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110819\
Data File : FB022938.D
Signal(s) : FID2B.CH
Acq On : 8 Nov 2019 12:44
Operator : DD/AJ
Sample : K5742-12
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
K5742-10MSD

Integration File: Calibration.e
Quant Time: Nov 08 23:41:33 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB103119.M
Quant Title :
QLast Update : Thu Oct 31 14:57:42 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.796	456836	20.293 ng/ml

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110819\
Data File : FB022938.D
Signal(s) : FID2B.CH
Acq On : 8 Nov 2019 12:44
Operator : DD/AJ
Sample : K5742-12
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
K5742-10MSD

Integration File: Calibration.e
Quant Time: Nov 08 23:41:33 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB103119.M
Quant Title :
QLast Update : Thu Oct 31 14:57:42 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

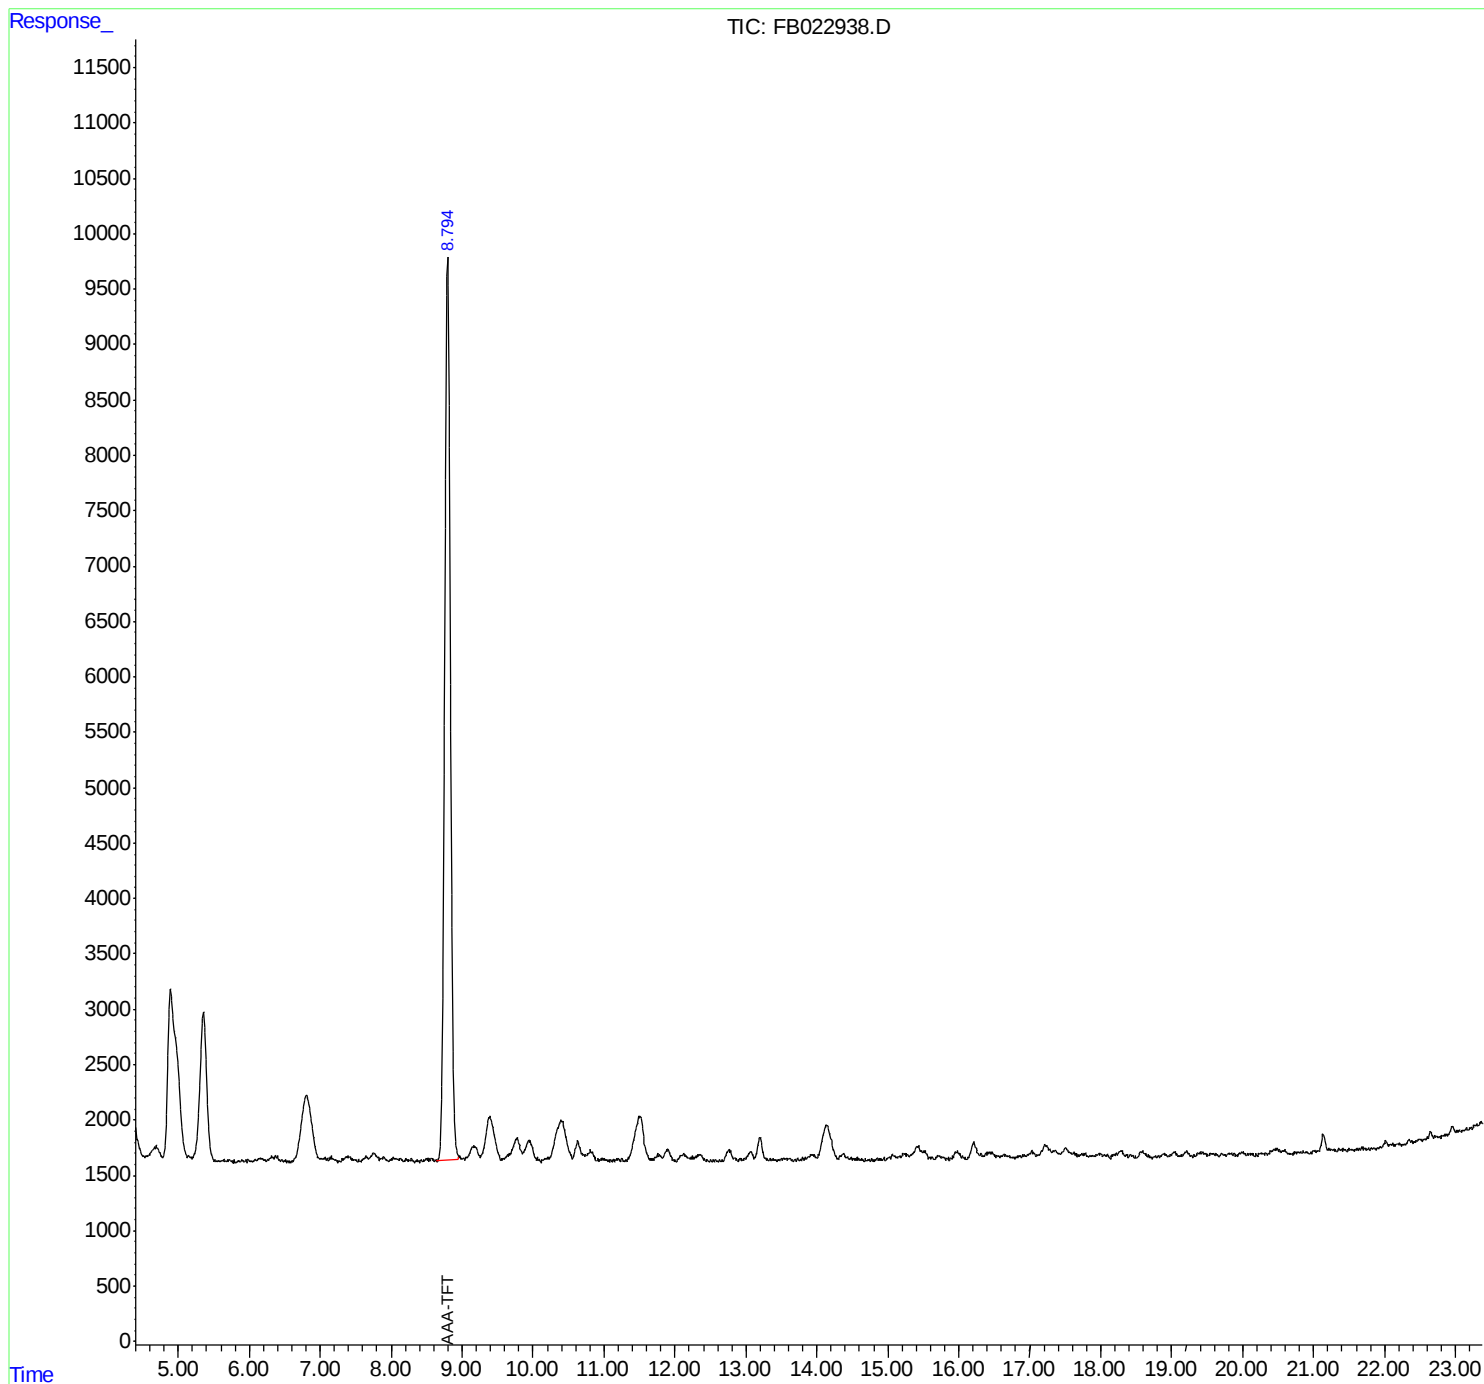

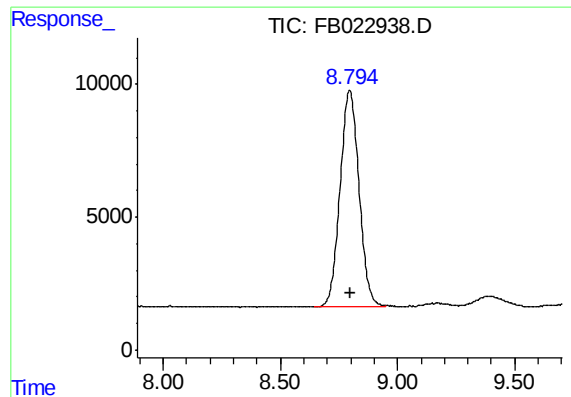

#5 AAA-TFT

R.T.: 8.796 min
Delta R.T.: -0.004 min
Response: 456836
Conc: 20.29 ng/ml

Instrument :
FID_B
ClientSampleId :
K5742-10MSD