

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110821\
 Data File : FB026345.D
 Signal(s) : FID2B.CH
 Acq On : 8 Nov 2021 18:13
 Operator : AJ/MA
 Sample : M4475-07MS
 Misc : 5.02G\5.00ML DI WATER
 ALS Vial : 8 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Nov 09 00:30:56 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB102721.M
 Quant Title :
 QLast Update : Thu Oct 28 05:34:31 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.794	214291	18.088 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.708	471446	28.314 ng/ml
2) t 2,2,4-Trimethylpentane	7.440	574815	29.479 ng/ml
3) t n-Heptane	7.753	176280	9.554 ng/ml
4) t Benzene	7.889	202882	9.306 ng/ml
6) t Toluene	10.621	594793	28.677 ng/ml
7) t Ethylbenzene	13.058	189196	10.019 ng/ml
8) t m-Xylene	13.190	376638	19.802 ng/ml
9) t O-Xylene	13.918	362562	19.630 ng/ml
10) t 1,2,4-Trimethylbenzene	16.193	383568	20.232 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110821\
Data File : FB026345.D
Signal(s) : FID2B.CH
Acq On : 8 Nov 2021 18:13
Operator : AJ/MA
Sample : M4475-07MS
Misc : 5.02G\5.00ML DI WATER
ALS Vial : 8 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Nov 09 00:30:56 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB102721.M
Quant Title :
QLast Update : Thu Oct 28 05:34:31 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

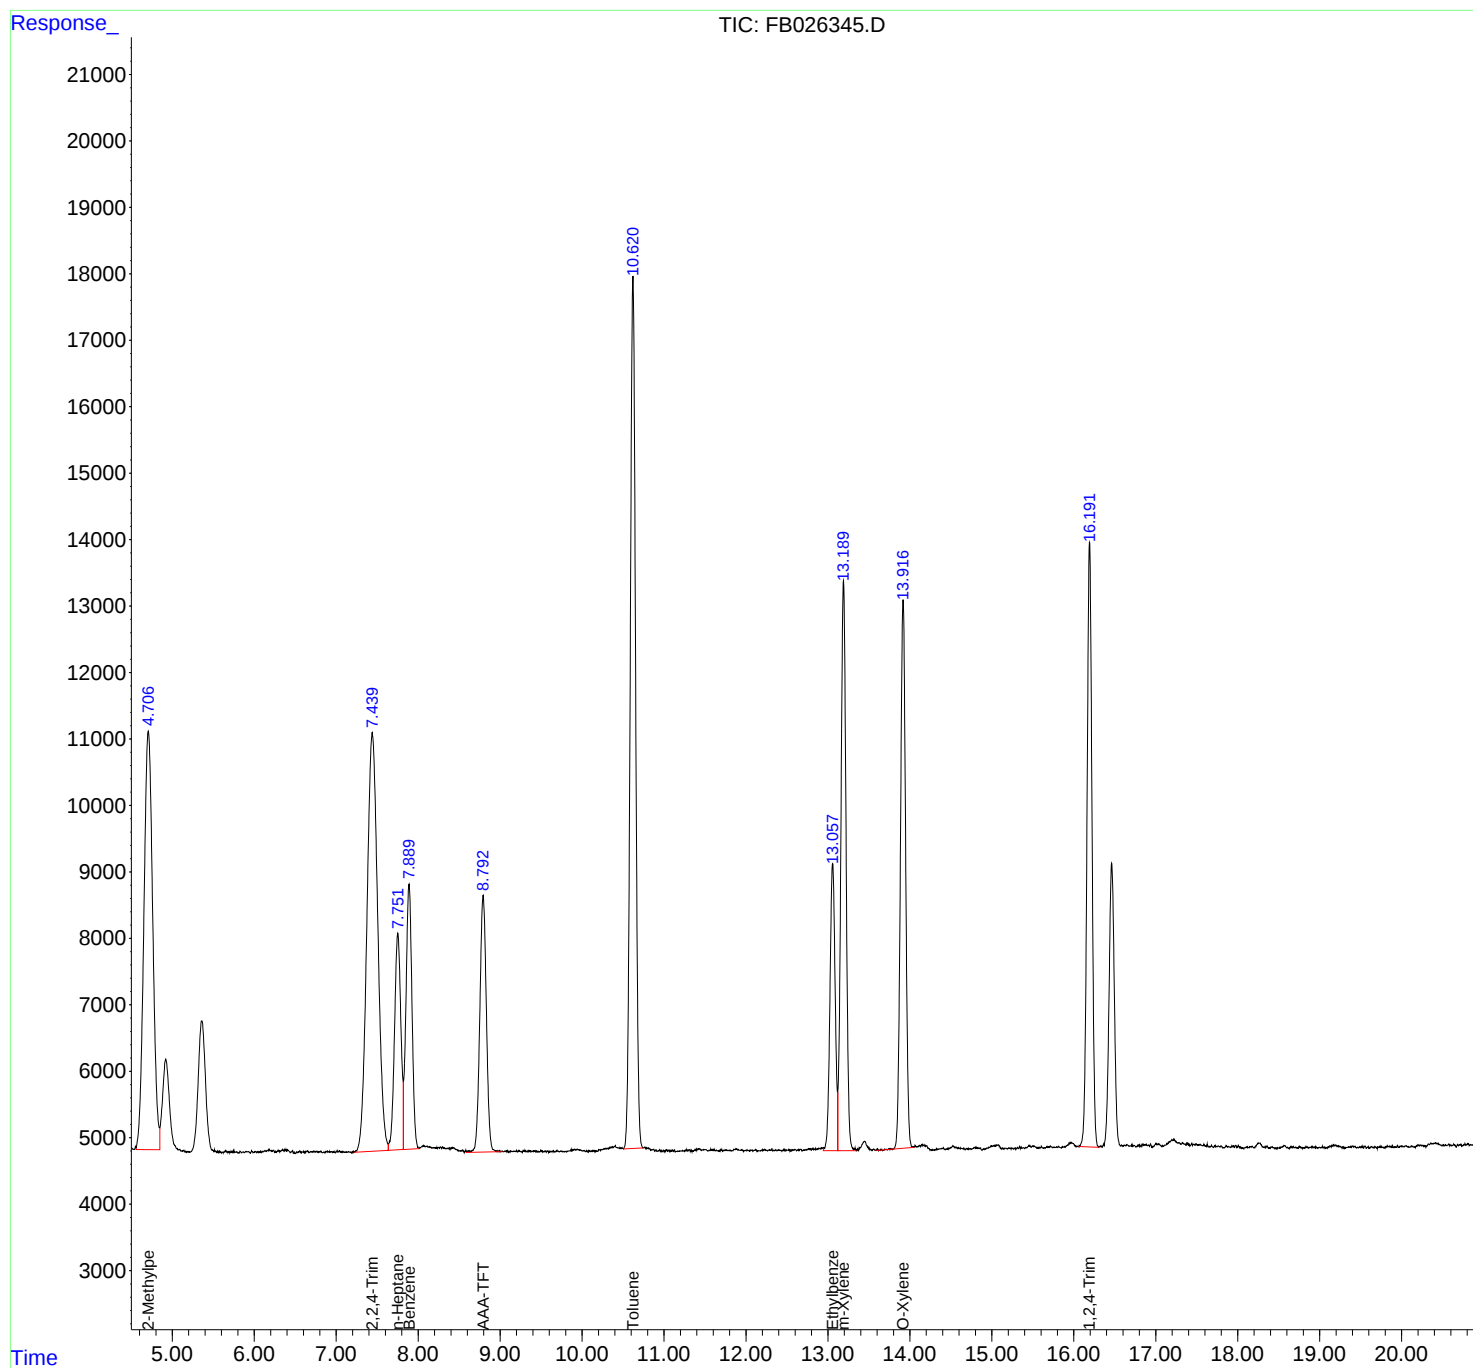

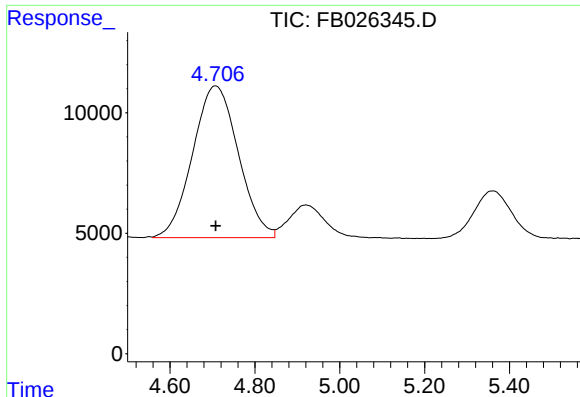


#1 2-Methylpentane

R.T.: 4.708 min
Delta R.T.: 0.000 min
Response: 471446
Conc: 28.31 ng/ml

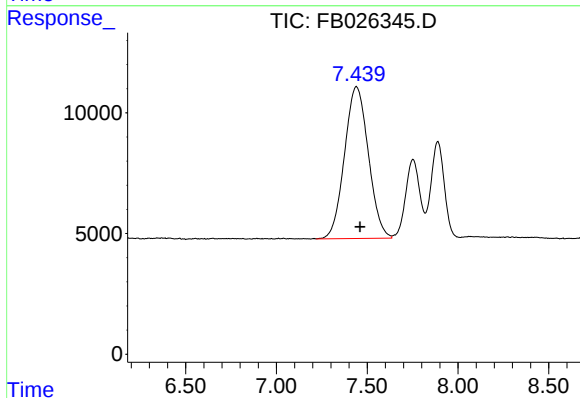


#2 2,2,4-Trimethylpentane

R.T.: 7.440 min
Delta R.T.: -0.020 min
Response: 574815
Conc: 29.48 ng/ml

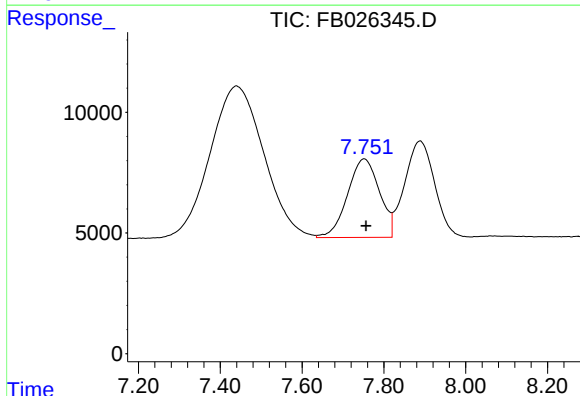


#3 n-Heptane

R.T.: 7.753 min
Delta R.T.: -0.004 min
Response: 176280
Conc: 9.55 ng/ml

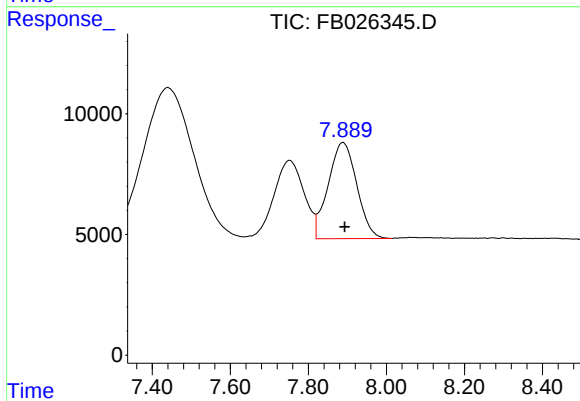


#4 Benzene

R.T.: 7.889 min
Delta R.T.: -0.004 min
Response: 202882
Conc: 9.31 ng/ml

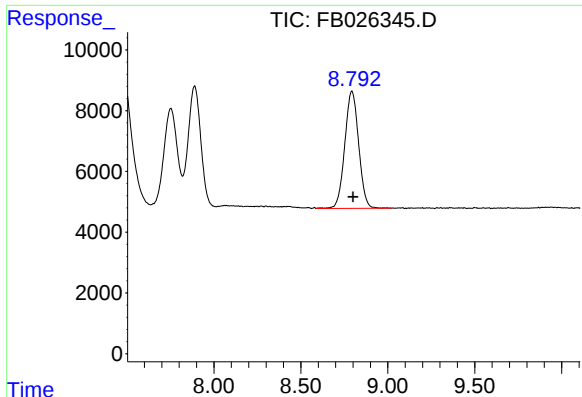


#5 AAA-TFT

R.T.: 8.794 min
Delta R.T.: -0.007 min
Response: 214291
Conc: 18.09 ng/ml

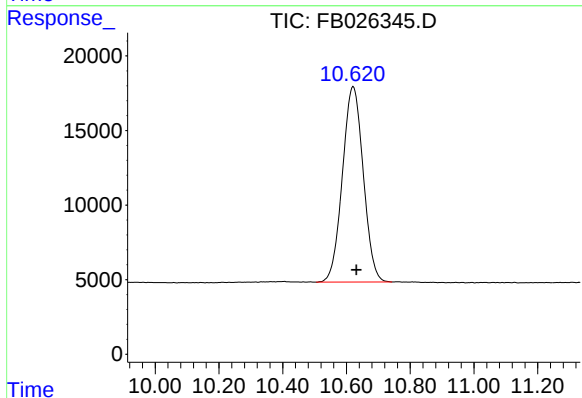


#6 Toluene

R.T.: 10.621 min
Delta R.T.: -0.010 min
Response: 594793
Conc: 28.68 ng/ml

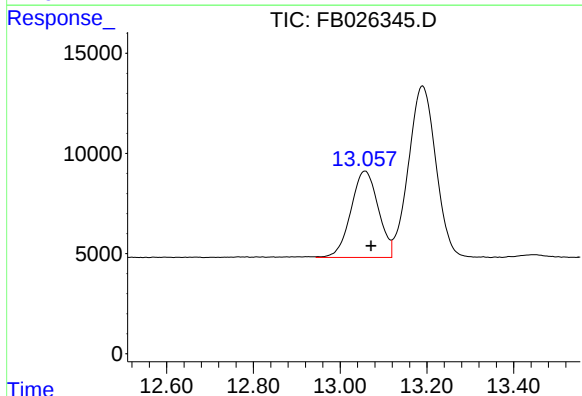


#7 Ethylbenzene

R.T.: 13.058 min
Delta R.T.: -0.014 min
Response: 189196
Conc: 10.02 ng/ml

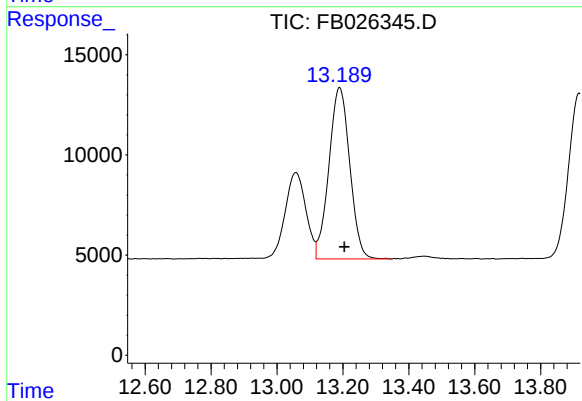

#8 m-Xylene

R.T.: 13.190 min
Delta R.T.: -0.014 min
Response: 376638
Conc: 19.80 ng/ml

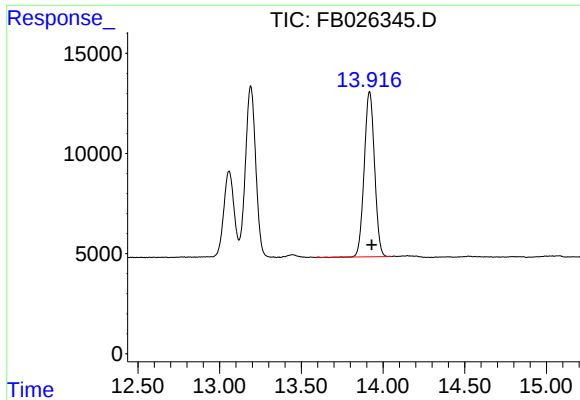


#9 O-Xylene

R.T.: 13.918 min

Delta R.T.: -0.014 min

Response: 362562

Conc: 19.63 ng/ml

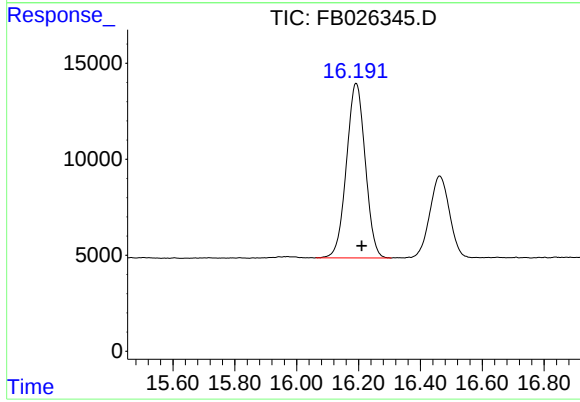

#10 1,2,4-Trimethylbenzene

R.T.: 16.193 min

Delta R.T.: -0.018 min

Response: 383568

Conc: 20.23 ng/ml