

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110821\
 Data File : FB026341.D
 Signal(s) : FID2B.CH
 Acq On : 8 Nov 2021 14:28
 Operator : AJ/MA
 Sample : BSF1108S1
 Misc : 5.02G\5.00ML DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: SAMPLE.e
 Quant Time: Nov 08 15:55:37 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB102721.M
 Quant Title :
 QLast Update : Thu Oct 28 05:34:31 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.792	238947	20.170 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.707	495641	29.767 ng/ml
2) t 2,2,4-Trimethylpentane	7.440	587121	30.110 ng/ml
3) t n-Heptane	7.750	187987	10.189 ng/ml
4) t Benzene	7.887	216125	9.914 ng/ml
6) t Toluene	10.620	636891	30.707 ng/ml
7) t Ethylbenzene	13.056	197851	10.477 ng/ml
8) t m-Xylene	13.189	387817	20.390 ng/ml
9) t O-Xylene	13.916	375134	20.311 ng/ml
10) t 1,2,4-Trimethylbenzene	16.191	385945	20.358 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110821\
Data File : FB026341.D
Signal(s) : FID2B.CH
Acq On : 8 Nov 2021 14:28
Operator : AJ/MA
Sample : BSF1108S1
Misc : 5.02G\5.00ML DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: SAMPLE.e
Quant Time: Nov 08 15:55:37 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB102721.M
Quant Title :
QLast Update : Thu Oct 28 05:34:31 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

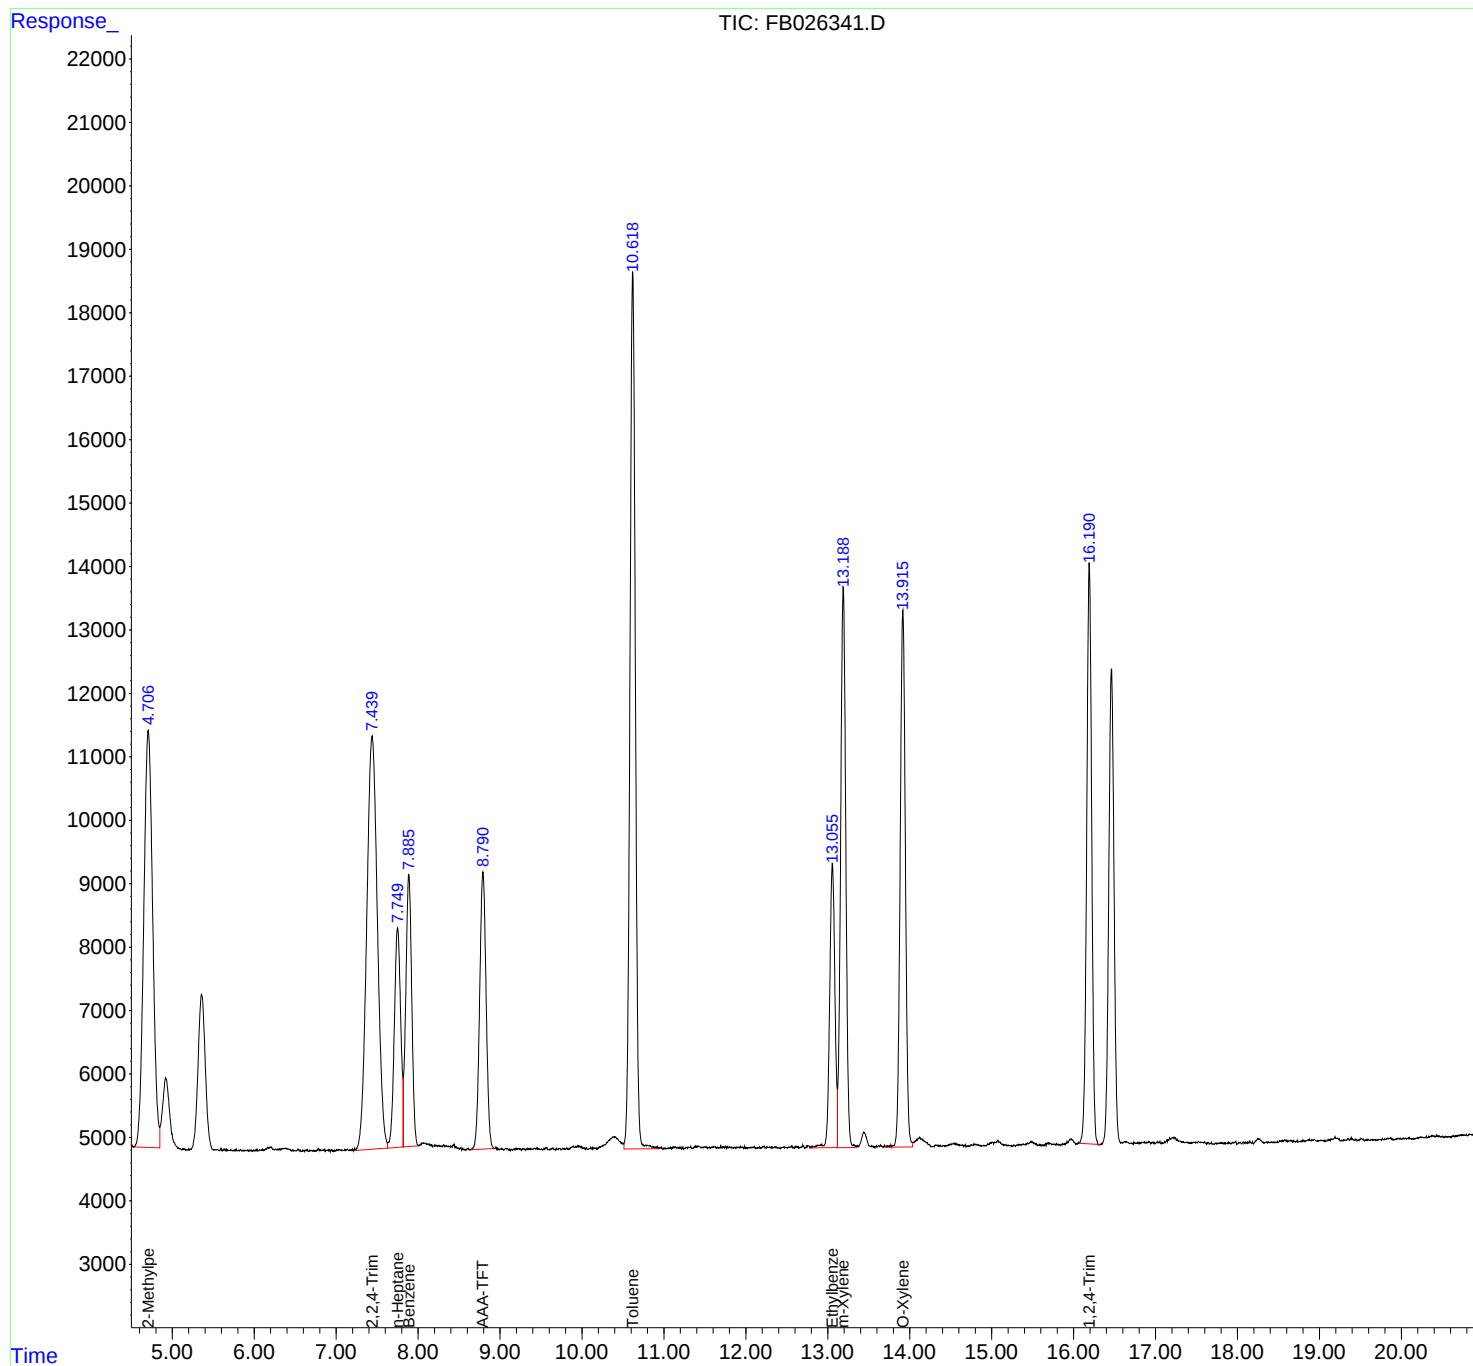

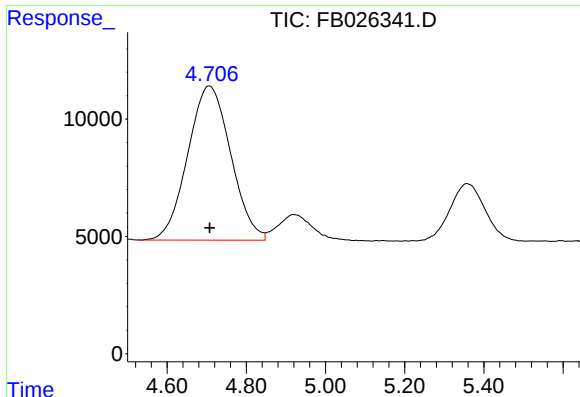


#1 2-Methylpentane

R.T.: 4.707 min
Delta R.T.: 0.000 min
Response: 495641
Conc: 29.77 ng/ml

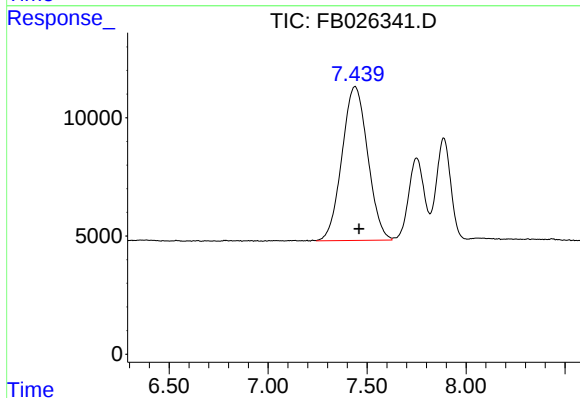


#2 2,2,4-Trimethylpentane

R.T.: 7.440 min
Delta R.T.: -0.020 min
Response: 587121
Conc: 30.11 ng/ml

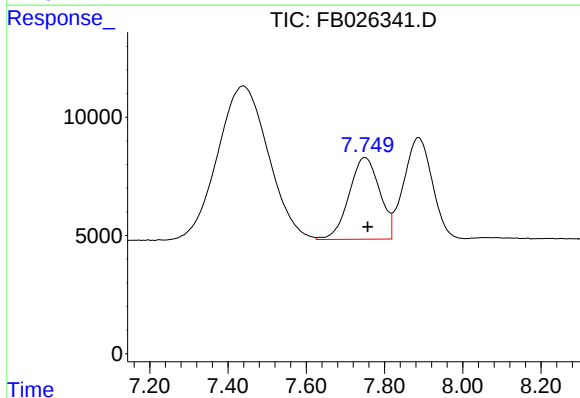


#3 n-Heptane

R.T.: 7.750 min
Delta R.T.: -0.006 min
Response: 187987
Conc: 10.19 ng/ml

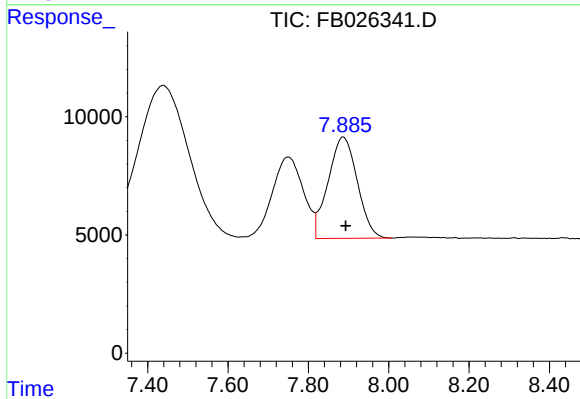


#4 Benzene

R.T.: 7.887 min
Delta R.T.: -0.006 min
Response: 216125
Conc: 9.91 ng/ml

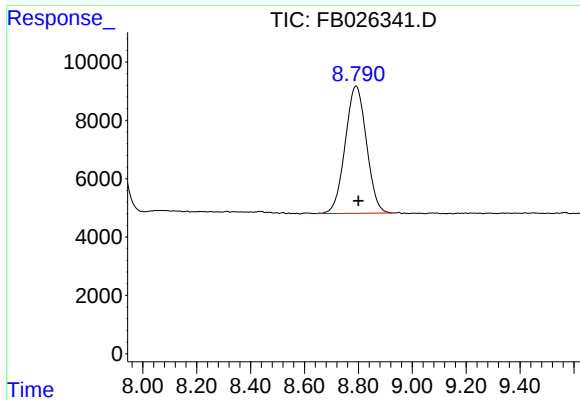


#5 AAA-TFT

R.T.: 8.792 min
Delta R.T.: -0.008 min
Response: 238947
Conc: 20.17 ng/ml

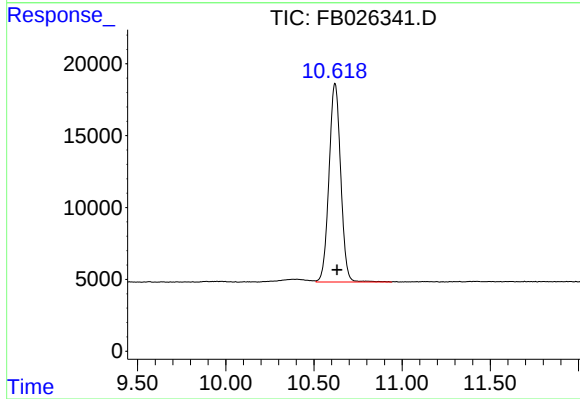


#6 Toluene

R.T.: 10.620 min
Delta R.T.: -0.011 min
Response: 636891
Conc: 30.71 ng/ml

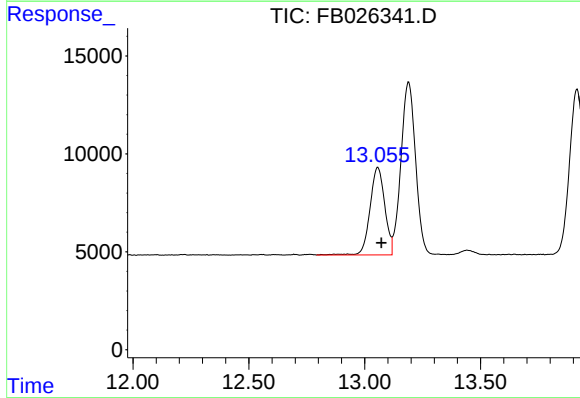


#7 Ethylbenzene

R.T.: 13.056 min
Delta R.T.: -0.015 min
Response: 197851
Conc: 10.48 ng/ml

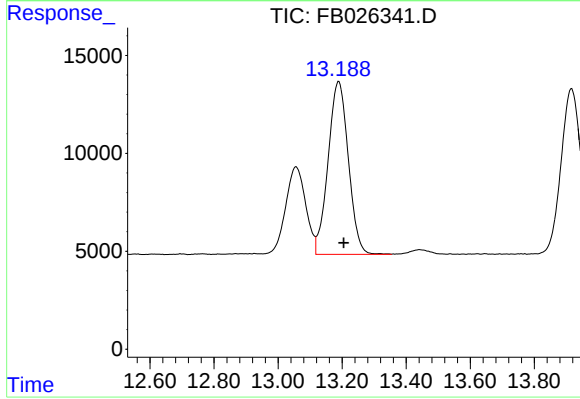


#8 m-Xylene

R.T.: 13.189 min
Delta R.T.: -0.015 min
Response: 387817
Conc: 20.39 ng/ml

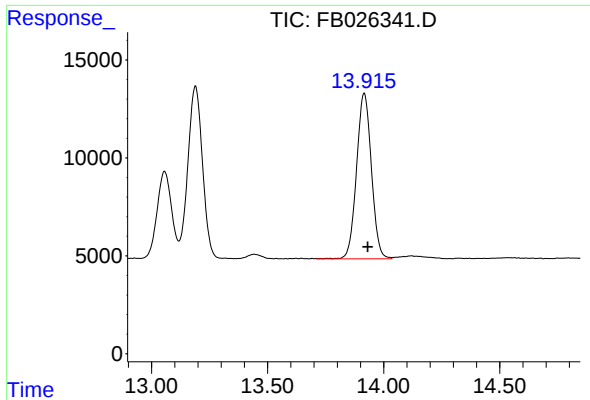

#9 O-Xylene

R.T.: 13.916 min
Delta R.T.: -0.015 min
Response: 375134
Conc: 20.31 ng/ml

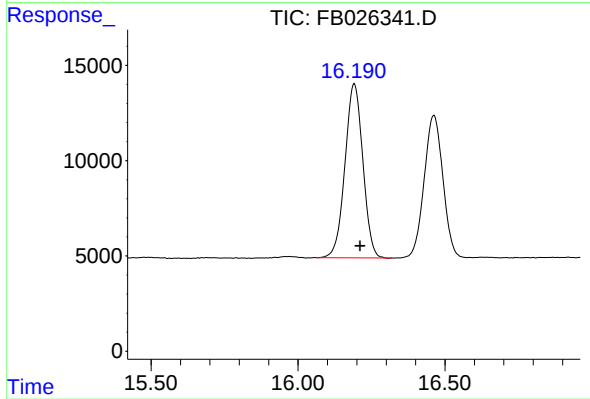

#10 1,2,4-Trimethylbenzene

R.T.: 16.191 min
Delta R.T.: -0.020 min
Response: 385945
Conc: 20.36 ng/ml