

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110821\
 Data File : FB026346.D
 Signal(s) : FID2B.CH
 Acq On : 8 Nov 2021 18:49
 Operator : AJ/MA
 Sample : M4475-07MSD
 Misc : 5.00G\5.00ML DI WATER
 ALS Vial : 9 Sample Multiplier: 1

Integration File: SAMPLE.e
 Quant Time: Nov 09 00:31:17 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB102721.M
 Quant Title :
 QLast Update : Thu Oct 28 05:34:31 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.793	239287	20.198 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.706	492782	29.595 ng/ml
2) t 2,2,4-Trimethylpentane	7.440	590604	30.289 ng/ml
3) t n-Heptane	7.751	187155	10.144 ng/ml
4) t Benzene	7.888	213533	9.795 ng/ml
6) t Toluene	10.621	635632	30.646 ng/ml
7) t Ethylbenzene	13.058	200548	10.620 ng/ml
8) t m-Xylene	13.190	393478	20.687 ng/ml
9) t O-Xylene	13.917	376533	20.386 ng/ml
10) t 1,2,4-Trimethylbenzene	16.192	391472	20.649 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110821\
Data File : FB026346.D
Signal(s) : FID2B.CH
Acq On : 8 Nov 2021 18:49
Operator : AJ/MA
Sample : M4475-07MSD
Misc : 5.00G\5.00ML DI WATER
ALS Vial : 9 Sample Multiplier: 1

Integration File: SAMPLE.e
Quant Time: Nov 09 00:31:17 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB102721.M
Quant Title :
QLast Update : Thu Oct 28 05:34:31 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

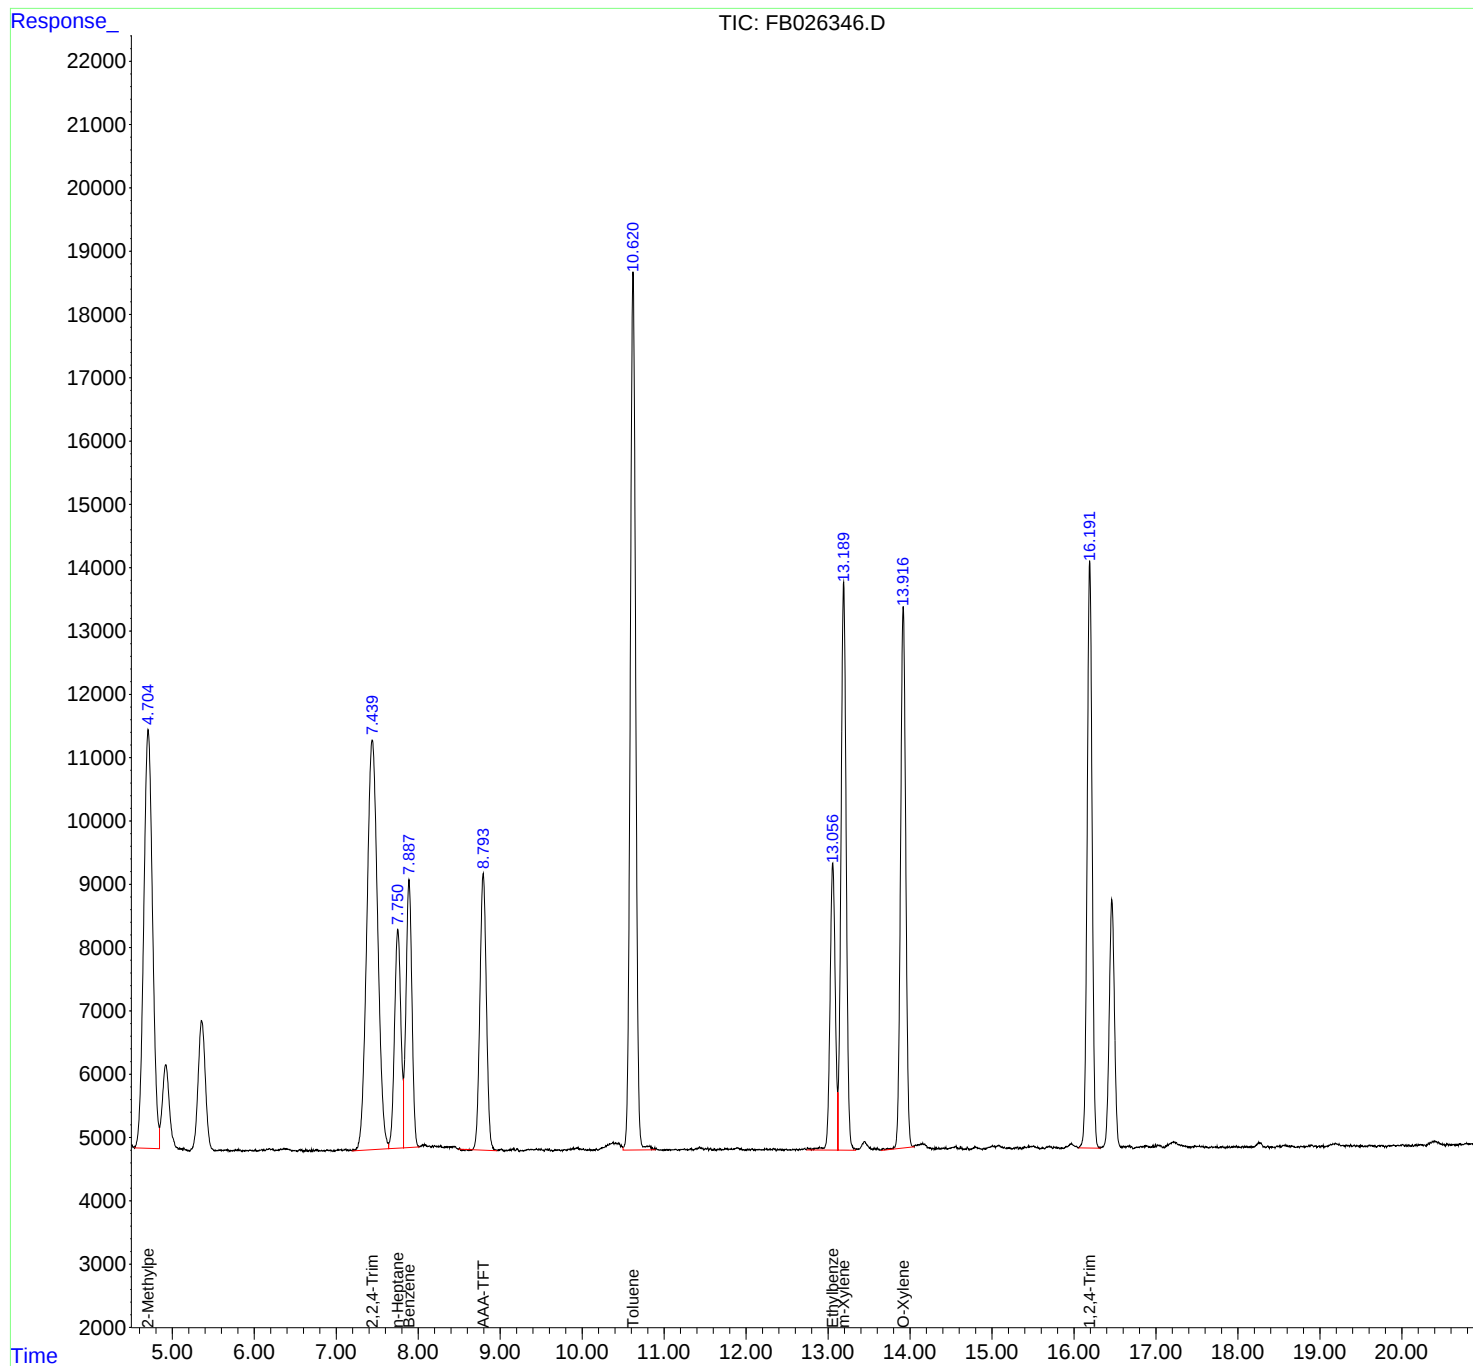

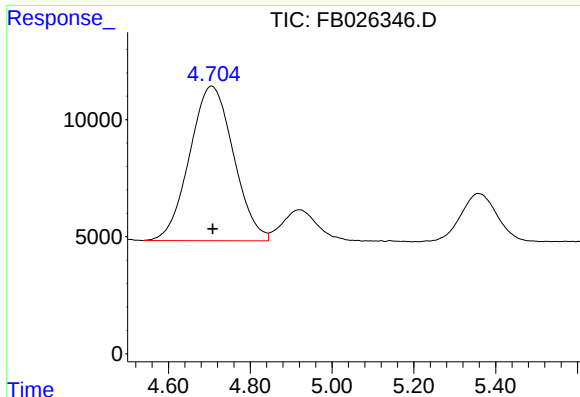


#1 2-Methylpentane

R.T.: 4.706 min
Delta R.T.: -0.002 min
Response: 492782
Conc: 29.59 ng/ml

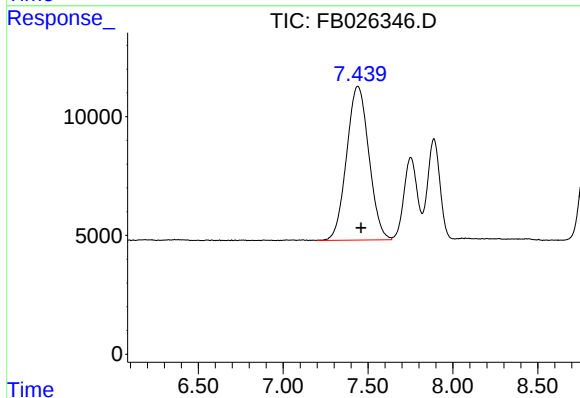


#2 2,2,4-Trimethylpentane

R.T.: 7.440 min
Delta R.T.: -0.020 min
Response: 590604
Conc: 30.29 ng/ml

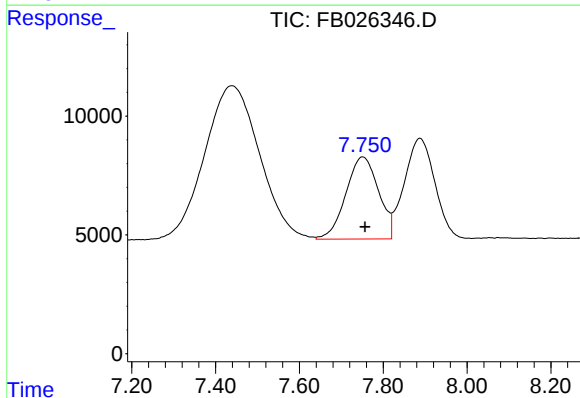


#3 n-Heptane

R.T.: 7.751 min
Delta R.T.: -0.005 min
Response: 187155
Conc: 10.14 ng/ml

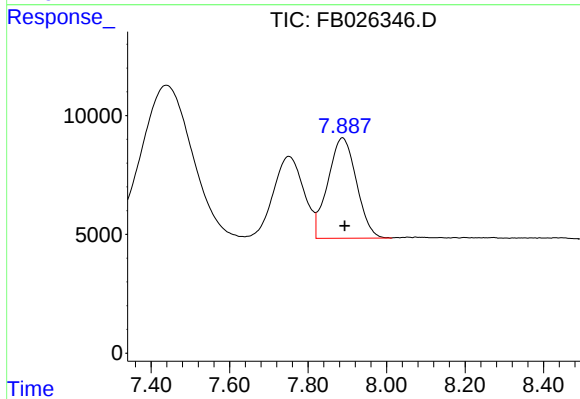


#4 Benzene

R.T.: 7.888 min
Delta R.T.: -0.005 min
Response: 213533
Conc: 9.79 ng/ml

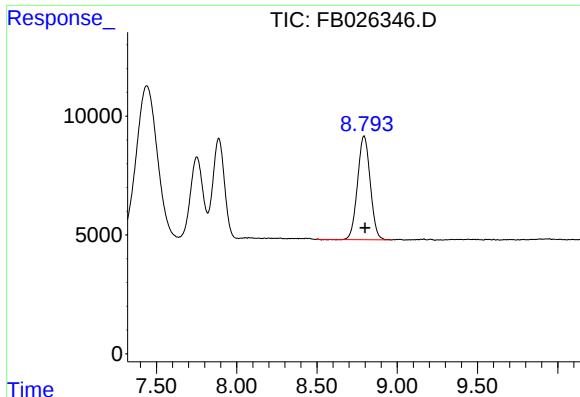


#5 AAA-TFT

R.T.: 8.793 min
Delta R.T.: -0.007 min
Response: 239287
Conc: 20.20 ng/ml

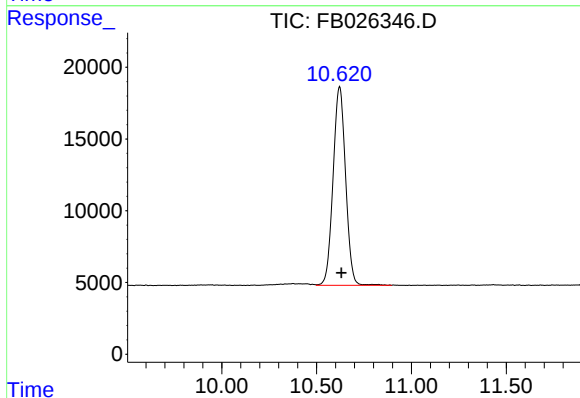


#6 Toluene

R.T.: 10.621 min
Delta R.T.: -0.010 min
Response: 635632
Conc: 30.65 ng/ml

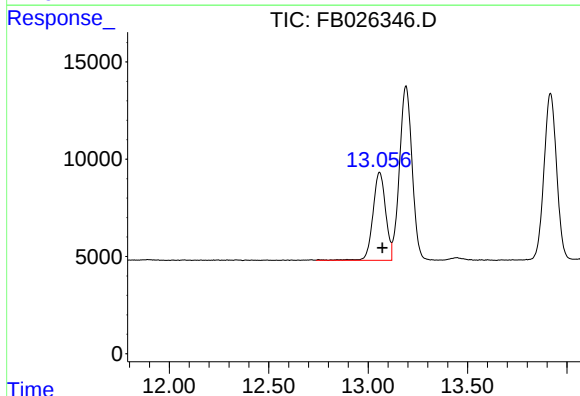


#7 Ethylbenzene

R.T.: 13.058 min
Delta R.T.: -0.014 min
Response: 200548
Conc: 10.62 ng/ml

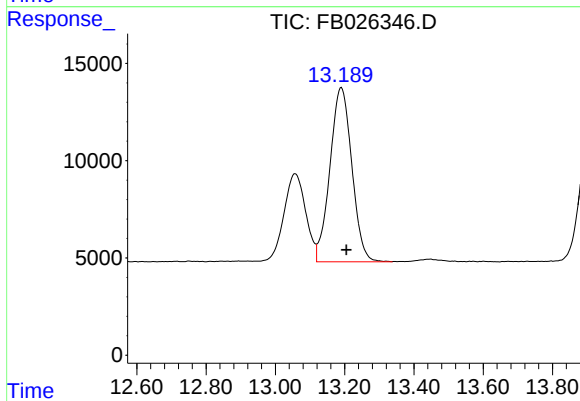


#8 m-Xylene

R.T.: 13.190 min
Delta R.T.: -0.014 min
Response: 393478
Conc: 20.69 ng/ml

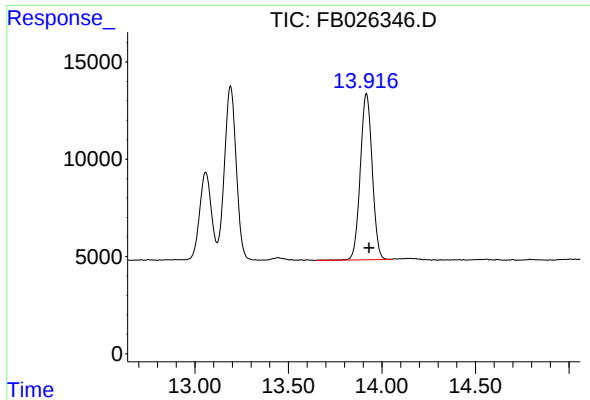

#9 O-Xylene

R.T.: 13.917 min
Delta R.T.: -0.014 min
Response: 376533
Conc: 20.39 ng/ml

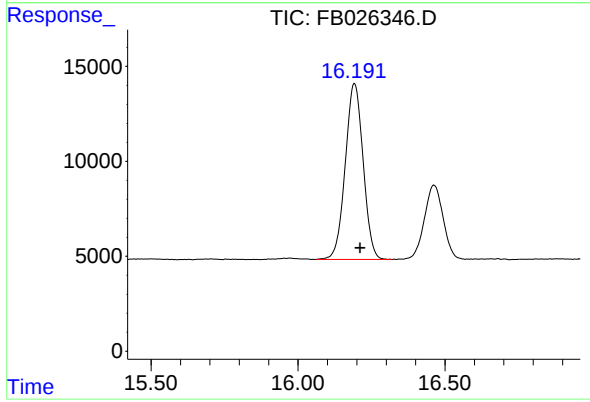

#10 1,2,4-Trimethylbenzene

R.T.: 16.192 min
Delta R.T.: -0.019 min
Response: 391472
Conc: 20.65 ng/ml