

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110822\
 Data File : FB028860.D
 Signal(s) : FID2B.CH
 Acq On : 8 Nov 2022 12:14
 Operator : AJ/MA
 Sample : BSF1108S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Nov 09 05:55:21 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110122.M
 Quant Title :
 QLast Update : Tue Nov 01 12:44:12 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.791	264666	20.828 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.711	445395	27.325 ng/ml
2) t 2,2,4-Trimethylpentane	7.419	483283	27.504 ng/ml
3) t n-Heptane	7.749	159726	9.085 ng/ml
4) t Benzene	7.886	190620	9.296 ng/ml
6) t Toluene	10.618	552608	27.475 ng/ml
7) t Ethylbenzene	13.054	172907	9.117 ng/ml
8) t m-Xylene	13.187	347052	18.448 ng/ml
9) t O-Xylene	13.913	344962	18.804 ng/ml
10) t 1,2,4-Trimethylbenzene	16.189	335352	18.204 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110822\
Data File : FB028860.D
Signal(s) : FID2B.CH
Acq On : 8 Nov 2022 12:14
Operator : AJ/MA
Sample : BSF1108S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Nov 09 05:55:21 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110122.M
Quant Title :
QLast Update : Tue Nov 01 12:44:12 2022
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

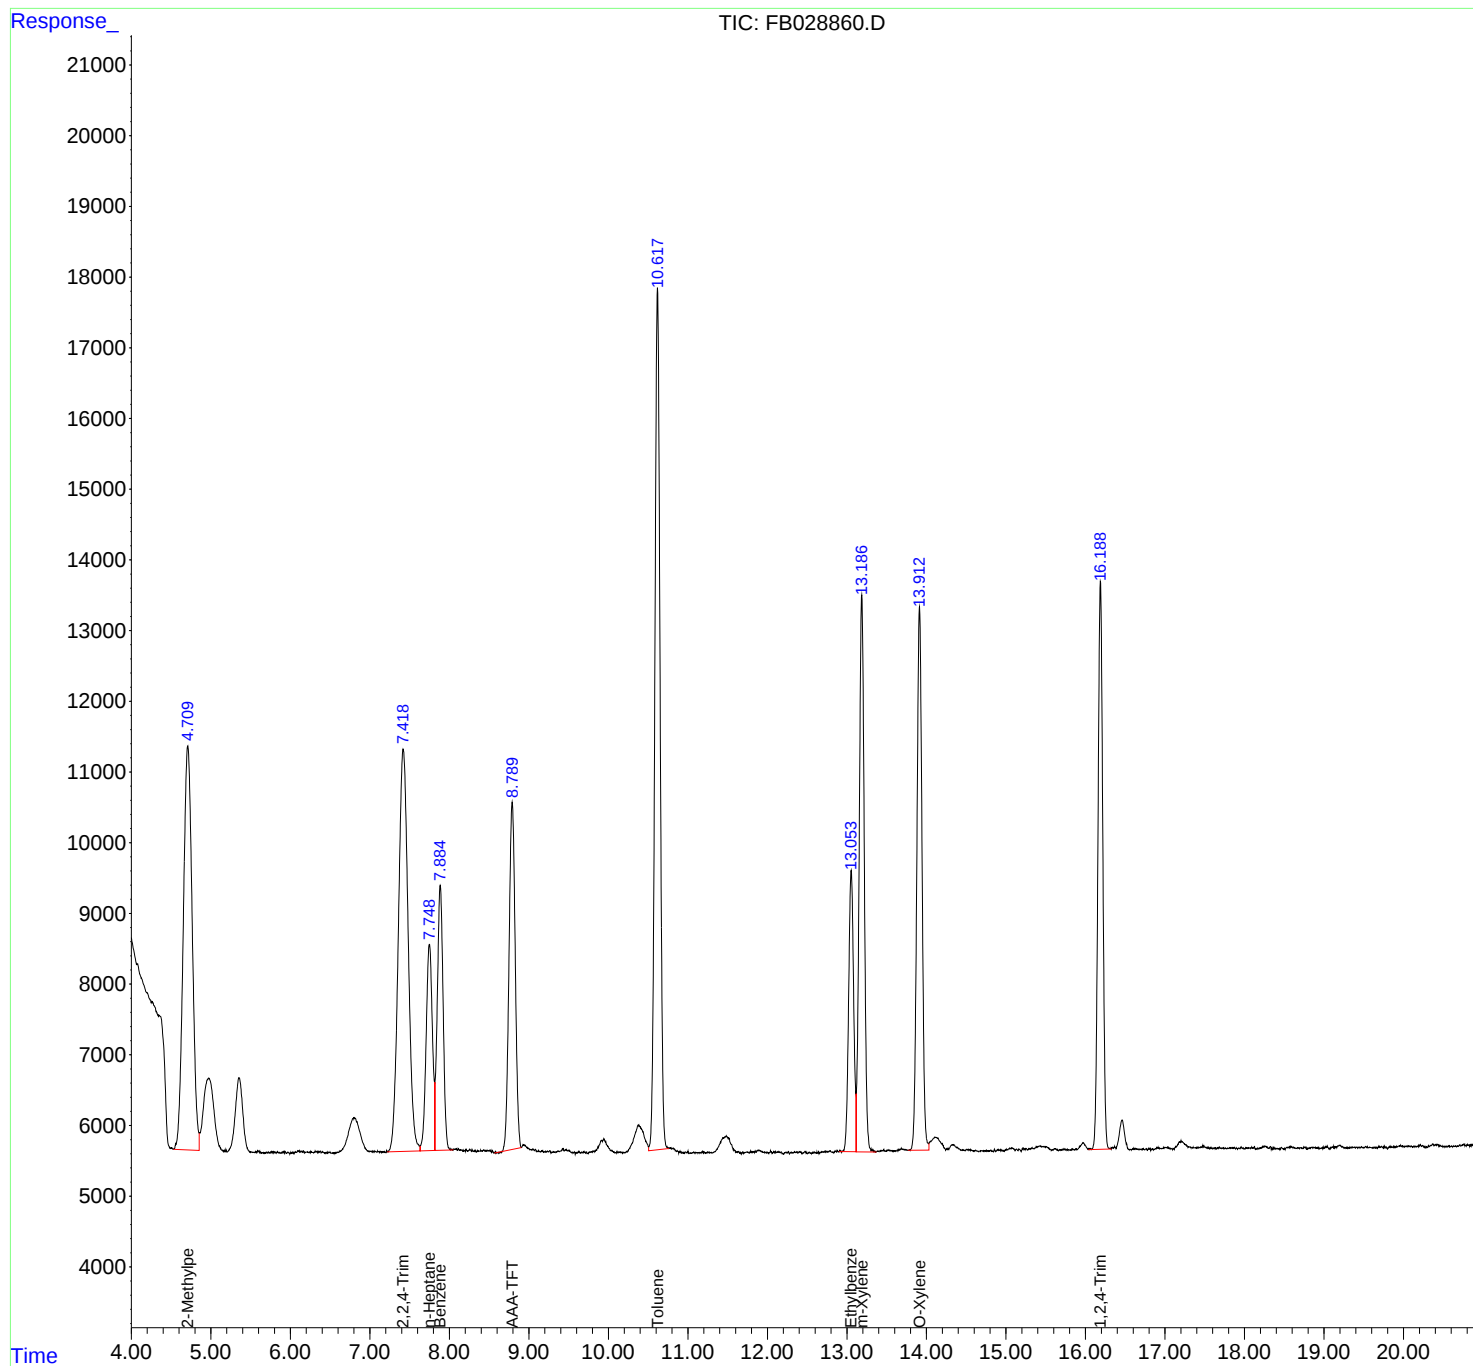

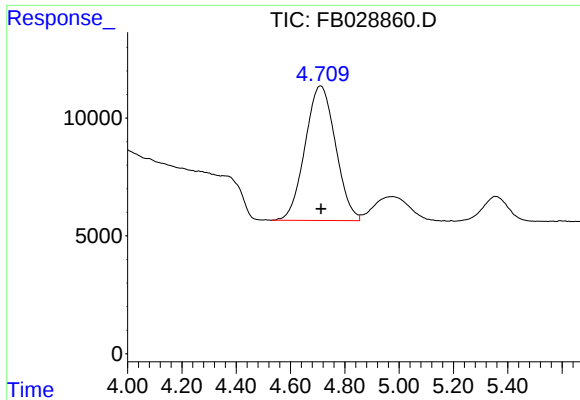


#1 2-Methylpentane

R.T.: 4.711 min
Delta R.T.: -0.001 min
Response: 445395
Conc: 27.33 ng/ml

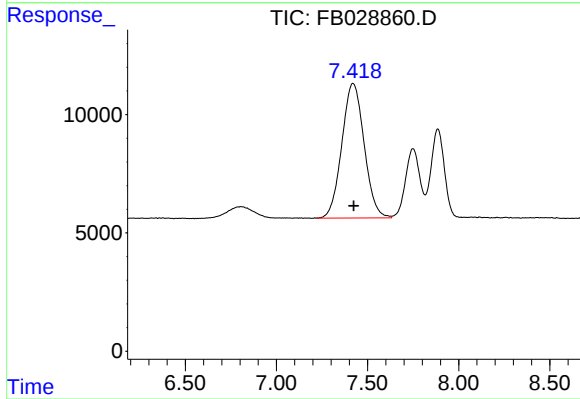


#2 2,2,4-Trimethylpentane

R.T.: 7.419 min
Delta R.T.: -0.006 min
Response: 483283
Conc: 27.50 ng/ml

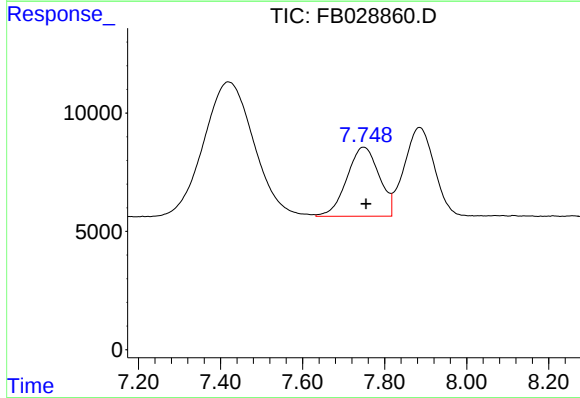


#3 n-Heptane

R.T.: 7.749 min
Delta R.T.: -0.005 min
Response: 159726
Conc: 9.08 ng/ml

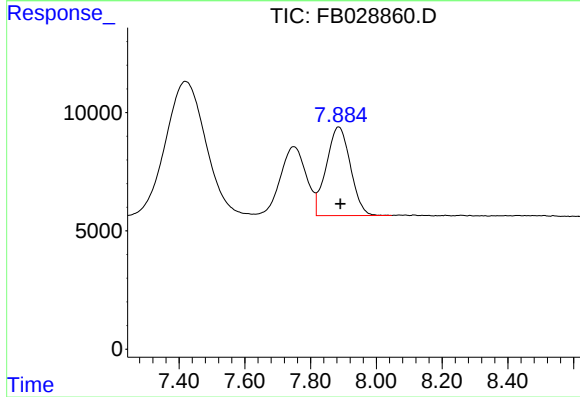


#4 Benzene

R.T.: 7.886 min
Delta R.T.: -0.005 min
Response: 190620
Conc: 9.30 ng/ml

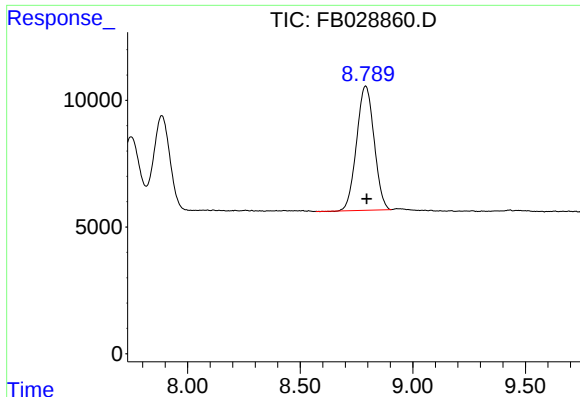


#5 AAA-TFT

R.T.: 8.791 min
Delta R.T.: -0.004 min
Response: 264666
Conc: 20.83 ng/ml

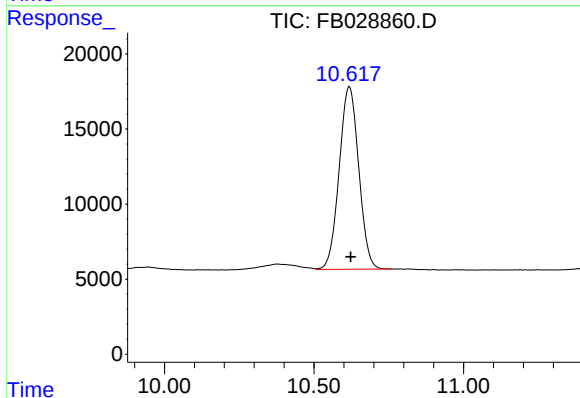


#6 Toluene

R.T.: 10.618 min
Delta R.T.: -0.005 min
Response: 552608
Conc: 27.48 ng/ml

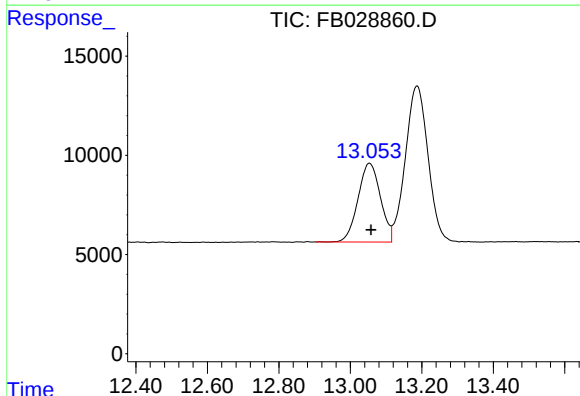


#7 Ethylbenzene

R.T.: 13.054 min
Delta R.T.: -0.004 min
Response: 172907
Conc: 9.12 ng/ml

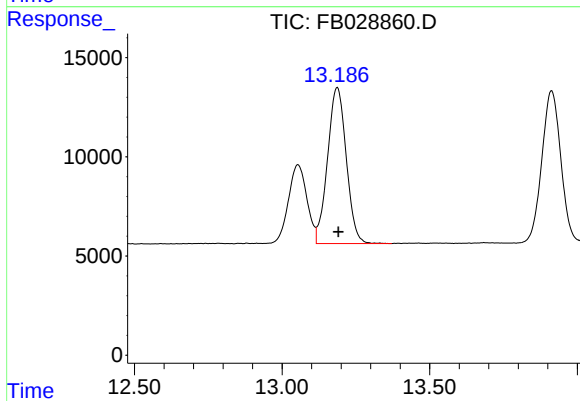

#8 m-Xylene

R.T.: 13.187 min
Delta R.T.: -0.004 min
Response: 347052
Conc: 18.45 ng/ml

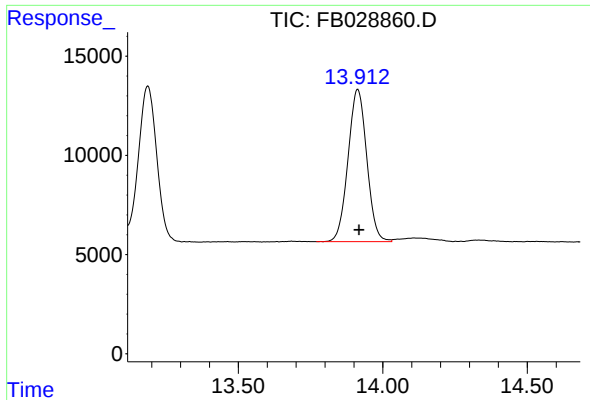


#9 O-Xylene

R.T.: 13.913 min

Delta R.T.: -0.005 min

Response: 344962

Conc: 18.80 ng/ml

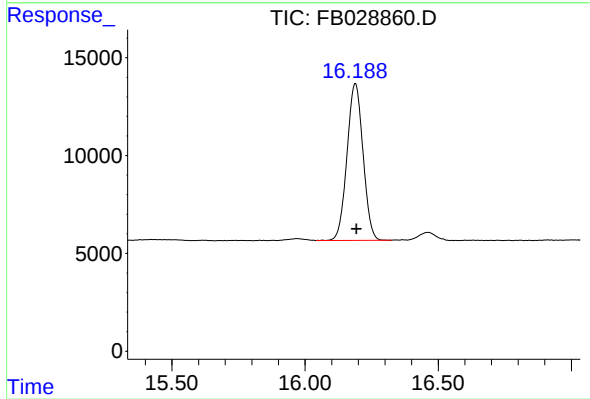

#10 1,2,4-Trimethylbenzene

R.T.: 16.189 min

Delta R.T.: -0.004 min

Response: 335352

Conc: 18.20 ng/ml