

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110822\
 Data File : FB028886.D
 Signal(s) : FID2B.CH
 Acq On : 9 Nov 2022 6:47
 Operator : AJ/MA
 Sample : BSF1108S3
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 34 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Nov 09 07:11:19 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110122.M
 Quant Title :
 QLast Update : Tue Nov 01 12:44:12 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.784	267425	21.045 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.699	479378	29.410 ng/ml
2) t	2,2,4-Trimethylpentane	7.409	501074	28.517 ng/ml
3) t	n-Heptane	7.742	169462	9.638 ng/ml
4) t	Benzene	7.879	208984	10.191 ng/ml
6) t	Toluene	10.611	610184	30.338 ng/ml
7) t	Ethylbenzene	13.047	191489	10.097 ng/ml
8) t	m-Xylene	13.180	381475	20.277 ng/ml
9) t	O-Xylene	13.906	380406	20.736 ng/ml
10) t	1,2,4-Trimethylbenzene	16.181	383400	20.812 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110822\
Data File : FB028886.D
Signal(s) : FID2B.CH
Acq On : 9 Nov 2022 6:47
Operator : AJ/MA
Sample : BSF1108S3
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 34 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Nov 09 07:11:19 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110122.M
Quant Title :
QLast Update : Tue Nov 01 12:44:12 2022
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

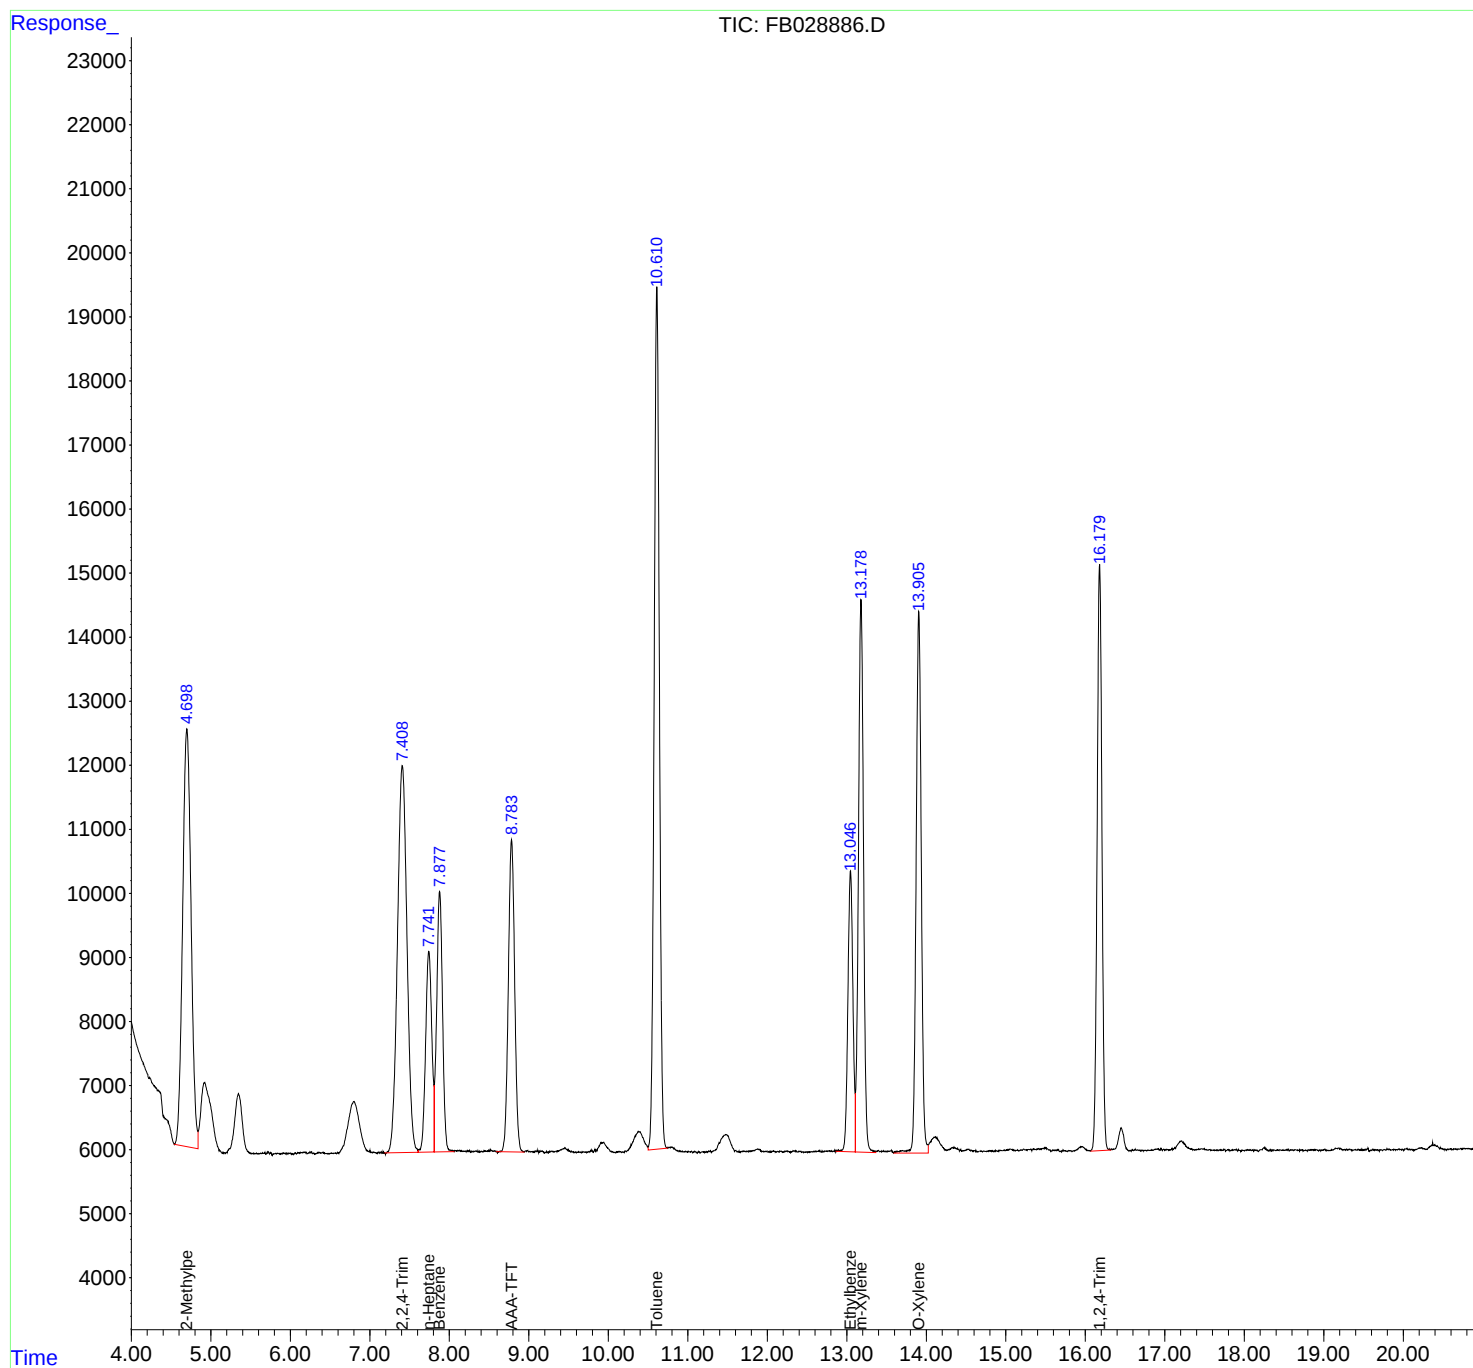

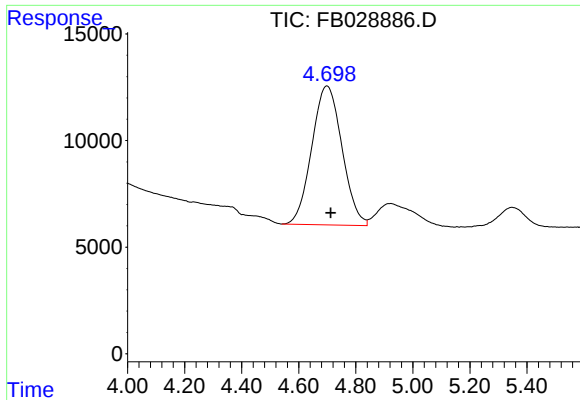


#1 2-Methylpentane

R.T.: 4.699 min
Delta R.T.: -0.013 min
Response: 479378
Conc: 29.41 ng/ml

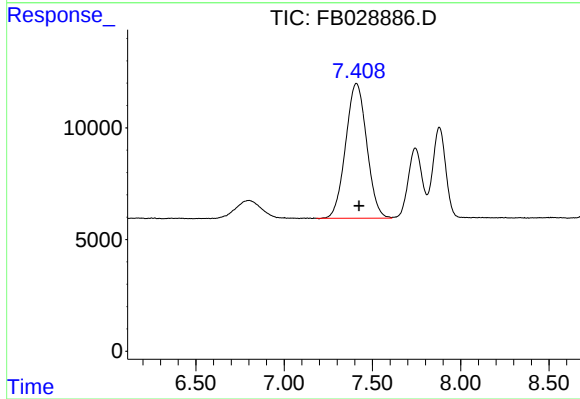


#2 2,2,4-Trimethylpentane

R.T.: 7.409 min
Delta R.T.: -0.016 min
Response: 501074
Conc: 28.52 ng/ml

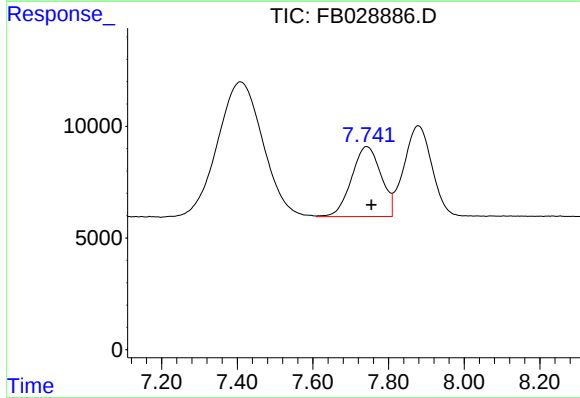


#3 n-Heptane

R.T.: 7.742 min
Delta R.T.: -0.012 min
Response: 169462
Conc: 9.64 ng/ml

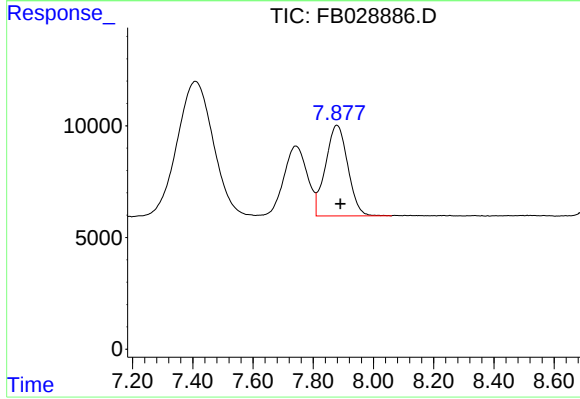


#4 Benzene

R.T.: 7.879 min
Delta R.T.: -0.012 min
Response: 208984
Conc: 10.19 ng/ml

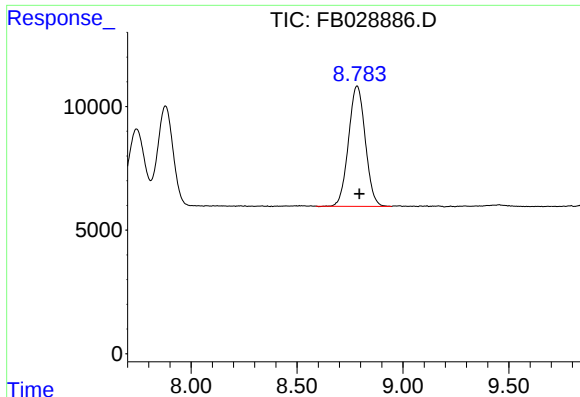


#5 AAA-TFT

R.T.: 8.784 min
Delta R.T.: -0.011 min
Response: 267425
Conc: 21.04 ng/ml

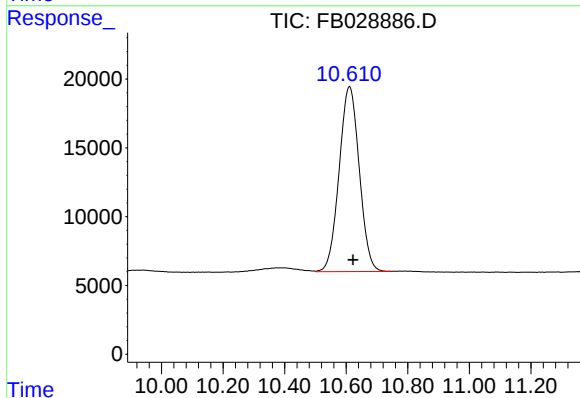


#6 Toluene

R.T.: 10.611 min
Delta R.T.: -0.011 min
Response: 610184
Conc: 30.34 ng/ml

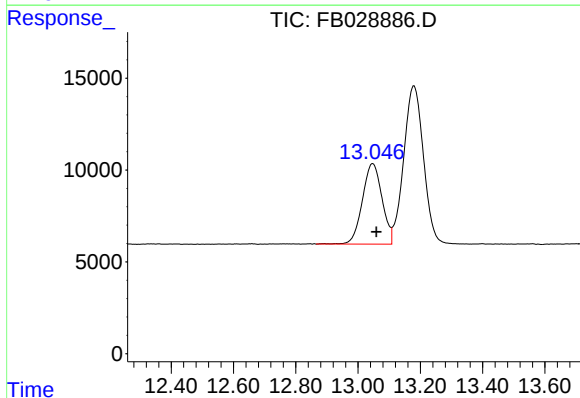


#7 Ethylbenzene

R.T.: 13.047 min
Delta R.T.: -0.011 min
Response: 191489
Conc: 10.10 ng/ml

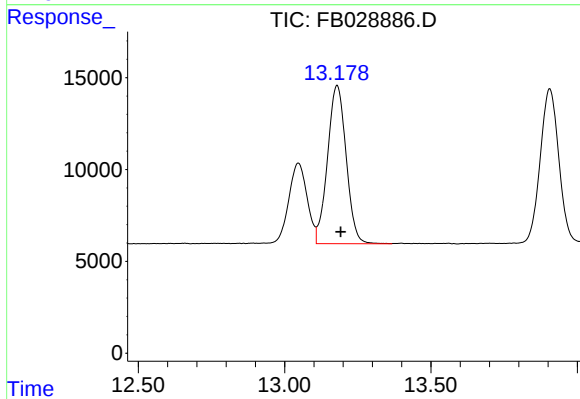

#8 m-Xylene

R.T.: 13.180 min
Delta R.T.: -0.012 min
Response: 381475
Conc: 20.28 ng/ml

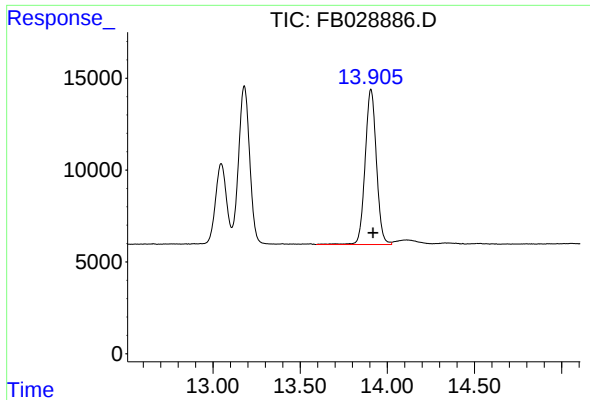


#9 O-Xylene

R.T.: 13.906 min

Delta R.T.: -0.012 min

Response: 380406

Conc: 20.74 ng/ml

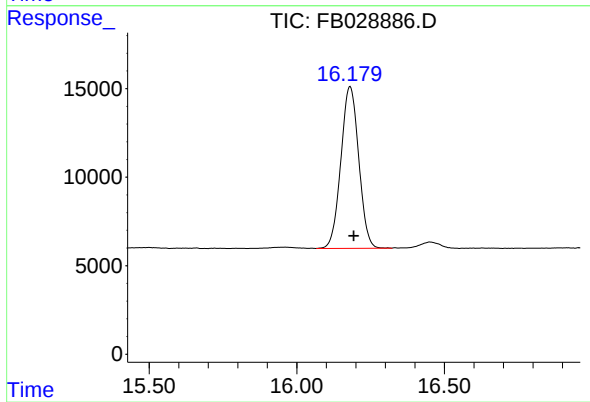

#10 1,2,4-Trimethylbenzene

R.T.: 16.181 min

Delta R.T.: -0.012 min

Response: 383400

Conc: 20.81 ng/ml