

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110823\
 Data File : FB030454.D
 Signal(s) : FID2B.CH
 Acq On : 8 Nov 2023 9:59
 Operator : YP/AJ
 Sample : 5 GRO STD
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 5 GRO STD

Integration File: Calibration.e
 Quant Time: Nov 08 10:36:32 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110823.M
 Quant Title :
 QLast Update : Wed Nov 08 10:33:55 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.779	87075	6.304 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.702	156394	7.971 ng/ml
2) t 2,2,4-Trimethylpentane	7.404	149475	7.624 ng/ml
3) t n-Heptane	7.737	55531	2.477 ng/ml
4) t Benzene	7.875	62836	2.471 ng/ml
6) t Toluene	10.606	185983	7.487 ng/ml
7) t Ethylbenzene	13.043	59438	2.565 ng/ml
8) t m-Xylene	13.175	119308	5.180 ng/ml
9) t O-Xylene	13.902	117824	5.279 ng/ml
10) t 1,2,4-Trimethylbenzene	16.179	124039	5.525 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110823\
Data File : FB030454.D
Signal(s) : FID2B.CH
Acq On : 8 Nov 2023 9:59
Operator : YP/AJ
Sample : 5 GRO STD
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
5 GRO STD

Integration File: Calibration.e
Quant Time: Nov 08 10:36:32 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110823.M
Quant Title :
QLast Update : Wed Nov 08 10:33:55 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

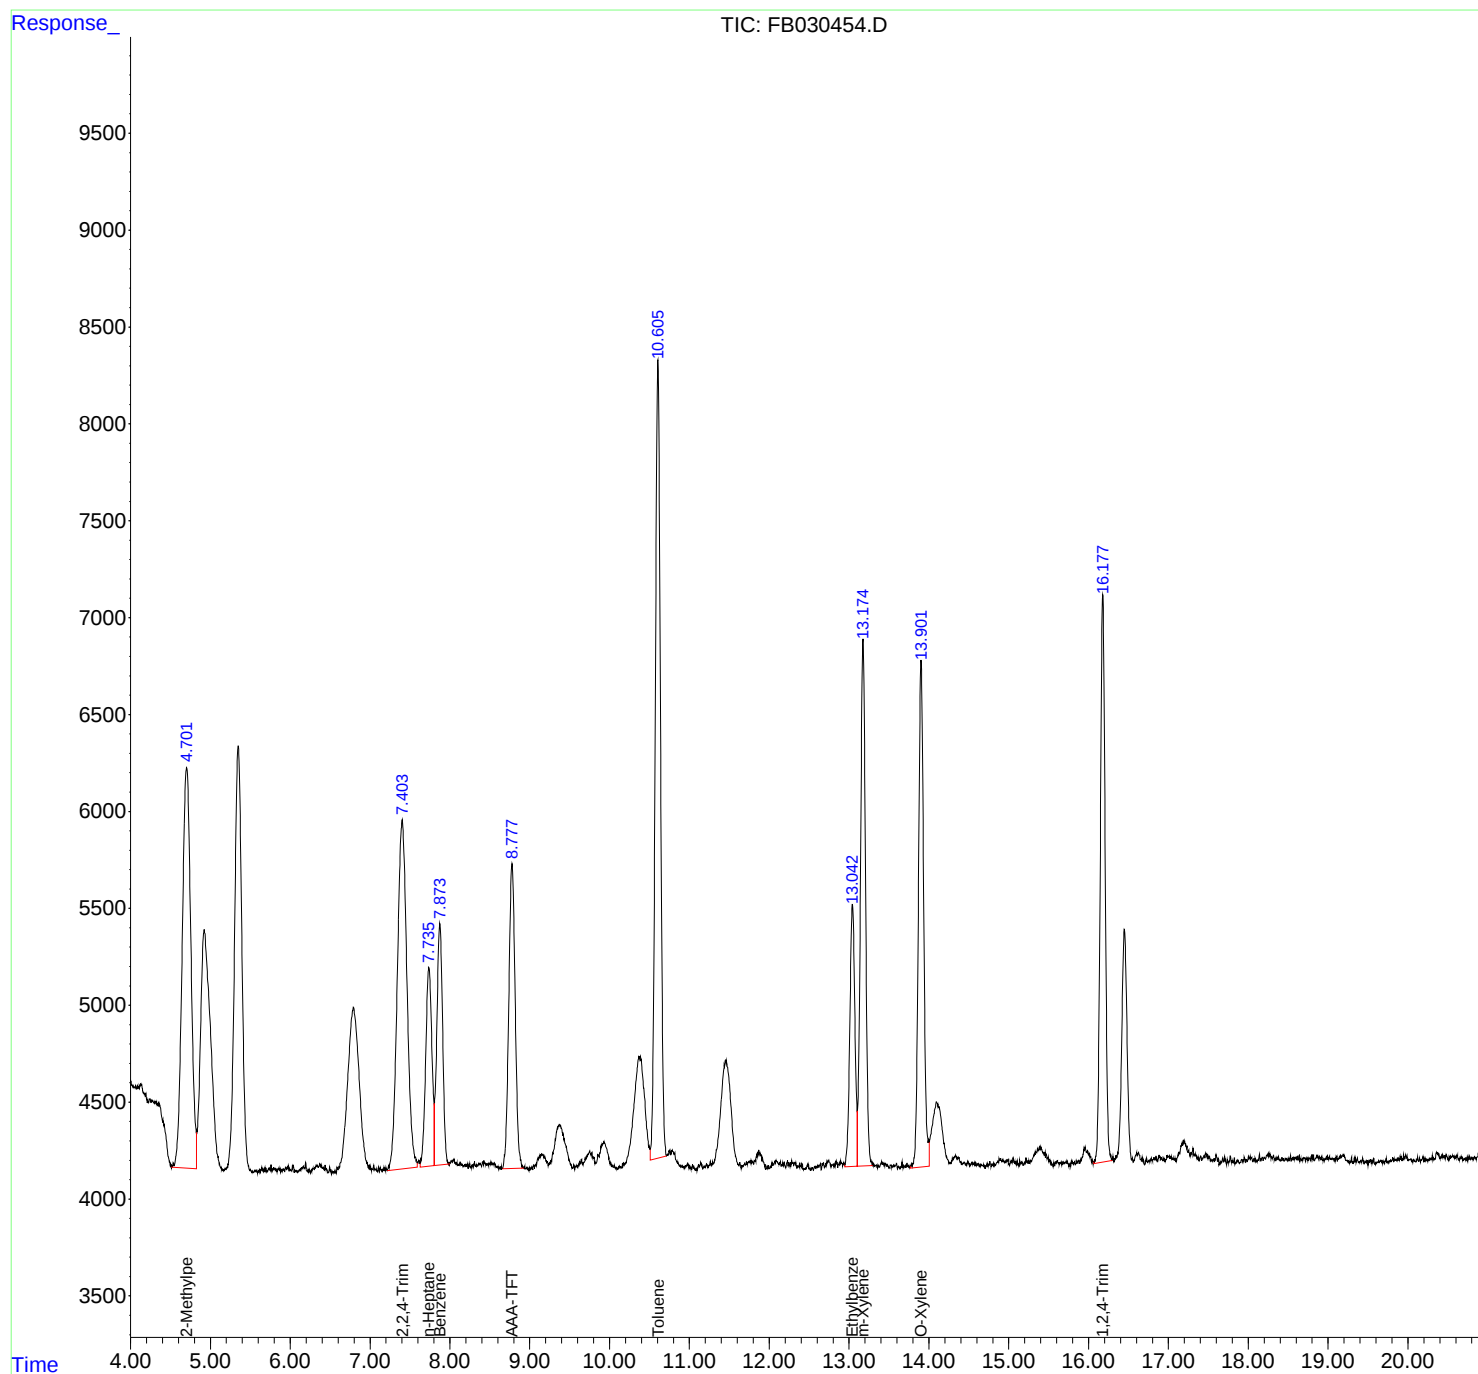


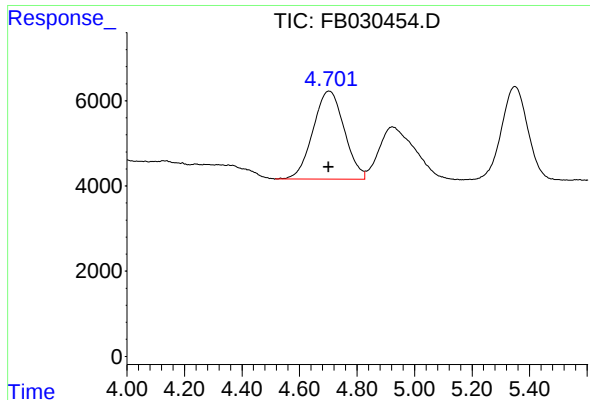

#1 2-Methylpentane


R.T.: 4.702 min
Delta R.T.: 0.000 min
Response: 156394
Conc: 7.97 ng/ml

Instrument :
FID_B
ClientSampleId :
5 GRO STD

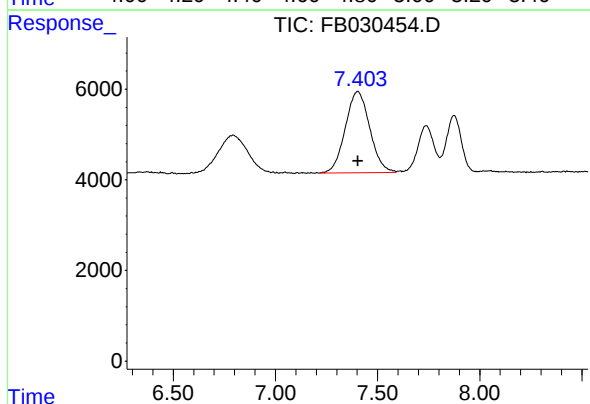


#2 2,2,4-Trimethylpentane

R.T.: 7.404 min
Delta R.T.: 0.000 min
Response: 149475
Conc: 7.62 ng/ml

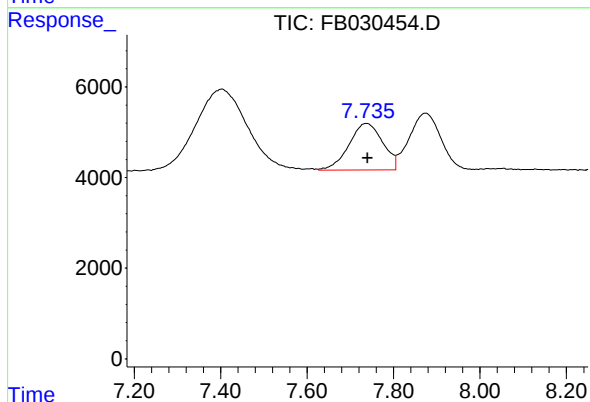


#3 n-Heptane

R.T.: 7.737 min
Delta R.T.: -0.004 min
Response: 55531
Conc: 2.48 ng/ml

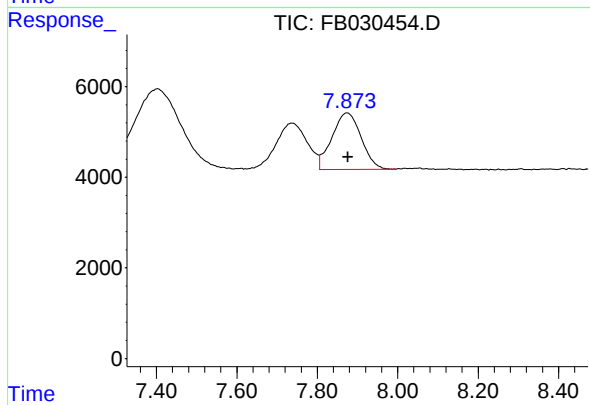

#4 Benzene


R.T.: 7.875 min
Delta R.T.: -0.002 min
Response: 62836
Conc: 2.47 ng/ml

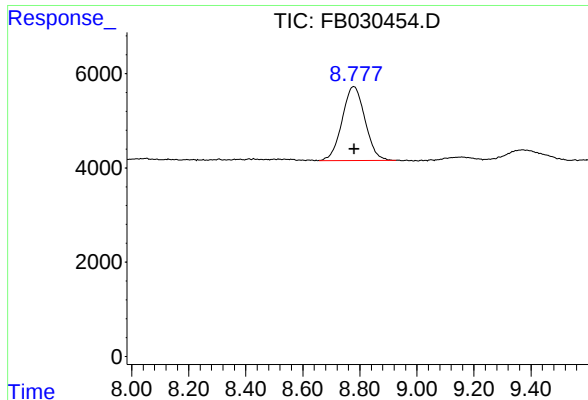

#5 AAA-TFT


R.T.: 8.779 min
Delta R.T.: -0.001 min
Response: 87075
Conc: 6.30 ng/ml

Instrument :
FID_B
ClientSampleId :
5 GRO STD

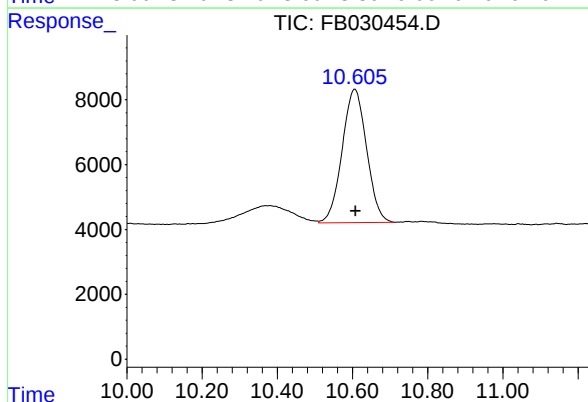


#6 Toluene

R.T.: 10.606 min
Delta R.T.: -0.002 min
Response: 185983
Conc: 7.49 ng/ml

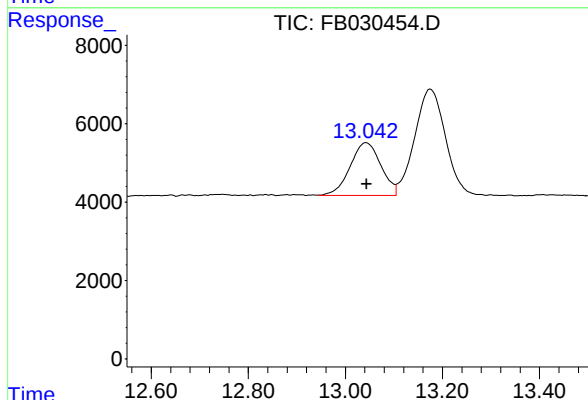


#7 Ethylbenzene

R.T.: 13.043 min
Delta R.T.: 0.000 min
Response: 59438
Conc: 2.56 ng/ml

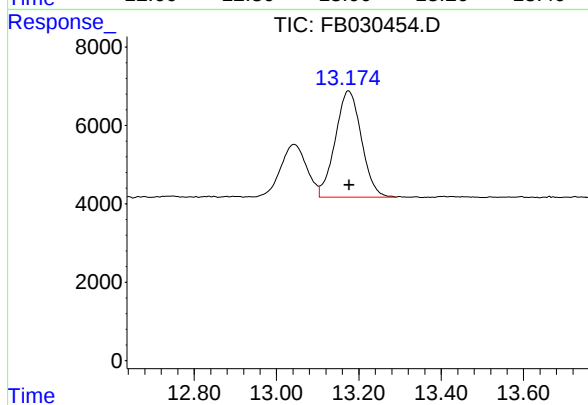

#8 m-Xylene


R.T.: 13.175 min
Delta R.T.: -0.002 min
Response: 119308
Conc: 5.18 ng/ml

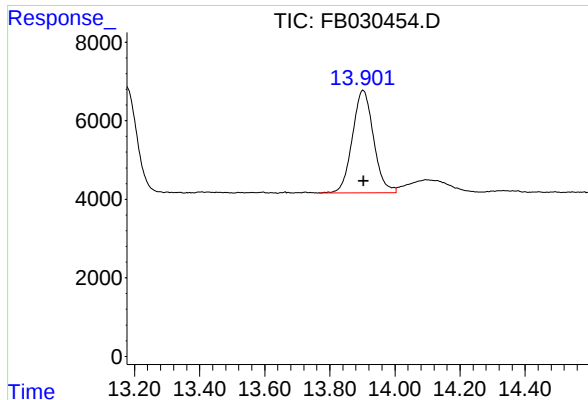

#9 O-Xylene

R.T.: 13.902 min
Delta R.T.: -0.001 min
Response: 117824
Conc: 5.28 ng/ml

Instrument :
FID_B
ClientSampleId :
5 GRO STD

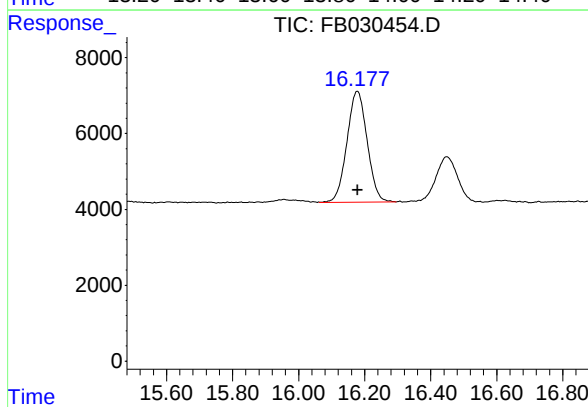

#10 1,2,4-Trimethylbenzene

R.T.: 16.179 min
Delta R.T.: 0.000 min
Response: 124039
Conc: 5.53 ng/ml