

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110823\
 Data File : FB030456.D
 Signal(s) : FID2B.CH
 Acq On : 8 Nov 2023 11:15
 Operator : YP/AJ
 Sample : 20 GRO STD
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 20 GRO STD

Integration File: Calibration.e
 Quant Time: Nov 08 10:34:25 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110823.M
 Quant Title :
 QLast Update : Wed Nov 08 10:33:55 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.780	276253	20.000 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.702	588615	30.000 ng/ml
2) t	2,2,4-Trimethylpentane	7.405	588153	30.000 ng/ml
3) t	n-Heptane	7.740	224144	10.000 ng/ml
4) t	Benzene	7.876	254345	10.000 ng/ml
6) t	Toluene	10.608	745245	30.000 ng/ml
7) t	Ethylbenzene	13.044	231730	10.000 ng/ml
8) t	m-Xylene	13.177	460619	20.000 ng/ml
9) t	O-Xylene	13.904	446426	20.000 ng/ml
10) t	1,2,4-Trimethylbenzene	16.179	449008	20.000 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110823\
Data File : FB030456.D
Signal(s) : FID2B.CH
Acq On : 8 Nov 2023 11:15
Operator : YP/AJ
Sample : 20 GRO STD
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
20 GRO STD

Integration File: Calibration.e
Quant Time: Nov 08 10:34:25 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110823.M
Quant Title :
QLast Update : Wed Nov 08 10:33:55 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

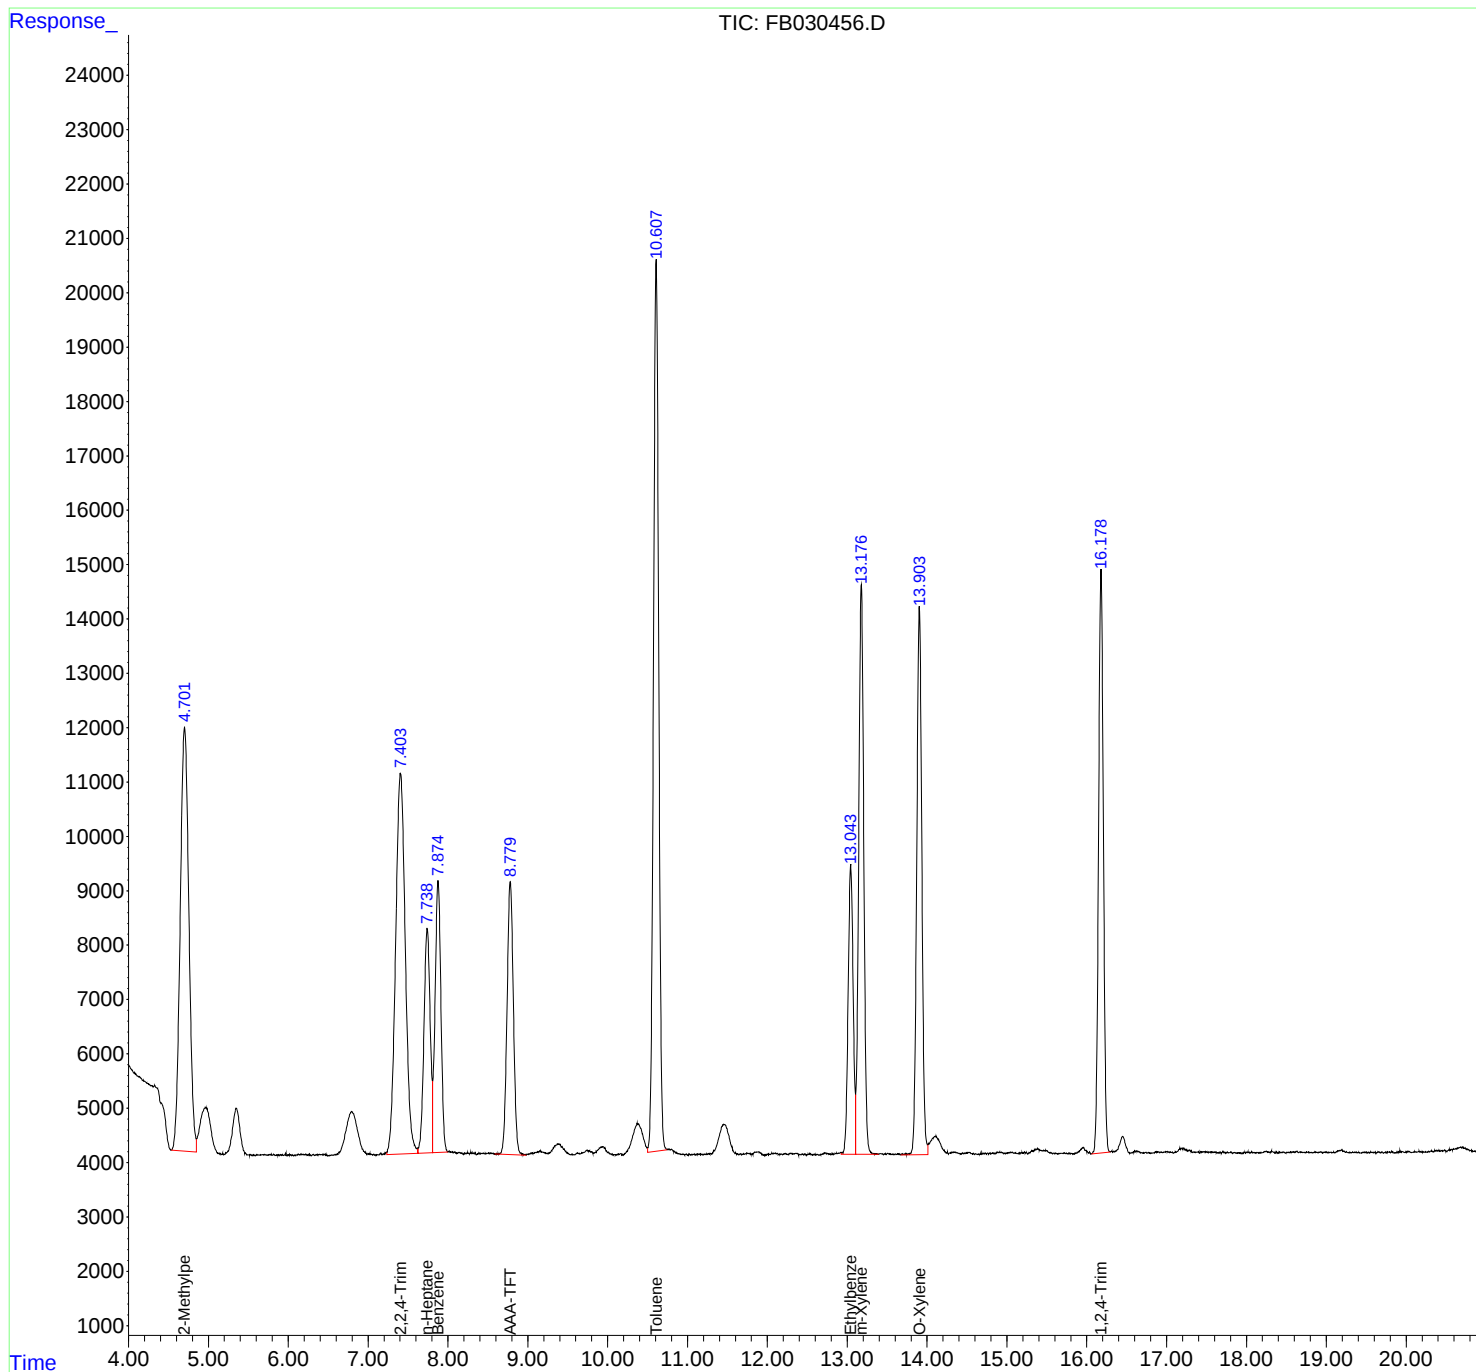


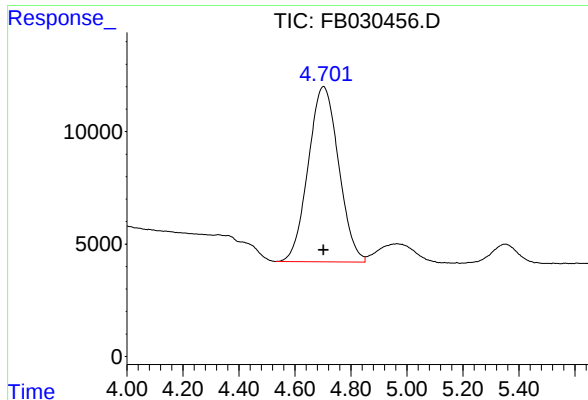

#1 2-Methylpentane


R.T.: 4.702 min
Delta R.T.: 0.000 min
Response: 588615
Conc: 30.00 ng/ml

Instrument :
FID_B
ClientSampleId :
20 GRO STD

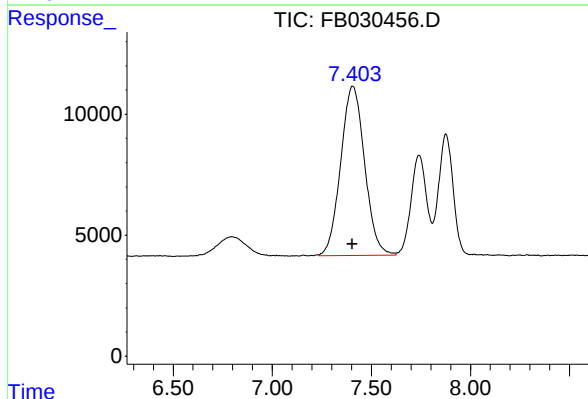


#2 2,2,4-Trimethylpentane

R.T.: 7.405 min
Delta R.T.: 0.000 min
Response: 588153
Conc: 30.00 ng/ml

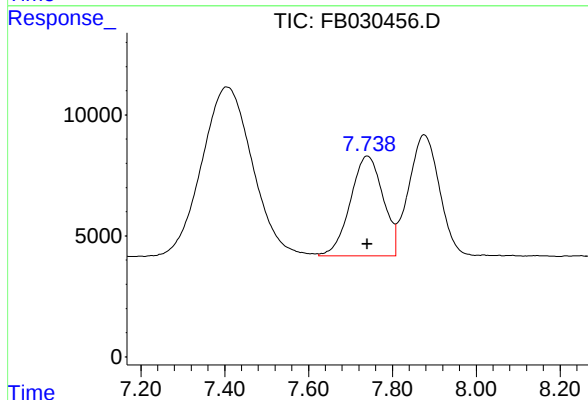


#3 n-Heptane

R.T.: 7.740 min
Delta R.T.: 0.000 min
Response: 224144
Conc: 10.00 ng/ml

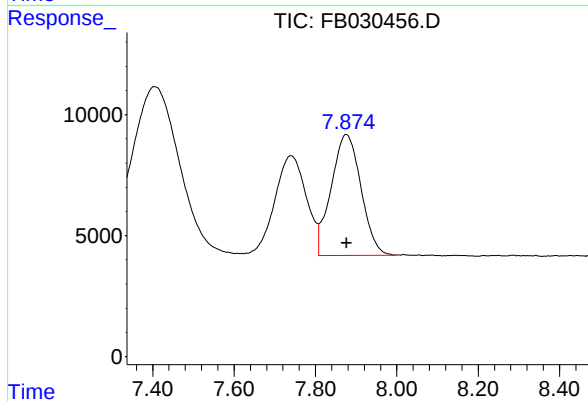

#4 Benzene


R.T.: 7.876 min
Delta R.T.: 0.000 min
Response: 254345
Conc: 10.00 ng/ml

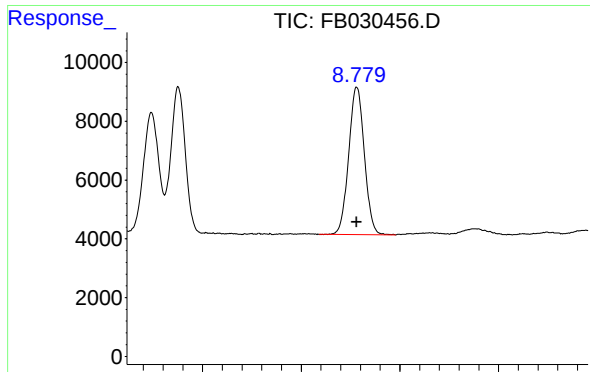

#5 AAA-TFT


R.T.: 8.780 min
Delta R.T.: 0.000 min
Response: 276253
Conc: 20.00 ng/ml

Instrument :
FID_B
ClientSampleId :
20 GRO STD

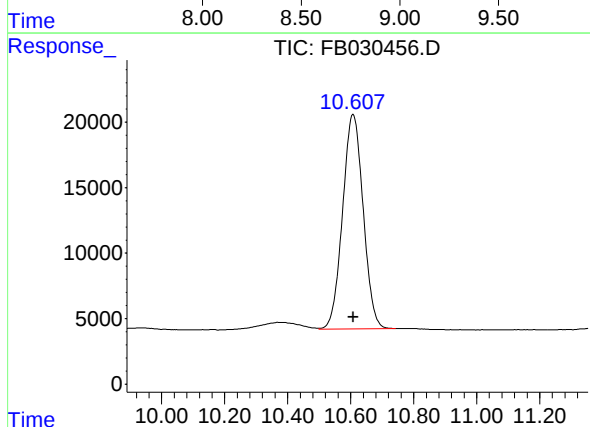


#6 Toluene

R.T.: 10.608 min
Delta R.T.: 0.000 min
Response: 745245
Conc: 30.00 ng/ml

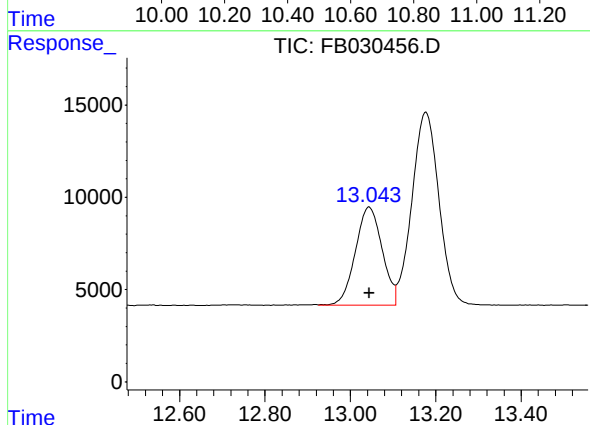


#7 Ethylbenzene

R.T.: 13.044 min
Delta R.T.: 0.000 min
Response: 231730
Conc: 10.00 ng/ml

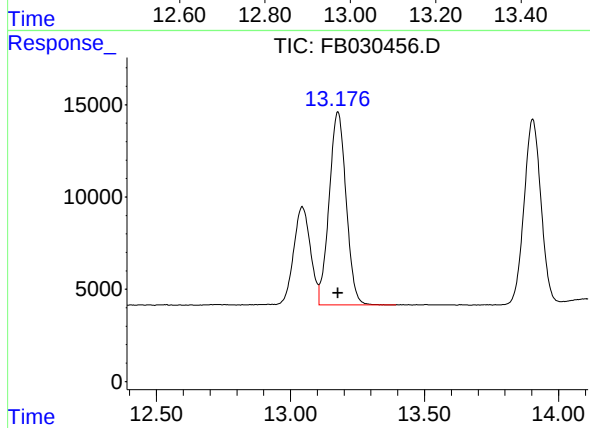

#8 m-Xylene


R.T.: 13.177 min
Delta R.T.: 0.000 min
Response: 460619
Conc: 20.00 ng/ml

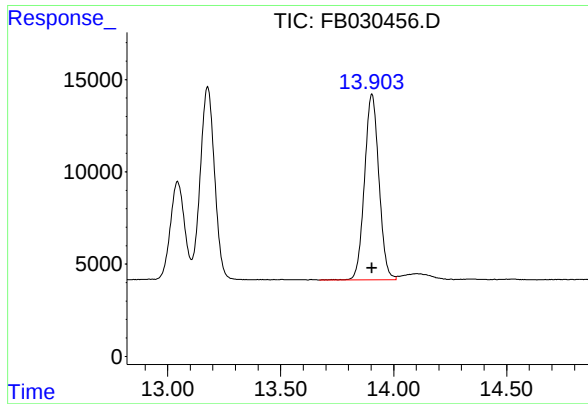

#9 O-Xylene

R.T.: 13.904 min
Delta R.T.: 0.000 min
Response: 446426
Conc: 20.00 ng/ml

Instrument :
FID_B
ClientSampleId :
20 GRO STD

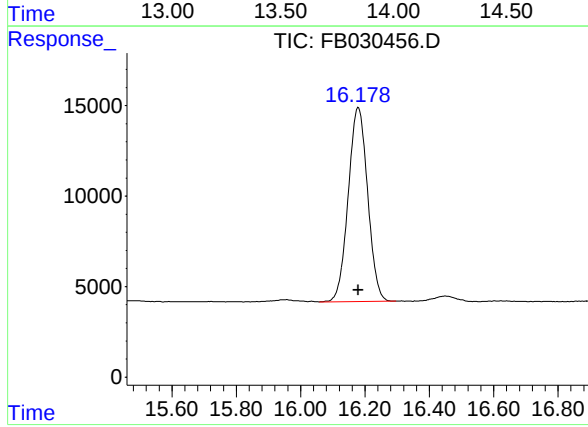

#10 1,2,4-Trimethylbenzene

R.T.: 16.179 min
Delta R.T.: 0.000 min
Response: 449008
Conc: 20.00 ng/ml