

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110823\
 Data File : FB030459.D
 Signal(s) : FID2B.CH
 Acq On : 8 Nov 2023 13:09
 Operator : YP/AJ
 Sample : FB110823GROICV
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 FB110823GROICV

Integration File: Calibration.e
 Quant Time: Nov 08 12:12:37 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110823.M
 Quant Title :
 QLast Update : Wed Nov 08 11:36:32 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.782	229091	16.856 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.699	595241	29.854 ng/ml
2) t 2,2,4-Trimethylpentane	7.404	586135	29.582 ng/ml
3) t n-Heptane	7.741	229069	10.137 ng/ml
4) t Benzene	7.877	256311	9.876 ng/ml
6) t Toluene	10.608	752803	30.034 ng/ml
7) t Ethylbenzene	13.044	233494	10.012 ng/ml
8) t m-Xylene	13.177	464162	19.999 ng/ml
9) t O-Xylene	13.904	446997	19.865 ng/ml
10) t 1,2,4-Trimethylbenzene	16.179	449043	19.959 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110823\
Data File : FB030459.D
Signal(s) : FID2B.CH
Acq On : 8 Nov 2023 13:09
Operator : YP/AJ
Sample : FB110823GROICV
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
FB110823GROICV

Integration File: Calibration.e
Quant Time: Nov 08 12:12:37 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110823.M
Quant Title :
QLast Update : Wed Nov 08 11:36:32 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

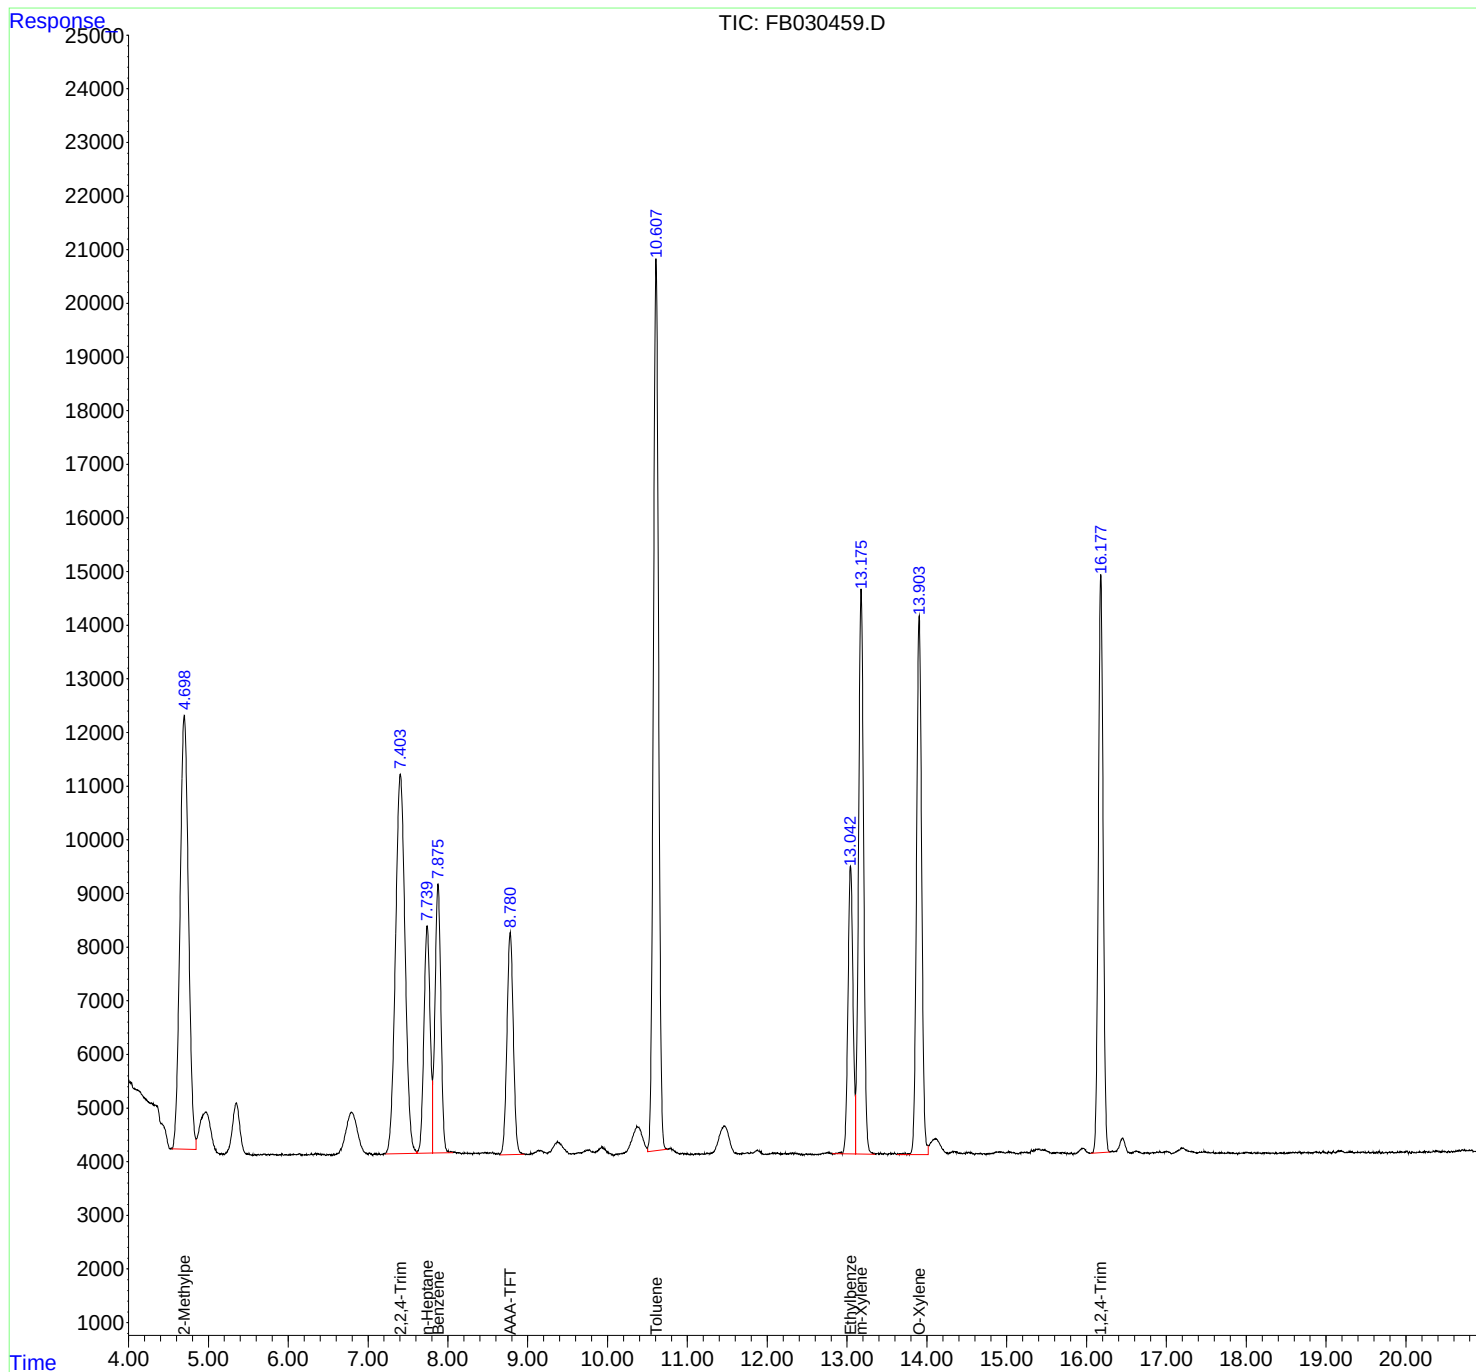


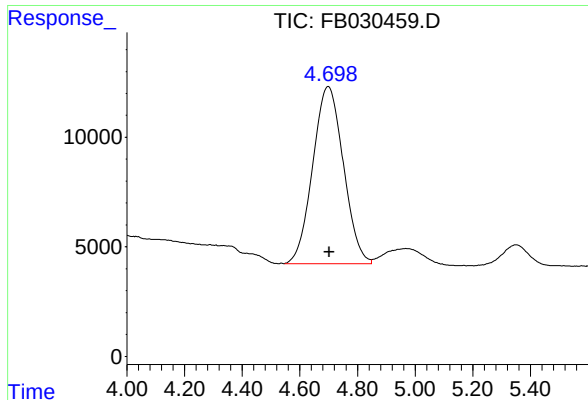

#1 2-Methylpentane


R.T.: 4.699 min
Delta R.T.: -0.003 min
Response: 595241
Conc: 29.85 ng/ml

Instrument :
FID_B
ClientSampleId :
FB110823GROICV

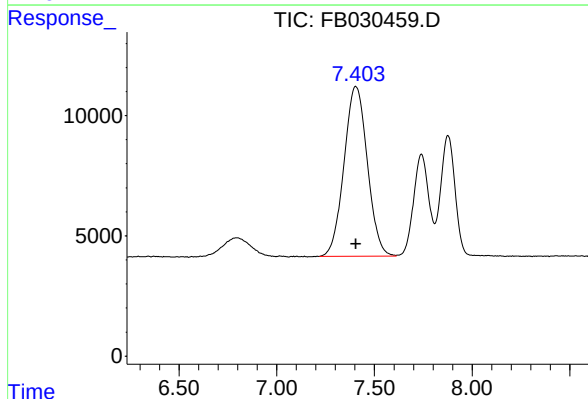


#2 2,2,4-Trimethylpentane

R.T.: 7.404 min
Delta R.T.: 0.000 min
Response: 586135
Conc: 29.58 ng/ml

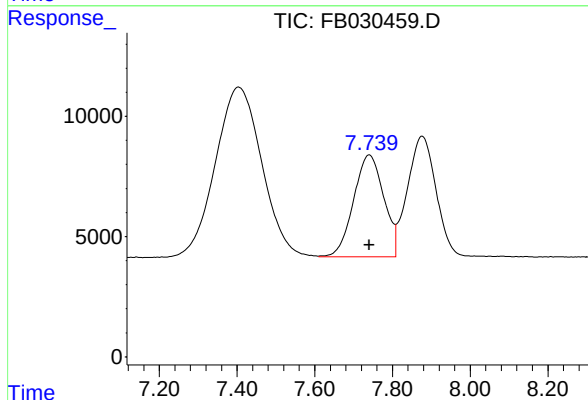


#3 n-Heptane

R.T.: 7.741 min
Delta R.T.: 0.000 min
Response: 229069
Conc: 10.14 ng/ml

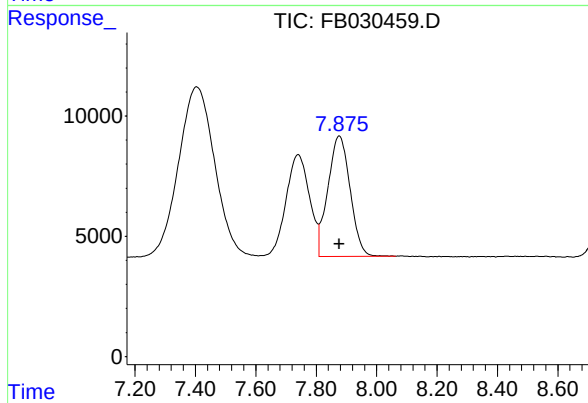

#4 Benzene


R.T.: 7.877 min
Delta R.T.: 0.000 min
Response: 256311
Conc: 9.88 ng/ml

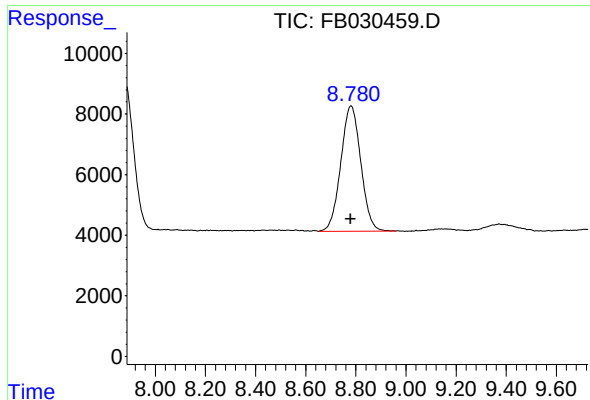

#5 AAA-TFT


R.T.: 8.782 min
Delta R.T.: 0.001 min
Response: 229091
Conc: 16.86 ng/ml

Instrument :
FID_B
ClientSampleId :
FB110823GROICV

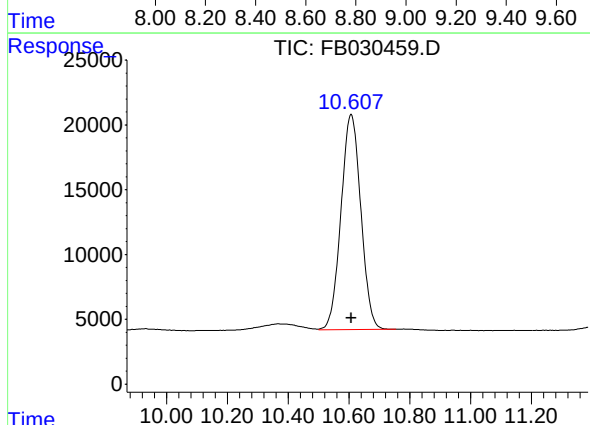


#6 Toluene

R.T.: 10.608 min
Delta R.T.: 0.000 min
Response: 752803
Conc: 30.03 ng/ml

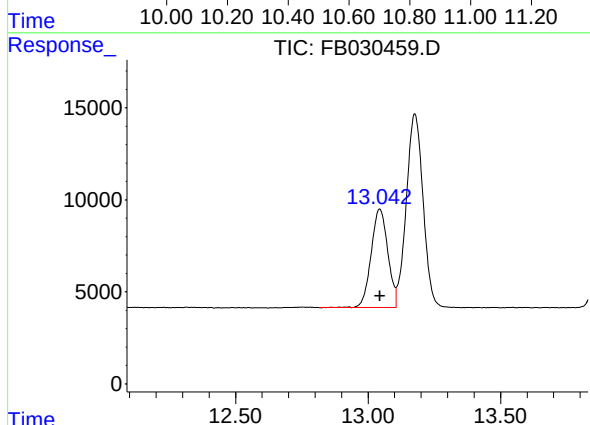


#7 Ethylbenzene

R.T.: 13.044 min
Delta R.T.: 0.000 min
Response: 233494
Conc: 10.01 ng/ml

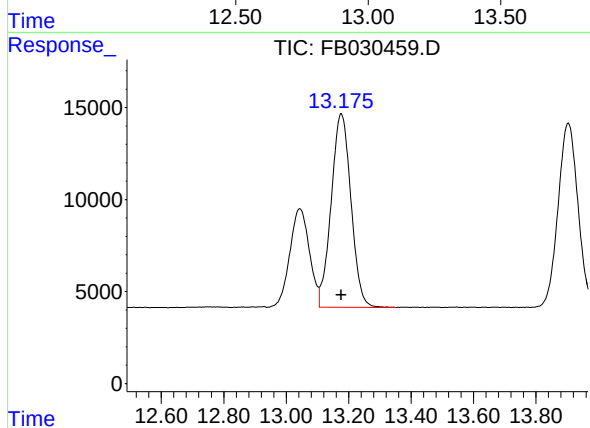

#8 m-Xylene


R.T.: 13.177 min
Delta R.T.: 0.000 min
Response: 464162
Conc: 20.00 ng/ml

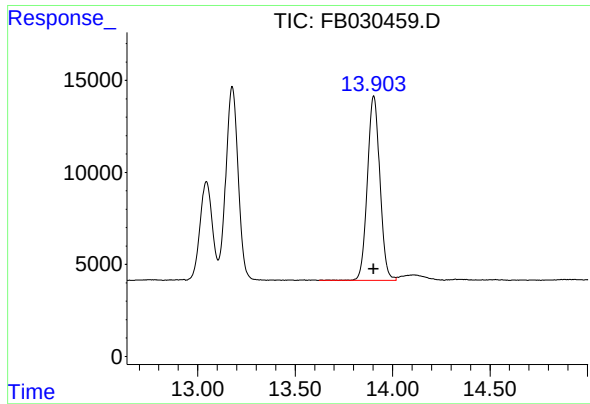

#9 O-Xylene

R.T.: 13.904 min
Delta R.T.: 0.000 min
Response: 446997
Conc: 19.87 ng/ml

Instrument :
FID_B
ClientSampleId :
FB110823GROICV

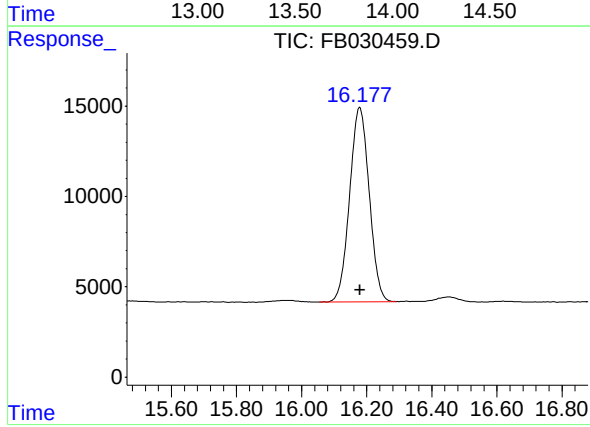

#10 1,2,4-Trimethylbenzene

R.T.: 16.179 min
Delta R.T.: 0.000 min
Response: 449043
Conc: 19.96 ng/ml