

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111022\
Data File : FB028902.D
Signal(s) : FID2B.CH
Acq On : 10 Nov 2022 13:34
Operator : AJ/MA
Sample : N5494-16 50X
Misc : 5.03G/5.00 ML MEOH
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Nov 10 13:54:42 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110122.M
Quant Title :
QLast Update : Tue Nov 01 12:44:12 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.790	241417	18.998 ng/ml
Target Compounds			
9) t O-Xylene	13.964	2931	0.160 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111022\
Data File : FB028902.D
Signal(s) : FID2B.CH
Acq On : 10 Nov 2022 13:34
Operator : AJ/MA
Sample : N5494-16 50X
Misc : 5.03G/5.00 ML MEOH
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Nov 10 13:54:42 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110122.M
Quant Title :
QLast Update : Tue Nov 01 12:44:12 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

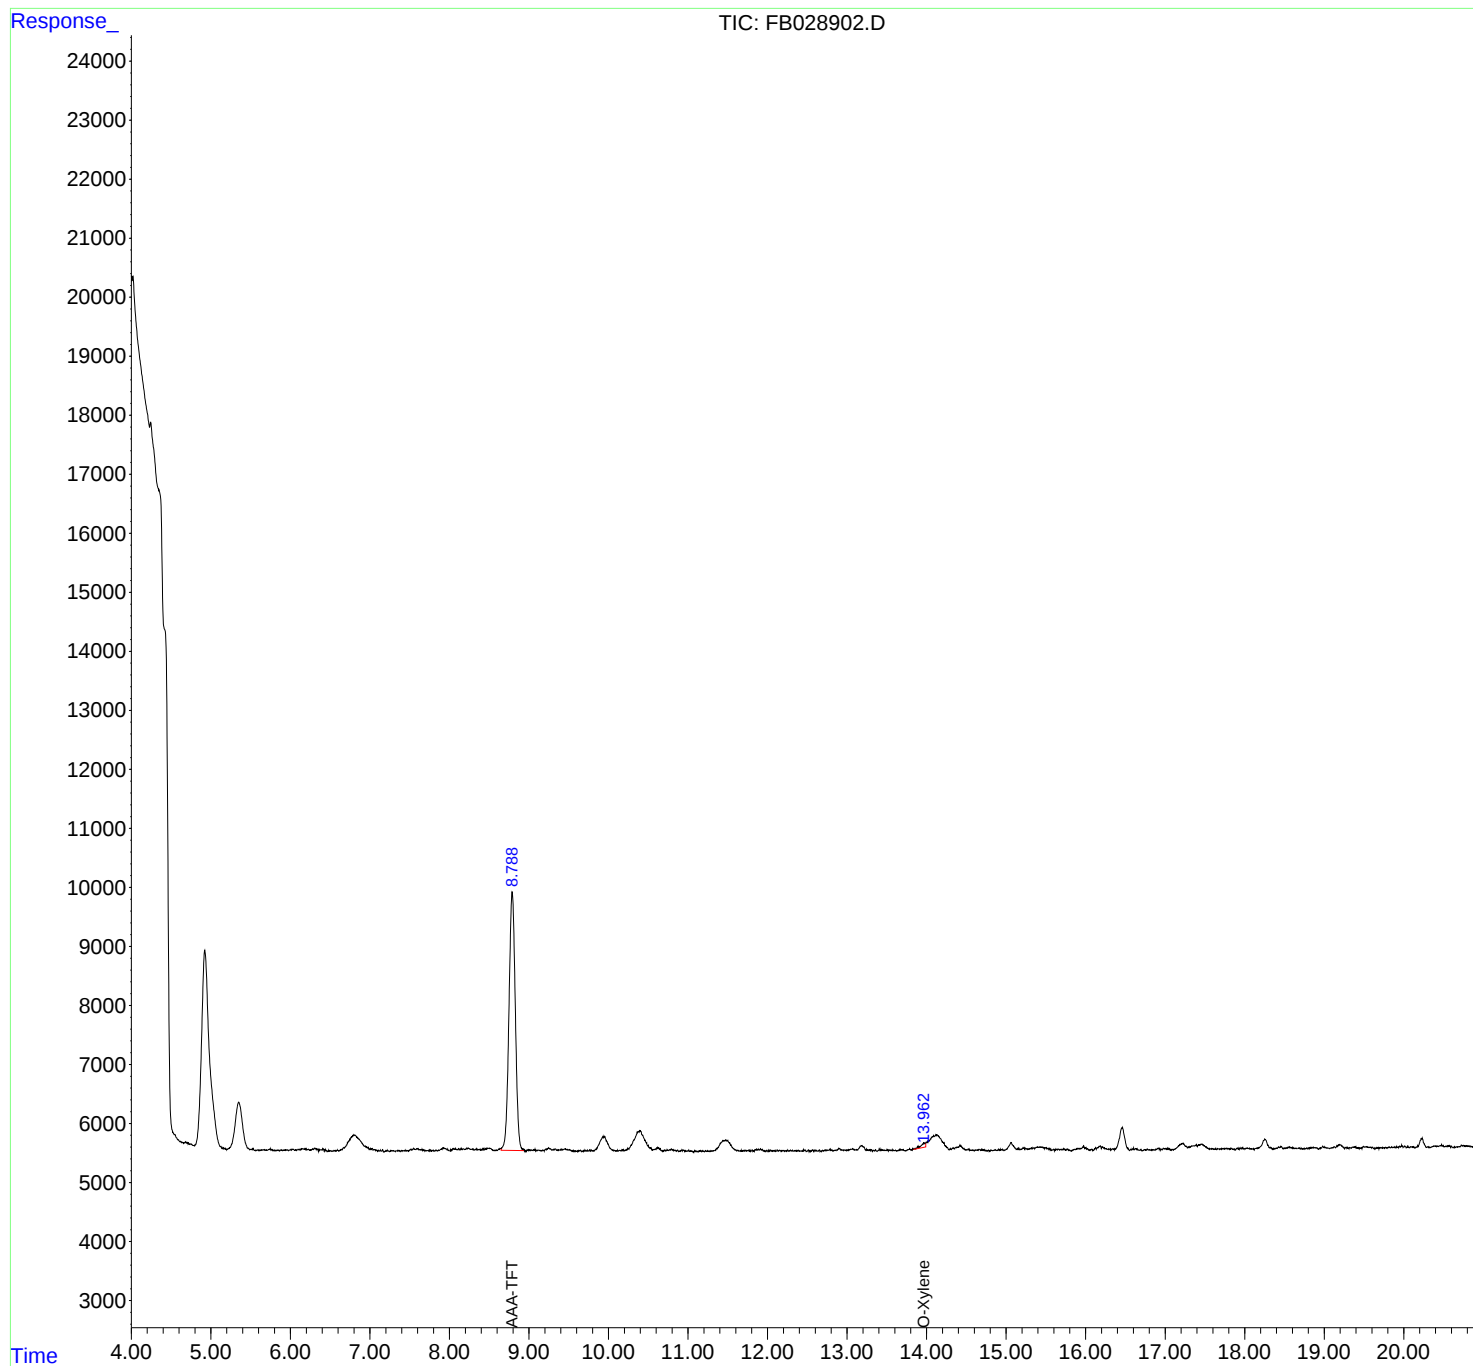


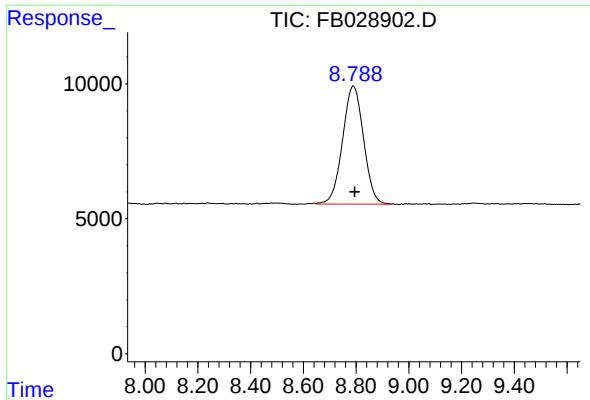

#5 AAA-TFT

R.T.: 8.790 min
Delta R.T.: -0.005 min
Response: 241417
Conc: 19.00 ng/ml

Instrument :
FID_B
ClientSampleId :

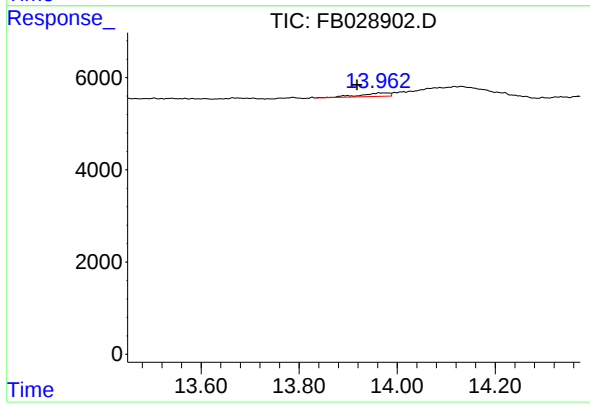

#9 O-Xylene

R.T.: 13.964 min
Delta R.T.: 0.045 min
Response: 2931
Conc: 0.16 ng/ml