

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111022\
 Data File : FB028915.D
 Signal(s) : FID2B.CH
 Acq On : 10 Nov 2022 22:19
 Operator : AJ/MA
 Sample : 20 PPB GRO STD
 Misc : 1.23G/5.00 ML DI WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 20 PPB GRO STD

Integration File: Calibration.e
 Quant Time: Nov 11 07:34:35 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110122.M
 Quant Title :
 QLast Update : Tue Nov 01 12:44:12 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.795	237396	18.682 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.713	408567	25.066 ng/ml
2) t 2,2,4-Trimethylpentane	7.426	470416	26.772 ng/ml
3) t n-Heptane	7.753	145062	8.250 ng/ml
4) t Benzene	7.889	183467	8.947 ng/ml
6) t Toluene	10.622	530527	26.377 ng/ml
7) t Ethylbenzene	13.059	165809	8.743 ng/ml
8) t m-Xylene	13.191	331424	17.617 ng/ml
9) t O-Xylene	13.918	330850	18.035 ng/ml
10) t 1,2,4-Trimethylbenzene	16.192	325554	17.672 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111022\
Data File : FB028915.D
Signal(s) : FID2B.CH
Acq On : 10 Nov 2022 22:19
Operator : AJ/MA
Sample : 20 PPB GRO STD
Misc : 1.23G/5.00 ML DI WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
20 PPB GRO STD

Integration File: Calibration.e
Quant Time: Nov 11 07:34:35 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110122.M
Quant Title :
QLast Update : Tue Nov 01 12:44:12 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

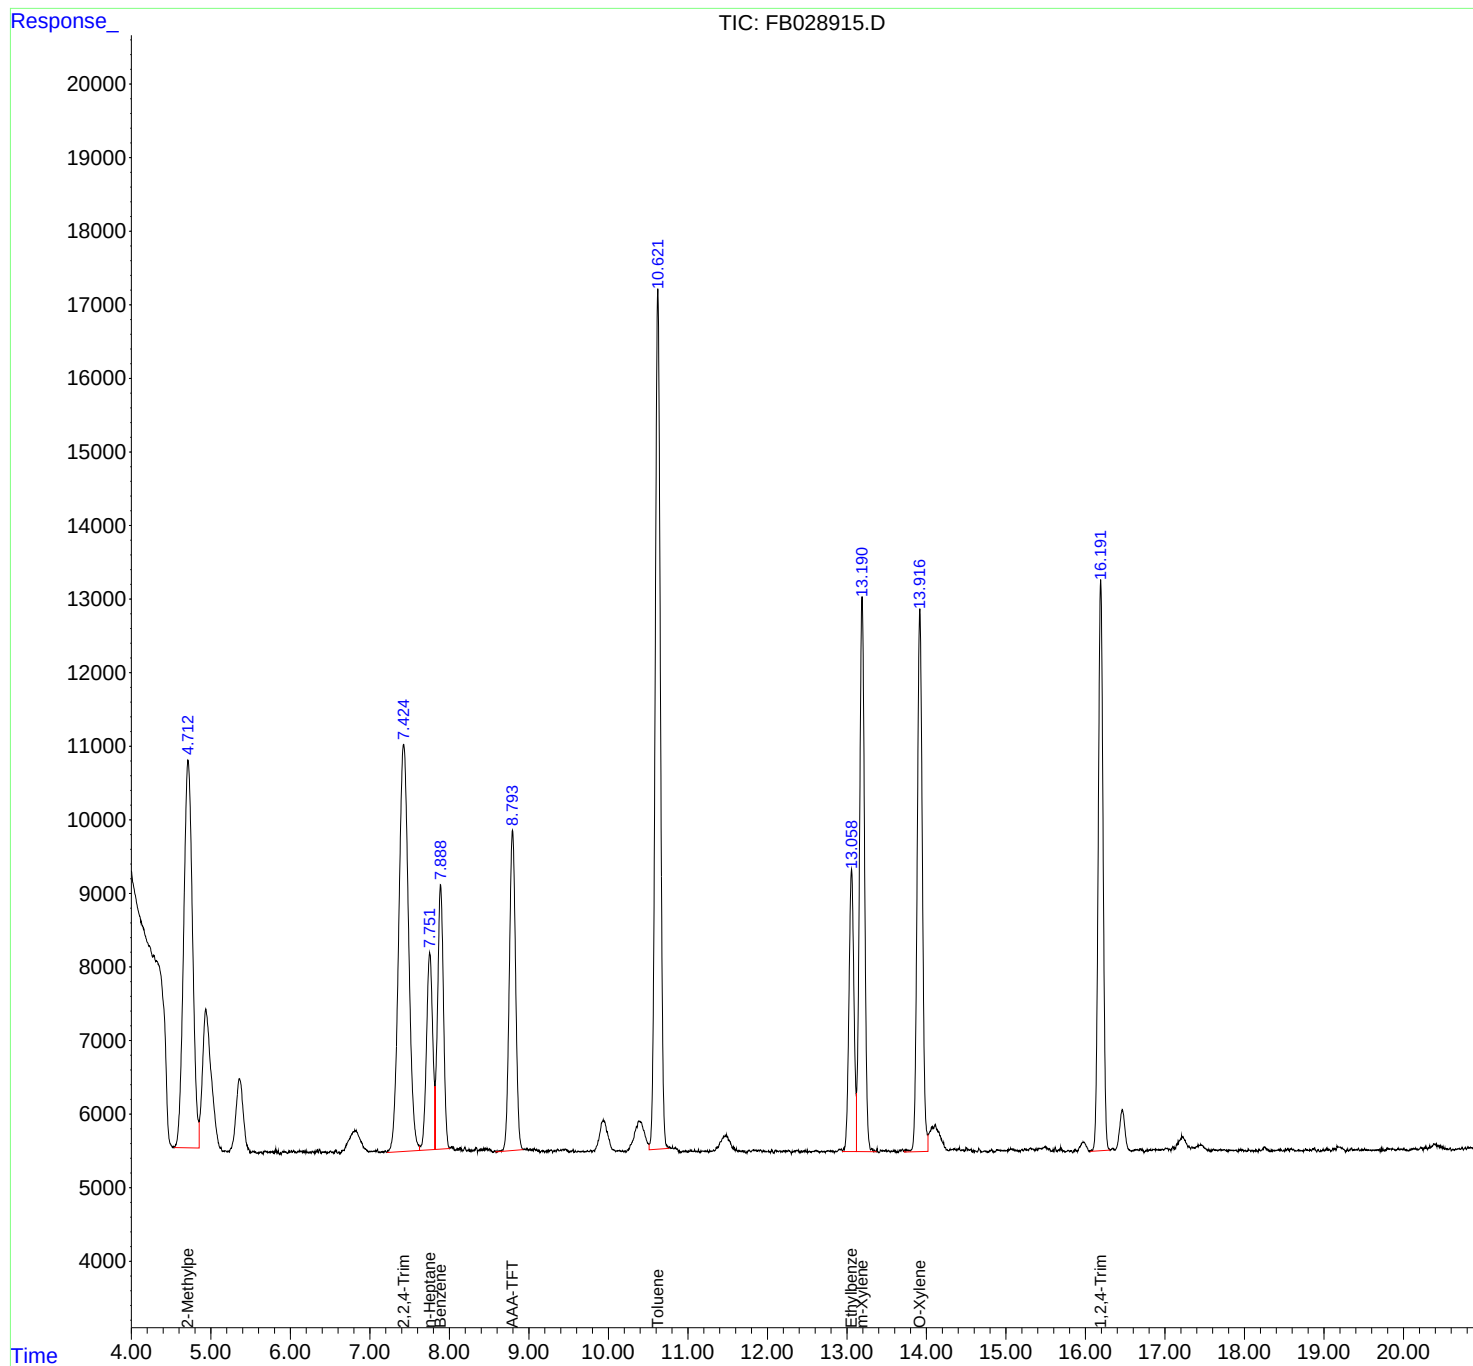


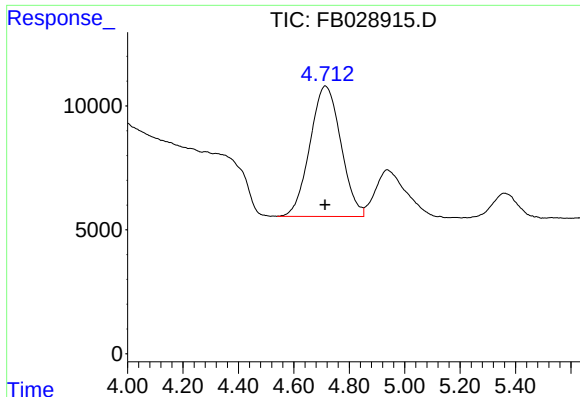

#1 2-Methylpentane


R.T.: 4.713 min
Delta R.T.: 0.001 min
Response: 408567
Conc: 25.07 ng/ml

Instrument :
FID_B
ClientSampleId :
20 PPB GRO STD

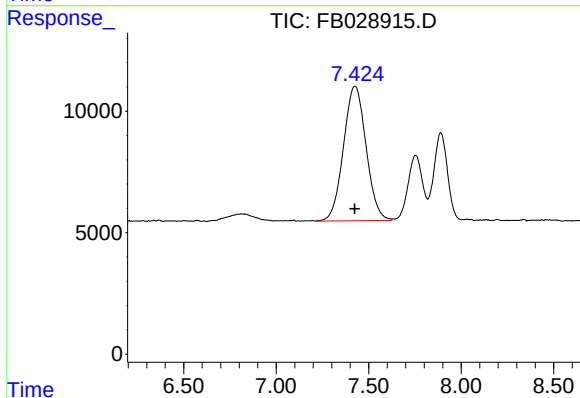


#2 2,2,4-Trimethylpentane

R.T.: 7.426 min
Delta R.T.: 0.001 min
Response: 470416
Conc: 26.77 ng/ml

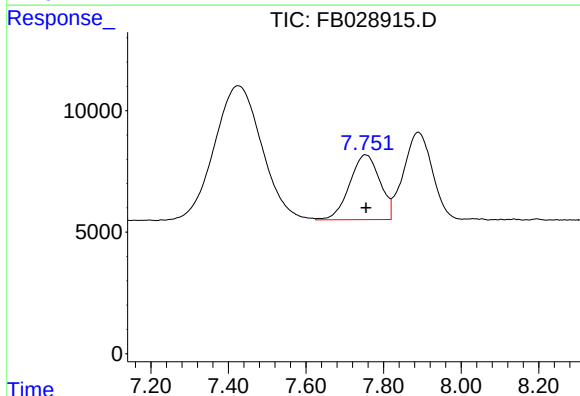


#3 n-Heptane

R.T.: 7.753 min
Delta R.T.: -0.002 min
Response: 145062
Conc: 8.25 ng/ml

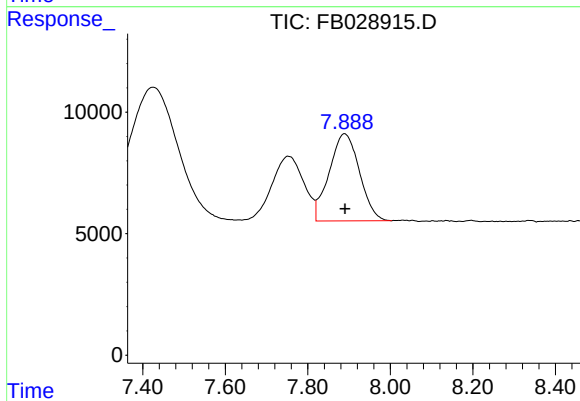

#4 Benzene


R.T.: 7.889 min
Delta R.T.: -0.001 min
Response: 183467
Conc: 8.95 ng/ml

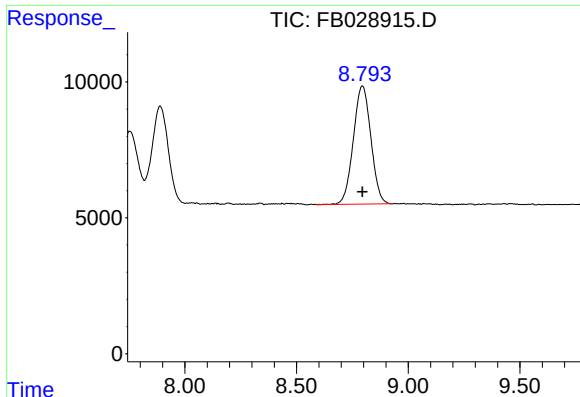

#5 AAA-TFT


R.T.: 8.795 min
Delta R.T.: 0.000 min
Response: 237396
Conc: 18.68 ng/ml

Instrument :
FID_B
ClientSampleId :
20 PPB GRO STD

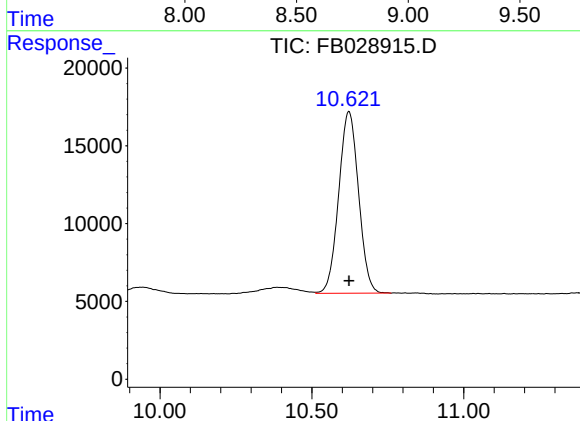


#6 Toluene

R.T.: 10.622 min
Delta R.T.: 0.000 min
Response: 530527
Conc: 26.38 ng/ml

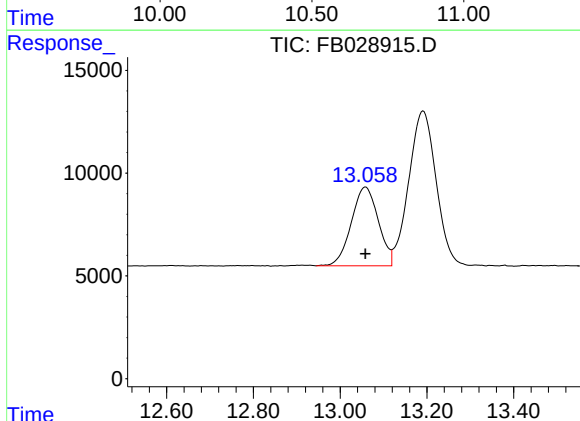


#7 Ethylbenzene

R.T.: 13.059 min
Delta R.T.: 0.000 min
Response: 165809
Conc: 8.74 ng/ml

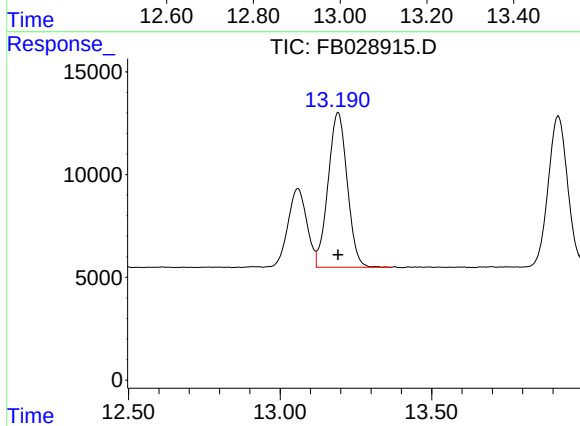

#8 m-Xylene


R.T.: 13.191 min
Delta R.T.: 0.000 min
Response: 331424
Conc: 17.62 ng/ml

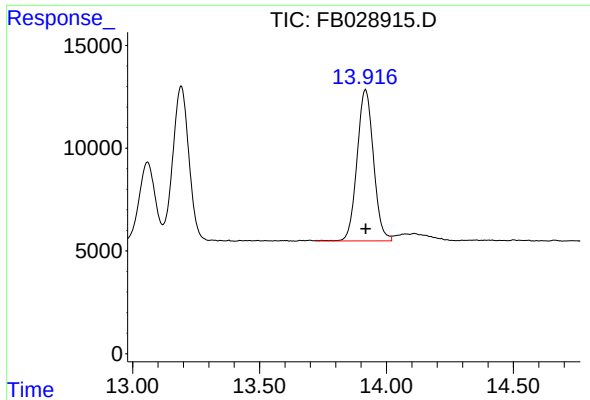

#9 O-Xylene

R.T.: 13.918 min
Delta R.T.: 0.000 min
Response: 330850
Conc: 18.03 ng/ml

Instrument :
FID_B
ClientSampleId :
20 PPB GRO STD

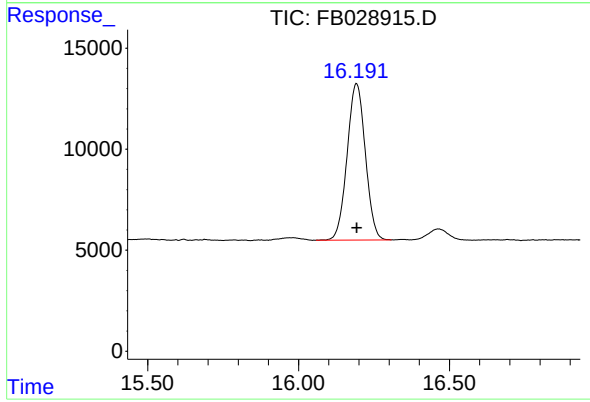

#10 1,2,4-Trimethylbenzene

R.T.: 16.192 min
Delta R.T.: 0.000 min
Response: 325554
Conc: 17.67 ng/ml