

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111022\
 Data File : FB028918.D
 Signal(s) : FID2B.CH
 Acq On : 11 Nov 2022 00:49
 Operator : AJ/MA
 Sample : N5495-09MS 50X
 Misc : 5.00G/5.00 ML MEOH
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Nov 11 07:34:48 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110122.M
 Quant Title :
 QLast Update : Tue Nov 01 12:44:12 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.791	246691	19.413 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.704	418749	25.691 ng/ml
2) t 2,2,4-Trimethylpentane	7.421	502345	28.589 ng/ml
3) t n-Heptane	7.749	156314	8.890 ng/ml
4) t Benzene	7.885	209676	10.225 ng/ml
6) t Toluene	10.619	584466	29.059 ng/ml
7) t Ethylbenzene	13.057	185601	9.786 ng/ml
8) t m-Xylene	13.189	371344	19.739 ng/ml
9) t O-Xylene	13.917	366063	19.954 ng/ml
10) t 1,2,4-Trimethylbenzene	16.191	344106	18.679 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111022\
Data File : FB028918.D
Signal(s) : FID2B.CH
Acq On : 11 Nov 2022 00:49
Operator : AJ/MA
Sample : N5495-09MS 50X
Misc : 5.00G/5.00 ML MEOH
ALS Vial : 26 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Nov 11 07:34:48 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110122.M
Quant Title :
QLast Update : Tue Nov 01 12:44:12 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

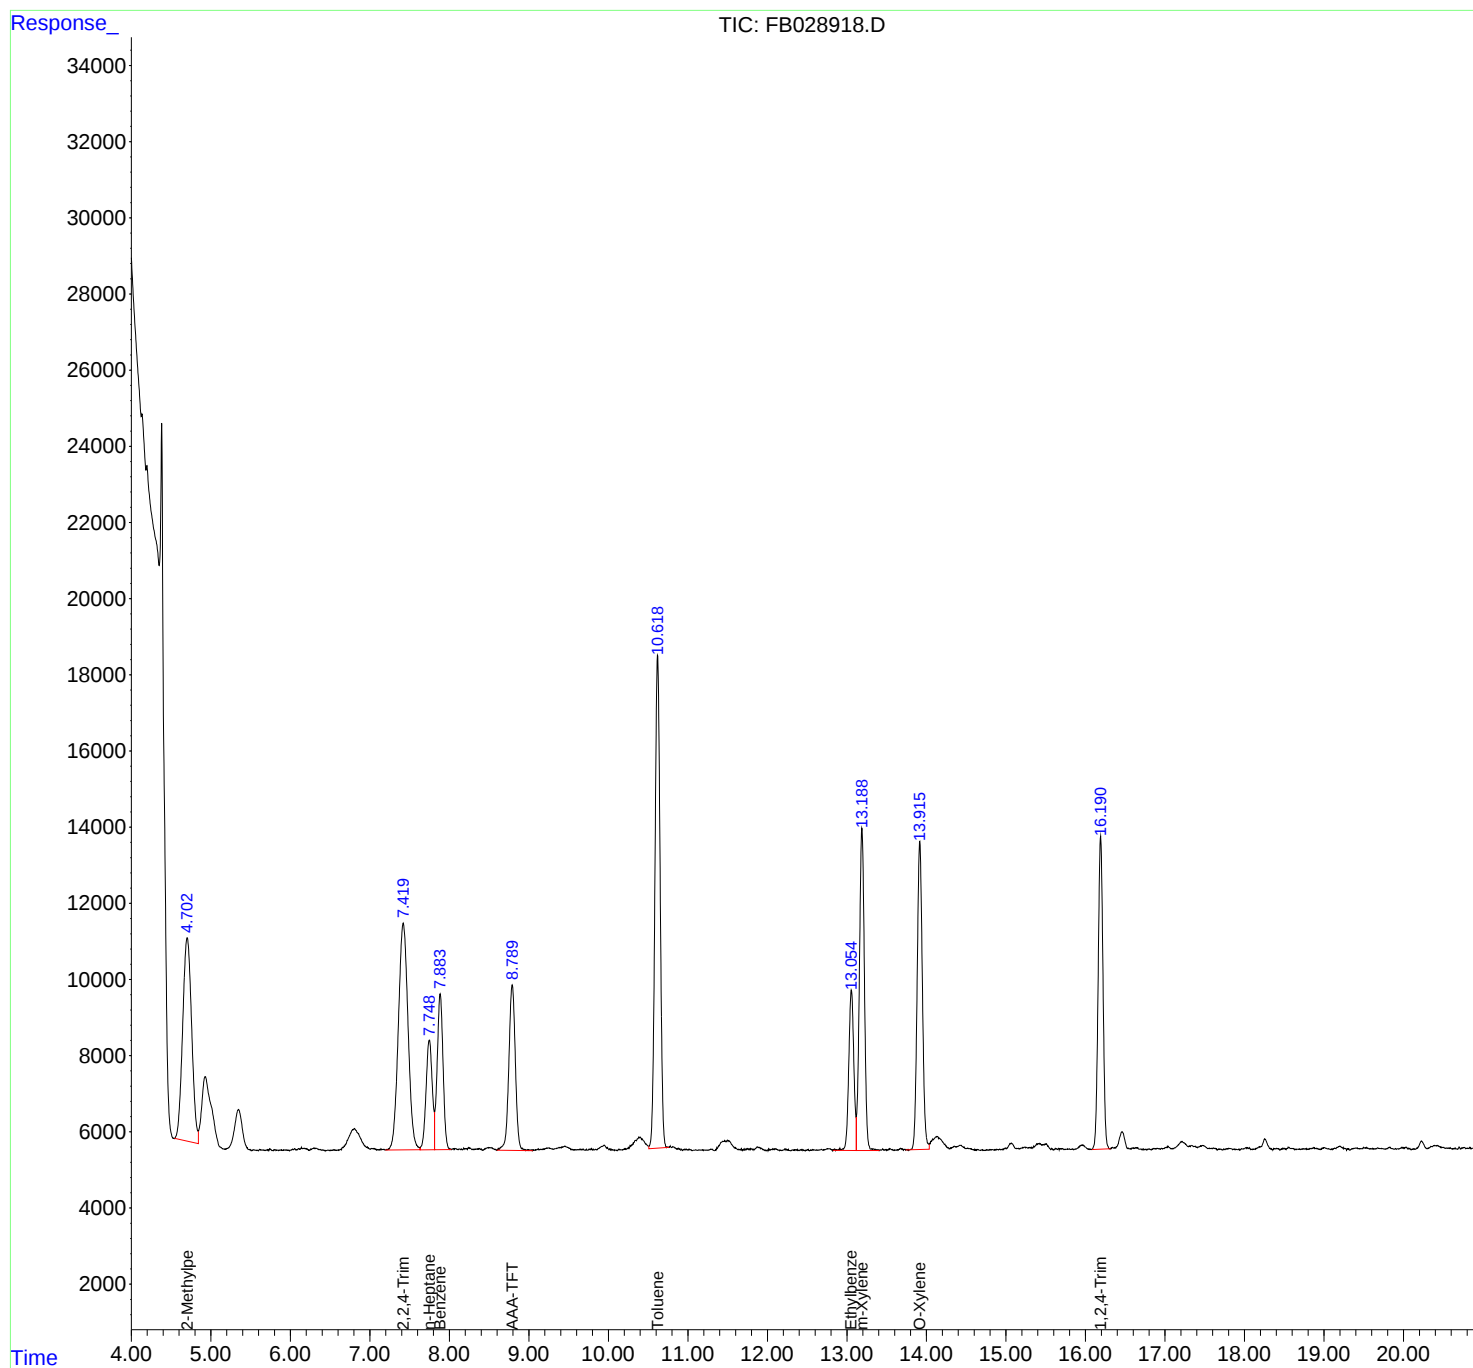


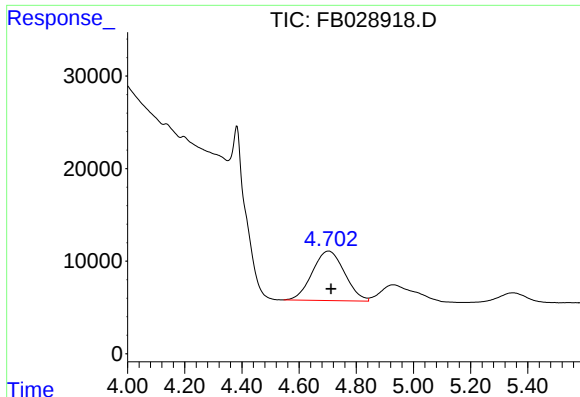

#1 2-Methylpentane


R.T.: 4.704 min
Delta R.T.: -0.008 min
Response: 418749
Conc: 25.69 ng/ml

Instrument :
FID_B
ClientSampleId :

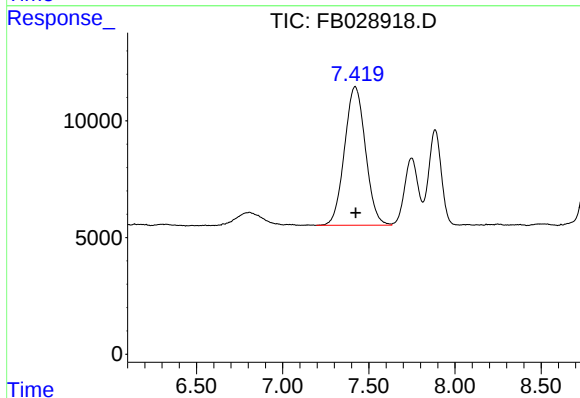


#2 2,2,4-Trimethylpentane

R.T.: 7.421 min
Delta R.T.: -0.004 min
Response: 502345
Conc: 28.59 ng/ml

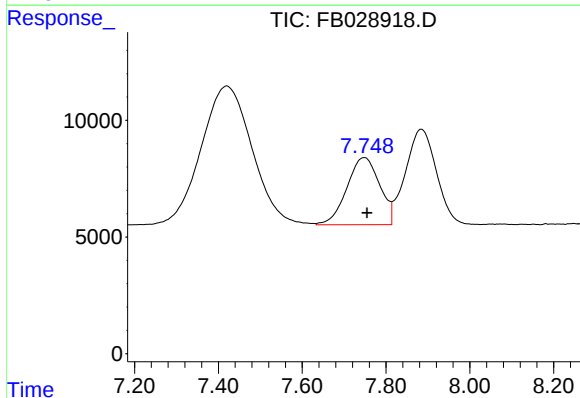


#3 n-Heptane

R.T.: 7.749 min
Delta R.T.: -0.006 min
Response: 156314
Conc: 8.89 ng/ml

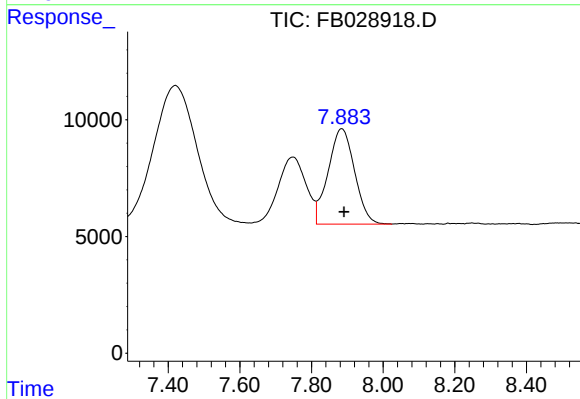

#4 Benzene


R.T.: 7.885 min
Delta R.T.: -0.006 min
Response: 209676
Conc: 10.22 ng/ml

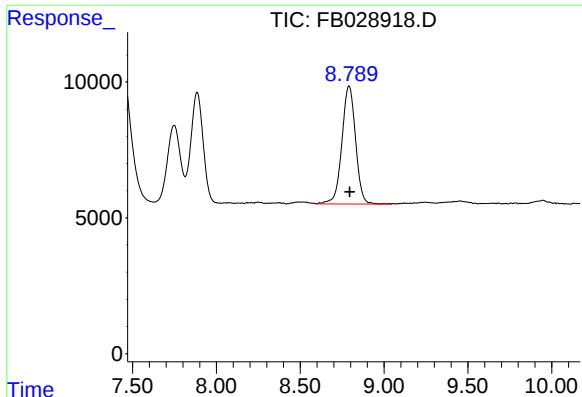

#5 AAA-TFT


R.T.: 8.791 min
Delta R.T.: -0.004 min
Response: 246691
Conc: 19.41 ng/ml

Instrument :
FID_B
ClientSampleId :

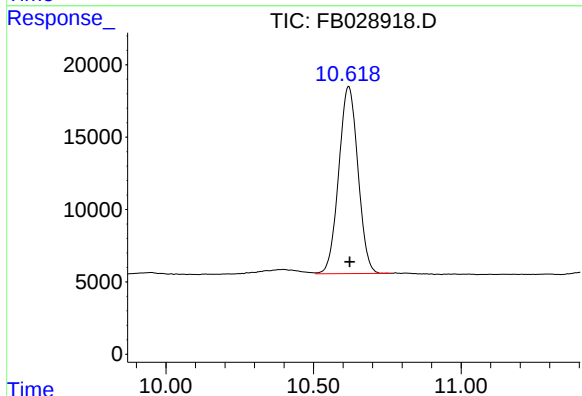


#6 Toluene

R.T.: 10.619 min
Delta R.T.: -0.004 min
Response: 584466
Conc: 29.06 ng/ml

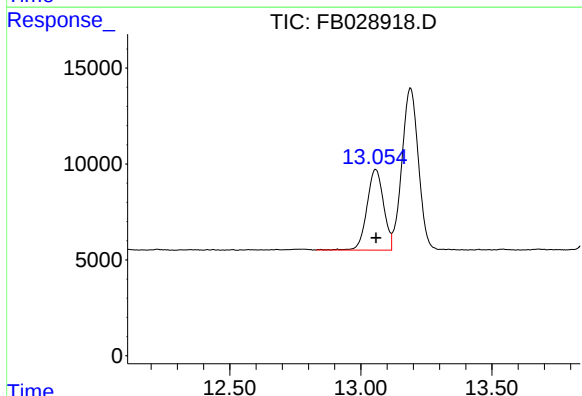


#7 Ethylbenzene

R.T.: 13.057 min
Delta R.T.: -0.002 min
Response: 185601
Conc: 9.79 ng/ml

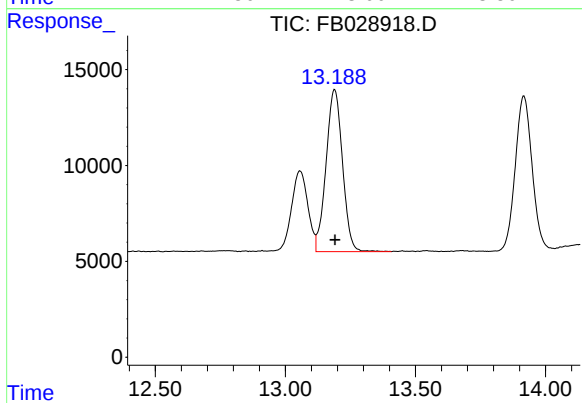

#8 m-Xylene


R.T.: 13.189 min
Delta R.T.: -0.002 min
Response: 371344
Conc: 19.74 ng/ml

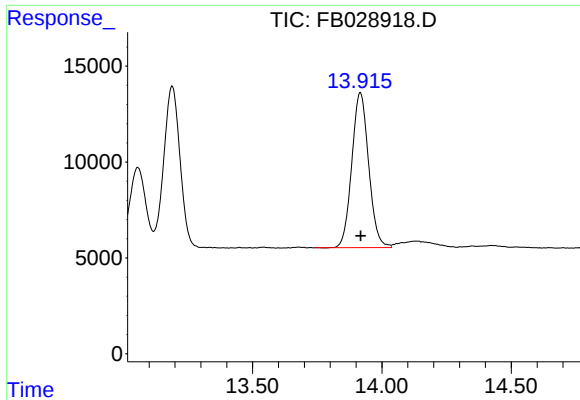

#9 O-Xylene

R.T.: 13.917 min
Delta R.T.: -0.001 min
Response: 366063
Conc: 19.95 ng/ml

Instrument :
FID_B
ClientSampleId :

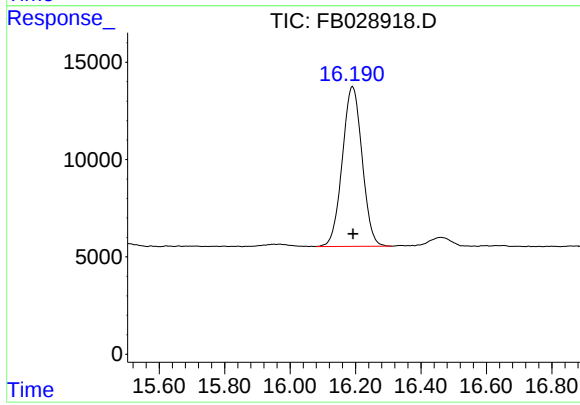

#10 1,2,4-Trimethylbenzene

R.T.: 16.191 min
Delta R.T.: -0.002 min
Response: 344106
Conc: 18.68 ng/ml