

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111022\
 Data File : FB028919.D
 Signal(s) : FID2B.CH
 Acq On : 11 Nov 2022 1:26
 Operator : AJ/MA
 Sample : N5495-09MSD 50X
 Misc : 5.00G/5.00 ML MEOH
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Nov 11 07:34:53 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110122.M
 Quant Title :
 QLast Update : Tue Nov 01 12:44:12 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.793	261412	20.572 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.703	366302	22.473 ng/ml
2) t 2,2,4-Trimethylpentane	7.420	416827	23.722 ng/ml
3) t n-Heptane	7.750	142093	8.082 ng/ml
4) t Benzene	7.887	184756	9.010 ng/ml
6) t Toluene	10.621	529488	26.326 ng/ml
7) t Ethylbenzene	13.057	166544	8.781 ng/ml
8) t m-Xylene	13.190	328591	17.466 ng/ml
9) t O-Xylene	13.918	319054	17.392 ng/ml
10) t 1,2,4-Trimethylbenzene	16.192	286629	15.559 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111022\
Data File : FB028919.D
Signal(s) : FID2B.CH
Acq On : 11 Nov 2022 1:26
Operator : AJ/MA
Sample : N5495-09MSD 50X
Misc : 5.00G/5.00 ML MEOH
ALS Vial : 27 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Nov 11 07:34:53 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110122.M
Quant Title :
QLast Update : Tue Nov 01 12:44:12 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

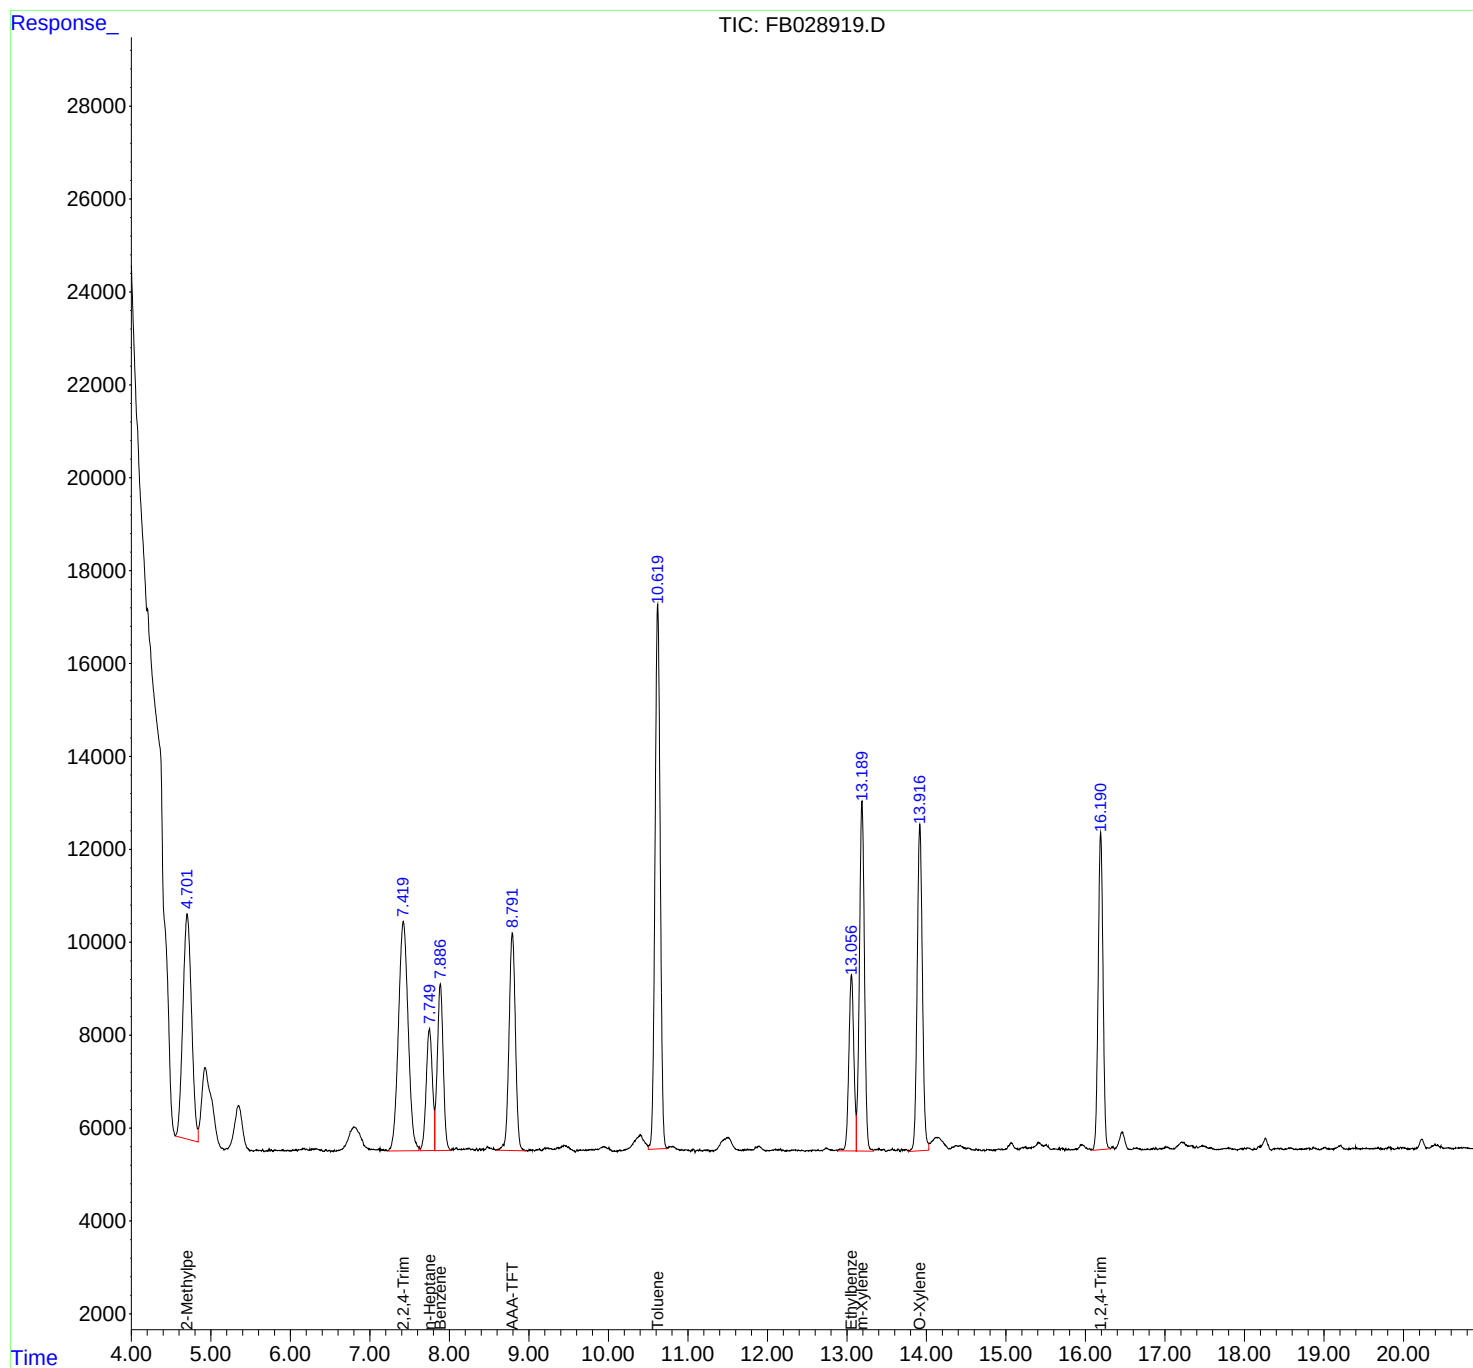


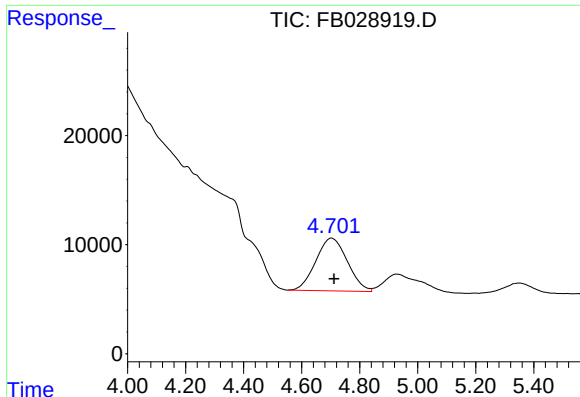

#1 2-Methylpentane


R.T.: 4.703 min
Delta R.T.: -0.009 min
Response: 366302
Conc: 22.47 ng/ml

Instrument :
FID_B
ClientSampleId :

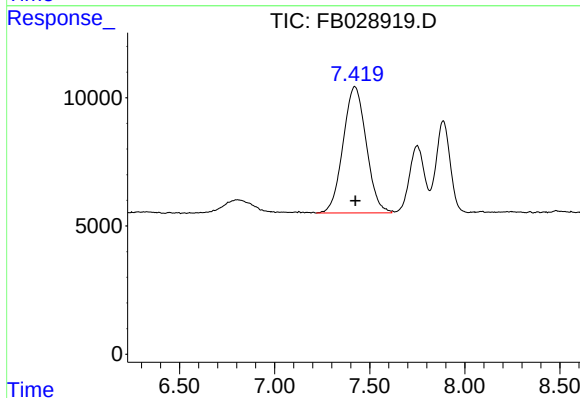


#2 2,2,4-Trimethylpentane

R.T.: 7.420 min
Delta R.T.: -0.004 min
Response: 416827
Conc: 23.72 ng/ml

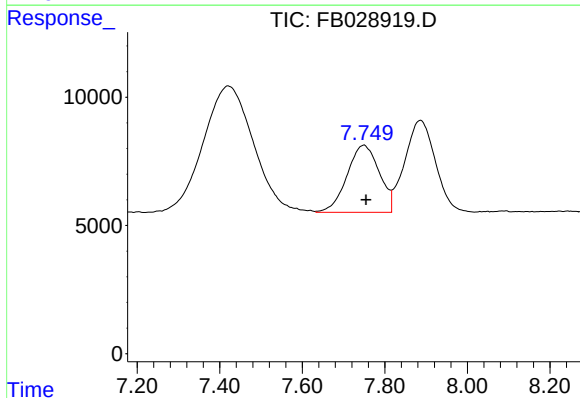


#3 n-Heptane

R.T.: 7.750 min
Delta R.T.: -0.004 min
Response: 142093
Conc: 8.08 ng/ml

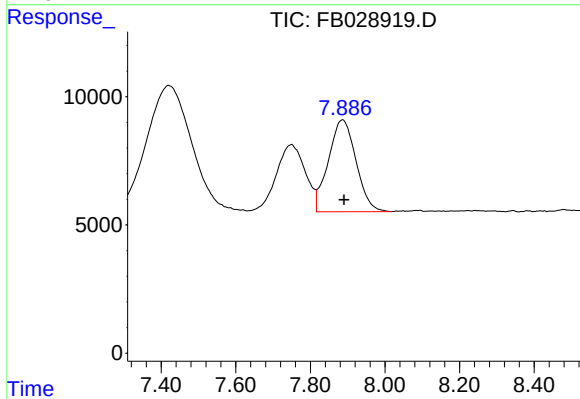

#4 Benzene


R.T.: 7.887 min
Delta R.T.: -0.003 min
Response: 184756
Conc: 9.01 ng/ml

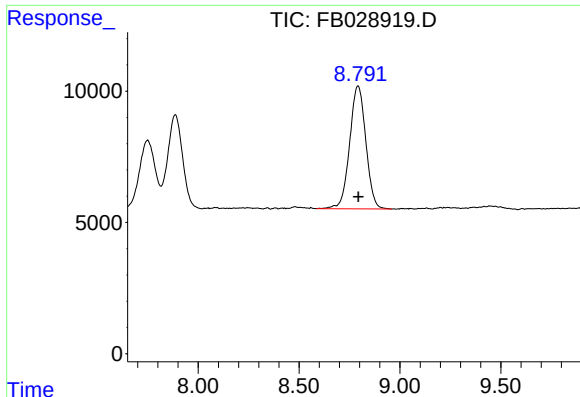

#5 AAA-TFT


R.T.: 8.793 min
Delta R.T.: -0.002 min
Response: 261412
Conc: 20.57 ng/ml

Instrument :
FID_B
ClientSampleId :

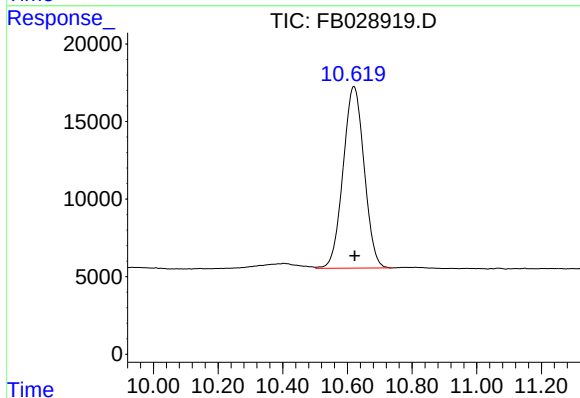


#6 Toluene

R.T.: 10.621 min
Delta R.T.: -0.002 min
Response: 529488
Conc: 26.33 ng/ml

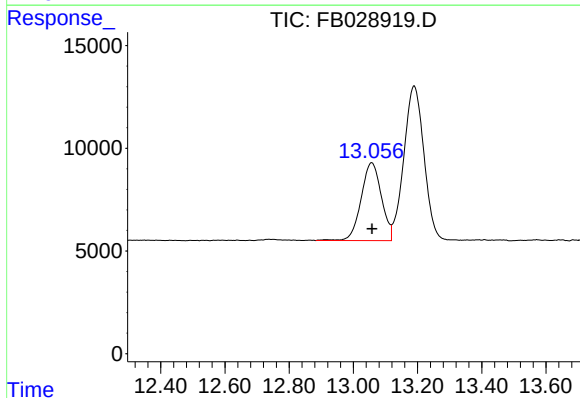


#7 Ethylbenzene

R.T.: 13.057 min
Delta R.T.: 0.000 min
Response: 166544
Conc: 8.78 ng/ml

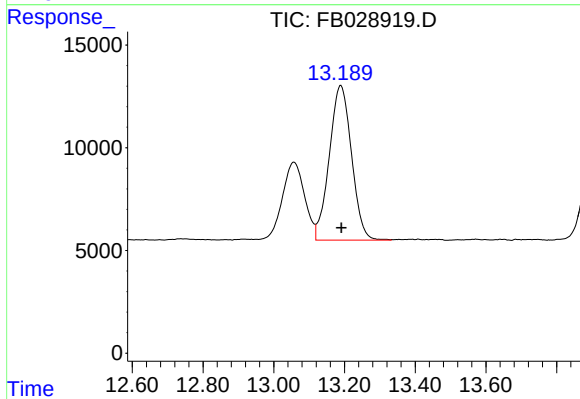

#8 m-Xylene


R.T.: 13.190 min
Delta R.T.: -0.001 min
Response: 328591
Conc: 17.47 ng/ml

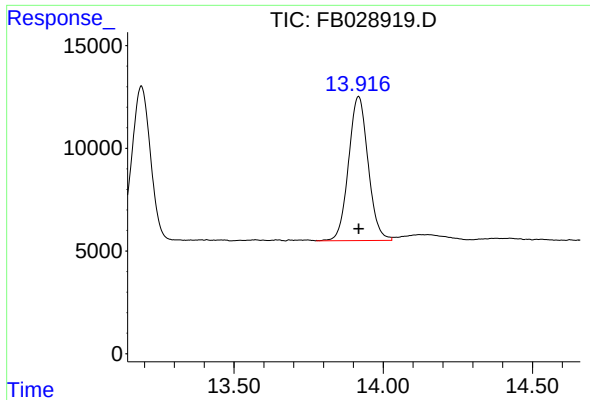

#9 O-Xylene

R.T.: 13.918 min
Delta R.T.: 0.000 min
Response: 319054
Conc: 17.39 ng/ml

Instrument :
FID_B
ClientSampleId :

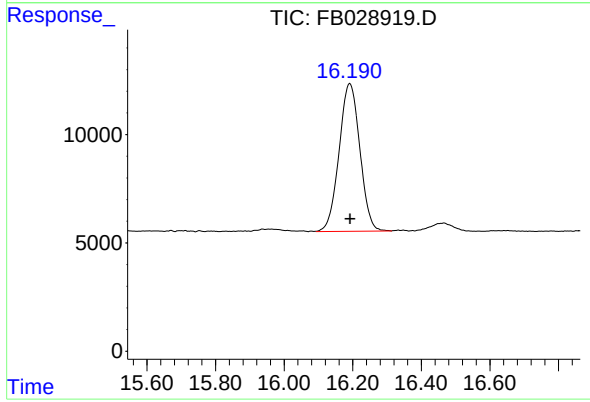

#10 1,2,4-Trimethylbenzene

R.T.: 16.192 min
Delta R.T.: 0.000 min
Response: 286629
Conc: 15.56 ng/ml