

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111022\
 Data File : FB028926.D
 Signal(s) : FID2B.CH
 Acq On : 11 Nov 2022 6:25
 Operator : AJ/MA
 Sample : 20 PPB GRO STD
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 20 PPB GRO STD

Integration File: Calibration.e
 Quant Time: Nov 11 07:35:24 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110122.M
 Quant Title :
 QLast Update : Tue Nov 01 12:44:12 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.793	262053	20.622 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.712	487544	29.911 ng/ml
2) t 2,2,4-Trimethylpentane	7.427	536844	30.552 ng/ml
3) t n-Heptane	7.752	177378	10.088 ng/ml
4) t Benzene	7.889	216822	10.573 ng/ml
6) t Toluene	10.622	621146	30.883 ng/ml
7) t Ethylbenzene	13.058	190067	10.022 ng/ml
8) t m-Xylene	13.190	377573	20.070 ng/ml
9) t O-Xylene	13.917	368494	20.087 ng/ml
10) t 1,2,4-Trimethylbenzene	16.191	347906	18.885 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111022\
Data File : FB028926.D
Signal(s) : FID2B.CH
Acq On : 11 Nov 2022 6:25
Operator : AJ/MA
Sample : 20 PPB GRO STD
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
20 PPB GRO STD

Integration File: Calibration.e
Quant Time: Nov 11 07:35:24 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110122.M
Quant Title :
QLast Update : Tue Nov 01 12:44:12 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

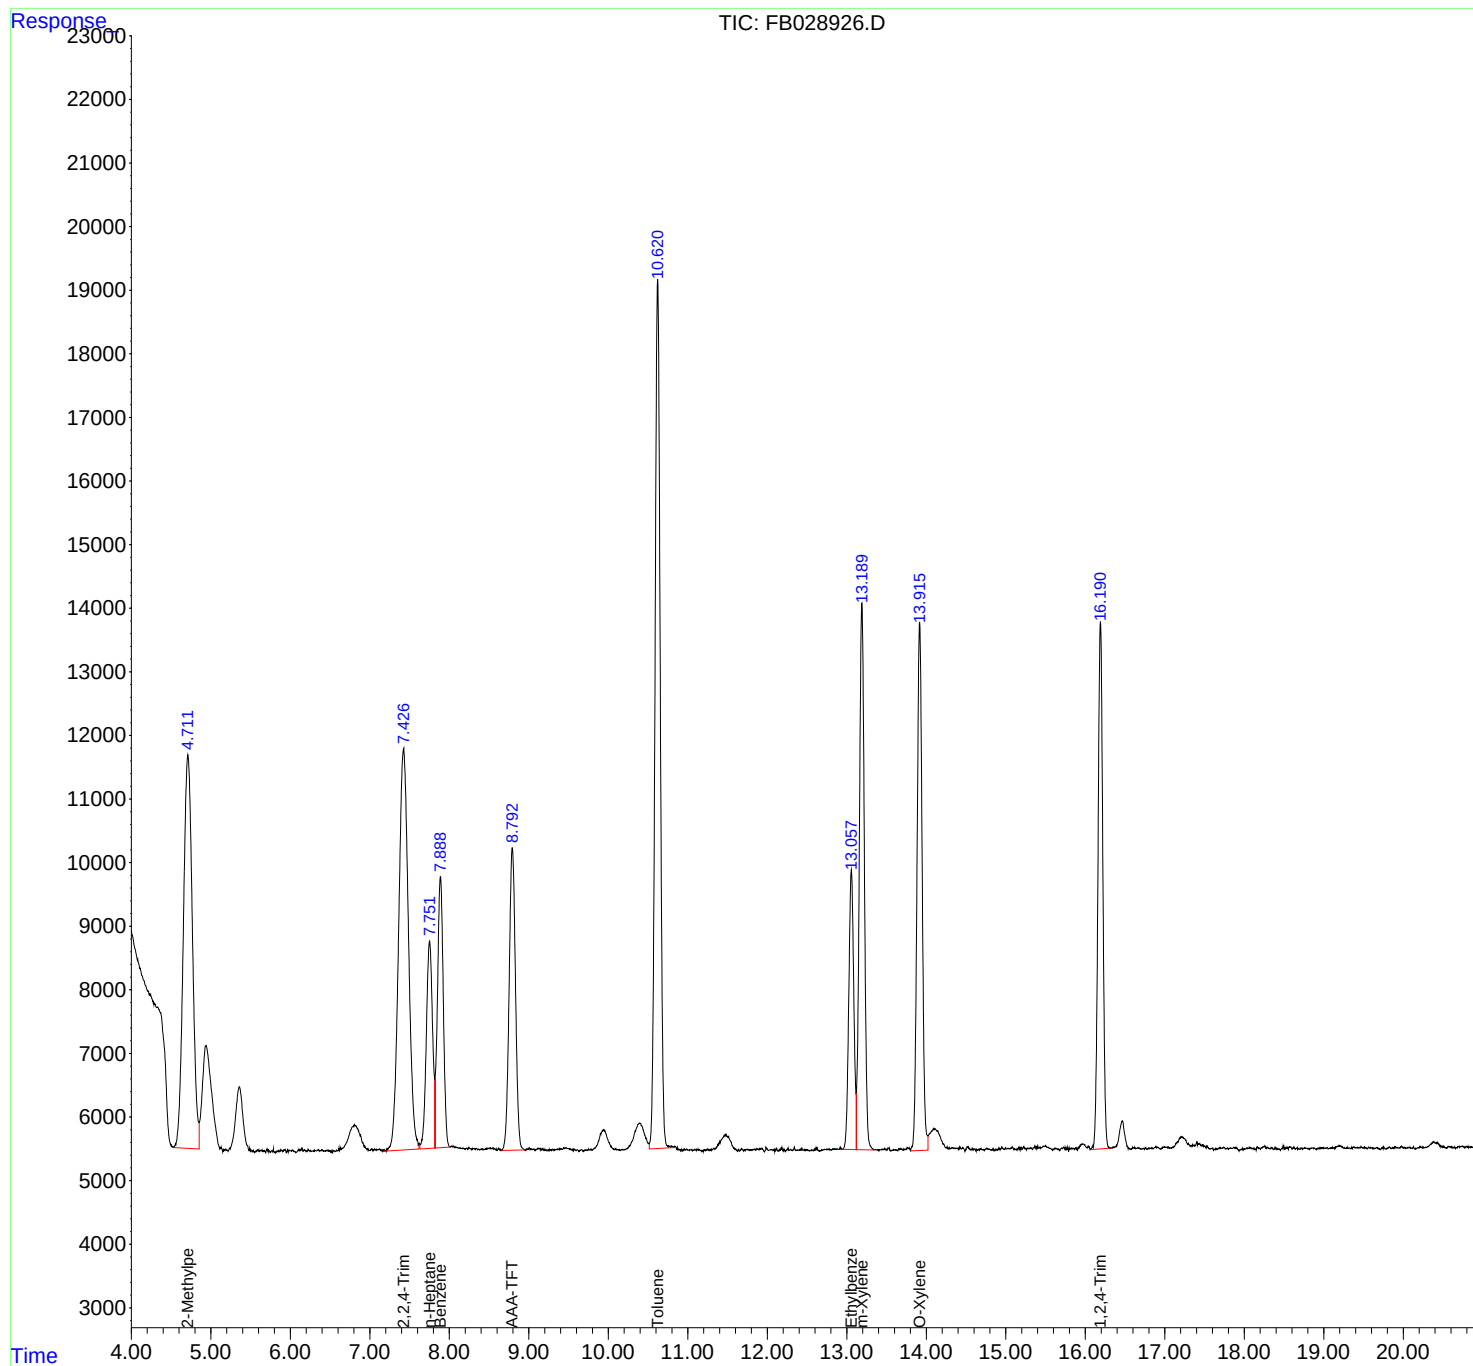


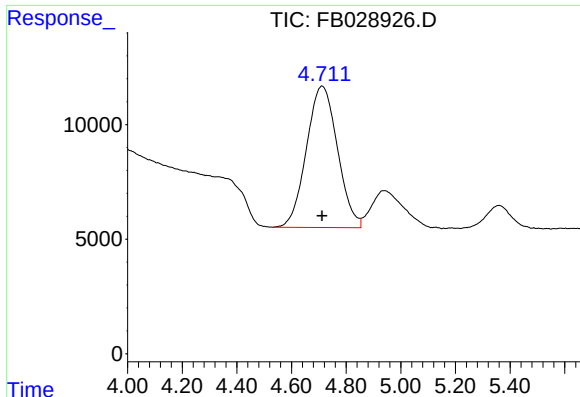

#1 2-Methylpentane


R.T.: 4.712 min
Delta R.T.: 0.000 min
Response: 487544
Conc: 29.91 ng/ml

Instrument :
FID_B
ClientSampleId :
20 PPB GRO STD

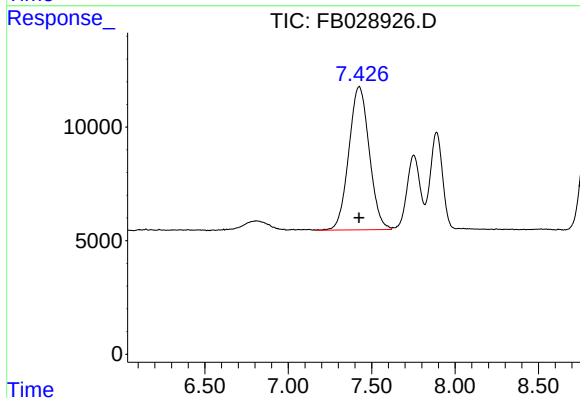


#2 2,2,4-Trimethylpentane

R.T.: 7.427 min
Delta R.T.: 0.002 min
Response: 536844
Conc: 30.55 ng/ml

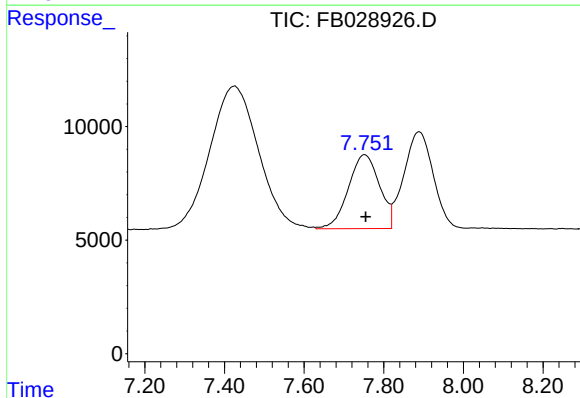


#3 n-Heptane

R.T.: 7.752 min
Delta R.T.: -0.002 min
Response: 177378
Conc: 10.09 ng/ml

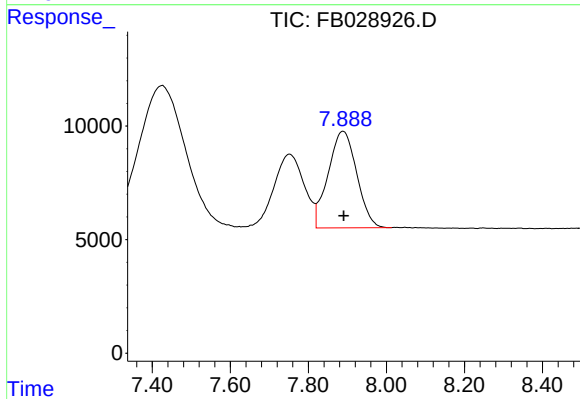

#4 Benzene


R.T.: 7.889 min
Delta R.T.: -0.001 min
Response: 216822
Conc: 10.57 ng/ml

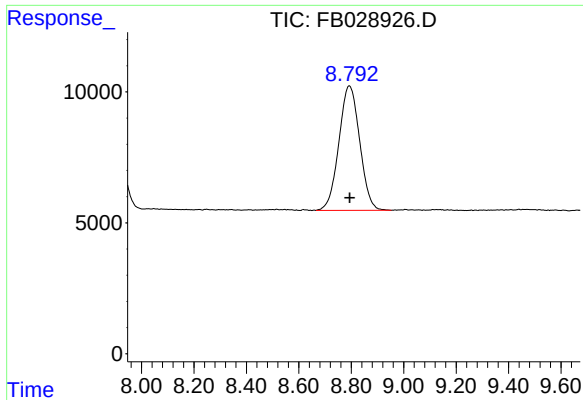

#5 AAA-TFT


R.T.: 8.793 min
Delta R.T.: -0.002 min
Response: 262053
Conc: 20.62 ng/ml

Instrument :
FID_B
ClientSampleId :
20 PPB GRO STD

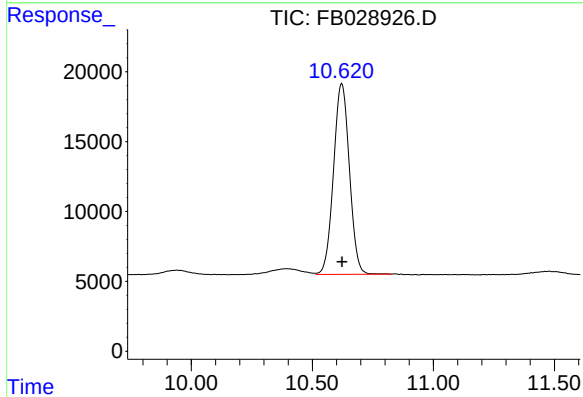


#6 Toluene

R.T.: 10.622 min
Delta R.T.: -0.001 min
Response: 621146
Conc: 30.88 ng/ml

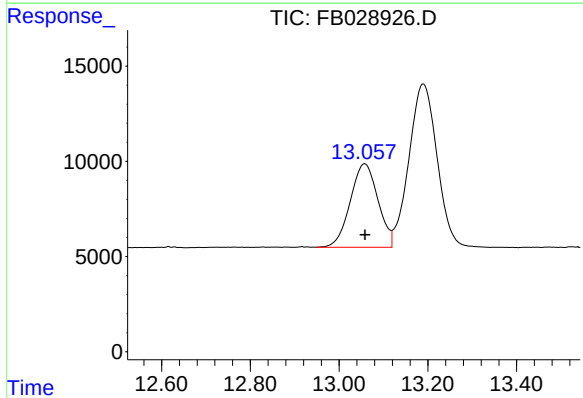


#7 Ethylbenzene

R.T.: 13.058 min
Delta R.T.: 0.000 min
Response: 190067
Conc: 10.02 ng/ml

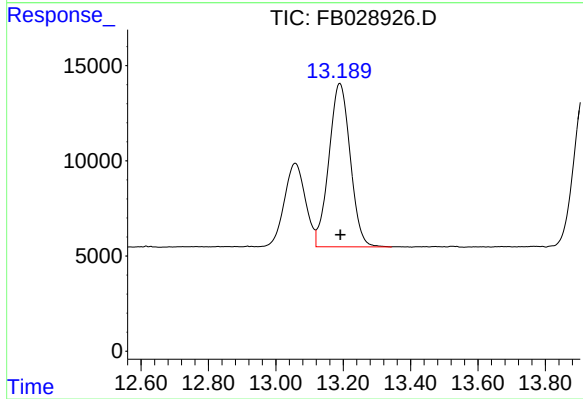

#8 m-Xylene


R.T.: 13.190 min
Delta R.T.: -0.001 min
Response: 377573
Conc: 20.07 ng/ml

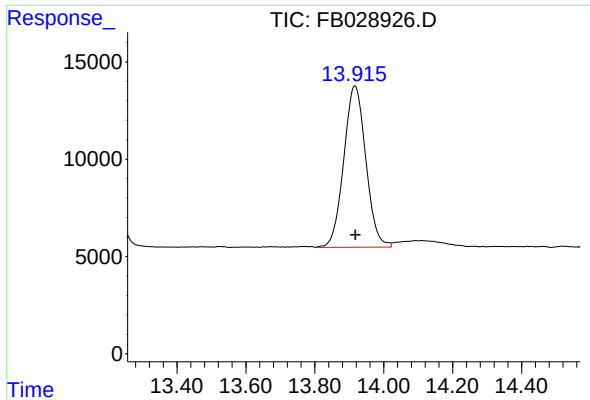

#9 O-Xylene

R.T.: 13.917 min
Delta R.T.: -0.001 min
Response: 368494
Conc: 20.09 ng/ml

Instrument :
FID_B
ClientSampleId :
20 PPB GRO STD

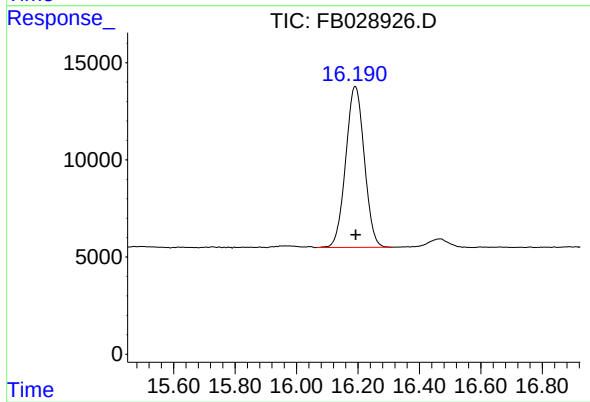

#10 1,2,4-Trimethylbenzene

R.T.: 16.191 min
Delta R.T.: -0.001 min
Response: 347906
Conc: 18.89 ng/ml