

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111119\
 Data File : FB022953.D
 Signal(s) : FID2B.CH
 Acq On : 11 Nov 2019 12:56
 Operator : DD/AJ
 Sample : BSF1111S1
 Misc : 5.00g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Nov 12 00:33:05 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB103119.M
 Quant Title :
 QLast Update : Thu Oct 31 14:57:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.797	480743	21.355 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.689	944249	29.354 ng/ml
2) t 2,2,4-Trimethylpentane	7.416	1090271	30.886 ng/ml
3) t n-Heptane	7.755	352458	10.132 ng/ml
4) t Benzene	7.890	432087	9.976 ng/ml
6) t Toluene	10.628	1268482	29.424 ng/ml
7) t Ethylbenzene	13.068	395816	9.915 ng/ml
8) t m-Xylene	13.201	747779	19.800 ng/ml
9) t O-Xylene	13.929	697323	19.565 ng/ml
10) t 1,2,4-Trimethylbenzene	16.207	575649	20.299 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111119\
Data File : FB022953.D
Signal(s) : FID2B.CH
Acq On : 11 Nov 2019 12:56
Operator : DD/AJ
Sample : BSF1111S1
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Nov 12 00:33:05 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB103119.M
Quant Title :
QLast Update : Thu Oct 31 14:57:42 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

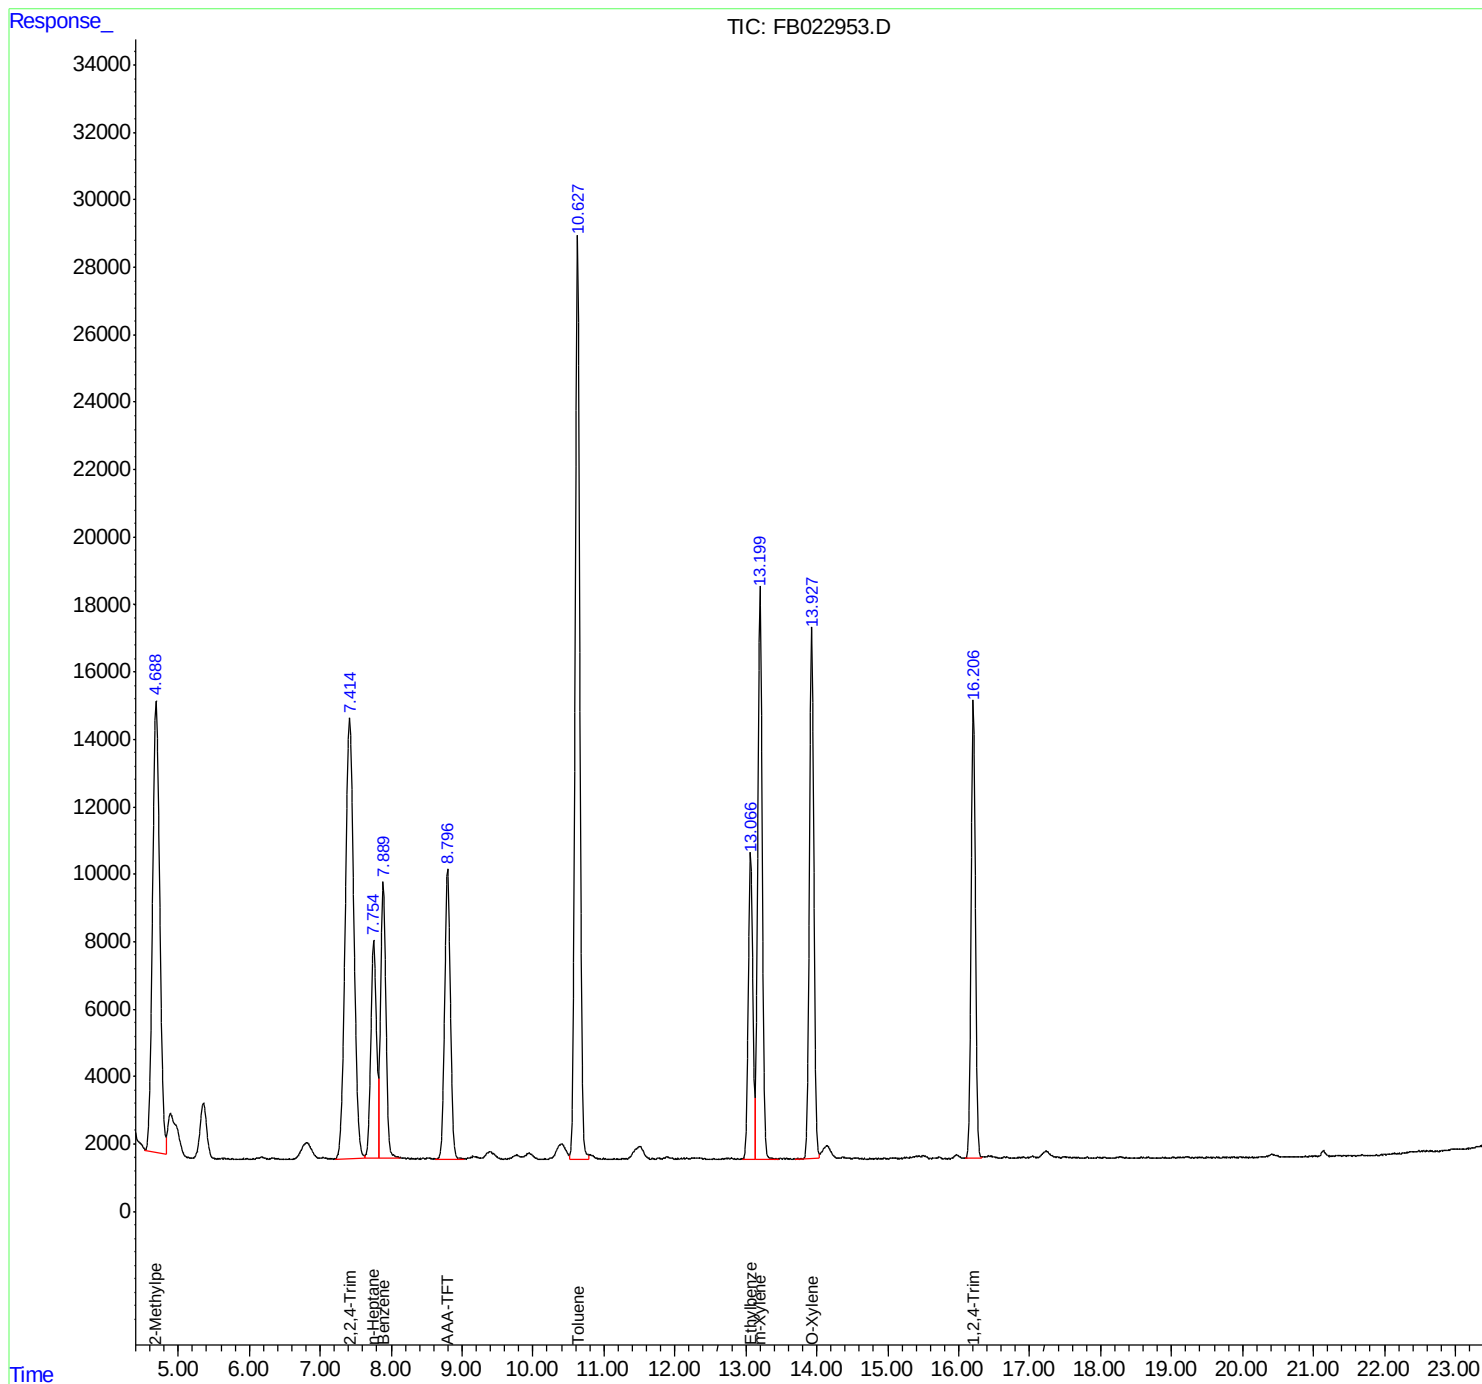

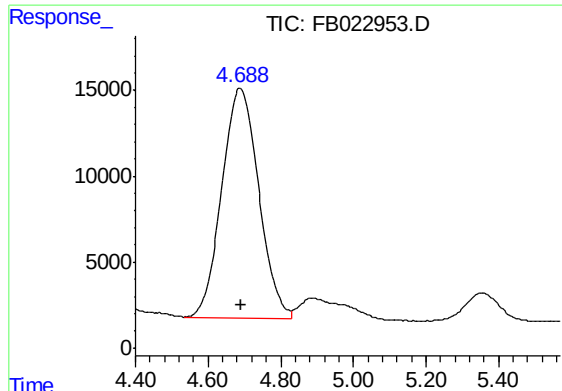


#1 2-Methylpentane

R.T.: 4.689 min
Delta R.T.: 0.000 min
Response: 944249
Conc: 29.35 ng/ml

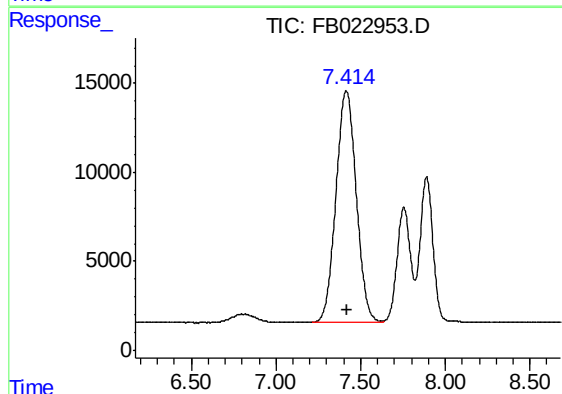


#2 2,2,4-Trimethylpentane

R.T.: 7.416 min
Delta R.T.: -0.002 min
Response: 1090271
Conc: 30.89 ng/ml

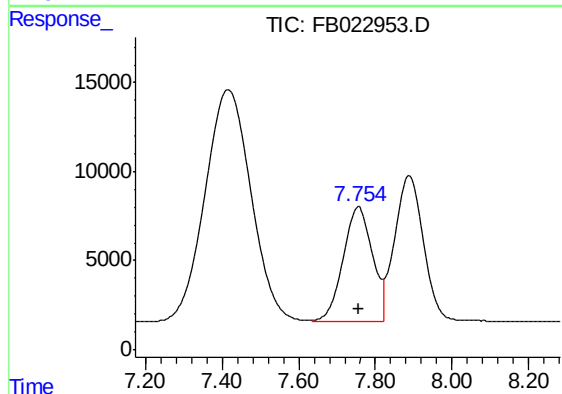


#3 n-Heptane

R.T.: 7.755 min
Delta R.T.: -0.003 min
Response: 352458
Conc: 10.13 ng/ml

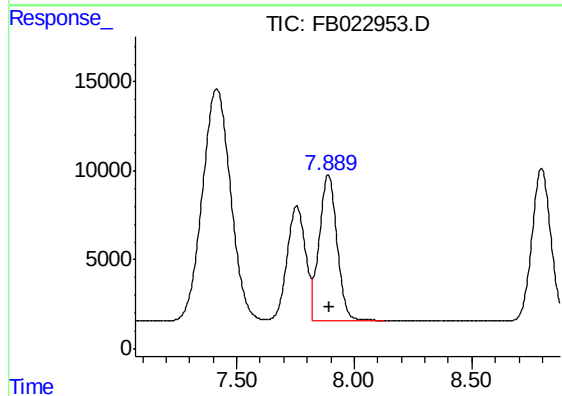


#4 Benzene

R.T.: 7.890 min
Delta R.T.: -0.003 min
Response: 432087
Conc: 9.98 ng/ml

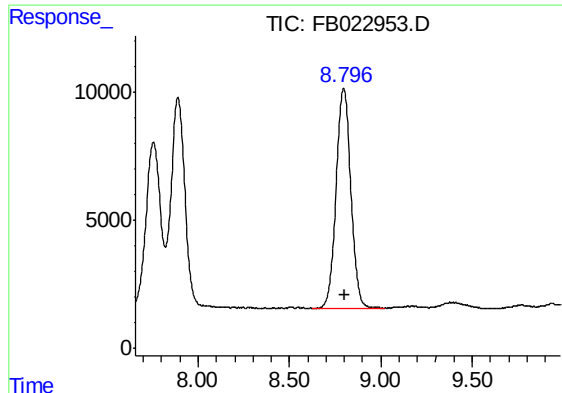


#5 AAA-TFT

R.T.: 8.797 min
Delta R.T.: -0.003 min
Response: 480743
Conc: 21.36 ng/ml

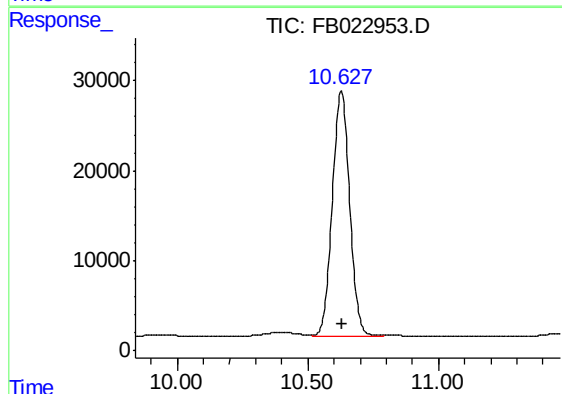


#6 Toluene

R.T.: 10.628 min
Delta R.T.: -0.004 min
Response: 1268482
Conc: 29.42 ng/ml

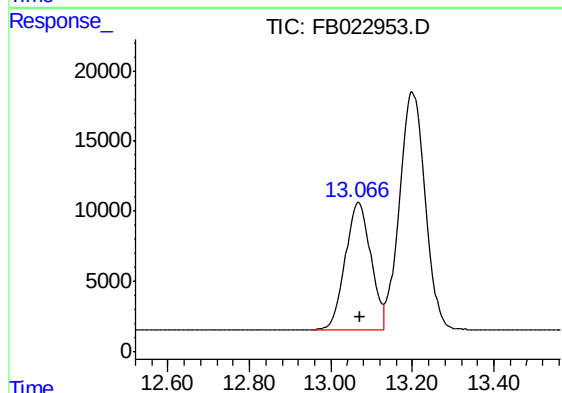


#7 Ethylbenzene

R.T.: 13.068 min
Delta R.T.: -0.004 min
Response: 395816
Conc: 9.91 ng/ml

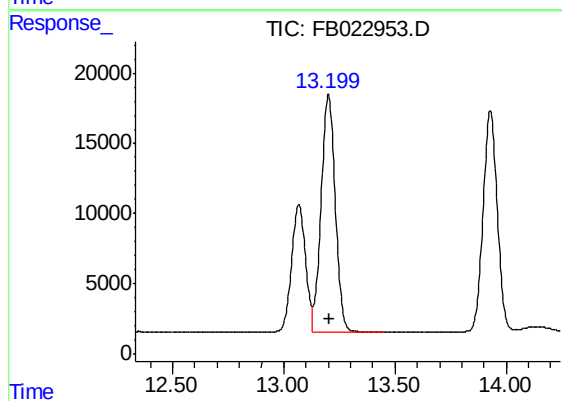


#8 m-Xylene

R.T.: 13.201 min
Delta R.T.: -0.004 min
Response: 747779
Conc: 19.80 ng/ml

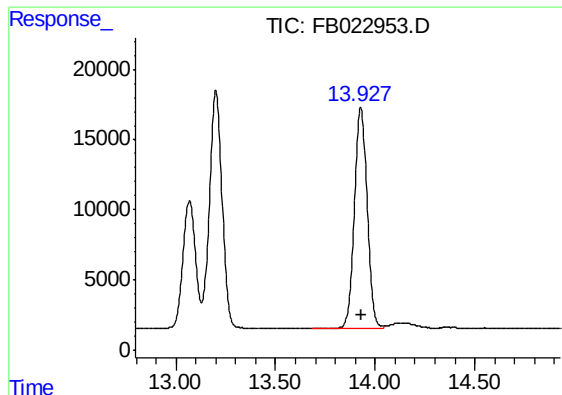

#9 O-Xylene

R.T.: 13.929 min
Delta R.T.: -0.004 min
Response: 697323
Conc: 19.57 ng/ml

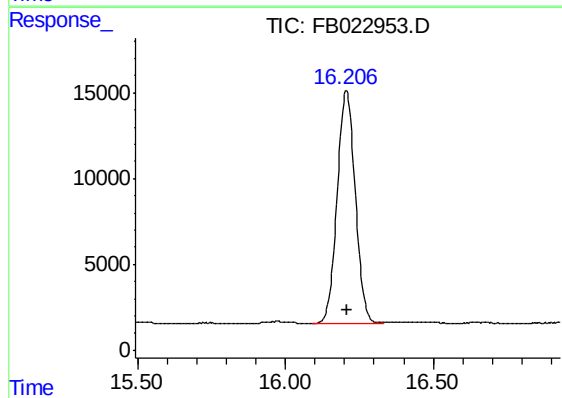

#10 1,2,4-Trimethylbenzene

R.T.: 16.207 min
Delta R.T.: -0.004 min
Response: 575649
Conc: 20.30 ng/ml