

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111119\
 Data File : FB022955.D
 Signal(s) : FID2B.CH
 Acq On : 11 Nov 2019 15:00
 Operator : DD/AJ
 Sample : K5676-12MS
 Misc : 5.03g/5.00ml DI WATER
 ALS Vial : 5 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Nov 12 00:33:23 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB103119.M
 Quant Title :
 QLast Update : Thu Oct 31 14:57:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.796	423175	18.798 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.688	825212	25.654 ng/ml
2) t 2,2,4-Trimethylpentane	7.414	835188	23.660 ng/ml
3) t n-Heptane	7.755	233753	6.720 ng/ml
4) t Benzene	7.889	420126	9.699 ng/ml
6) t Toluene	10.627	1206503	27.986 ng/ml
7) t Ethylbenzene	13.067	364115	9.121 ng/ml
8) t m-Xylene	13.200	665276	17.615 ng/ml
9) t O-Xylene	13.928	645856	18.121 ng/ml
10) t 1,2,4-Trimethylbenzene	16.207	488989	17.243 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111119\
Data File : FB022955.D
Signal(s) : FID2B.CH
Acq On : 11 Nov 2019 15:00
Operator : DD/AJ
Sample : K5676-12MS
Misc : 5.03g/5.00ml DI WATER
ALS Vial : 5 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Nov 12 00:33:23 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB103119.M
Quant Title :
QLast Update : Thu Oct 31 14:57:42 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

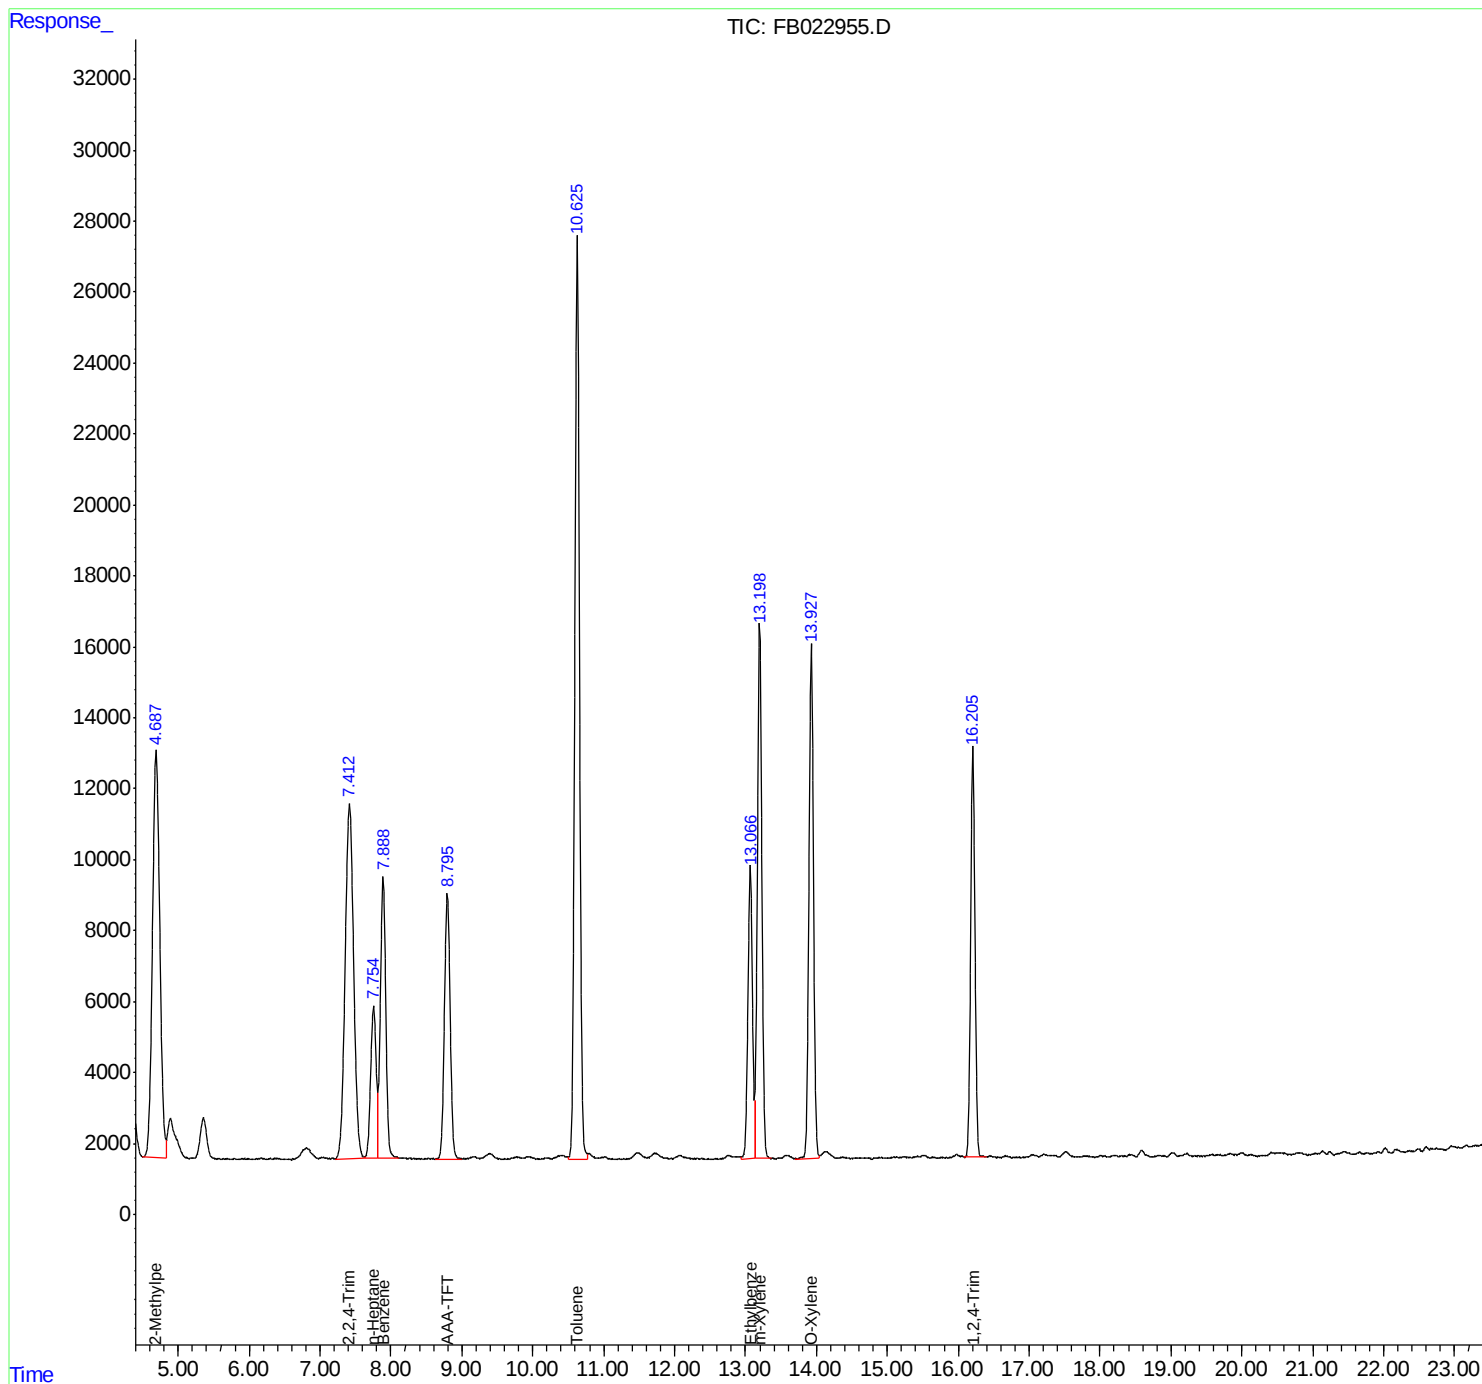

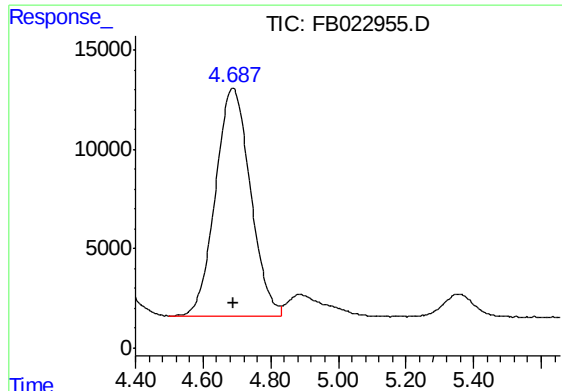


#1 2-Methylpentane

R.T.: 4.688 min
Delta R.T.: 0.000 min
Response: 825212
Conc: 25.65 ng/ml

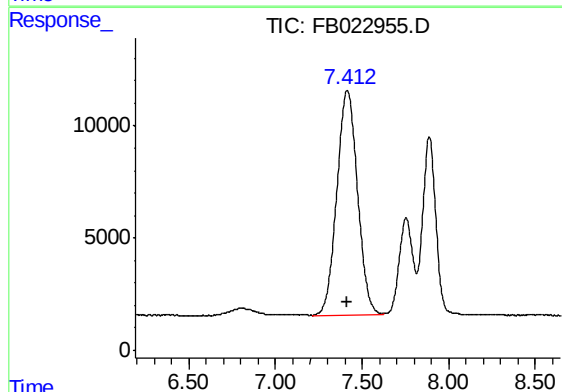


#2 2,2,4-Trimethylpentane

R.T.: 7.414 min
Delta R.T.: -0.004 min
Response: 835188
Conc: 23.66 ng/ml

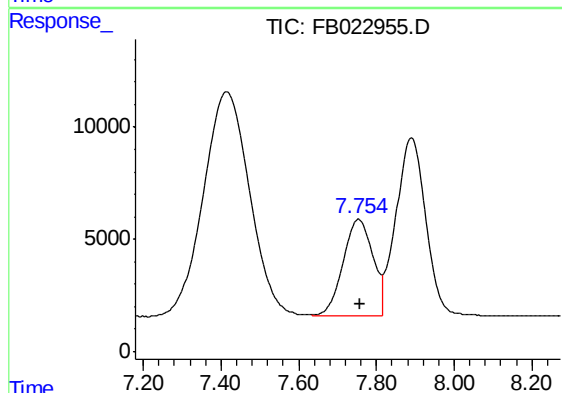


#3 n-Heptane

R.T.: 7.755 min
Delta R.T.: -0.003 min
Response: 233753
Conc: 6.72 ng/ml

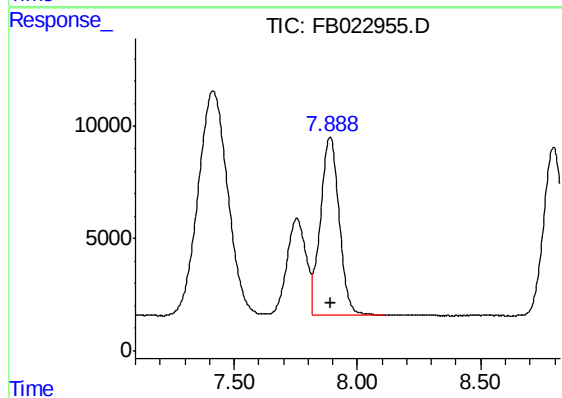


#4 Benzene

R.T.: 7.889 min
Delta R.T.: -0.004 min
Response: 420126
Conc: 9.70 ng/ml

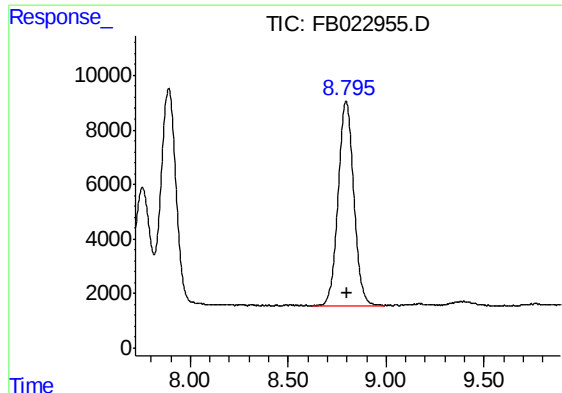


#5 AAA-TFT

R.T.: 8.796 min
Delta R.T.: -0.004 min
Response: 423175
Conc: 18.80 ng/ml

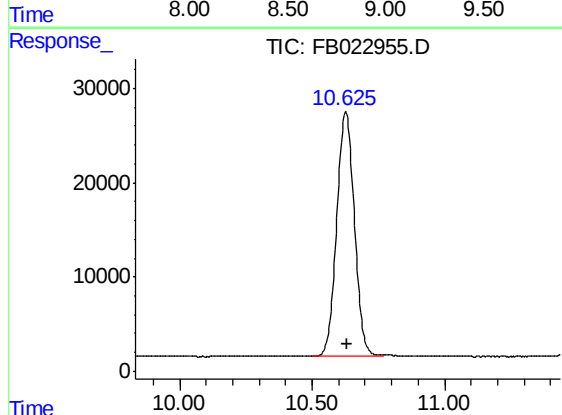


#6 Toluene

R.T.: 10.627 min
Delta R.T.: -0.005 min
Response: 1206503
Conc: 27.99 ng/ml

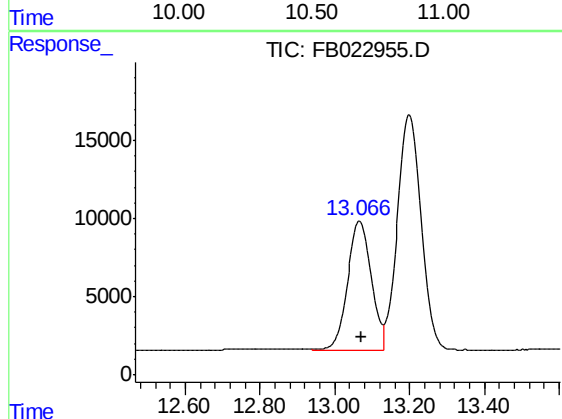


#7 Ethylbenzene

R.T.: 13.067 min
Delta R.T.: -0.005 min
Response: 364115
Conc: 9.12 ng/ml

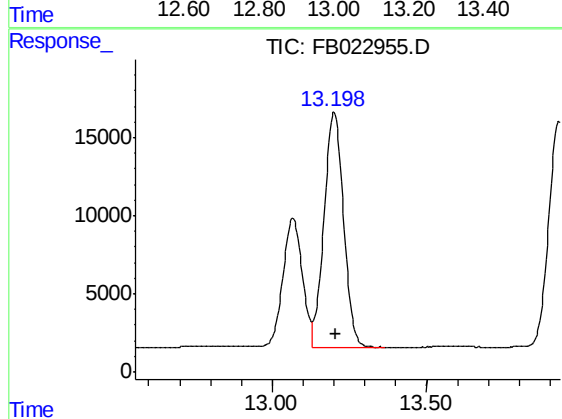


#8 m-Xylene

R.T.: 13.200 min
Delta R.T.: -0.005 min
Response: 665276
Conc: 17.62 ng/ml

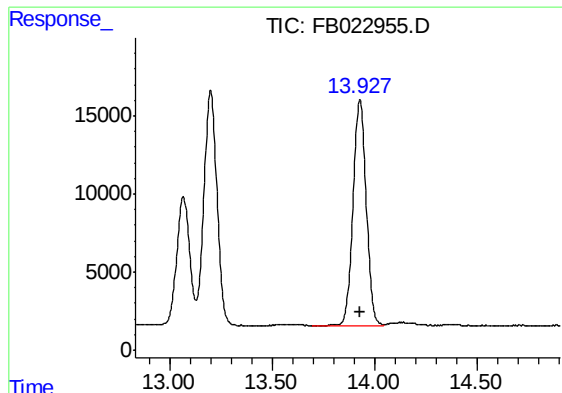

#9 O-Xylene

R.T.: 13.928 min
Delta R.T.: -0.004 min
Response: 645856
Conc: 18.12 ng/ml

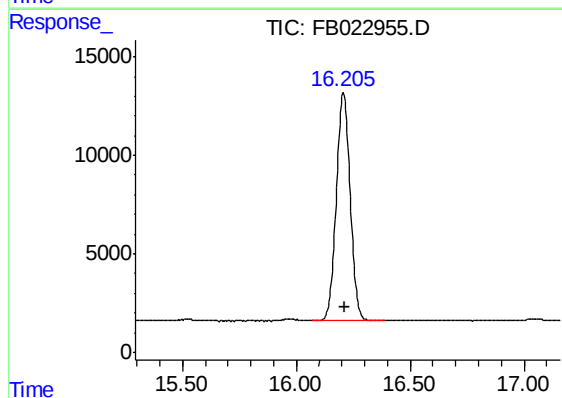

#10 1,2,4-Trimethylbenzene

R.T.: 16.207 min
Delta R.T.: -0.004 min
Response: 488989
Conc: 17.24 ng/ml