

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111119\
 Data File : FB022956.D
 Signal(s) : FID2B.CH
 Acq On : 11 Nov 2019 15:30
 Operator : DD/AJ
 Sample : K5676-12MSD
 Misc : 5.04g/5.00ml DI WATER
 ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Nov 12 00:33:32 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB103119.M
 Quant Title :
 QLast Update : Thu Oct 31 14:57:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.796	401549	17.837 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.689	771492	23.984 ng/ml
2) t 2,2,4-Trimethylpentane	7.415	790314	22.388 ng/ml
3) t n-Heptane	7.756	216706	6.230 ng/ml
4) t Benzene	7.890	399762	9.229 ng/ml
6) t Toluene	10.628	1177921	27.323 ng/ml
7) t Ethylbenzene	13.068	364190	9.122 ng/ml
8) t m-Xylene	13.201	673462	17.832 ng/ml
9) t O-Xylene	13.929	653111	18.325 ng/ml
10) t 1,2,4-Trimethylbenzene	16.207	476081	16.788 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111119\
Data File : FB022956.D
Signal(s) : FID2B.CH
Acq On : 11 Nov 2019 15:30
Operator : DD/AJ
Sample : K5676-12MSD
Misc : 5.04g/5.00ml DI WATER
ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Nov 12 00:33:32 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB103119.M
Quant Title :
QLast Update : Thu Oct 31 14:57:42 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

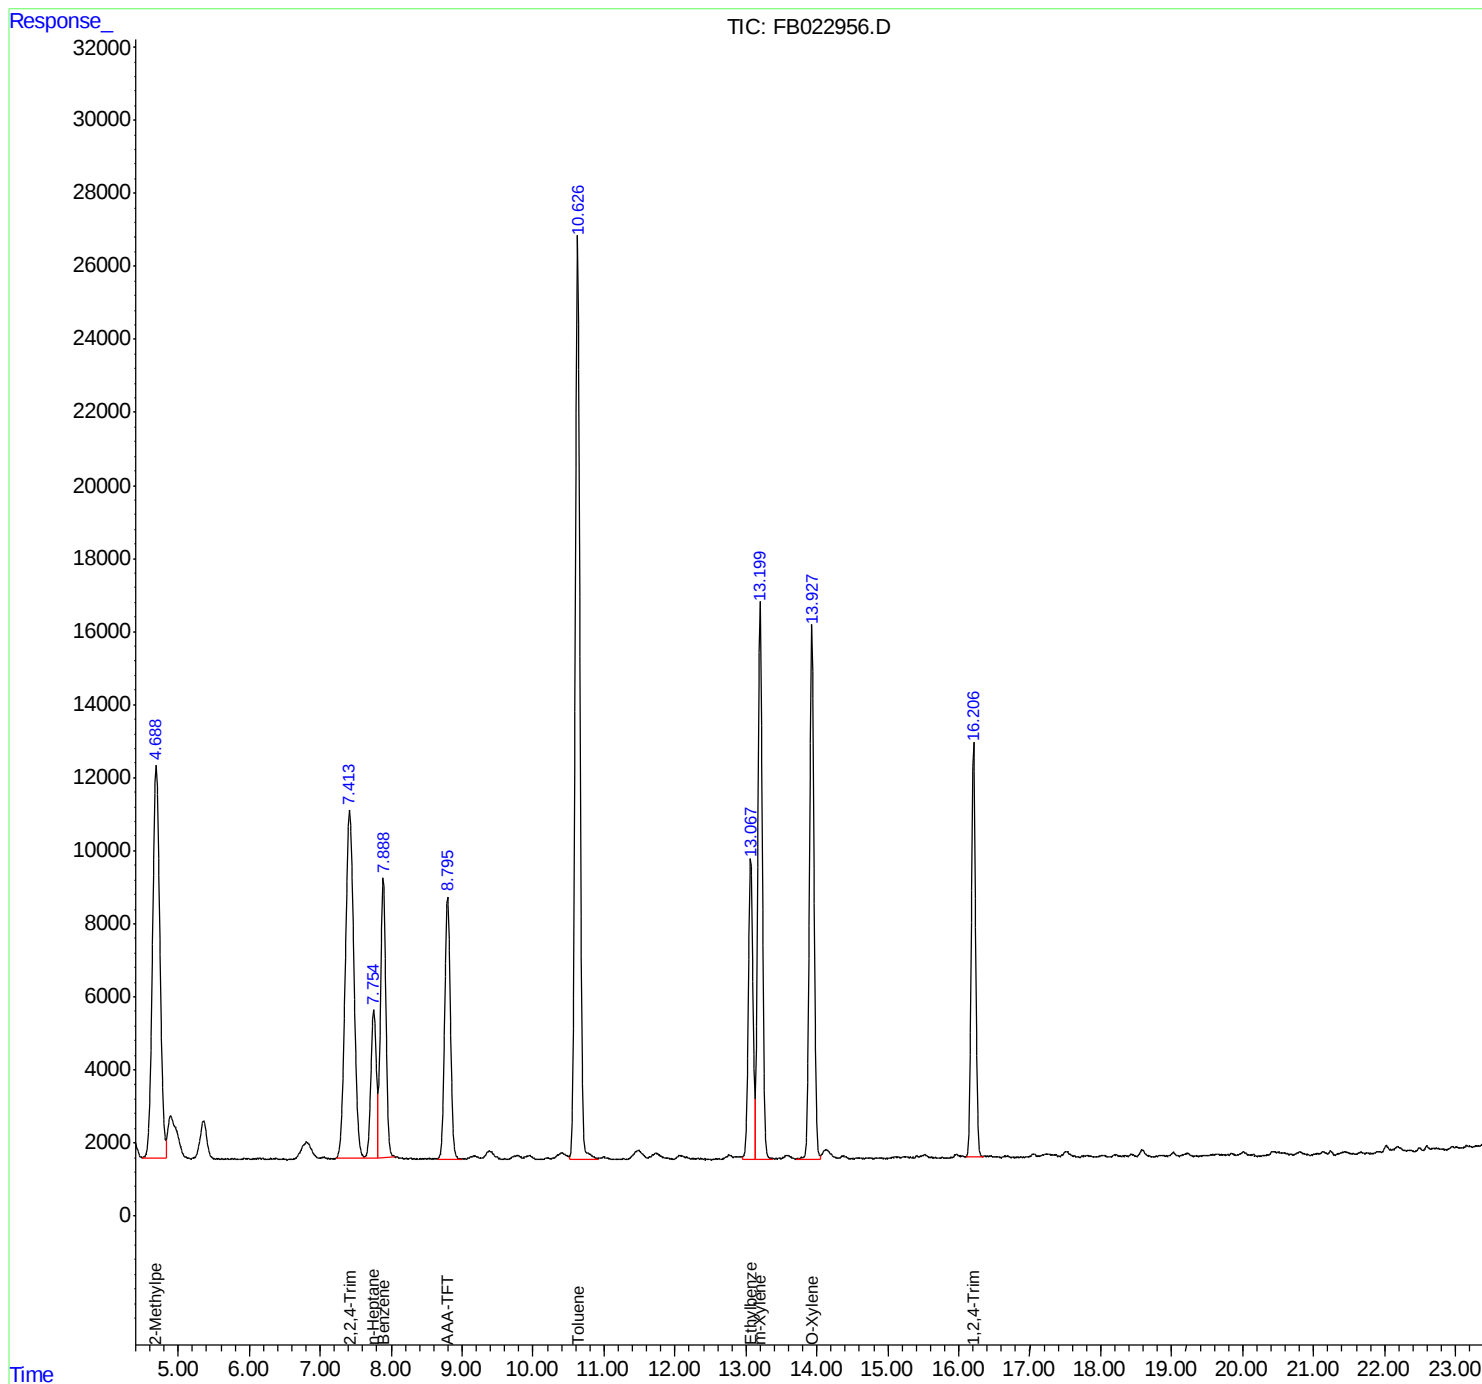

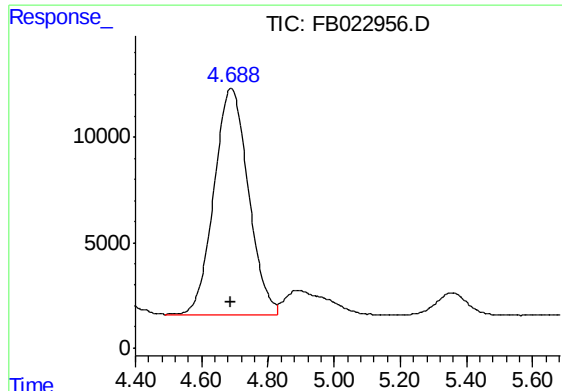


#1 2-Methylpentane

R.T.: 4.689 min
Delta R.T.: 0.000 min
Response: 771492
Conc: 23.98 ng/ml

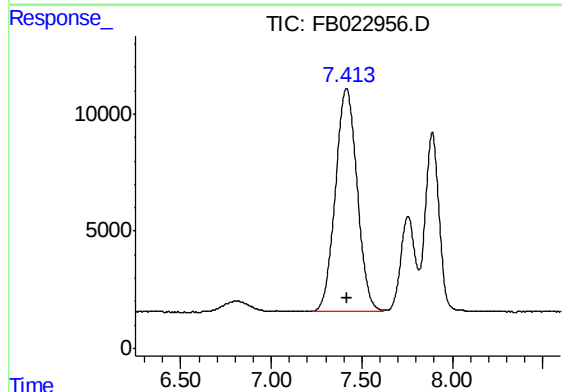


#2 2,2,4-Trimethylpentane

R.T.: 7.415 min
Delta R.T.: -0.003 min
Response: 790314
Conc: 22.39 ng/ml

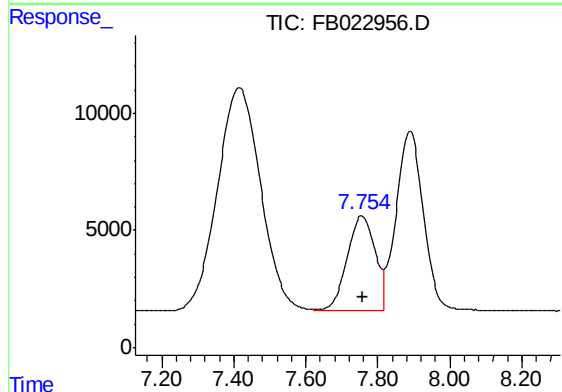


#3 n-Heptane

R.T.: 7.756 min
Delta R.T.: -0.003 min
Response: 216706
Conc: 6.23 ng/ml

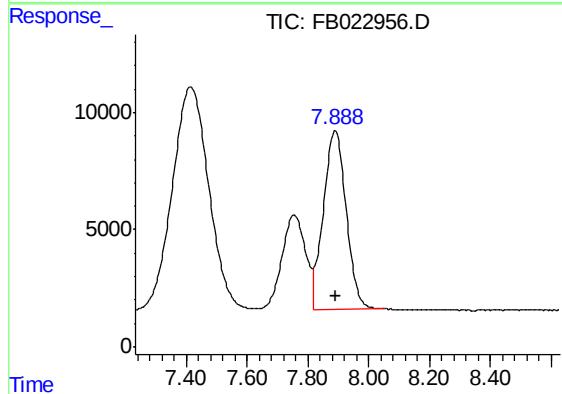


#4 Benzene

R.T.: 7.890 min
Delta R.T.: -0.003 min
Response: 399762
Conc: 9.23 ng/ml

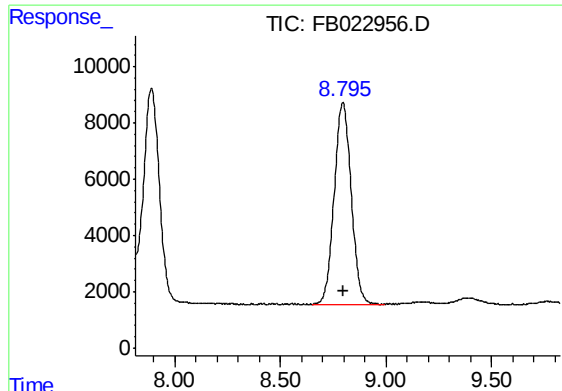


#5 AAA-TFT

R.T.: 8.796 min
Delta R.T.: -0.004 min
Response: 401549
Conc: 17.84 ng/ml

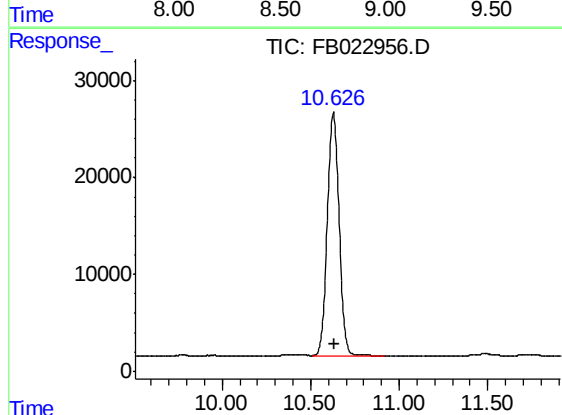


#6 Toluene

R.T.: 10.628 min
Delta R.T.: -0.004 min
Response: 1177921
Conc: 27.32 ng/ml

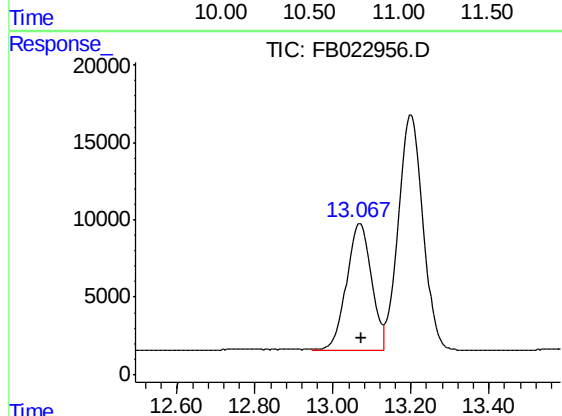


#7 Ethylbenzene

R.T.: 13.068 min
Delta R.T.: -0.004 min
Response: 364190
Conc: 9.12 ng/ml

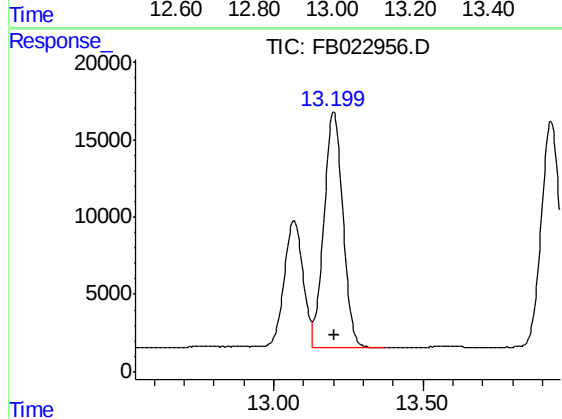


#8 m-Xylene

R.T.: 13.201 min
Delta R.T.: -0.004 min
Response: 673462
Conc: 17.83 ng/ml

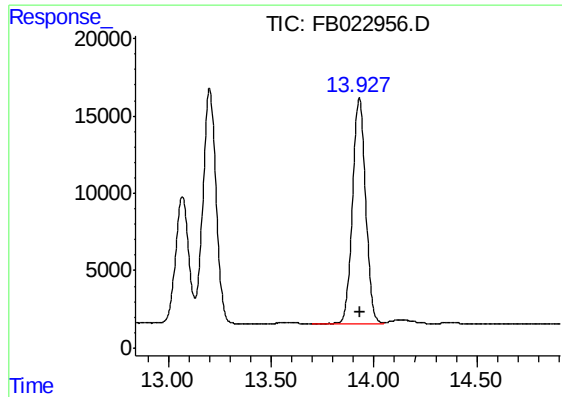

#9 O-Xylene

R.T.: 13.929 min
Delta R.T.: -0.004 min
Response: 653111
Conc: 18.32 ng/ml

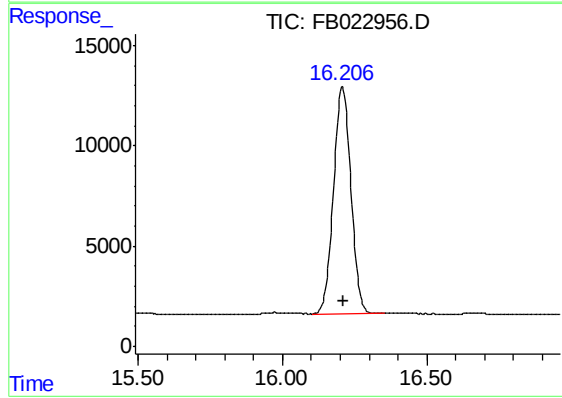

#10 1,2,4-Trimethylbenzene

R.T.: 16.207 min
Delta R.T.: -0.004 min
Response: 476081
Conc: 16.79 ng/ml