

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111122\
 Data File : FB028930.D
 Signal(s) : FID2B.CH
 Acq On : 11 Nov 2022 8:54
 Operator : AJ/MA
 Sample : BSF1111S1
 Misc : 5.00G/5.00 ML MEOH
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF1111S1

Integration File: Calibration.e
 Quant Time: Nov 14 02:08:29 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110122.M
 Quant Title :
 QLast Update : Tue Nov 01 12:44:12 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.793	224900	17.699 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.715	459588	28.196 ng/ml
2) t 2,2,4-Trimethylpentane	7.425	555066	31.590 ng/ml
3) t n-Heptane	7.753	147543	8.392 ng/ml
4) t Benzene	7.889	192464	9.386 ng/ml
6) t Toluene	10.621	554684	27.578 ng/ml
7) t Ethylbenzene	13.057	184569	9.732 ng/ml
8) t m-Xylene	13.190	369639	19.648 ng/ml
9) t O-Xylene	13.916	370510	20.197 ng/ml
10) t 1,2,4-Trimethylbenzene	16.191	395814	21.486 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111122\
Data File : FB028930.D
Signal(s) : FID2B.CH
Acq On : 11 Nov 2022 8:54
Operator : AJ/MA
Sample : BSF1111S1
Misc : 5.00G/5.00 ML MEOH
ALS Vial : 39 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF1111S1

Integration File: Calibration.e
Quant Time: Nov 14 02:08:29 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110122.M
Quant Title :
QLast Update : Tue Nov 01 12:44:12 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

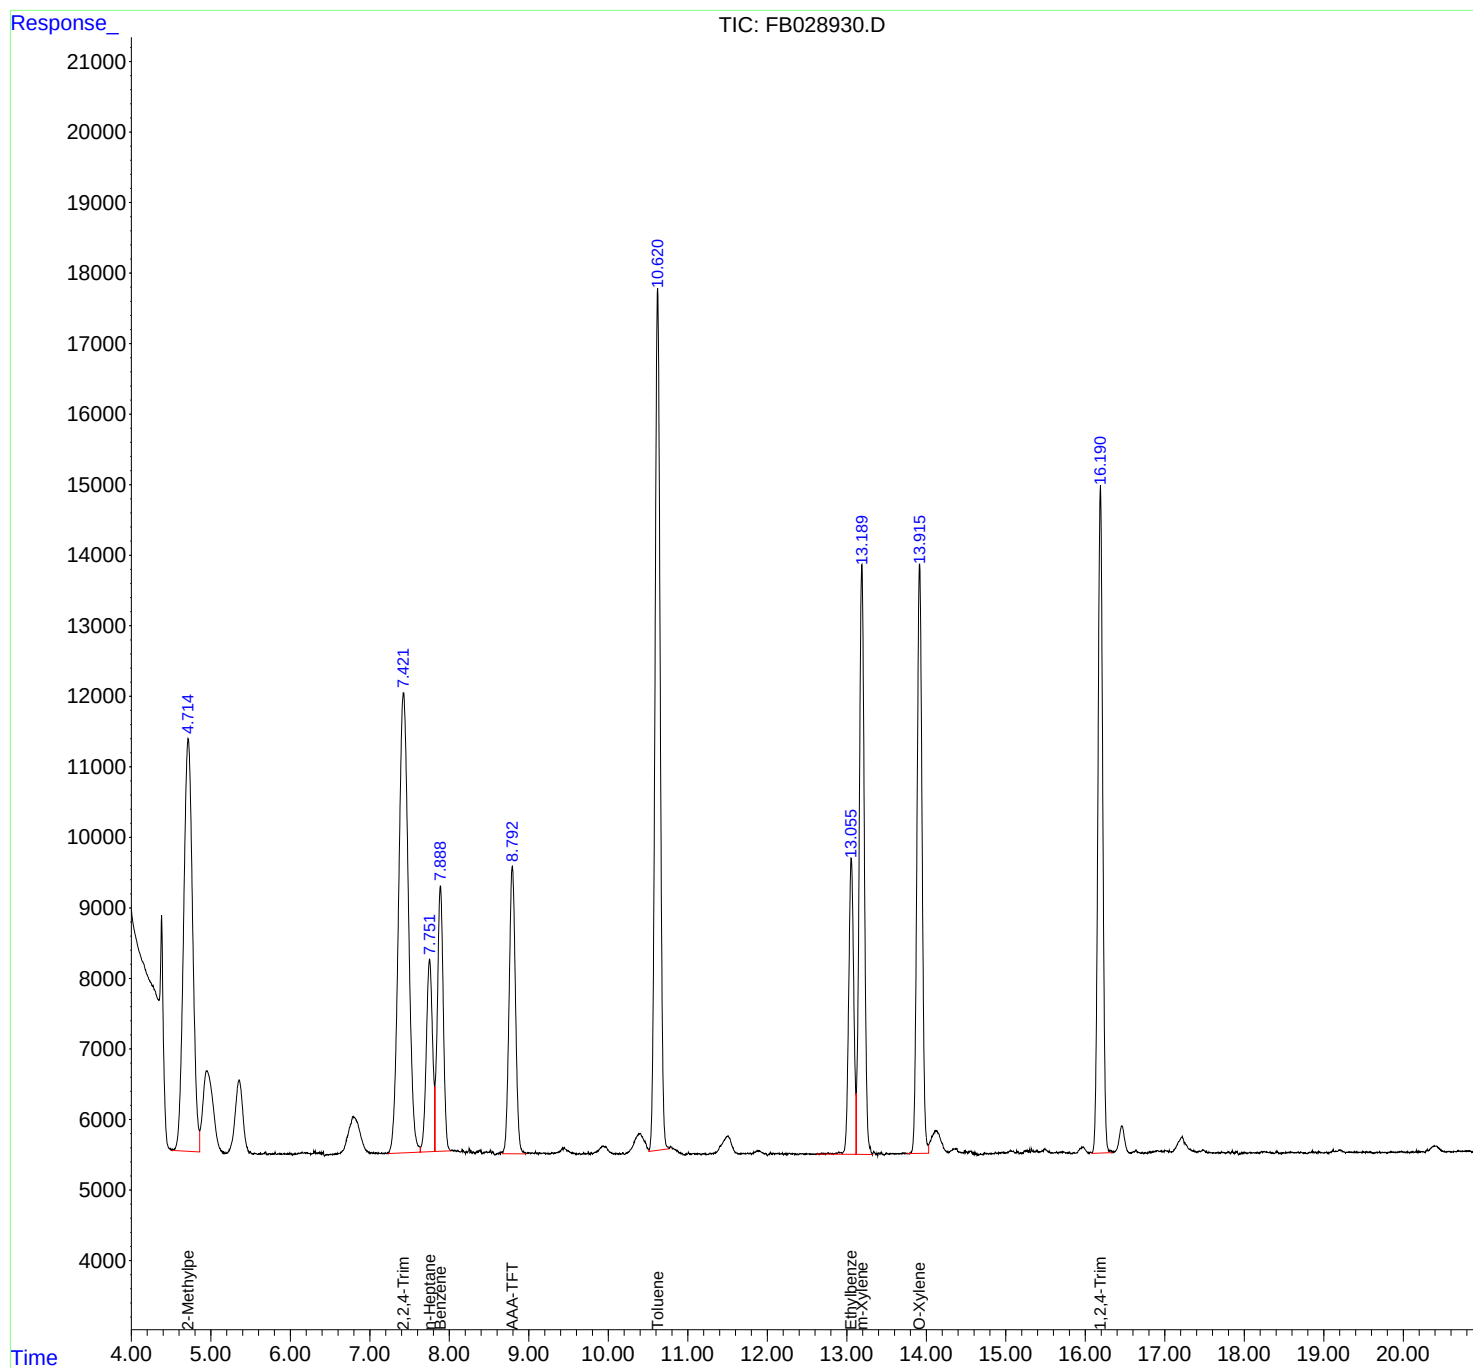


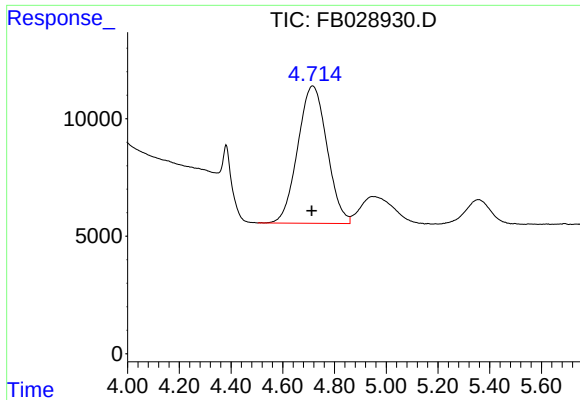

#1 2-Methylpentane


R.T.: 4.715 min
Delta R.T.: 0.003 min
Response: 459588
Conc: 28.20 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1111S1

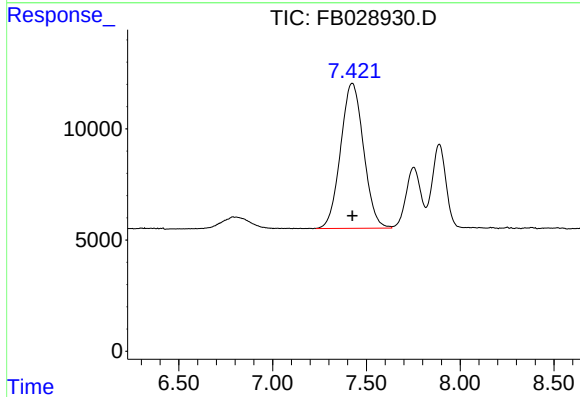


#2 2,2,4-Trimethylpentane

R.T.: 7.425 min
Delta R.T.: 0.000 min
Response: 555066
Conc: 31.59 ng/ml

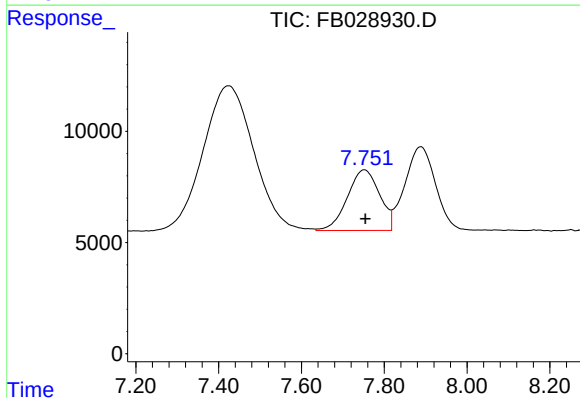


#3 n-Heptane

R.T.: 7.753 min
Delta R.T.: -0.002 min
Response: 147543
Conc: 8.39 ng/ml

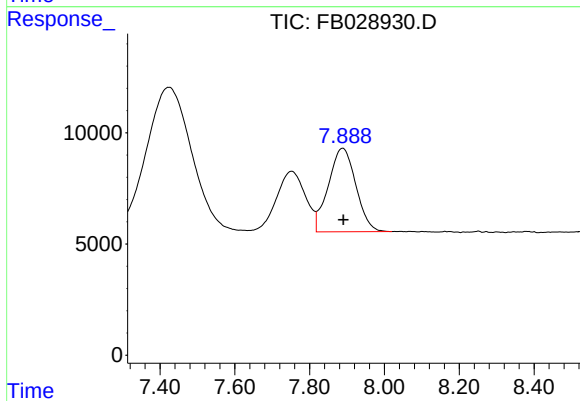

#4 Benzene


R.T.: 7.889 min
Delta R.T.: -0.002 min
Response: 192464
Conc: 9.39 ng/ml

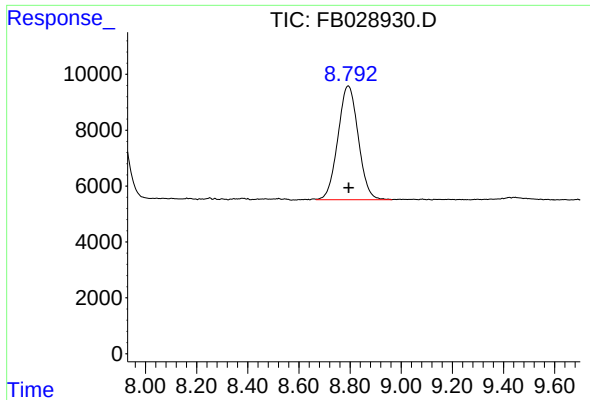

#5 AAA-TFT


R.T.: 8.793 min
Delta R.T.: -0.002 min
Response: 224900
Conc: 17.70 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1111S1

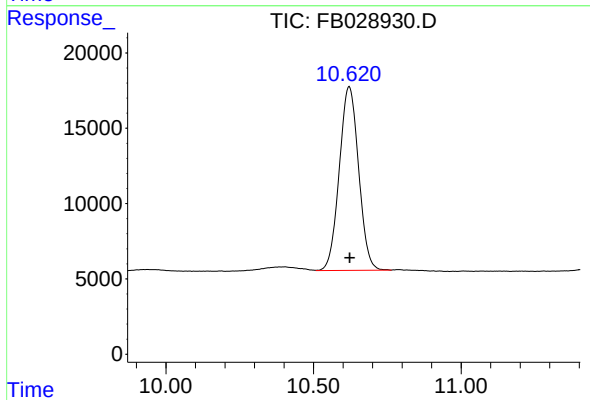


#6 Toluene

R.T.: 10.621 min
Delta R.T.: -0.002 min
Response: 554684
Conc: 27.58 ng/ml

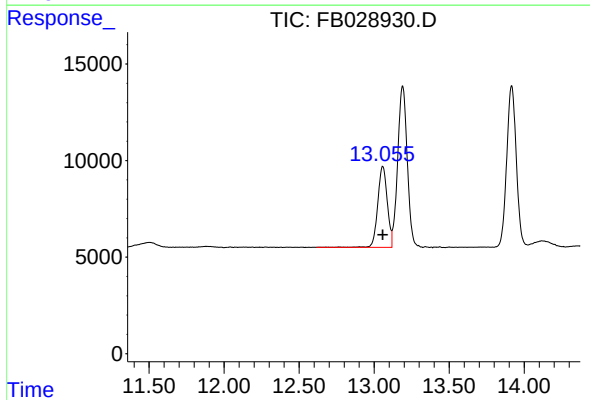


#7 Ethylbenzene

R.T.: 13.057 min
Delta R.T.: -0.001 min
Response: 184569
Conc: 9.73 ng/ml

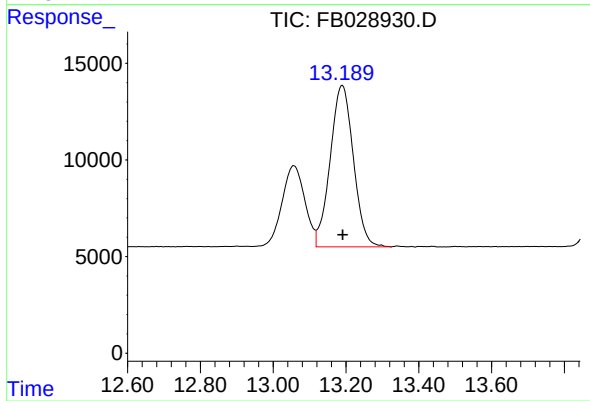

#8 m-Xylene


R.T.: 13.190 min
Delta R.T.: -0.001 min
Response: 369639
Conc: 19.65 ng/ml

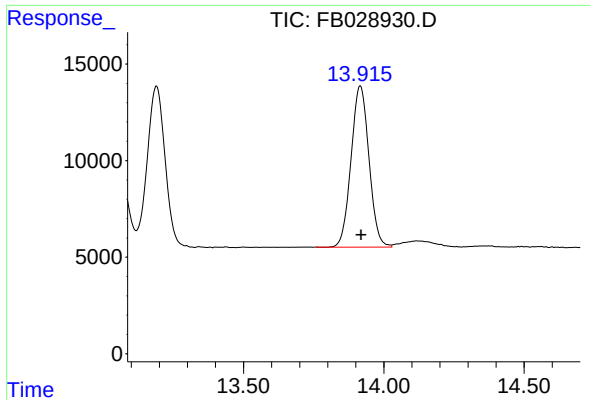

#9 O-Xylene

R.T.: 13.916 min
Delta R.T.: -0.002 min
Response: 370510
Conc: 20.20 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1111S1

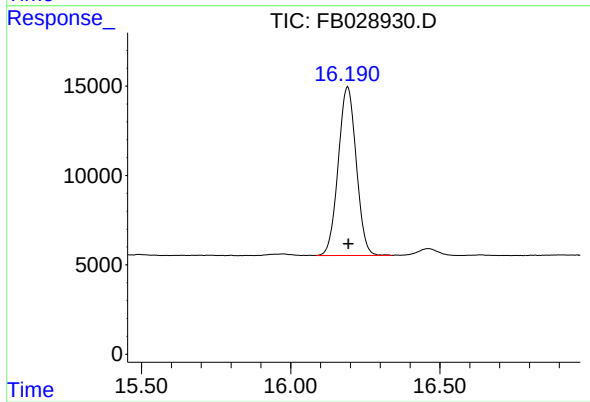

#10 1,2,4-Trimethylbenzene

R.T.: 16.191 min
Delta R.T.: -0.002 min
Response: 395814
Conc: 21.49 ng/ml