

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111122\
 Data File : FB028931.D
 Signal(s) : FID2B.CH
 Acq On : 11 Nov 2022 9:31
 Operator : AJ/MA
 Sample : BSF1111S2
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF1111S2

Integration File: Calibration.e
 Quant Time: Nov 14 02:08:36 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110122.M
 Quant Title :
 QLast Update : Tue Nov 01 12:44:12 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.793	259058	20.387 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.711	509415	31.253 ng/ml
2) t 2,2,4-Trimethylpentane	7.424	562538	32.015 ng/ml
3) t n-Heptane	7.752	184521	10.495 ng/ml
4) t Benzene	7.888	228357	11.136 ng/ml
6) t Toluene	10.621	658833	32.756 ng/ml
7) t Ethylbenzene	13.058	206874	10.908 ng/ml
8) t m-Xylene	13.190	405982	21.580 ng/ml
9) t O-Xylene	13.917	388886	21.198 ng/ml
10) t 1,2,4-Trimethylbenzene	16.191	375657	20.392 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111122\
Data File : FB028931.D
Signal(s) : FID2B.CH
Acq On : 11 Nov 2022 9:31
Operator : AJ/MA
Sample : BSF1111S2
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF1111S2

Integration File: Calibration.e
Quant Time: Nov 14 02:08:36 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110122.M
Quant Title :
QLast Update : Tue Nov 01 12:44:12 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

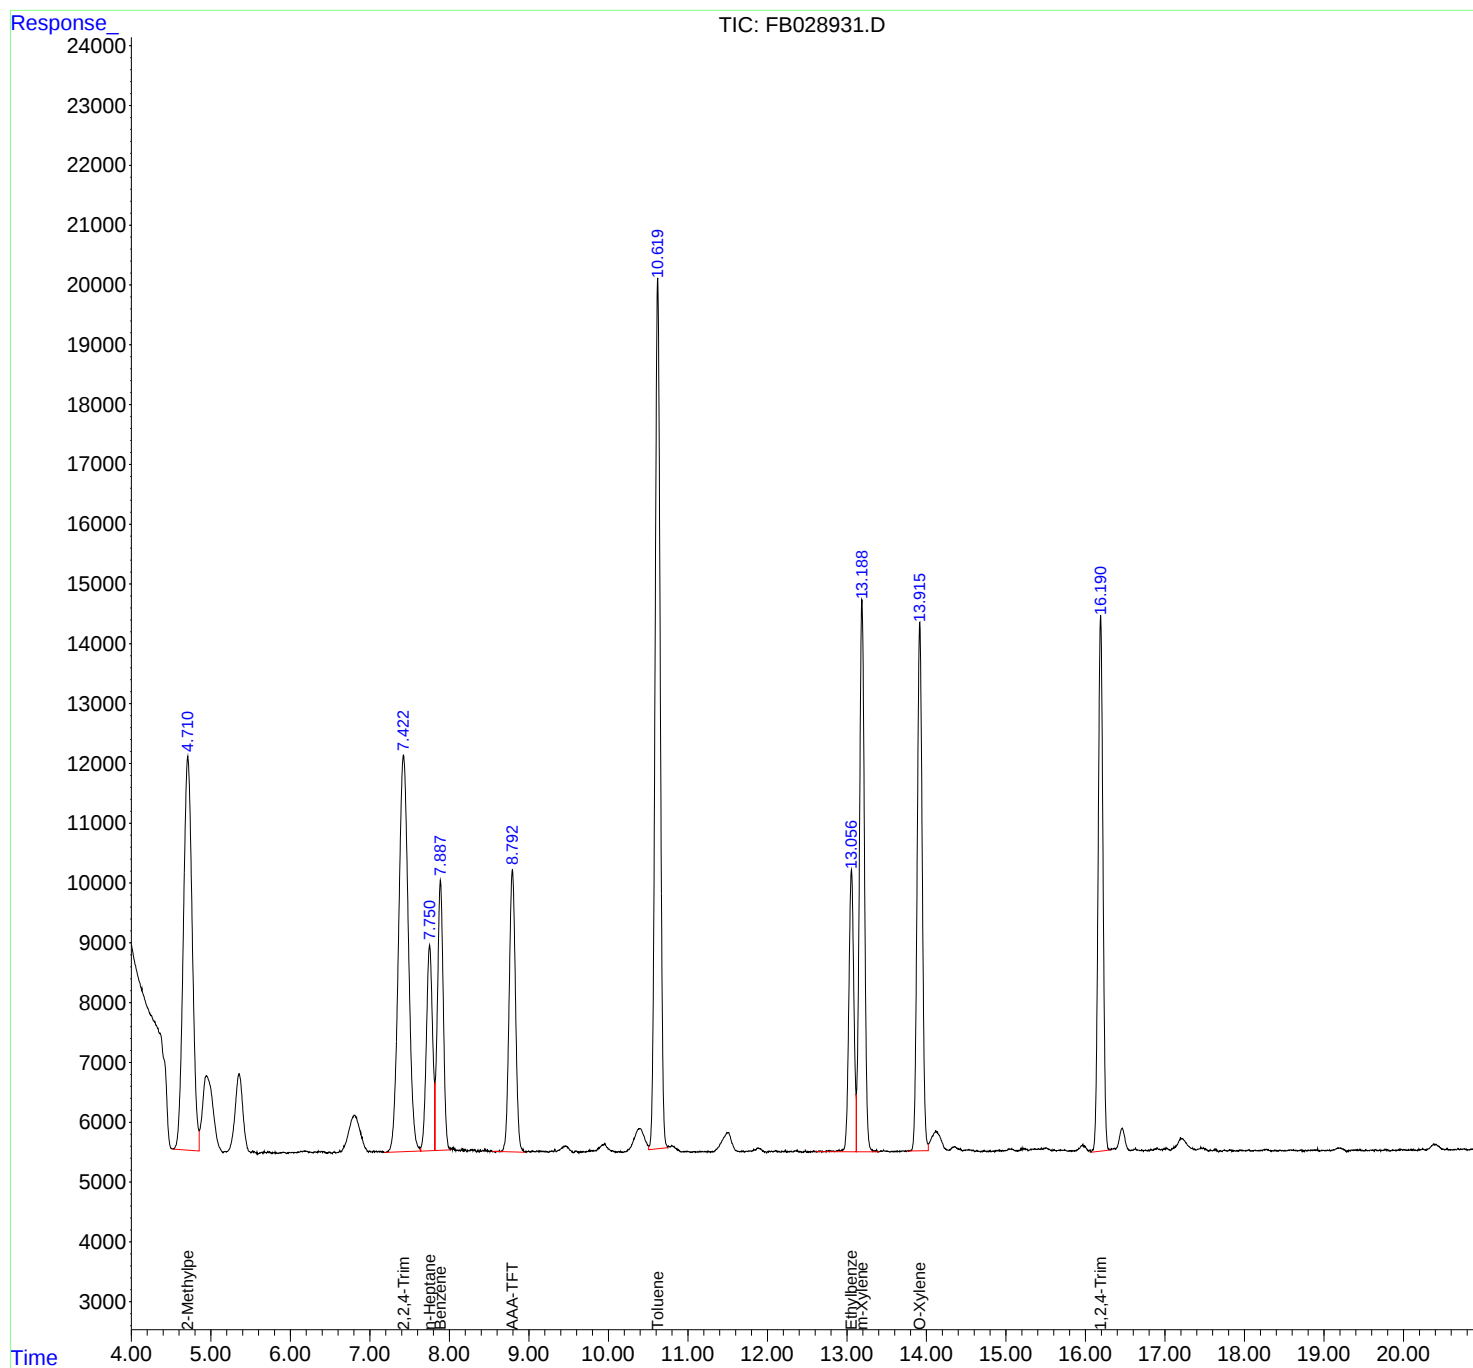


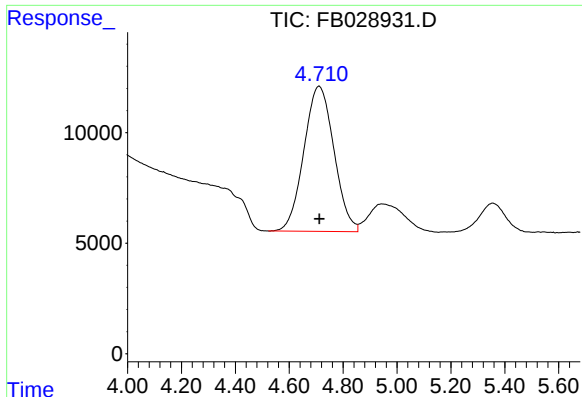

#1 2-Methylpentane


R.T.: 4.711 min
Delta R.T.: 0.000 min
Response: 509415
Conc: 31.25 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1111S2

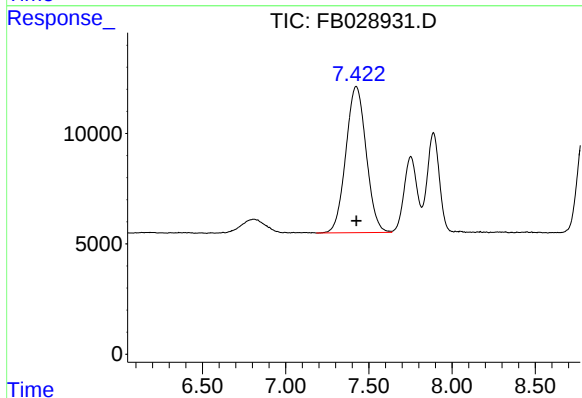


#2 2,2,4-Trimethylpentane

R.T.: 7.424 min
Delta R.T.: 0.000 min
Response: 562538
Conc: 32.01 ng/ml

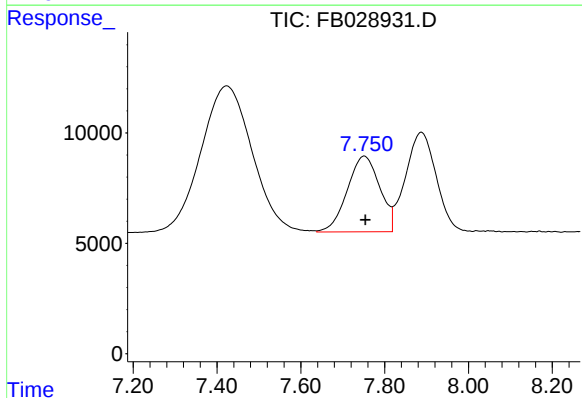


#3 n-Heptane

R.T.: 7.752 min
Delta R.T.: -0.003 min
Response: 184521
Conc: 10.49 ng/ml

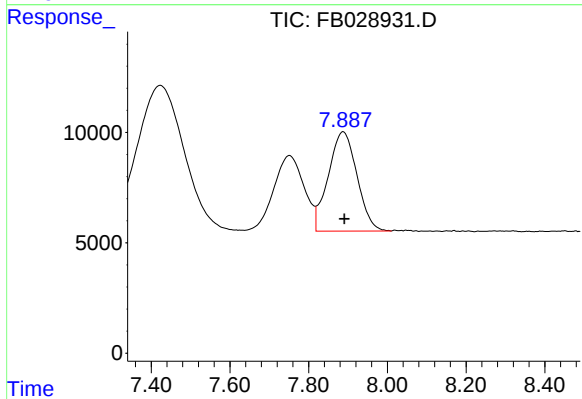

#4 Benzene


R.T.: 7.888 min
Delta R.T.: -0.002 min
Response: 228357
Conc: 11.14 ng/ml

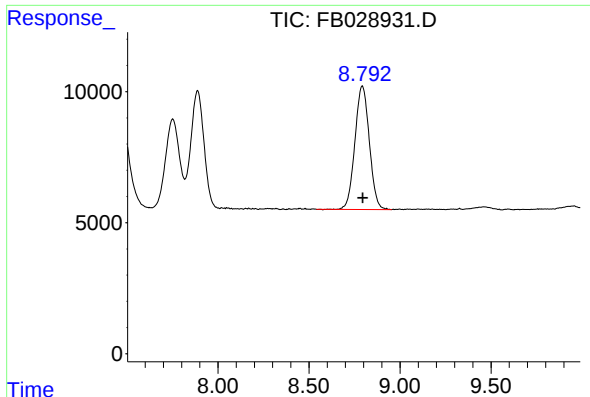

#5 AAA-TFT


R.T.: 8.793 min
Delta R.T.: -0.002 min
Response: 259058
Conc: 20.39 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1111S2

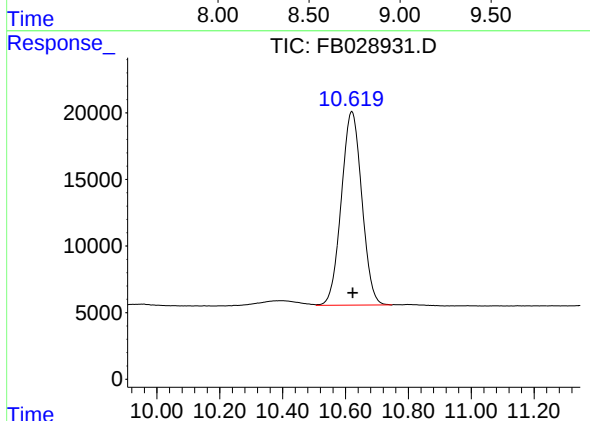


#6 Toluene

R.T.: 10.621 min
Delta R.T.: -0.002 min
Response: 658833
Conc: 32.76 ng/ml

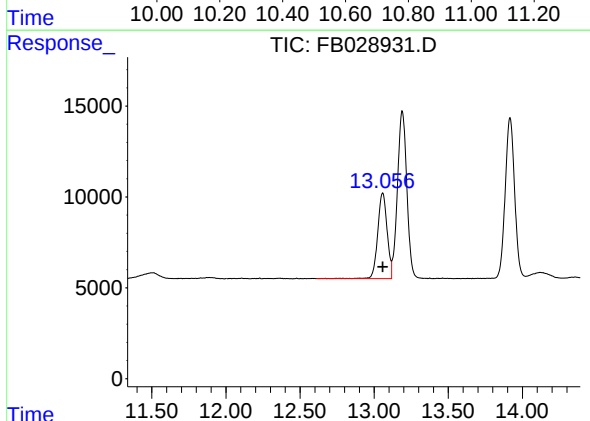


#7 Ethylbenzene

R.T.: 13.058 min
Delta R.T.: 0.000 min
Response: 206874
Conc: 10.91 ng/ml

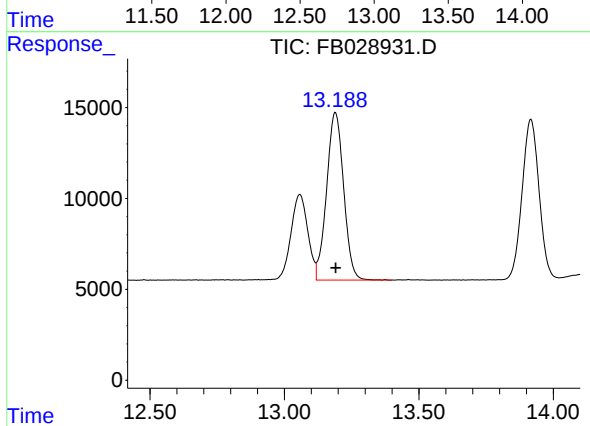

#8 m-Xylene


R.T.: 13.190 min
Delta R.T.: -0.002 min
Response: 405982
Conc: 21.58 ng/ml

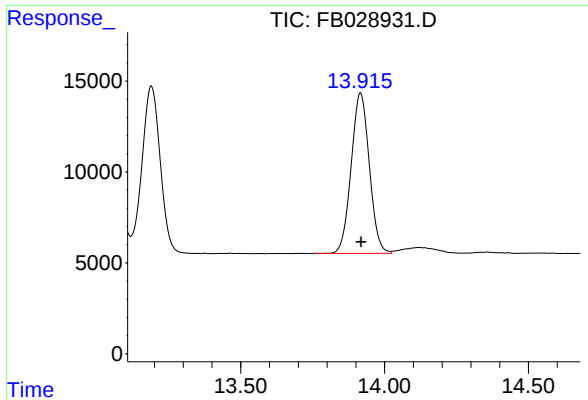

#9 O-Xylene

R.T.: 13.917 min
Delta R.T.: -0.002 min
Response: 388886
Conc: 21.20 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1111S2

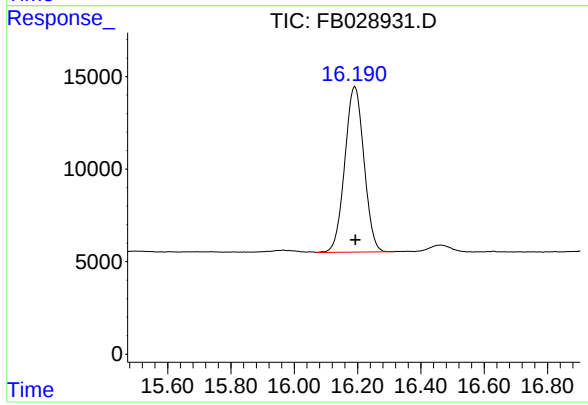

#10 1,2,4-Trimethylbenzene

R.T.: 16.191 min
Delta R.T.: -0.001 min
Response: 375657
Conc: 20.39 ng/ml