

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111219\
 Data File : FB022962.D
 Signal(s) : FID2B.CH
 Acq On : 12 Nov 2019 12:42
 Operator : DD/AJ
 Sample : K5670-02MS
 Misc : 5.05g/5.00ml DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Nov 13 00:11:42 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB103119.M
 Quant Title :
 QLast Update : Thu Oct 31 14:57:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.797	455796	20.247 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.687	962676	29.927 ng/ml
2) t 2,2,4-Trimethylpentane	7.415	1095720	31.040 ng/ml
3) t n-Heptane	7.755	355249	10.213 ng/ml
4) t Benzene	7.890	427208	9.863 ng/ml
6) t Toluene	10.629	1279977	29.691 ng/ml
7) t Ethylbenzene	13.069	400393	10.029 ng/ml
8) t m-Xylene	13.202	756828	20.039 ng/ml
9) t O-Xylene	13.930	713311	20.014 ng/ml
10) t 1,2,4-Trimethylbenzene	16.208	591888	20.871 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111219\
Data File : FB022962.D
Signal(s) : FID2B.CH
Acq On : 12 Nov 2019 12:42
Operator : DD/AJ
Sample : K5670-02MS
Misc : 5.05g/5.00ml DI WATER
ALS Vial : 4 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Nov 13 00:11:42 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB103119.M
Quant Title :
QLast Update : Thu Oct 31 14:57:42 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

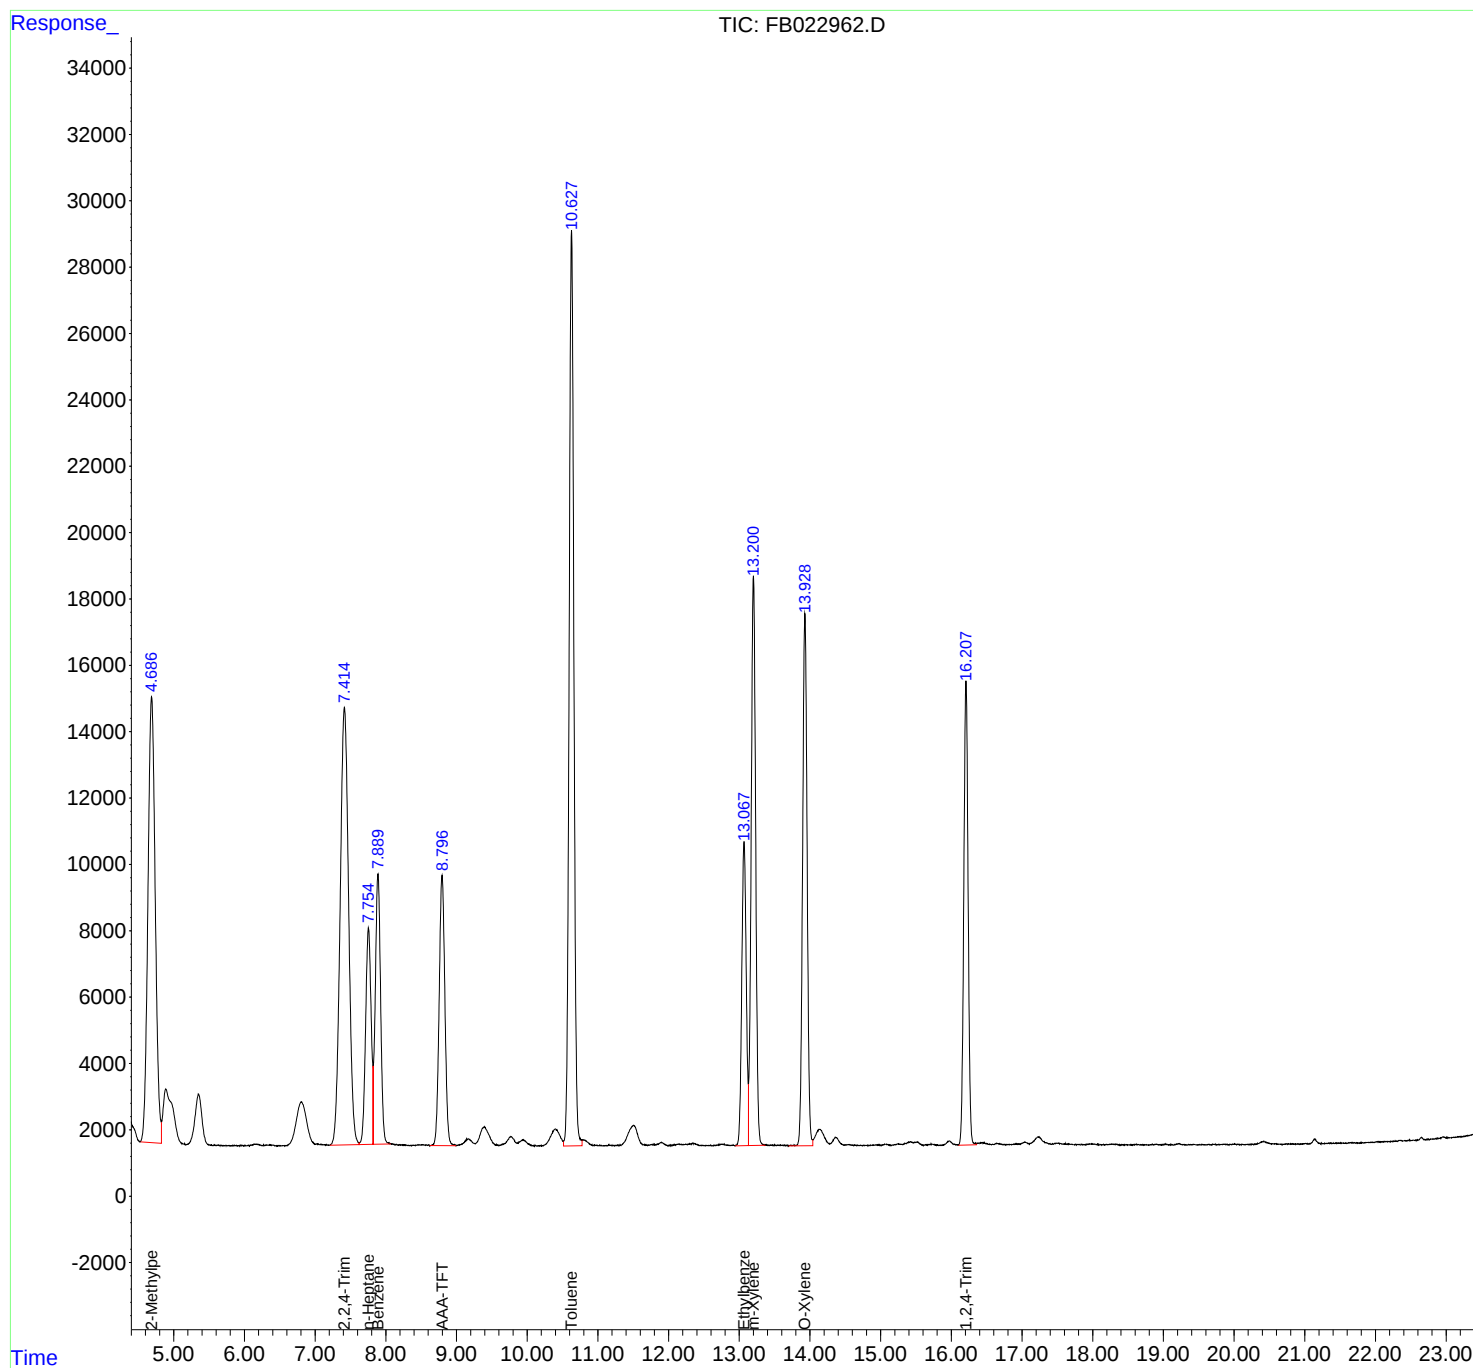

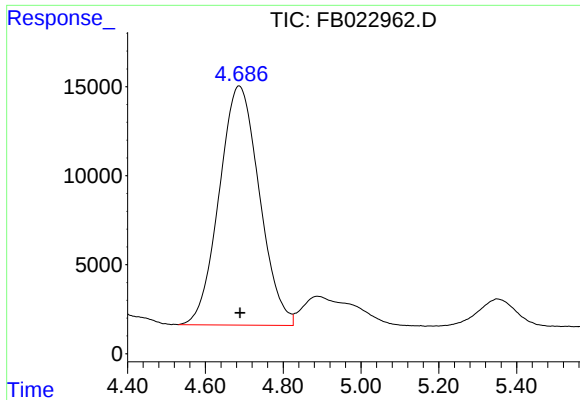


#1 2-Methylpentane

R.T.: 4.687 min
Delta R.T.: -0.002 min
Response: 962676
Conc: 29.93 ng/ml

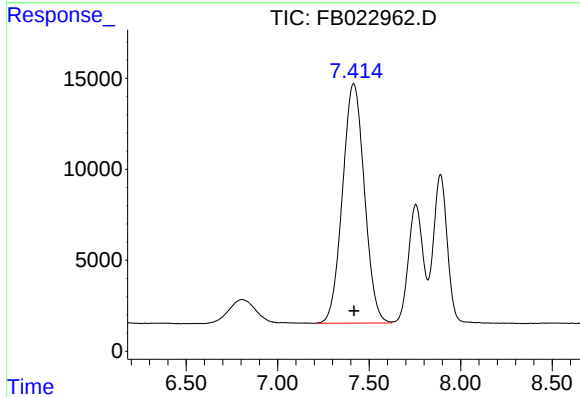


#2 2,2,4-Trimethylpentane

R.T.: 7.415 min
Delta R.T.: -0.003 min
Response: 1095720
Conc: 31.04 ng/ml

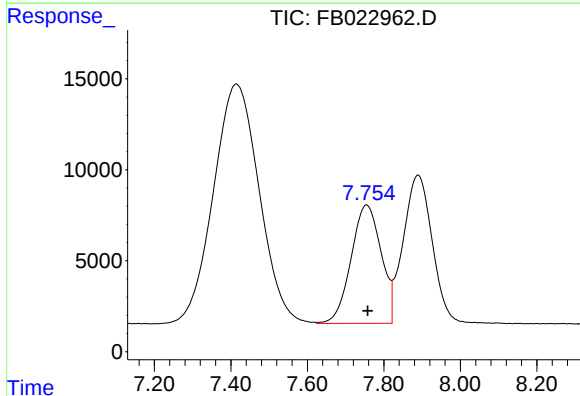


#3 n-Heptane

R.T.: 7.755 min
Delta R.T.: -0.003 min
Response: 355249
Conc: 10.21 ng/ml

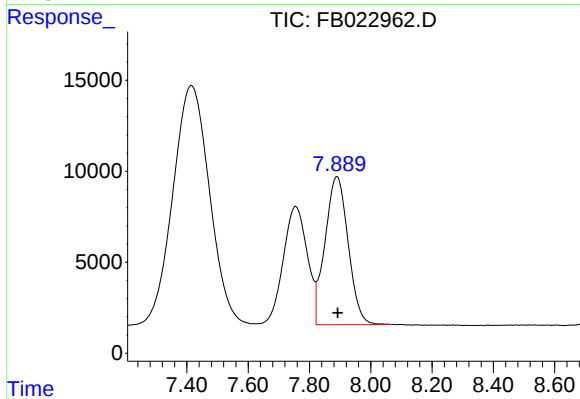


#4 Benzene

R.T.: 7.890 min
Delta R.T.: -0.003 min
Response: 427208
Conc: 9.86 ng/ml

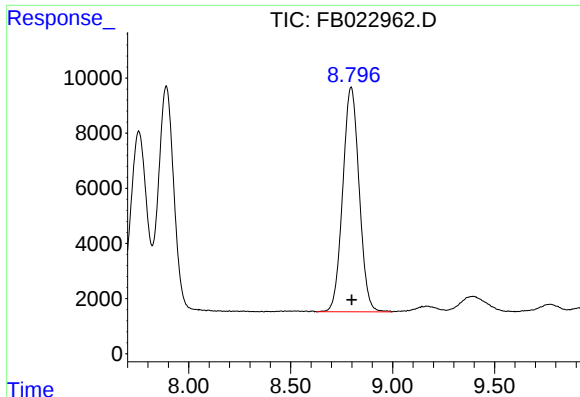


#5 AAA-TFT

R.T.: 8.797 min
Delta R.T.: -0.003 min
Response: 455796
Conc: 20.25 ng/ml

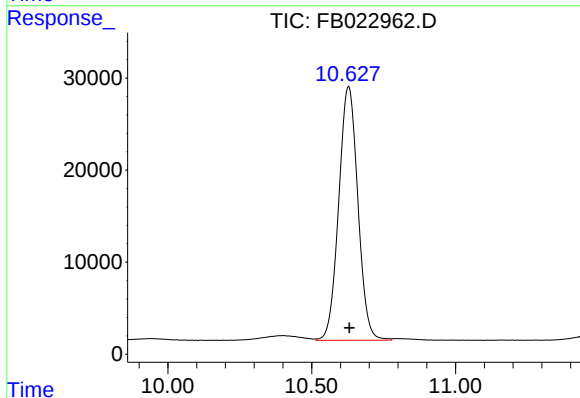


#6 Toluene

R.T.: 10.629 min
Delta R.T.: -0.003 min
Response: 1279977
Conc: 29.69 ng/ml

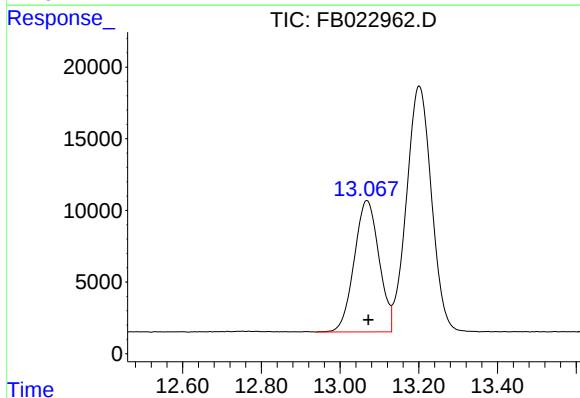


#7 Ethylbenzene

R.T.: 13.069 min
Delta R.T.: -0.003 min
Response: 400393
Conc: 10.03 ng/ml

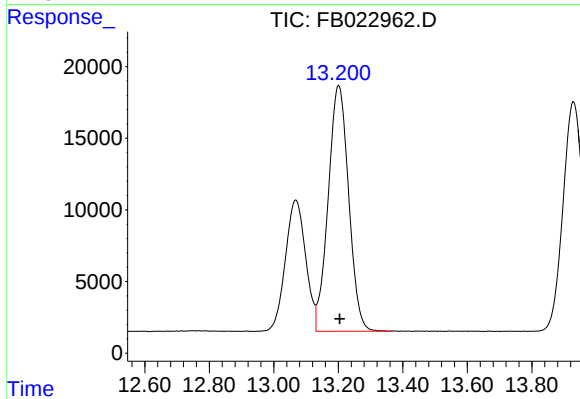


#8 m-Xylene

R.T.: 13.202 min
Delta R.T.: -0.003 min
Response: 756828
Conc: 20.04 ng/ml

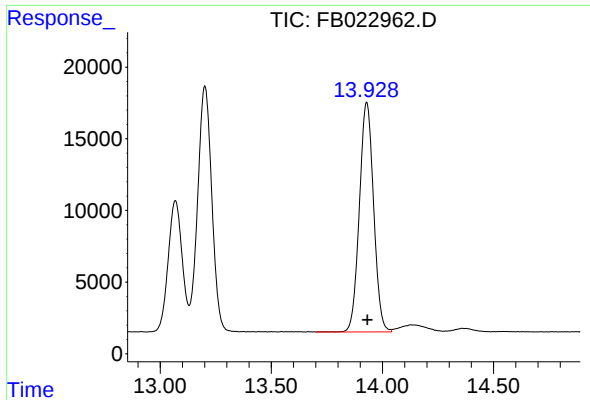

#9 O-Xylene

R.T.: 13.930 min
Delta R.T.: -0.003 min
Response: 713311
Conc: 20.01 ng/ml

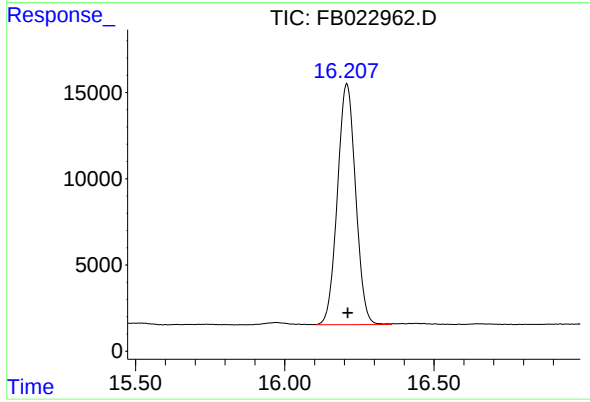

#10 1,2,4-Trimethylbenzene

R.T.: 16.208 min
Delta R.T.: -0.003 min
Response: 591888
Conc: 20.87 ng/ml