

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111220\
 Data File : FB025227.D
 Signal(s) : FID2B.CH
 Acq On : 12 Nov 2020 10:21
 Operator : DD/AJ
 Sample : BSF1112S1
 Misc : 5.00g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Nov 13 00:26:36 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110320.M
 Quant Title :
 QLast Update : Wed Nov 04 08:05:53 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.800	459268	20.340 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.687	1001728	31.035 ng/ml
2) t 2,2,4-Trimethylpentane	7.418	1060487	31.964 ng/ml
3) t n-Heptane	7.758	350561	10.673 ng/ml
4) t Benzene	7.893	418344	10.522 ng/ml
6) t Toluene	10.631	1177014	31.479 ng/ml
7) t Ethylbenzene	13.071	360895	10.509 ng/ml
8) t m-Xylene	13.204	714975	21.175 ng/ml
9) t O-Xylene	13.932	697298	21.326 ng/ml
10) t 1,2,4-Trimethylbenzene	16.209	586491	21.315 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111220\
Data File : FB025227.D
Signal(s) : FID2B.CH
Acq On : 12 Nov 2020 10:21
Operator : DD/AJ
Sample : BSF1112S1
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Nov 13 00:26:36 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110320.M
Quant Title :
QLast Update : Wed Nov 04 08:05:53 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

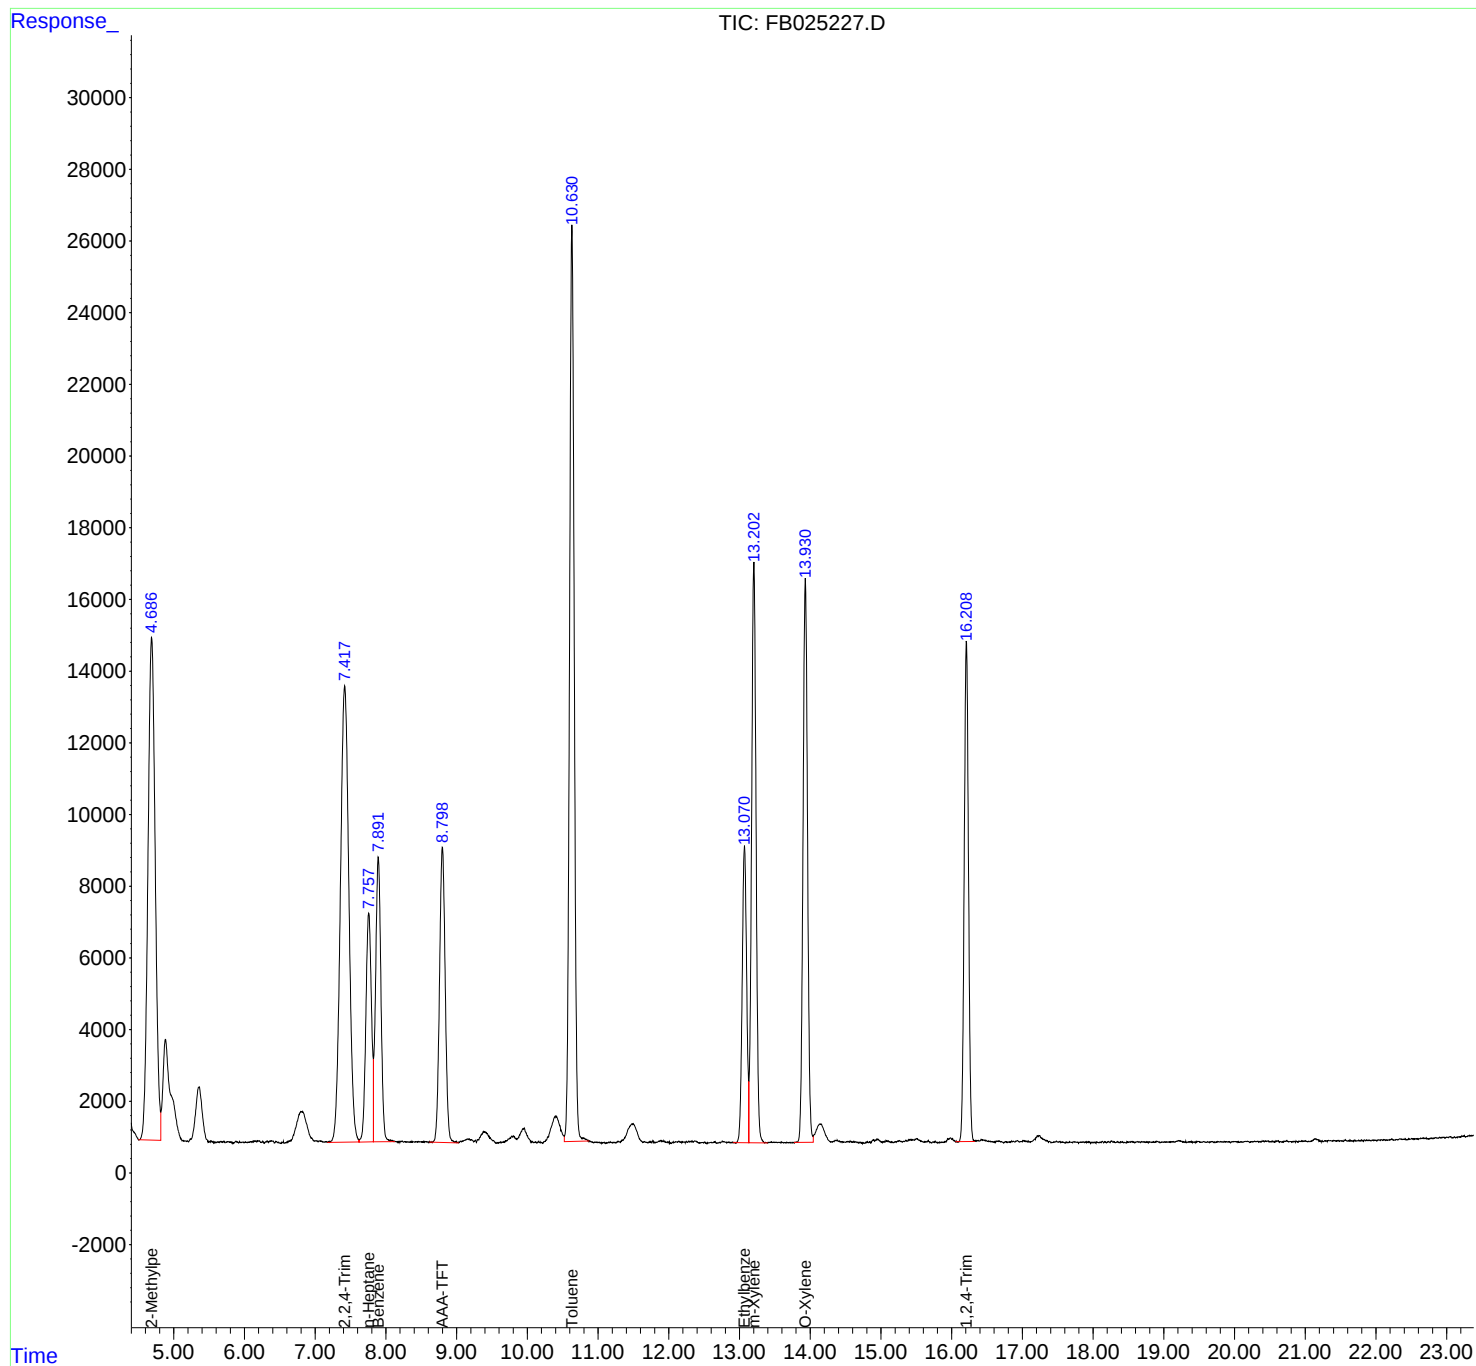


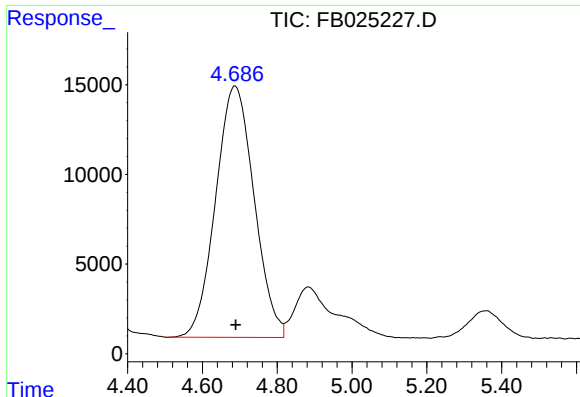

#1 2-Methylpentane


R.T.: 4.687 min
Delta R.T.: -0.002 min
Response: 1001728
Conc: 31.03 ng/ml

Instrument :
FID_B
ClientSampleId :

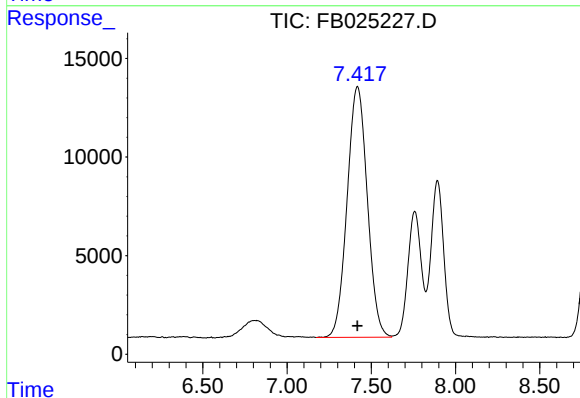


#2 2,2,4-Trimethylpentane

R.T.: 7.418 min
Delta R.T.: 0.000 min
Response: 1060487
Conc: 31.96 ng/ml

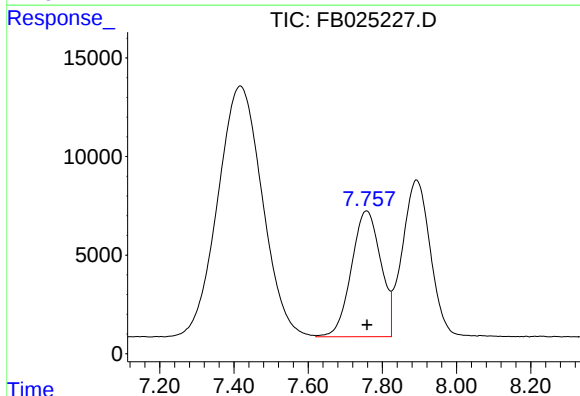


#3 n-Heptane

R.T.: 7.758 min
Delta R.T.: 0.000 min
Response: 350561
Conc: 10.67 ng/ml

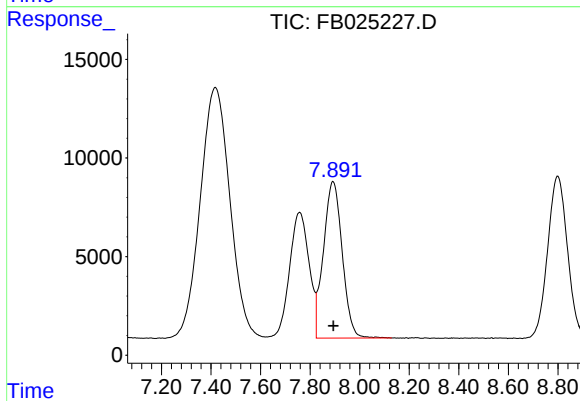

#4 Benzene


R.T.: 7.893 min
Delta R.T.: 0.000 min
Response: 418344
Conc: 10.52 ng/ml

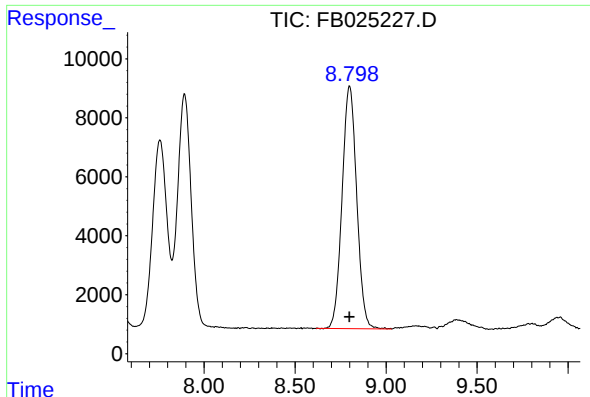

#5 AAA-TFT


R.T.: 8.800 min
Delta R.T.: 0.000 min
Response: 459268
Conc: 20.34 ng/ml

Instrument :
FID_B
ClientSampleId :

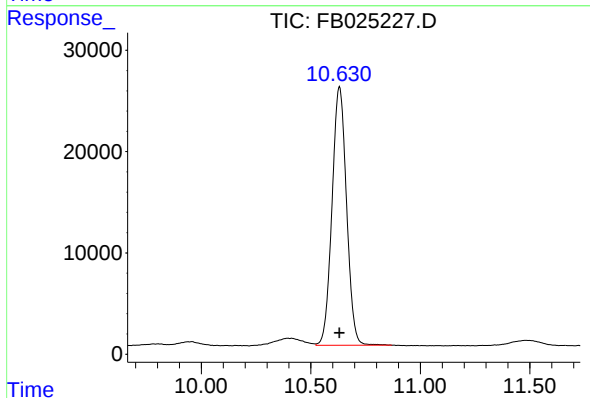


#6 Toluene

R.T.: 10.631 min
Delta R.T.: 0.000 min
Response: 1177014
Conc: 31.48 ng/ml

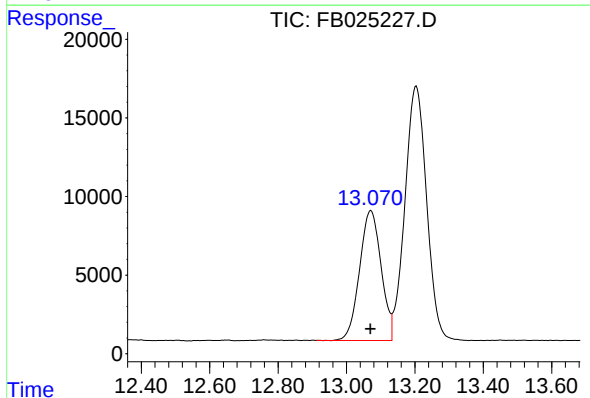


#7 Ethylbenzene

R.T.: 13.071 min
Delta R.T.: 0.000 min
Response: 360895
Conc: 10.51 ng/ml

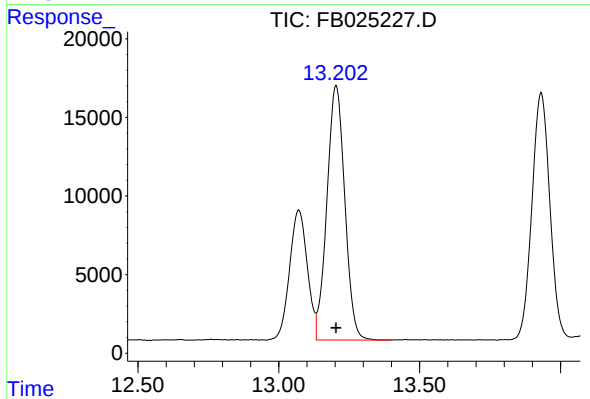

#8 m-Xylene


R.T.: 13.204 min
Delta R.T.: 0.000 min
Response: 714975
Conc: 21.18 ng/ml

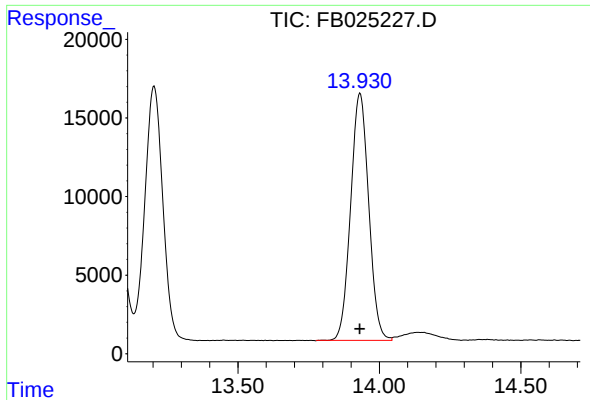

#9 O-Xylene

R.T.: 13.932 min
Delta R.T.: 0.000 min
Response: 697298
Conc: 21.33 ng/ml

Instrument :
FID_B
ClientSampleId :

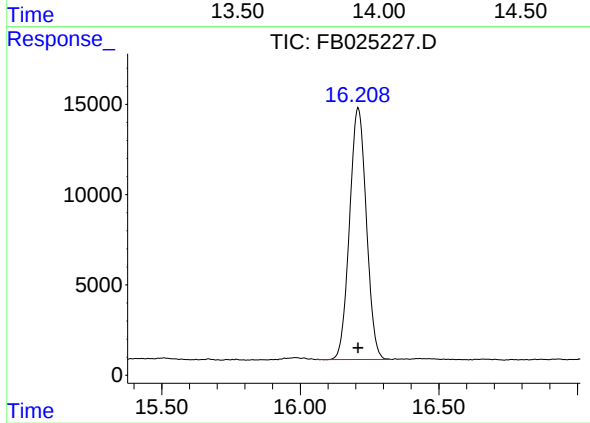

#10 1,2,4-Trimethylbenzene

R.T.: 16.209 min
Delta R.T.: 0.000 min
Response: 586491
Conc: 21.32 ng/ml