

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111220\
 Data File : FB025231.D
 Signal(s) : FID2B.CH
 Acq On : 12 Nov 2020 12:47
 Operator : DD/AJ
 Sample : L4622-05MSD
 Misc : 5.07g/5.00ml DI WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 PAV-B12-110320-10-17MSD

Integration File: Calibration.e
 Quant Time: Nov 13 00:27:07 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110320.M
 Quant Title :
 QLast Update : Wed Nov 04 08:05:53 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.802	519959	23.028 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.689	838773	25.986 ng/ml
2) t 2,2,4-Trimethylpentane	7.420	729113	21.976 ng/ml
3) t n-Heptane	7.760	240862	7.333 ng/ml
4) t Benzene	7.895	432657	10.882 ng/ml
6) t Toluene	10.633	1160764	31.044 ng/ml
7) t Ethylbenzene	13.072	336770	9.807 ng/ml
8) t m-Xylene	13.206	662046	19.608 ng/ml
9) t O-Xylene	13.933	645886	19.754 ng/ml
10) t 1,2,4-Trimethylbenzene	16.211	502607	18.267 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111220\
Data File : FB025231.D
Signal(s) : FID2B.CH
Acq On : 12 Nov 2020 12:47
Operator : DD/AJ
Sample : L4622-05MSD
Misc : 5.07g/5.00ml DI WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
PAV-B12-110320-10-17MSD

Integration File: Calibration.e
Quant Time: Nov 13 00:27:07 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110320.M
Quant Title :
QLast Update : Wed Nov 04 08:05:53 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

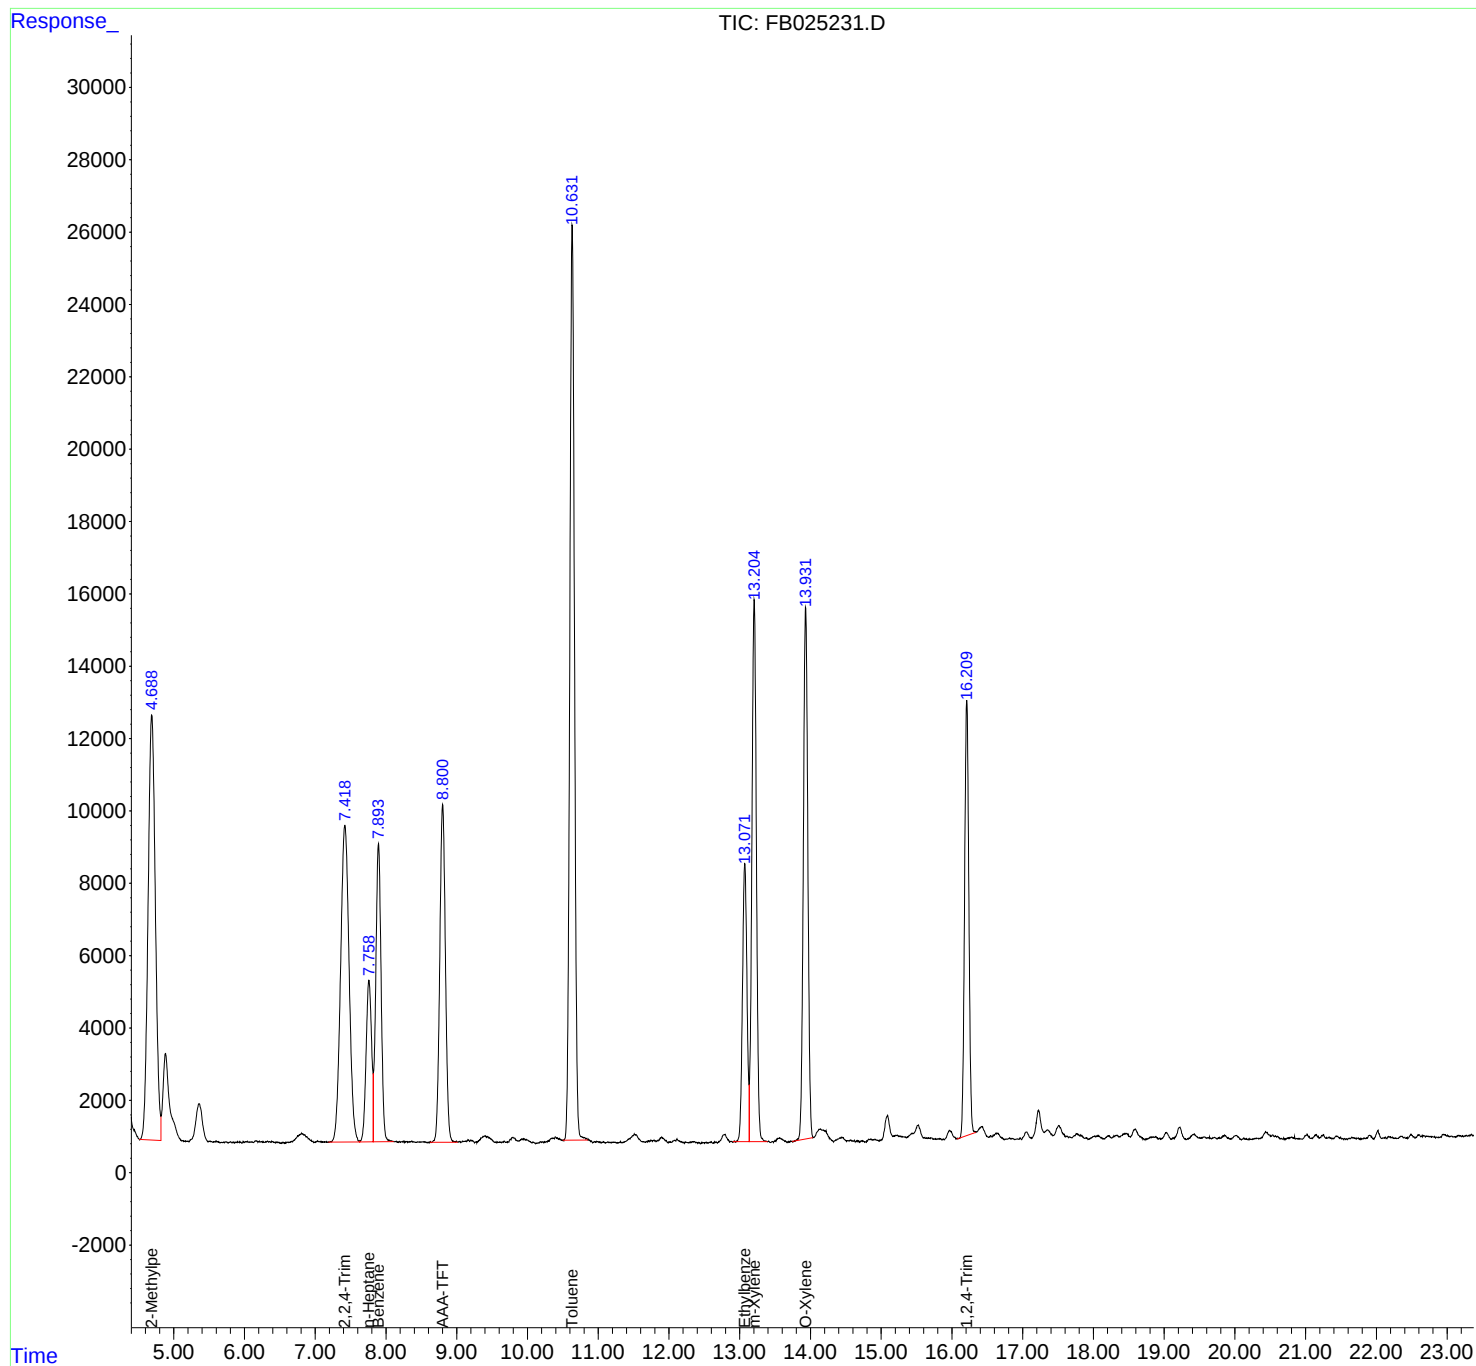


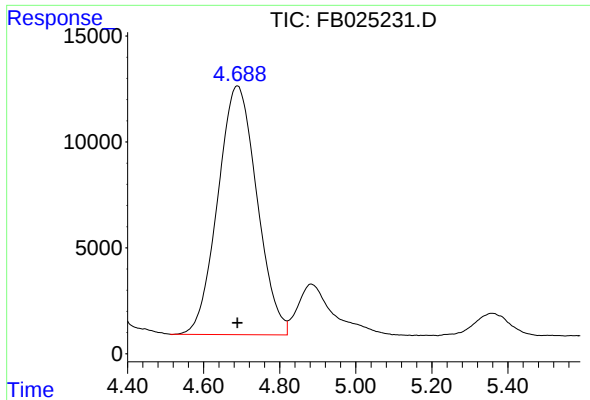

#1 2-Methylpentane


R.T.: 4.689 min
Delta R.T.: 0.000 min
Response: 838773
Conc: 25.99 ng/ml

Instrument :
FID_B
ClientSampleId :
PAV-B12-110320-10-17MSD

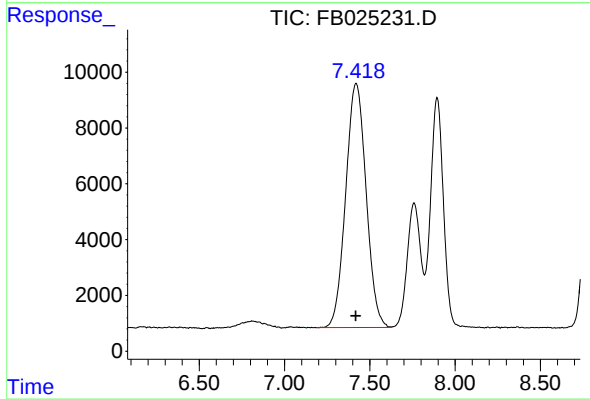


#2 2,2,4-Trimethylpentane

R.T.: 7.420 min
Delta R.T.: 0.002 min
Response: 729113
Conc: 21.98 ng/ml

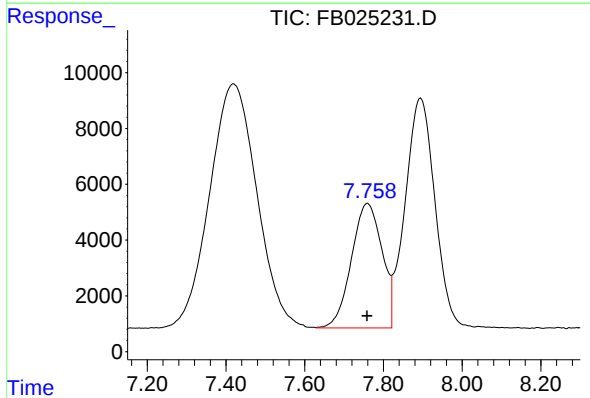


#3 n-Heptane

R.T.: 7.760 min
Delta R.T.: 0.000 min
Response: 240862
Conc: 7.33 ng/ml

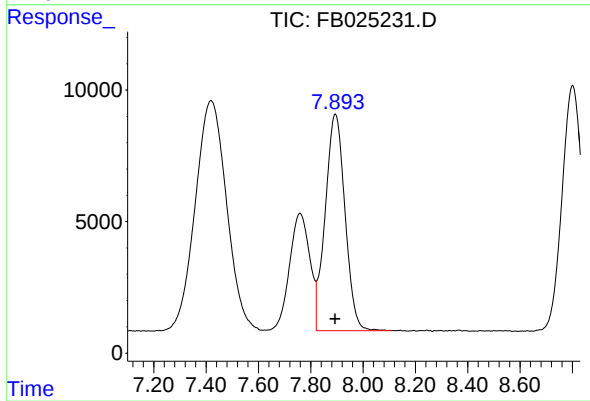

#4 Benzene


R.T.: 7.895 min
Delta R.T.: 0.002 min
Response: 432657
Conc: 10.88 ng/ml

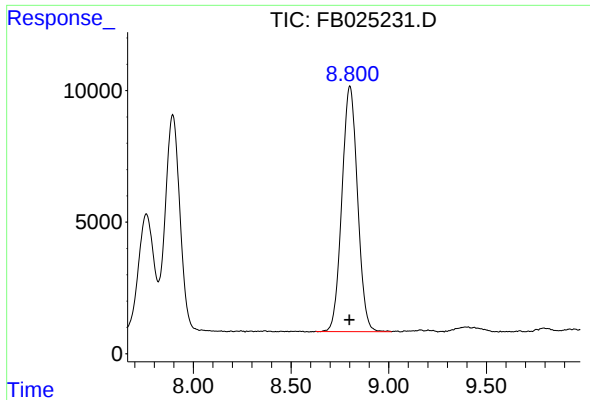

#5 AAA-TFT


R.T.: 8.802 min
Delta R.T.: 0.002 min
Response: 519959
Conc: 23.03 ng/ml

Instrument :
FID_B
ClientSampleId :
PAV-B12-110320-10-17MSD

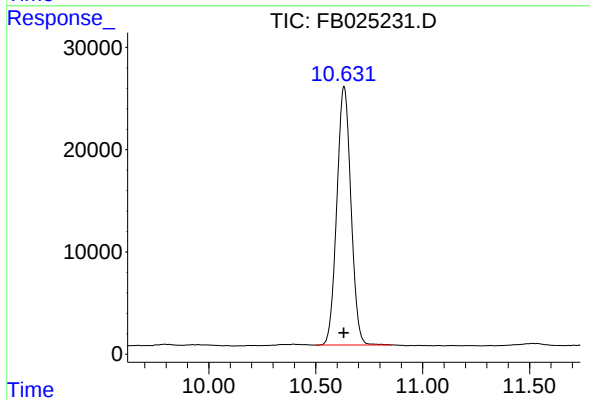


#6 Toluene

R.T.: 10.633 min
Delta R.T.: 0.002 min
Response: 1160764
Conc: 31.04 ng/ml

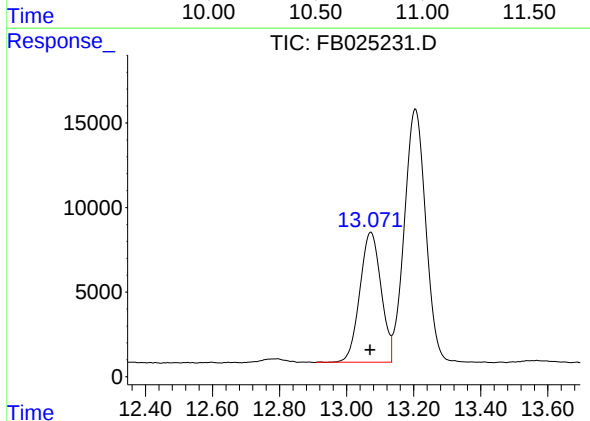


#7 Ethylbenzene

R.T.: 13.072 min
Delta R.T.: 0.002 min
Response: 336770
Conc: 9.81 ng/ml

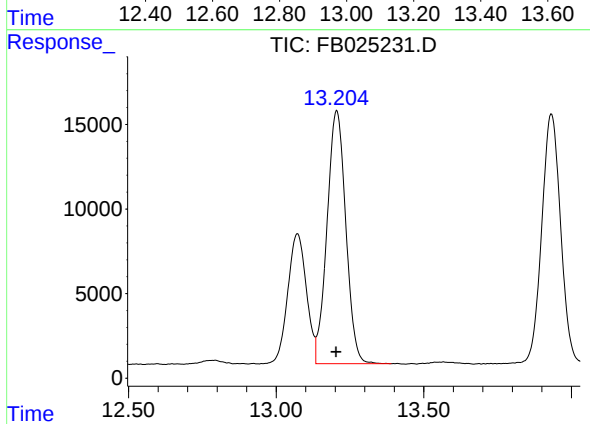

#8 m-Xylene


R.T.: 13.206 min
Delta R.T.: 0.002 min
Response: 662046
Conc: 19.61 ng/ml

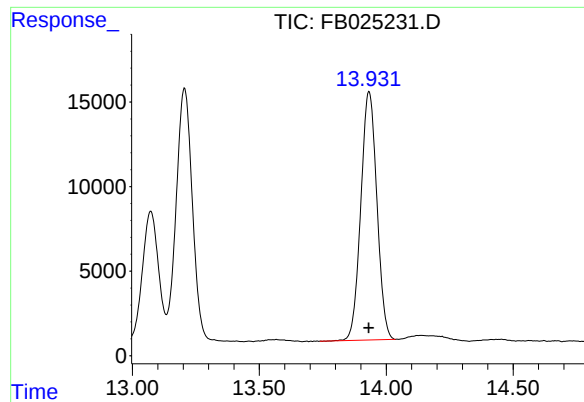

#9 O-Xylene

R.T.: 13.933 min
Delta R.T.: 0.002 min
Response: 645886
Conc: 19.75 ng/ml

Instrument :
FID_B
ClientSampleId :
PAV-B12-110320-10-17MSD

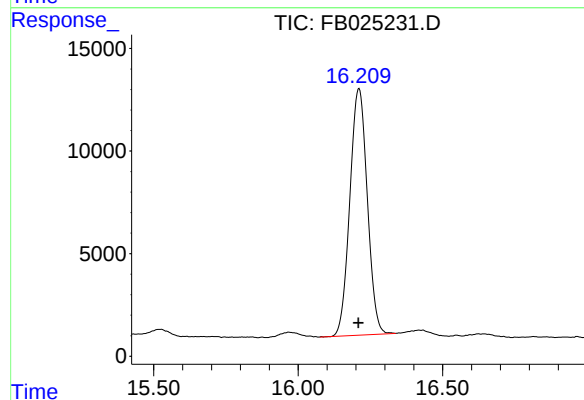

#10 1,2,4-Trimethylbenzene

R.T.: 16.211 min
Delta R.T.: 0.002 min
Response: 502607
Conc: 18.27 ng/ml