

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111319\
 Data File : FB022970.D
 Signal(s) : FID2B.CH
 Acq On : 13 Nov 2019 12:15
 Operator : DD/AJ
 Sample : BSF1113S1
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Nov 14 00:16:18 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB103119.M
 Quant Title :
 QLast Update : Thu Oct 31 14:57:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.796	410659	18.242 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.688	911111	28.324 ng/ml
2) t 2,2,4-Trimethylpentane	7.414	1008067	28.557 ng/ml
3) t n-Heptane	7.755	324330	9.324 ng/ml
4) t Benzene	7.889	399249	9.217 ng/ml
6) t Toluene	10.628	1197359	27.774 ng/ml
7) t Ethylbenzene	13.068	377460	9.455 ng/ml
8) t m-Xylene	13.201	716470	18.971 ng/ml
9) t O-Xylene	13.929	673705	18.903 ng/ml
10) t 1,2,4-Trimethylbenzene	16.208	564817	19.917 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111319\
Data File : FB022970.D
Signal(s) : FID2B.CH
Acq On : 13 Nov 2019 12:15
Operator : DD/AJ
Sample : BSF1113S1
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Nov 14 00:16:18 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB103119.M
Quant Title :
QLast Update : Thu Oct 31 14:57:42 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

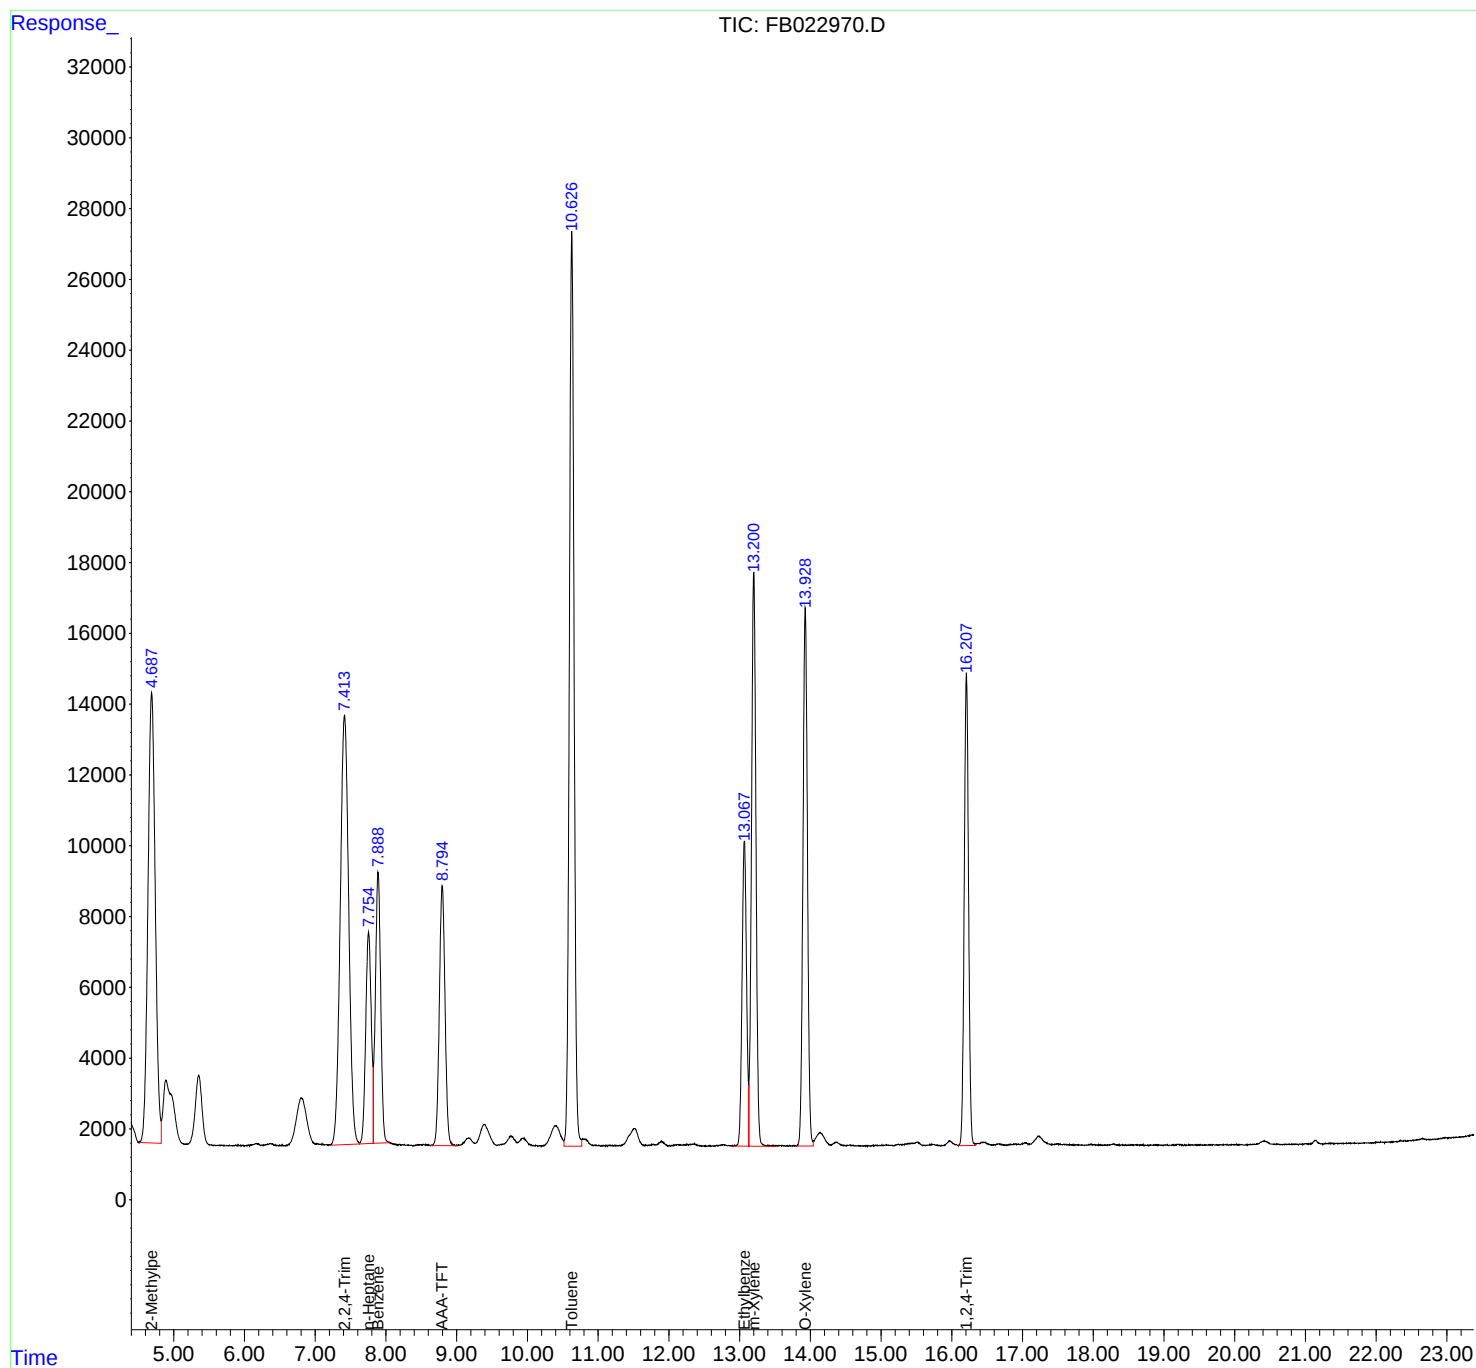

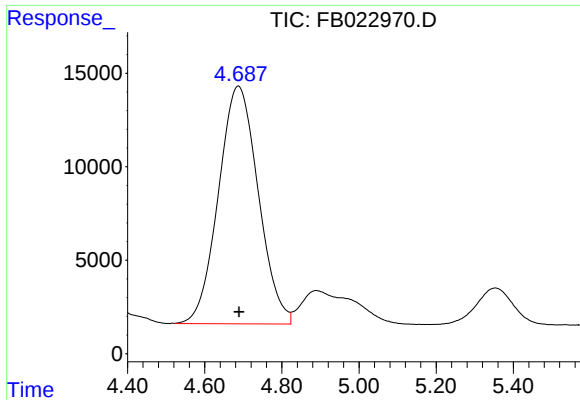


#1 2-Methylpentane

R.T.: 4.688 min
Delta R.T.: 0.000 min
Response: 911111
Conc: 28.32 ng/ml

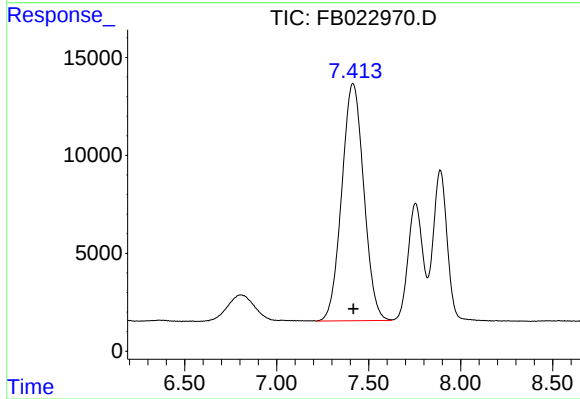


#2 2,2,4-Trimethylpentane

R.T.: 7.414 min
Delta R.T.: -0.004 min
Response: 1008067
Conc: 28.56 ng/ml

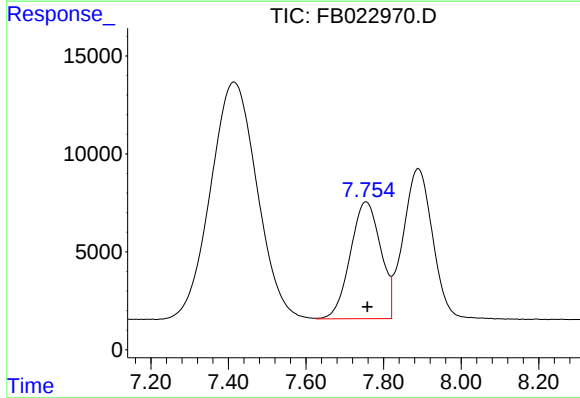


#3 n-Heptane

R.T.: 7.755 min
Delta R.T.: -0.003 min
Response: 324330
Conc: 9.32 ng/ml

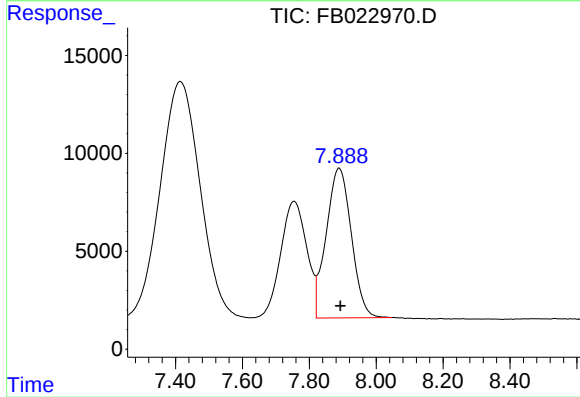


#4 Benzene

R.T.: 7.889 min
Delta R.T.: -0.004 min
Response: 399249
Conc: 9.22 ng/ml

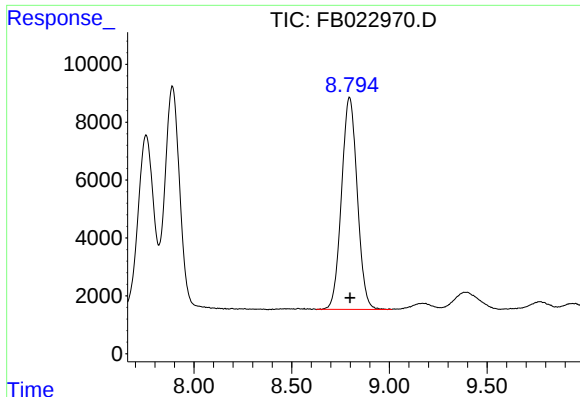


#5 AAA-TFT

R.T.: 8.796 min
Delta R.T.: -0.004 min
Response: 410659
Conc: 18.24 ng/ml

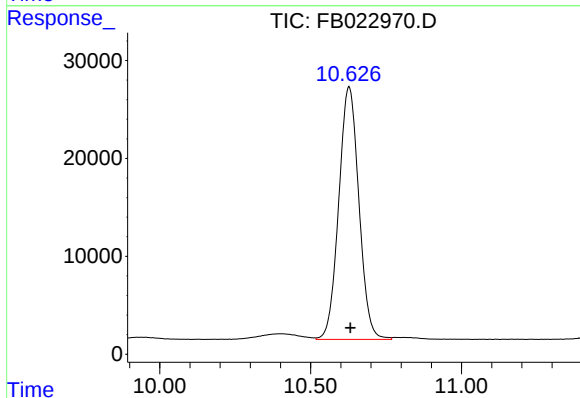


#6 Toluene

R.T.: 10.628 min
Delta R.T.: -0.004 min
Response: 1197359
Conc: 27.77 ng/ml

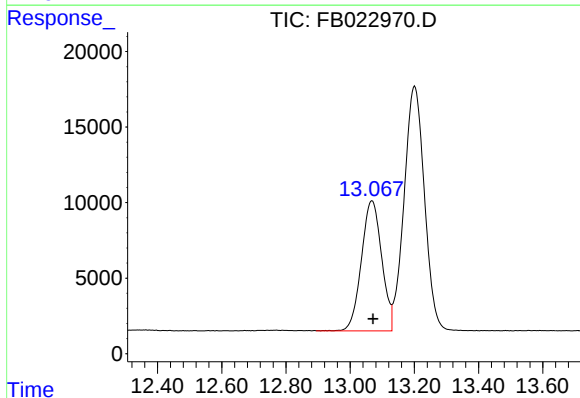


#7 Ethylbenzene

R.T.: 13.068 min
Delta R.T.: -0.004 min
Response: 377460
Conc: 9.45 ng/ml

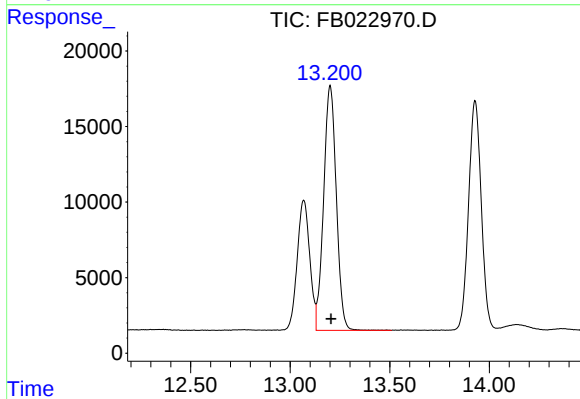


#8 m-Xylene

R.T.: 13.201 min
Delta R.T.: -0.004 min
Response: 716470
Conc: 18.97 ng/ml

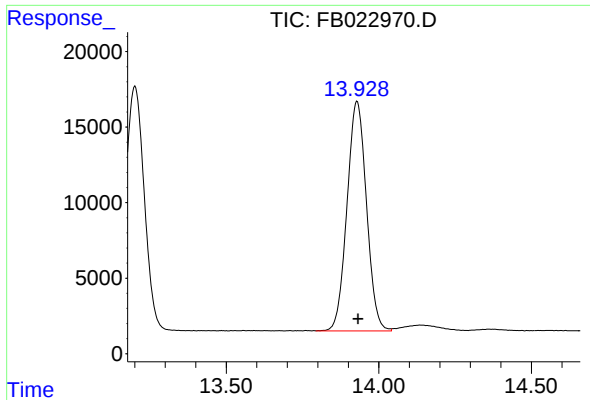

#9 O-Xylene

R.T.: 13.929 min
Delta R.T.: -0.004 min
Response: 673705
Conc: 18.90 ng/ml

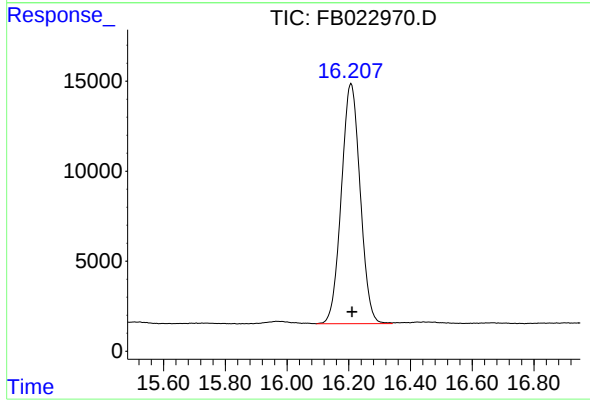

#10 1,2,4-Trimethylbenzene

R.T.: 16.208 min
Delta R.T.: -0.004 min
Response: 564817
Conc: 19.92 ng/ml