

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111319\
 Data File : FB022976.D
 Signal(s) : FID2B.CH
 Acq On : 13 Nov 2019 15:50
 Operator : DD/AJ
 Sample : K5670-06MSD
 Misc : 5.03g/5.00ml DI WATER
 ALS Vial : 9 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Nov 14 00:17:06 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB103119.M
 Quant Title :
 QLast Update : Thu Oct 31 14:57:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.796	379056	16.838 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.688	785957	24.433 ng/ml
2) t	2,2,4-Trimethylpentane	7.415	854403	24.204 ng/ml
3) t	n-Heptane	7.755	276697	7.954 ng/ml
4) t	Benzene	7.889	382794	8.838 ng/ml
6) t	Toluene	10.628	1120450	25.990 ng/ml
7) t	Ethylbenzene	13.068	339425	8.502 ng/ml
8) t	m-Xylene	13.201	642631	17.016 ng/ml
9) t	O-Xylene	13.929	607129	17.035 ng/ml
10) t	1,2,4-Trimethylbenzene	16.208	496485	17.507 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111319\
Data File : FB022976.D
Signal(s) : FID2B.CH
Acq On : 13 Nov 2019 15:50
Operator : DD/AJ
Sample : K5670-06MSD
Misc : 5.03g/5.00ml DI WATER
ALS Vial : 9 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Nov 14 00:17:06 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB103119.M
Quant Title :
QLast Update : Thu Oct 31 14:57:42 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

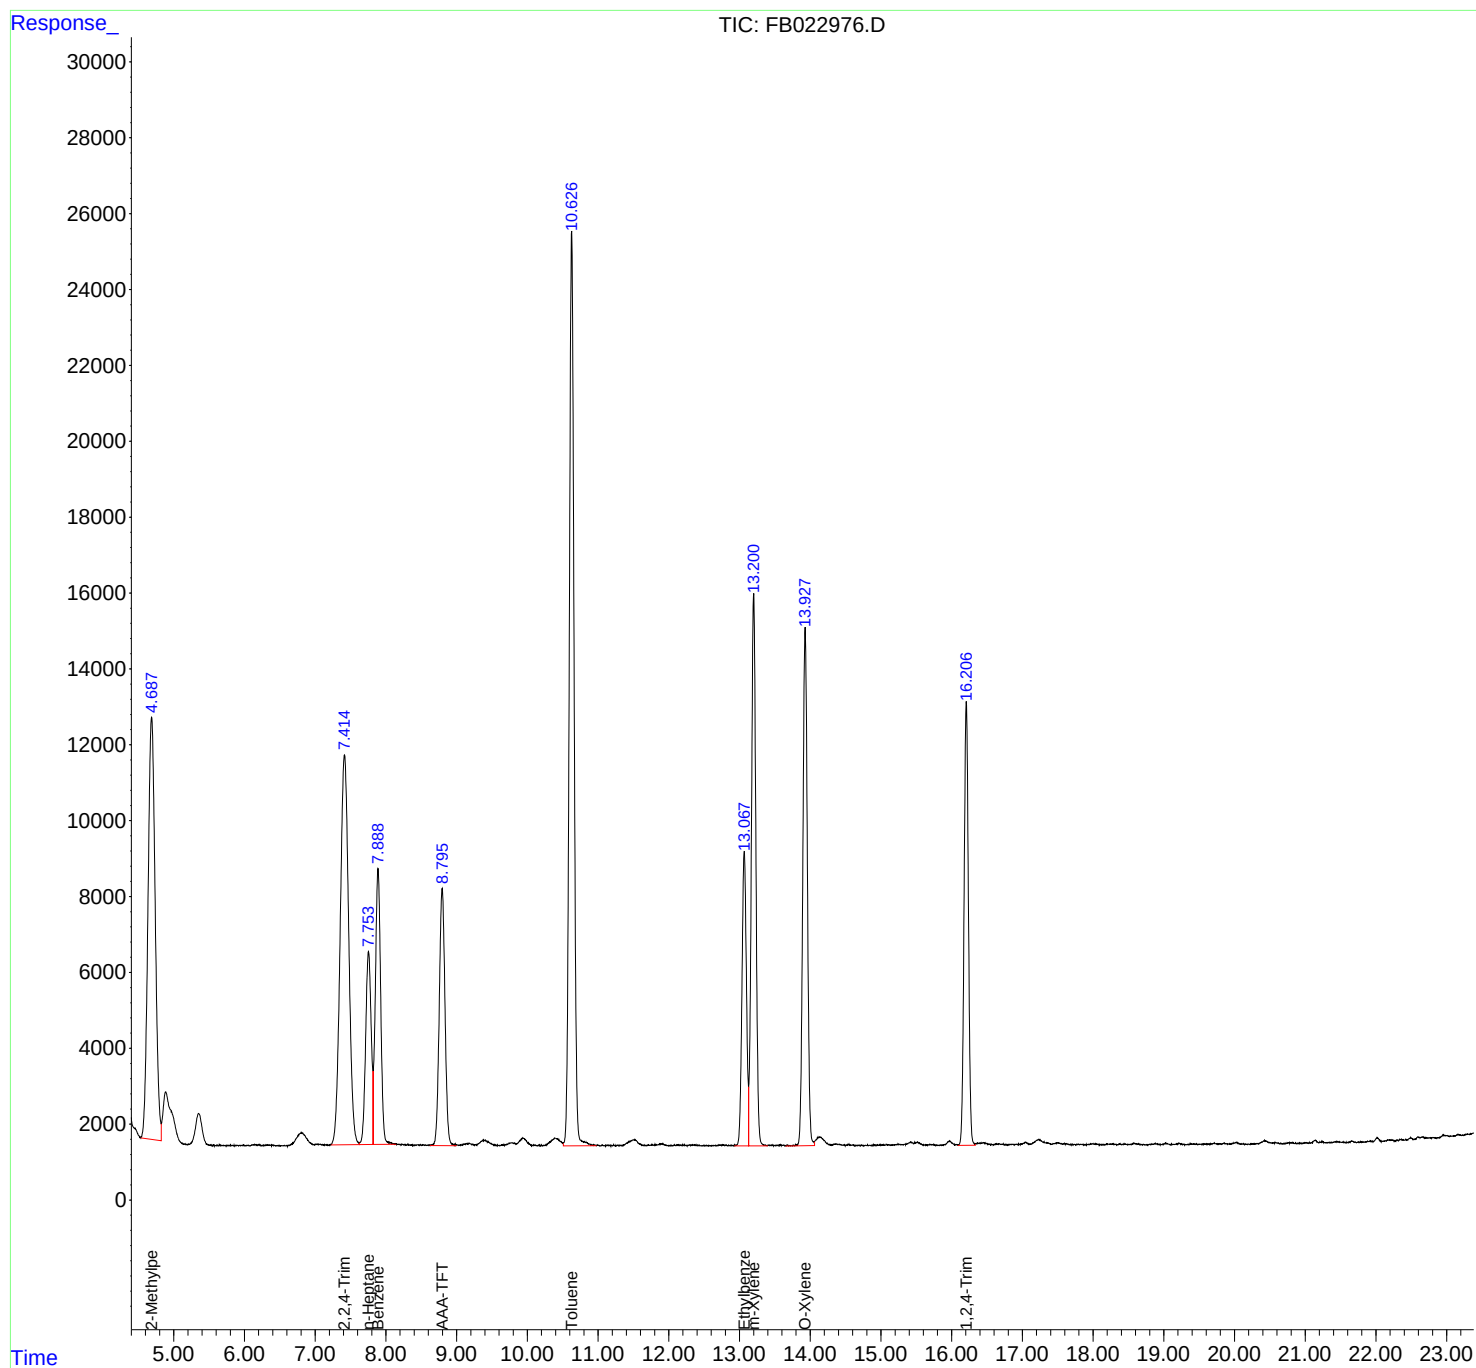

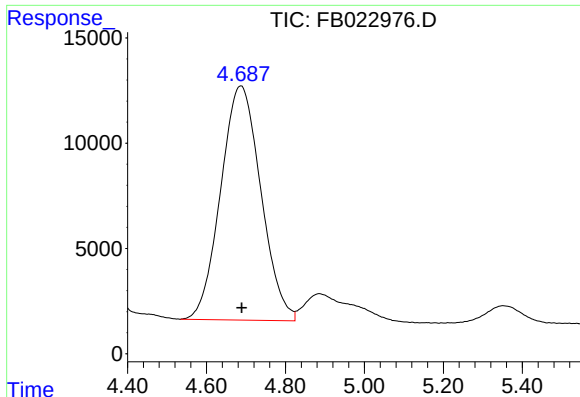


#1 2-Methylpentane

R.T.: 4.688 min
Delta R.T.: 0.000 min
Response: 785957
Conc: 24.43 ng/ml

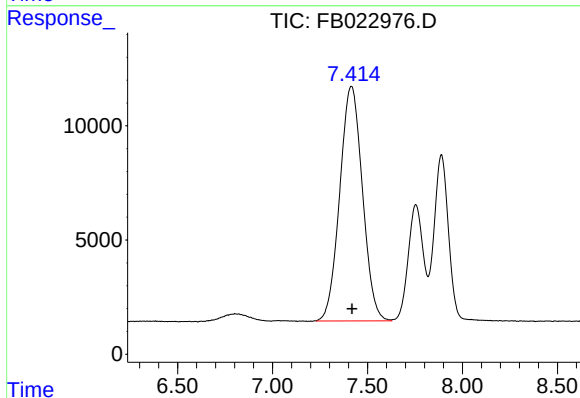


#2 2,2,4-Trimethylpentane

R.T.: 7.415 min
Delta R.T.: -0.003 min
Response: 854403
Conc: 24.20 ng/ml

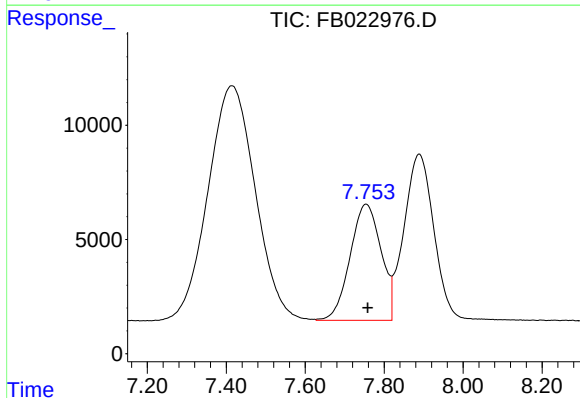


#3 n-Heptane

R.T.: 7.755 min
Delta R.T.: -0.004 min
Response: 276697
Conc: 7.95 ng/ml

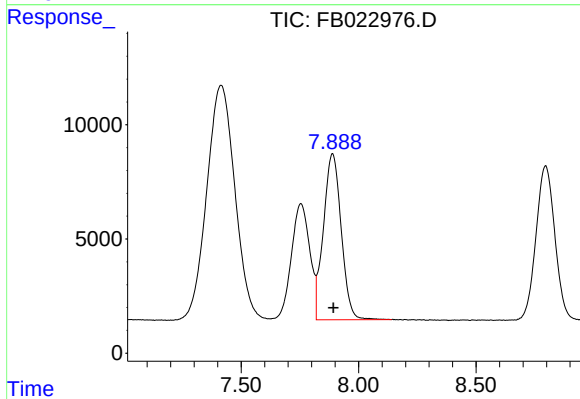


#4 Benzene

R.T.: 7.889 min
Delta R.T.: -0.004 min
Response: 382794
Conc: 8.84 ng/ml

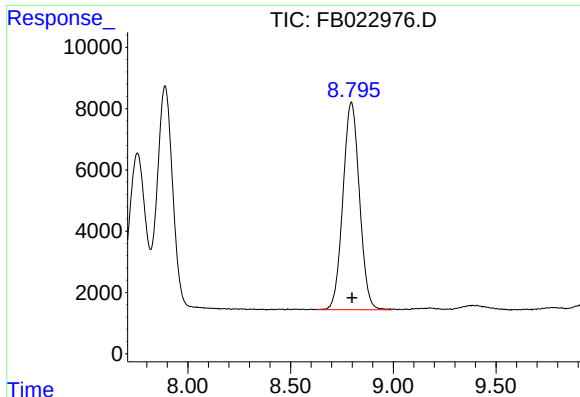


#5 AAA-TFT

R.T.: 8.796 min
Delta R.T.: -0.003 min
Response: 379056
Conc: 16.84 ng/ml

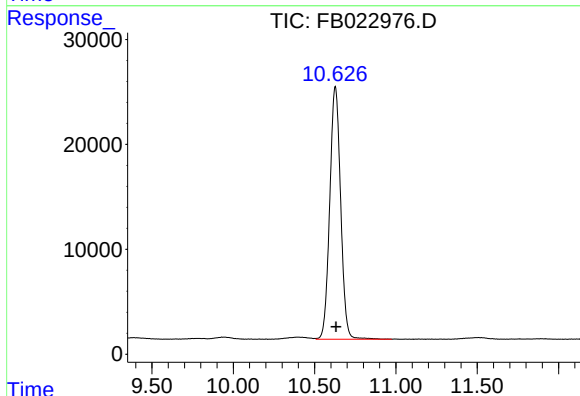


#6 Toluene

R.T.: 10.628 min
Delta R.T.: -0.004 min
Response: 1120450
Conc: 25.99 ng/ml

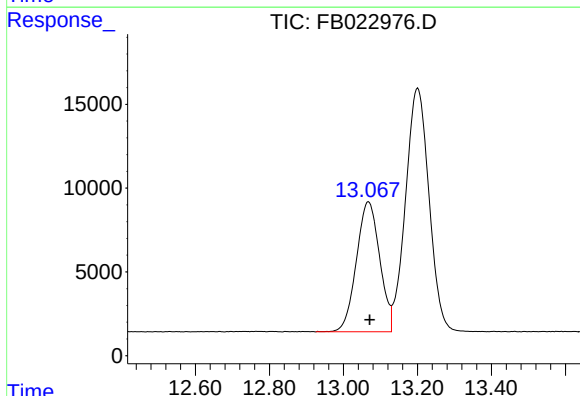


#7 Ethylbenzene

R.T.: 13.068 min
Delta R.T.: -0.004 min
Response: 339425
Conc: 8.50 ng/ml

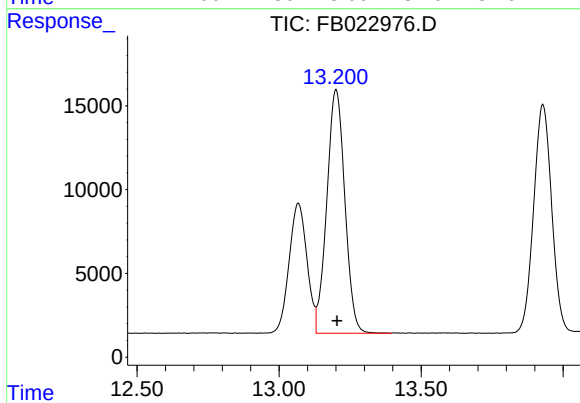


#8 m-Xylene

R.T.: 13.201 min
Delta R.T.: -0.004 min
Response: 642631
Conc: 17.02 ng/ml

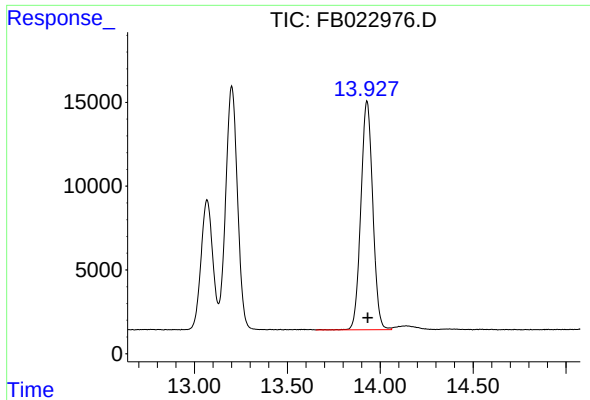

#9 O-Xylene

R.T.: 13.929 min
Delta R.T.: -0.003 min
Response: 607129
Conc: 17.03 ng/ml

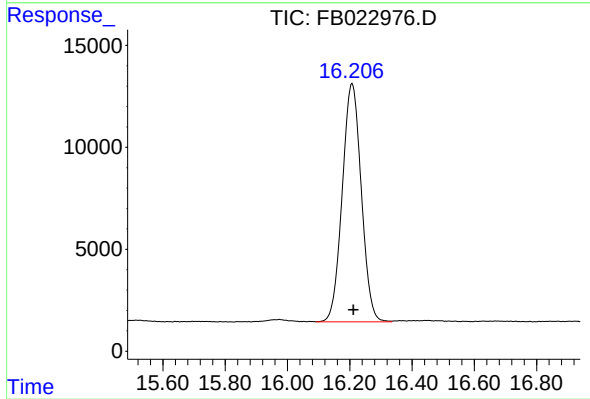

#10 1,2,4-Trimethylbenzene

R.T.: 16.208 min
Delta R.T.: -0.003 min
Response: 496485
Conc: 17.51 ng/ml