

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111320\
 Data File : FB025248.D
 Signal(s) : FID2B.CH
 Acq On : 13 Nov 2020 13:06
 Operator : DD/AJ
 Sample : L4680-05MSD
 Misc : 5.04g/5.00ml DI WATER
 ALS Vial : 8 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Nov 16 09:31:00 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110320.M
 Quant Title :
 QLast Update : Wed Nov 04 08:05:53 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.800	458220	20.294 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.688	846769	26.234 ng/ml
2) t	2,2,4-Trimethylpentane	7.417	825633	24.885 ng/ml
3) t	n-Heptane	7.760	244019	7.429 ng/ml
4) t	Benzene	7.894	363157	9.134 ng/ml
6) t	Toluene	10.632	1002207	26.803 ng/ml
7) t	Ethylbenzene	13.072	305568	8.898 ng/ml
8) t	m-Xylene	13.205	606067	17.950 ng/ml
9) t	O-Xylene	13.933	587556	17.970 ng/ml
10) t	1,2,4-Trimethylbenzene	16.210	480048	17.447 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111320\
Data File : FB025248.D
Signal(s) : FID2B.CH
Acq On : 13 Nov 2020 13:06
Operator : DD/AJ
Sample : L4680-05MSD
Misc : 5.04g/5.00ml DI WATER
ALS Vial : 8 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Nov 16 09:31:00 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110320.M
Quant Title :
QLast Update : Wed Nov 04 08:05:53 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

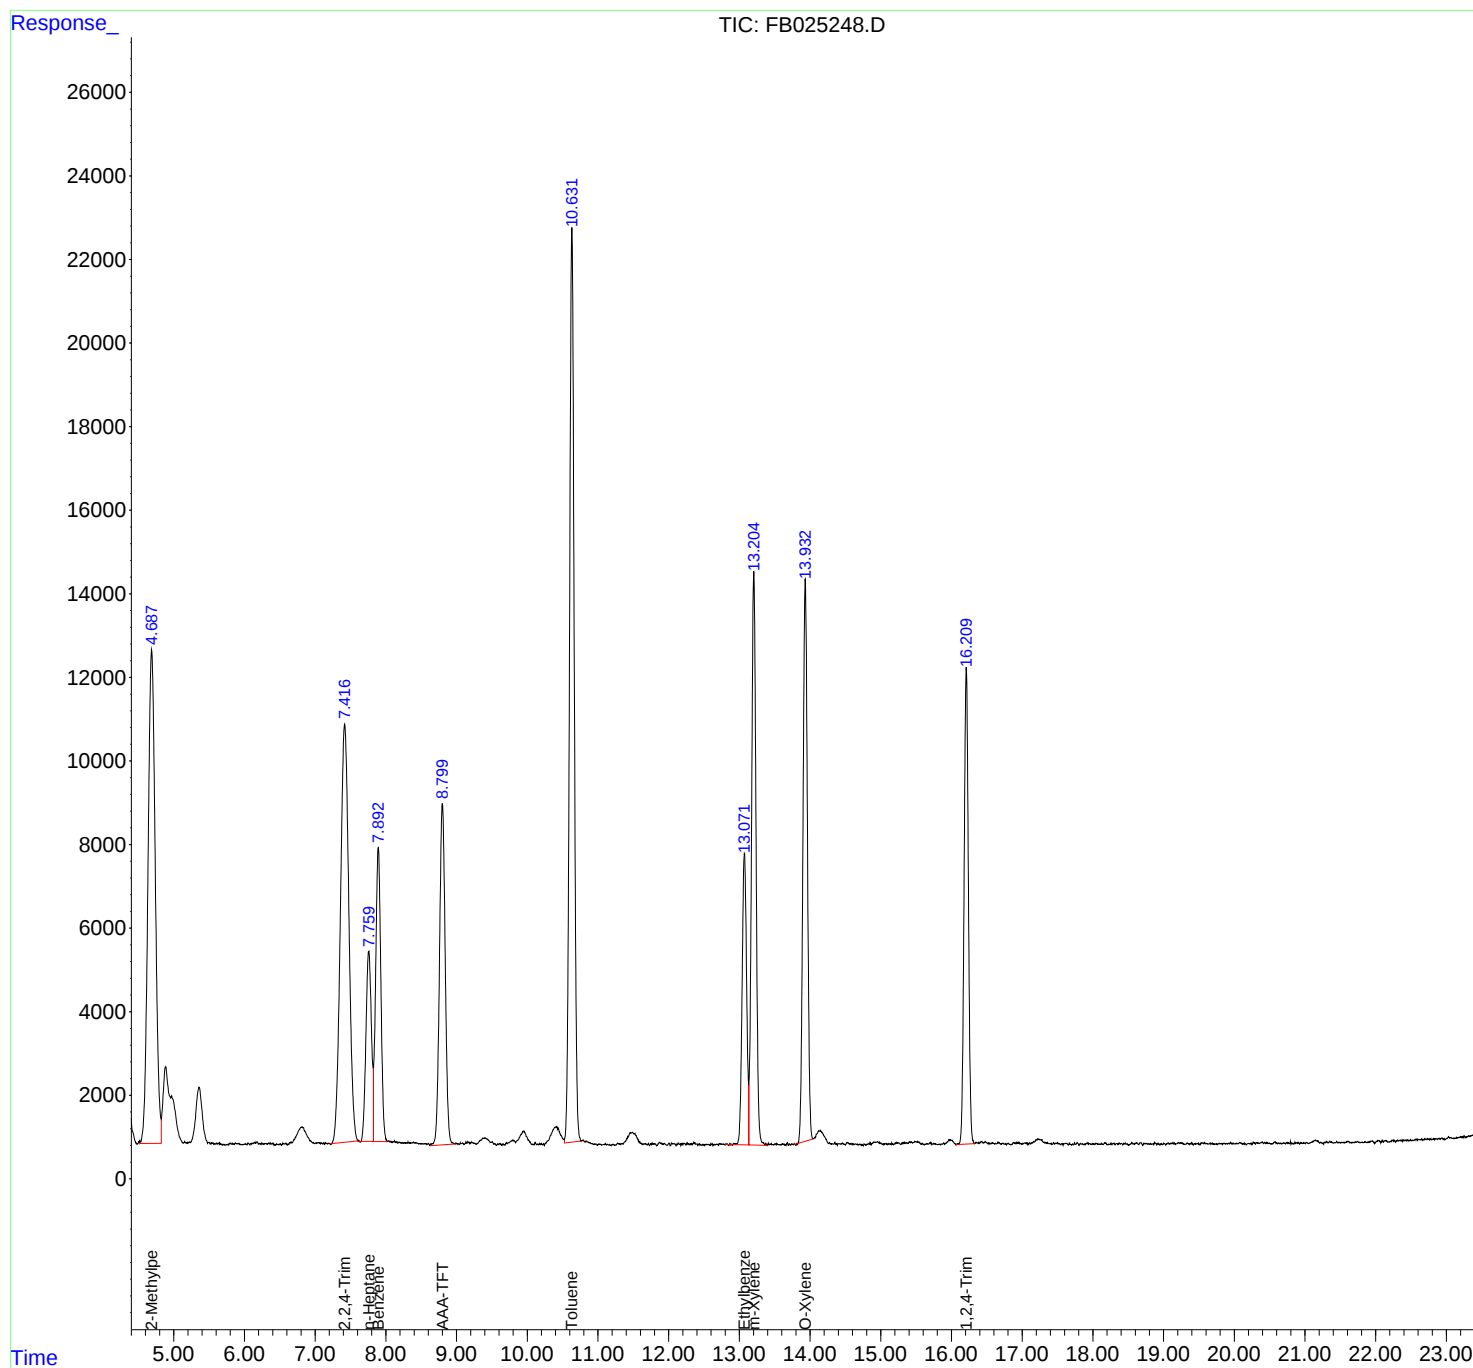

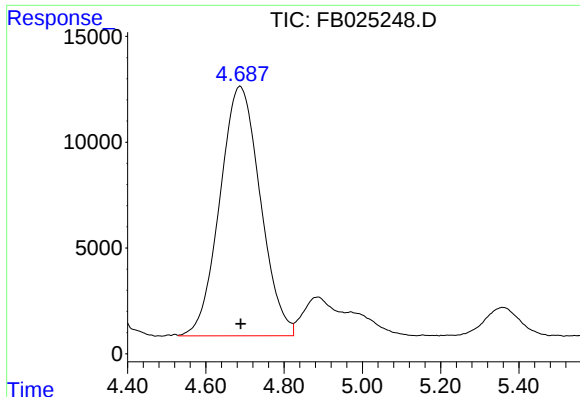


#1 2-Methylpentane

R.T.: 4.688 min
Delta R.T.: 0.000 min
Response: 846769
Conc: 26.23 ng/ml

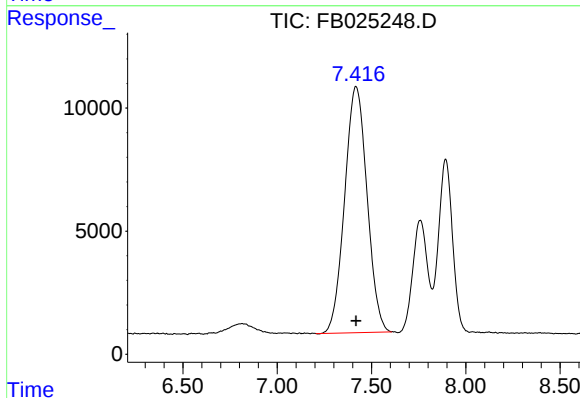


#2 2,2,4-Trimethylpentane

R.T.: 7.417 min
Delta R.T.: 0.000 min
Response: 825633
Conc: 24.88 ng/ml

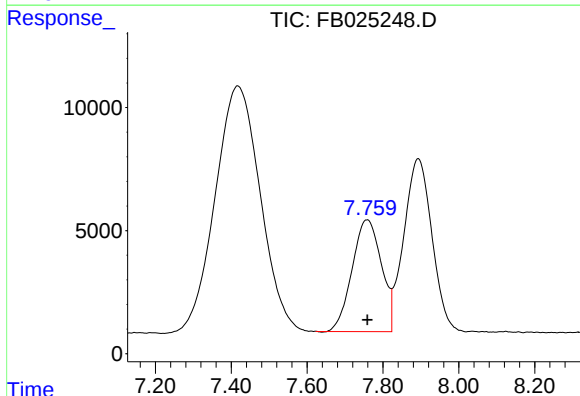


#3 n-Heptane

R.T.: 7.760 min
Delta R.T.: 0.000 min
Response: 244019
Conc: 7.43 ng/ml

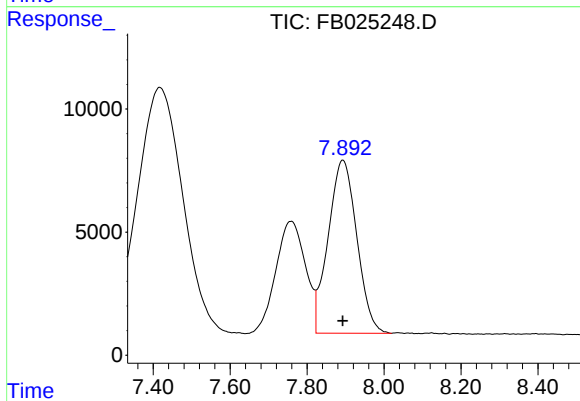


#4 Benzene

R.T.: 7.894 min
Delta R.T.: 0.000 min
Response: 363157
Conc: 9.13 ng/ml

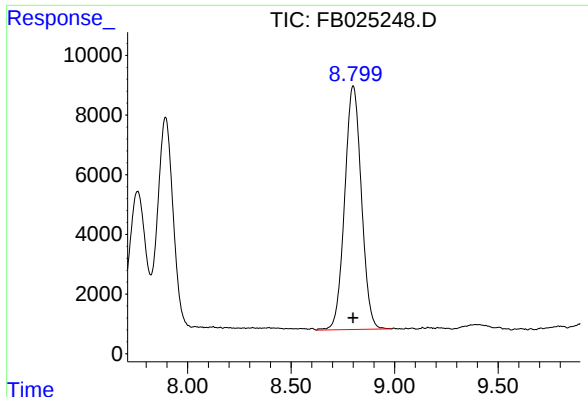


#5 AAA-TFT

R.T.: 8.800 min
Delta R.T.: 0.000 min
Response: 458220
Conc: 20.29 ng/ml

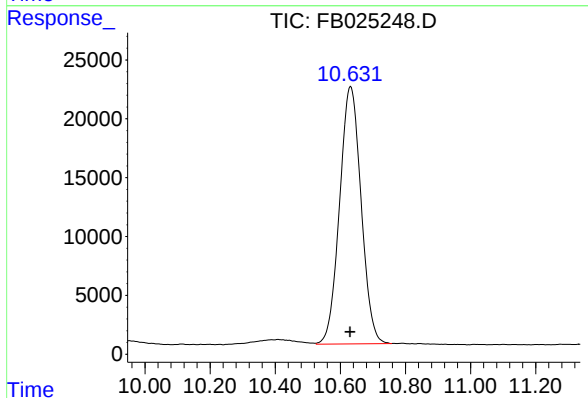


#6 Toluene

R.T.: 10.632 min
Delta R.T.: 0.002 min
Response: 1002207
Conc: 26.80 ng/ml

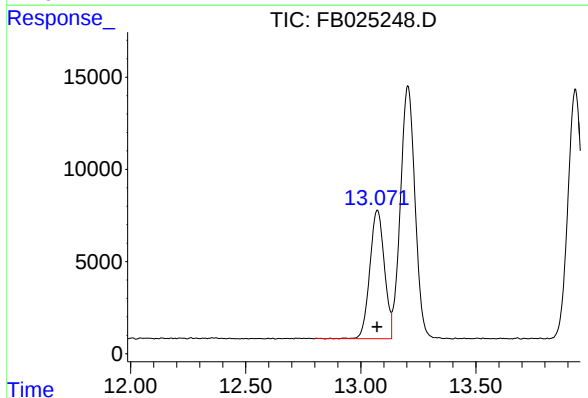


#7 Ethylbenzene

R.T.: 13.072 min
Delta R.T.: 0.002 min
Response: 305568
Conc: 8.90 ng/ml

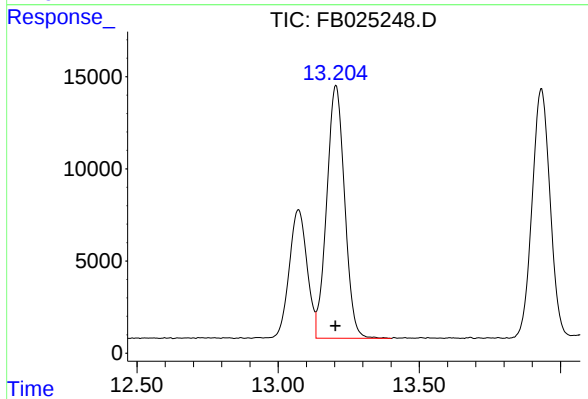

#8 m-Xylene

R.T.: 13.205 min
Delta R.T.: 0.002 min
Response: 606067
Conc: 17.95 ng/ml

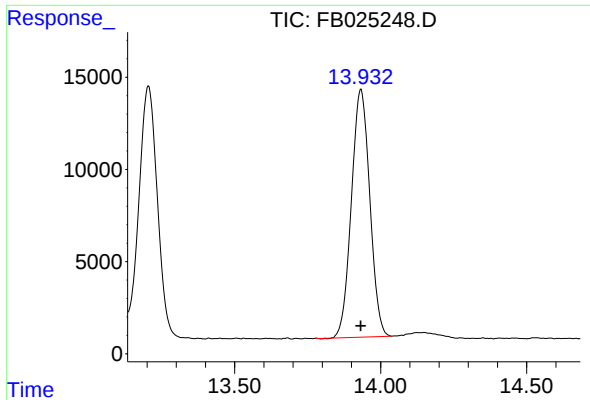


#9 O-Xylene

R.T.: 13.933 min

Delta R.T.: 0.001 min

Response: 587556

Conc: 17.97 ng/ml

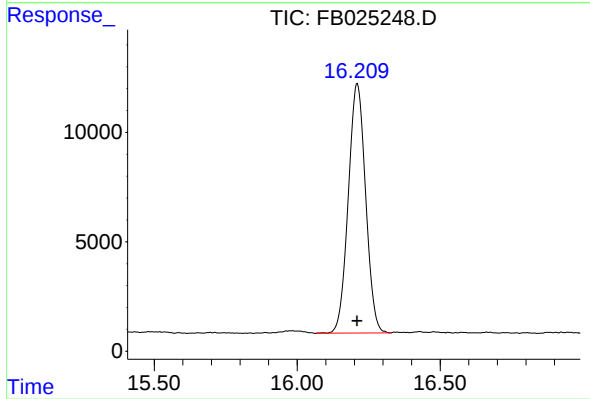

#10 1,2,4-Trimethylbenzene

R.T.: 16.210 min

Delta R.T.: 0.002 min

Response: 480048

Conc: 17.45 ng/ml