

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111418\
 Data File : FB018773.D
 Signal(s) : FID2B.CH
 Acq On : 14 Nov 2018 13:15
 Operator : MJ/SJ
 Sample : VBF1114S2
 Misc : 5.00g/5.00ml DI WATER
 ALS Vial : 5 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Nov 14 17:05:16 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110918.M
 Quant Title :
 QLast Update : Fri Nov 09 10:53:13 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.111	157529	18.263 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.957	5801	0.397 ng/ml
2) t 2,2,4-Trimethylpentane	7.712	804	0.055 ng/ml
3) t n-Heptane	8.051	2535	0.176 ng/ml
4) t Benzene	8.211	10854	0.599 ng/ml
6) t Toluene	10.958	69053	4.566 ng/ml
7) t Ethylbenzene	13.417	12888	0.826 ng/ml
8) t m-Xylene	13.539	57003	3.431 ng/ml
9) t O-Xylene	14.272	23912	1.394 ng/ml
10) t 1,2,4-Trimethylbenzene	16.555	25569	1.289 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111418\
Data File : FB018773.D
Signal(s) : FID2B.CH
Acq On : 14 Nov 2018 13:15
Operator : MJ/SJ
Sample : VBF1114S2
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 5 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Nov 14 17:05:16 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110918.M
Quant Title :
QLast Update : Fri Nov 09 10:53:13 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

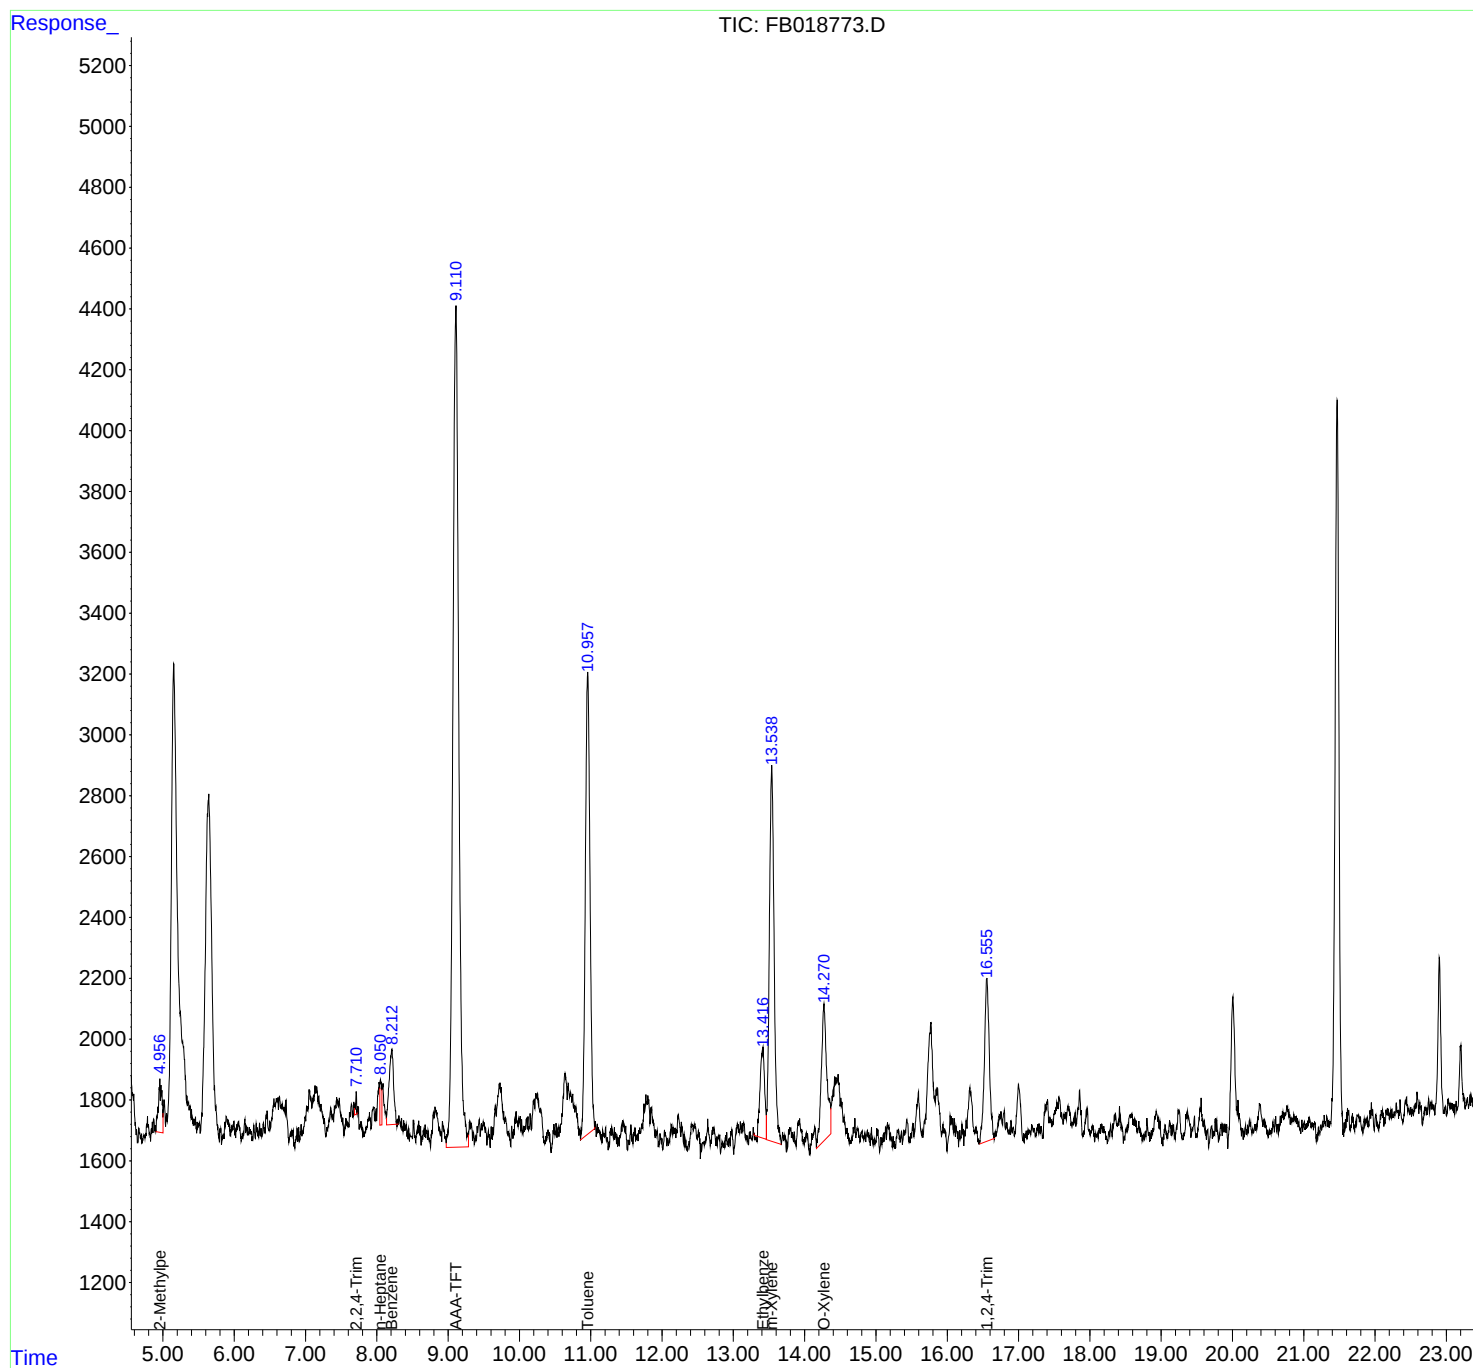

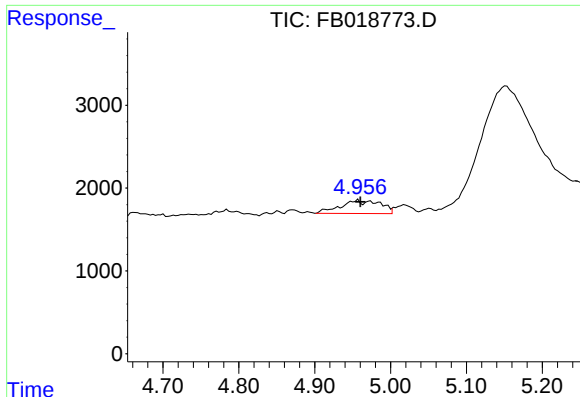


#1 2-Methylpentane

R.T.: 4.957 min
Delta R.T.: -0.003 min
Response: 5801
Conc: 0.40 ng/ml

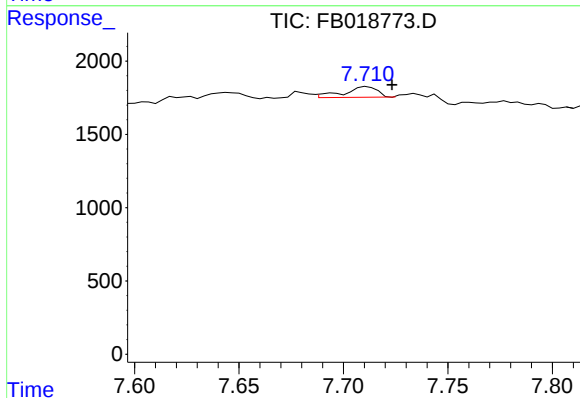


#2 2,2,4-Trimethylpentane

R.T.: 7.712 min
Delta R.T.: -0.011 min
Response: 804
Conc: 0.05 ng/ml

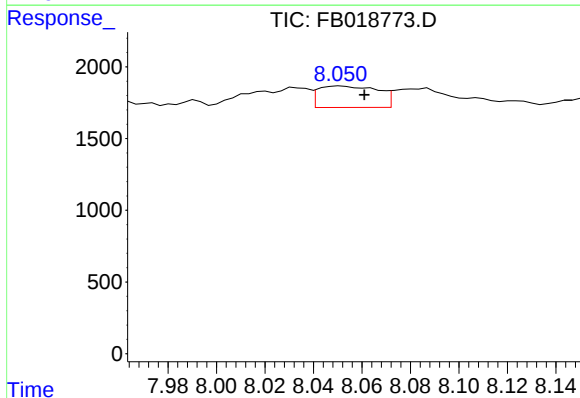


#3 n-Heptane

R.T.: 8.051 min
Delta R.T.: -0.010 min
Response: 2535
Conc: 0.18 ng/ml

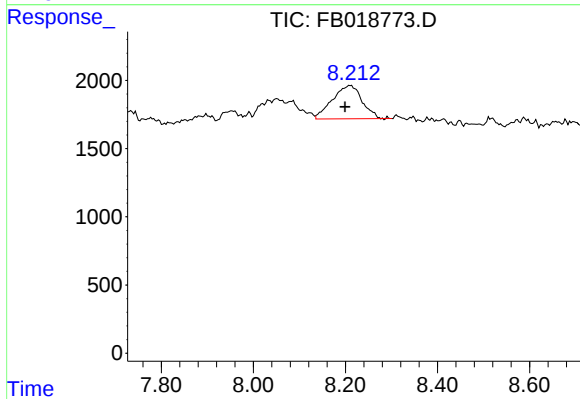


#4 Benzene

R.T.: 8.211 min
Delta R.T.: 0.012 min
Response: 10854
Conc: 0.60 ng/ml

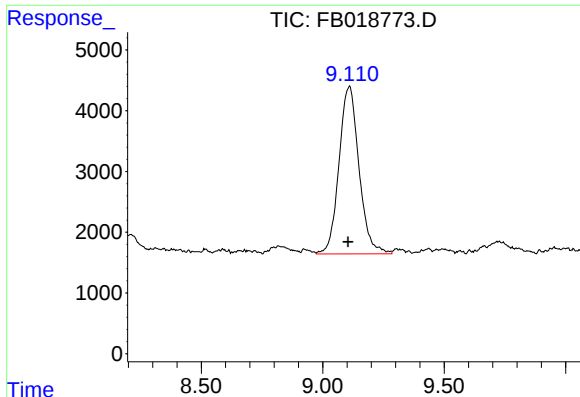


#5 AAA-TFT

R.T.: 9.111 min
Delta R.T.: 0.006 min
Response: 157529
Conc: 18.26 ng/ml

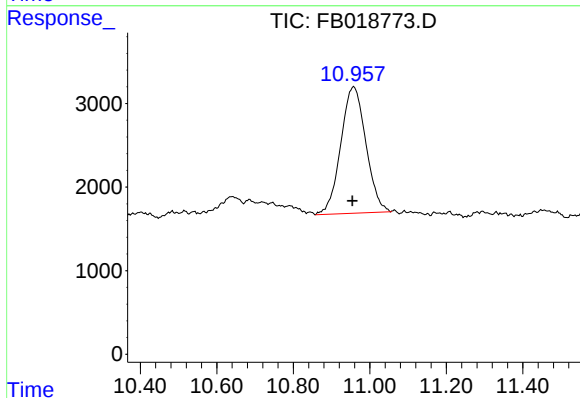


#6 Toluene

R.T.: 10.958 min
Delta R.T.: 0.004 min
Response: 69053
Conc: 4.57 ng/ml

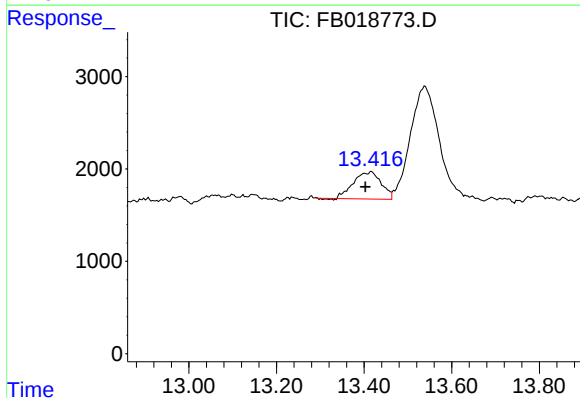


#7 Ethylbenzene

R.T.: 13.417 min
Delta R.T.: 0.014 min
Response: 12888
Conc: 0.83 ng/ml

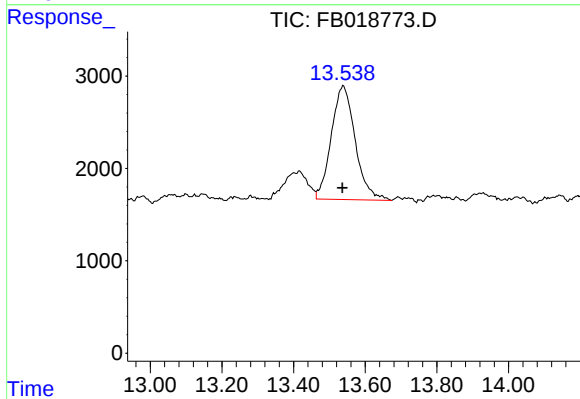


#8 m-Xylene

R.T.: 13.539 min
Delta R.T.: 0.003 min
Response: 57003
Conc: 3.43 ng/ml

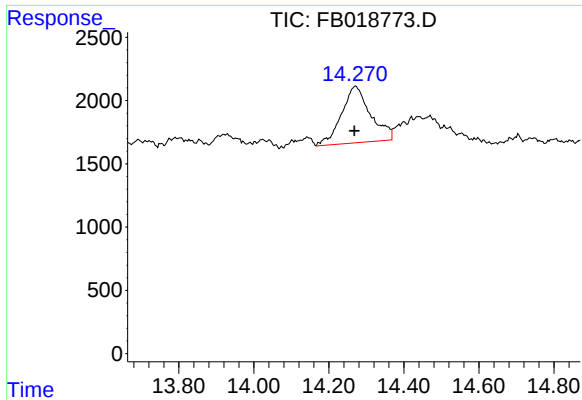

#9 O-Xylene

R.T.: 14.272 min
Delta R.T.: 0.004 min
Response: 23912
Conc: 1.39 ng/ml

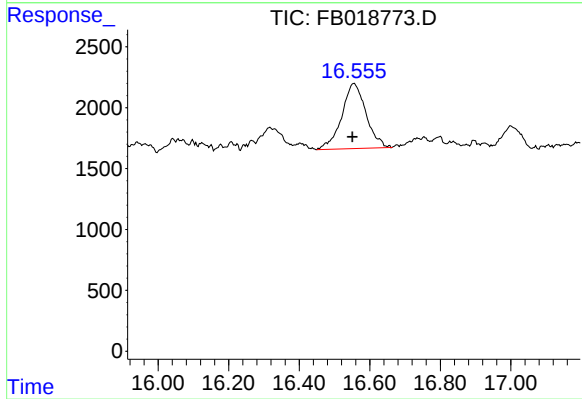

#10 1,2,4-Trimethylbenzene

R.T.: 16.555 min
Delta R.T.: 0.005 min
Response: 25569
Conc: 1.29 ng/ml