

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111419\
 Data File : FB022986.D
 Signal(s) : FID2B.CH
 Acq On : 14 Nov 2019 13:02
 Operator : DD/AJ
 Sample : BSF1114S1
 Misc : 5.04g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Nov 15 01:26:59 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB103119.M
 Quant Title :
 QLast Update : Thu Oct 31 14:57:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.798	469869	20.872 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.689	922992	28.693 ng/ml
2) t 2,2,4-Trimethylpentane	7.416	1041088	29.492 ng/ml
3) t n-Heptane	7.757	336975	9.687 ng/ml
4) t Benzene	7.891	431615	9.965 ng/ml
6) t Toluene	10.629	1261424	29.260 ng/ml
7) t Ethylbenzene	13.068	389578	9.758 ng/ml
8) t m-Xylene	13.202	732564	19.397 ng/ml
9) t O-Xylene	13.930	695874	19.525 ng/ml
10) t 1,2,4-Trimethylbenzene	16.208	589900	20.801 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111419\
Data File : FB022986.D
Signal(s) : FID2B.CH
Acq On : 14 Nov 2019 13:02
Operator : DD/AJ
Sample : BSF1114S1
Misc : 5.04g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Nov 15 01:26:59 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB103119.M
Quant Title :
QLast Update : Thu Oct 31 14:57:42 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

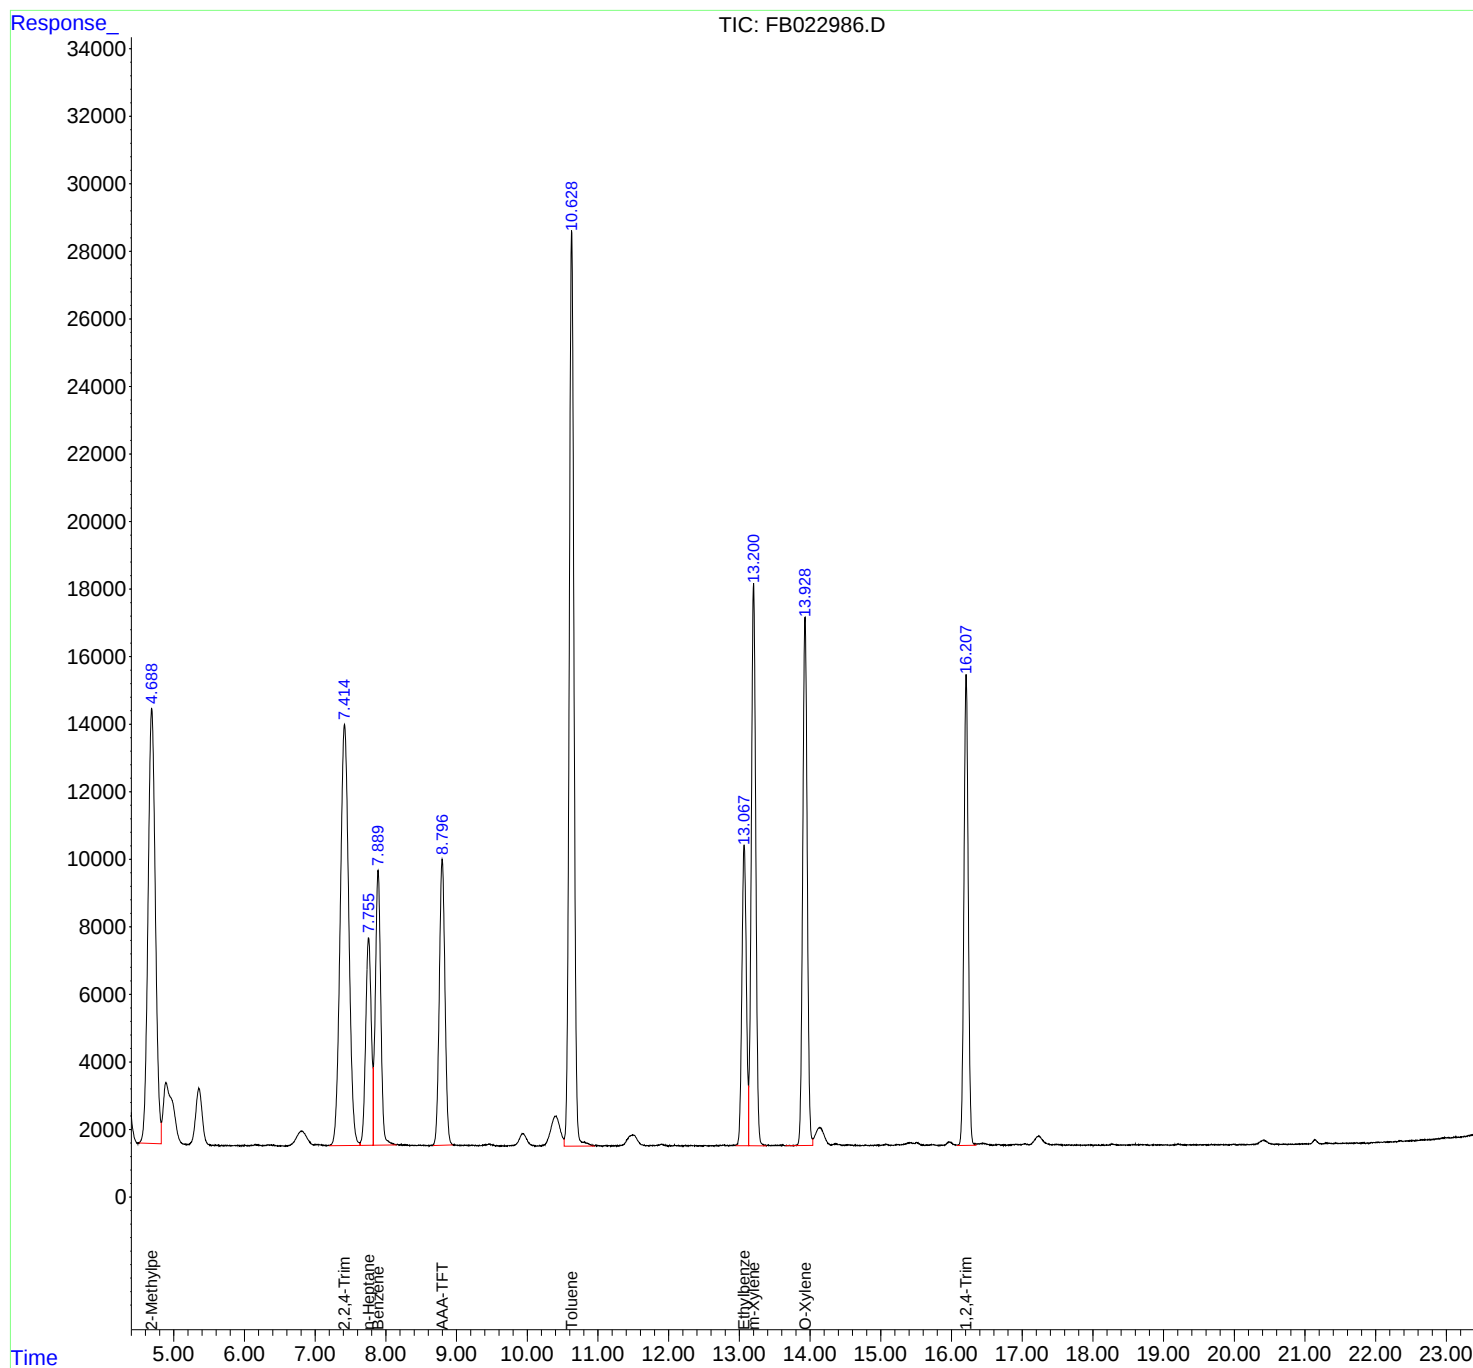

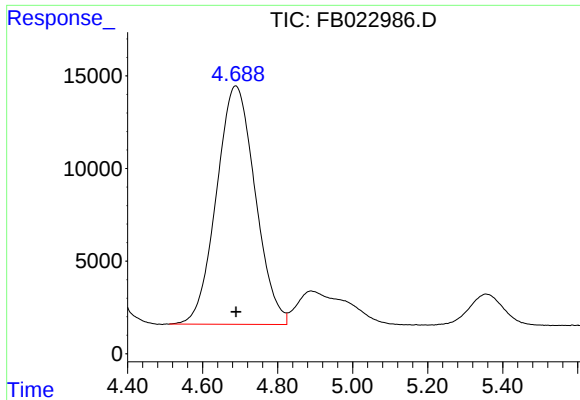


#1 2-Methylpentane

R.T.: 4.689 min
Delta R.T.: 0.000 min
Response: 922992
Conc: 28.69 ng/ml

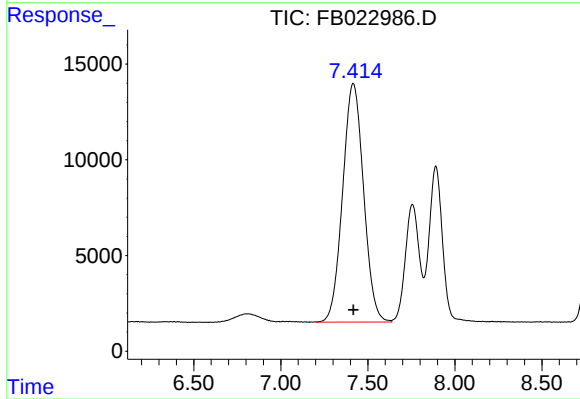


#2 2,2,4-Trimethylpentane

R.T.: 7.416 min
Delta R.T.: -0.002 min
Response: 1041088
Conc: 29.49 ng/ml

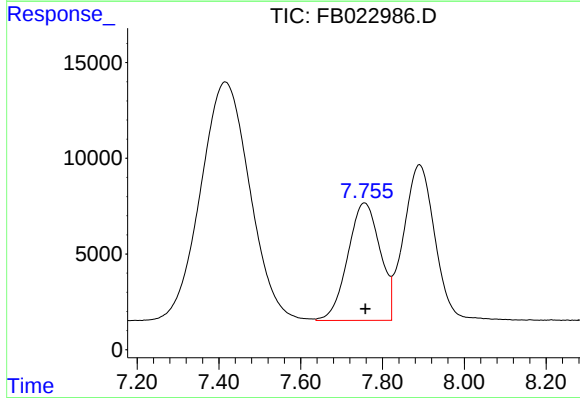


#3 n-Heptane

R.T.: 7.757 min
Delta R.T.: -0.002 min
Response: 336975
Conc: 9.69 ng/ml

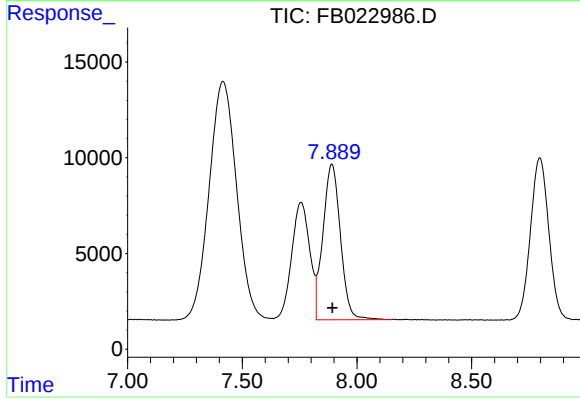


#4 Benzene

R.T.: 7.891 min
Delta R.T.: -0.002 min
Response: 431615
Conc: 9.96 ng/ml

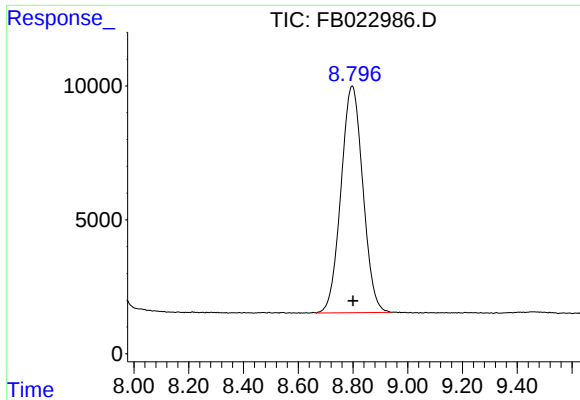


#5 AAA-TFT

R.T.: 8.798 min
Delta R.T.: -0.002 min
Response: 469869
Conc: 20.87 ng/ml

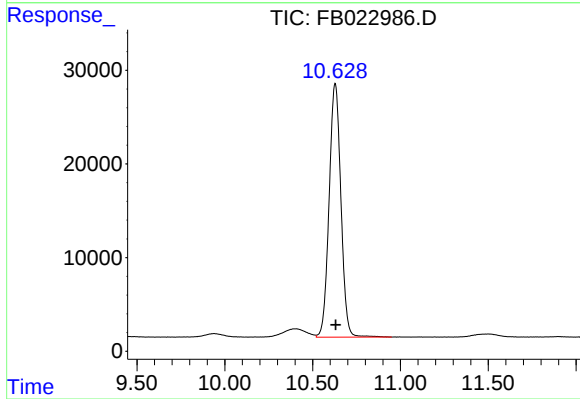


#6 Toluene

R.T.: 10.629 min
Delta R.T.: -0.003 min
Response: 1261424
Conc: 29.26 ng/ml

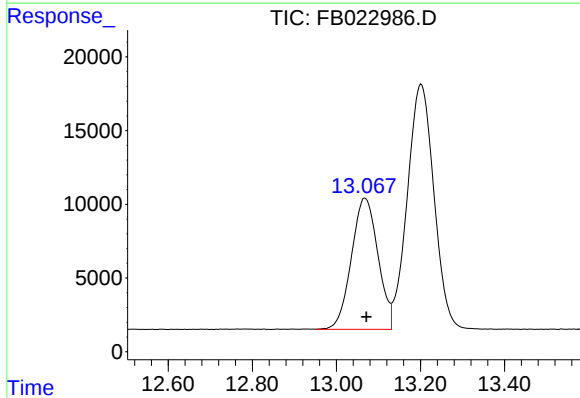


#7 Ethylbenzene

R.T.: 13.068 min
Delta R.T.: -0.004 min
Response: 389578
Conc: 9.76 ng/ml

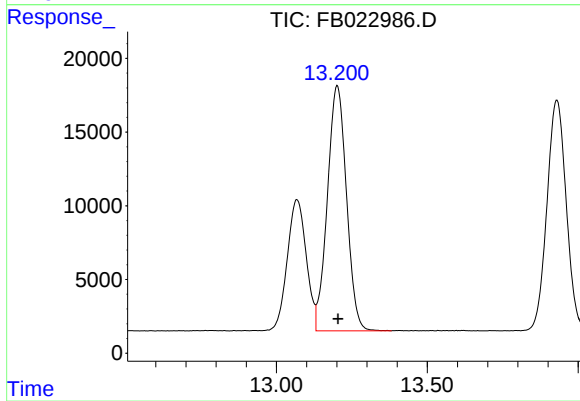


#8 m-Xylene

R.T.: 13.202 min
Delta R.T.: -0.003 min
Response: 732564
Conc: 19.40 ng/ml

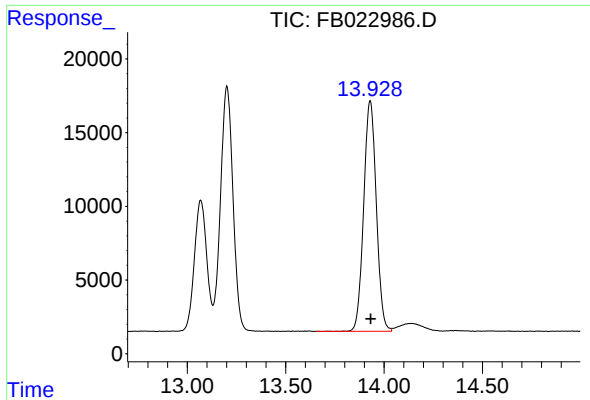

#9 O-Xylene

R.T.: 13.930 min
Delta R.T.: -0.003 min
Response: 695874
Conc: 19.52 ng/ml

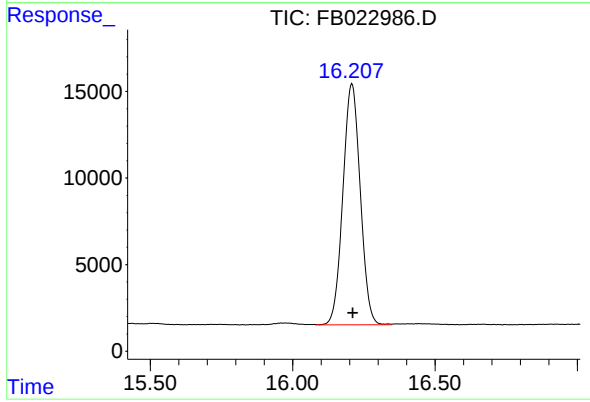

#10 1,2,4-Trimethylbenzene

R.T.: 16.208 min
Delta R.T.: -0.003 min
Response: 589900
Conc: 20.80 ng/ml