

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111419\
 Data File : FB022992.D
 Signal(s) : FID2B.CH
 Acq On : 14 Nov 2019 16:41
 Operator : DD/AJ
 Sample : K5668-06MSD
 Misc : 5.03g/5.00ml DI WATER
 ALS Vial : 9 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Nov 15 01:28:07 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB103119.M
 Quant Title :
 QLast Update : Thu Oct 31 14:57:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.796	460137	20.440 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.688	900985	28.009 ng/ml
2) t 2,2,4-Trimethylpentane	7.415	981696	27.810 ng/ml
3) t n-Heptane	7.755	307924	8.852 ng/ml
4) t Benzene	7.889	422270	9.749 ng/ml
6) t Toluene	10.628	1248465	28.960 ng/ml
7) t Ethylbenzene	13.068	395764	9.913 ng/ml
8) t m-Xylene	13.201	704551	18.655 ng/ml
9) t O-Xylene	13.929	700582	19.657 ng/ml
10) t 1,2,4-Trimethylbenzene	16.208	542849	19.142 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111419\
Data File : FB022992.D
Signal(s) : FID2B.CH
Acq On : 14 Nov 2019 16:41
Operator : DD/AJ
Sample : K5668-06MSD
Misc : 5.03g/5.00ml DI WATER
ALS Vial : 9 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Nov 15 01:28:07 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB103119.M
Quant Title :
QLast Update : Thu Oct 31 14:57:42 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

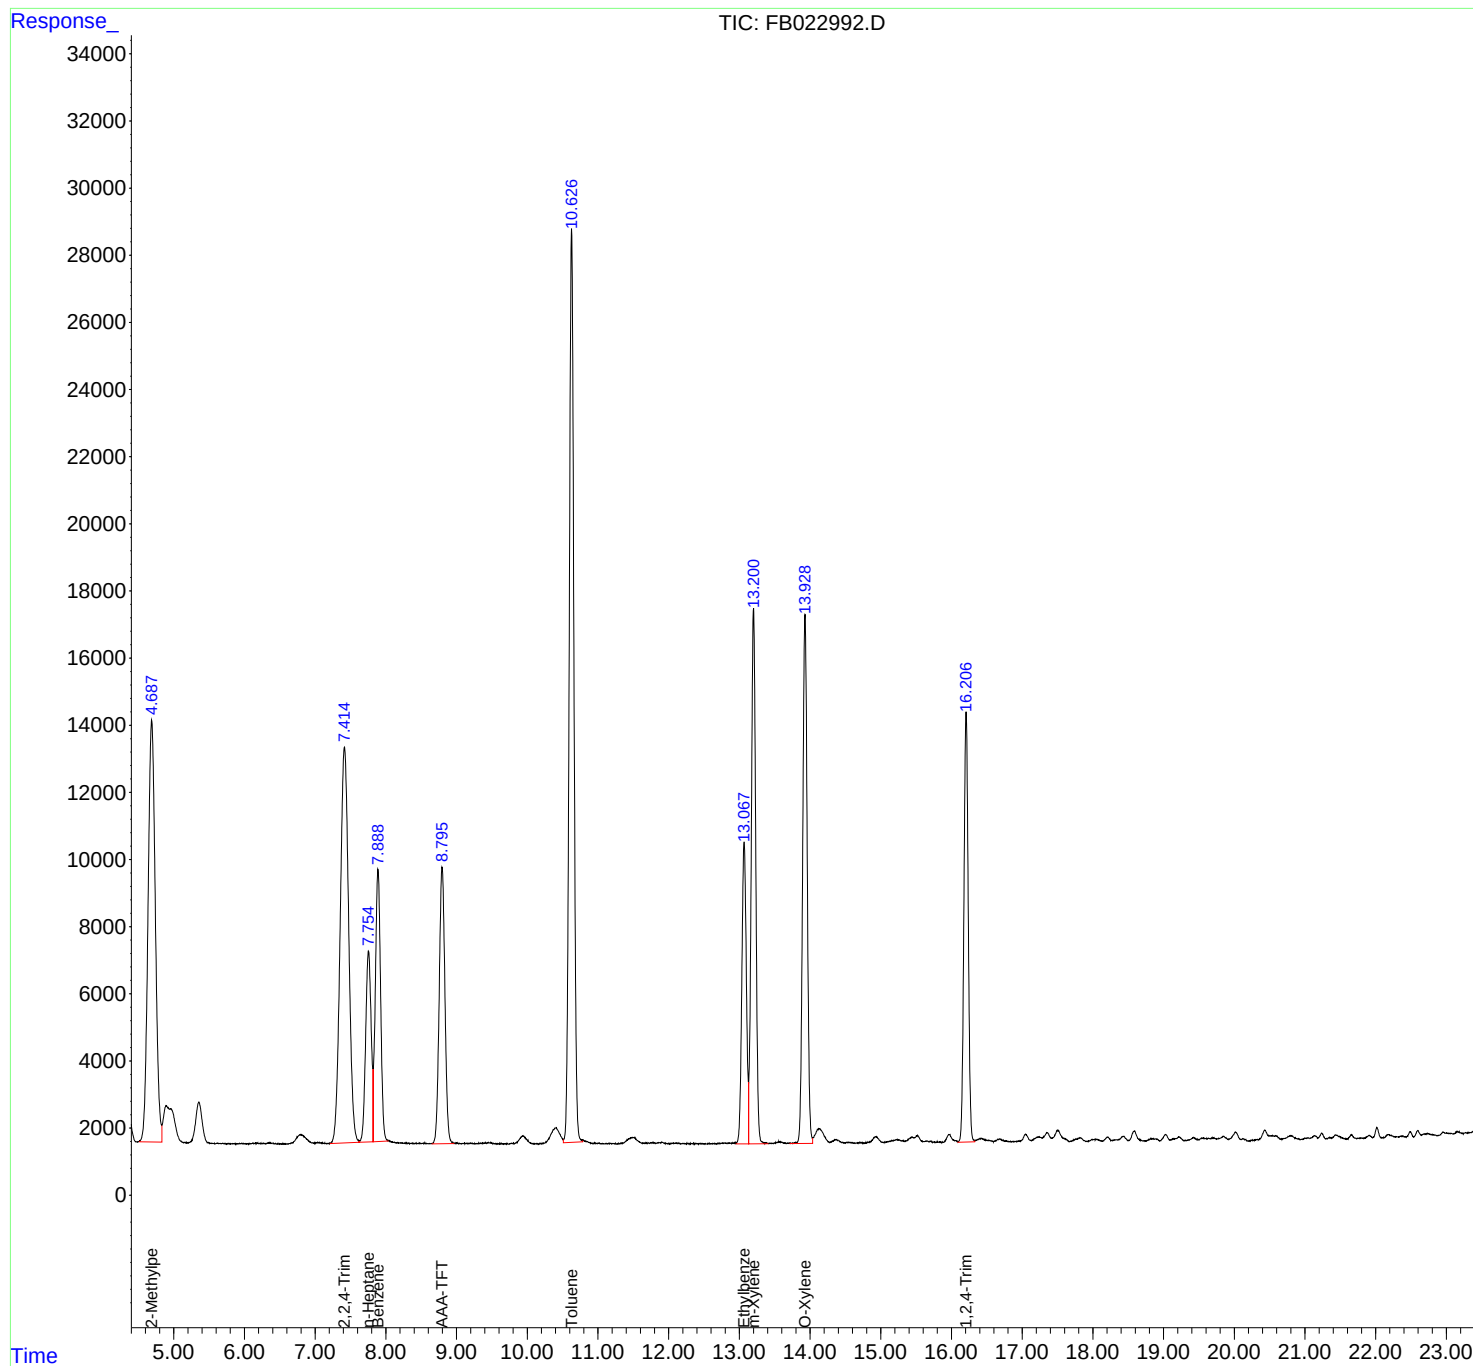

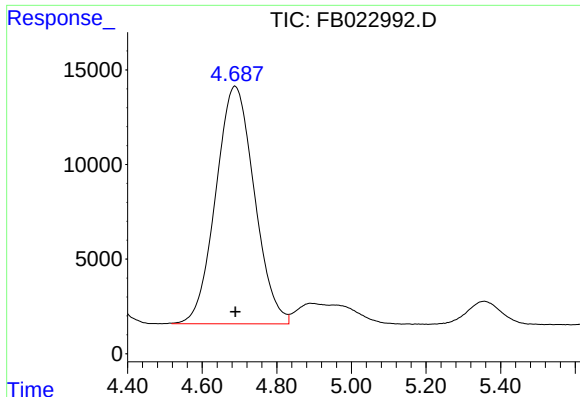


#1 2-Methylpentane

R.T.: 4.688 min
Delta R.T.: 0.000 min
Response: 900985
Conc: 28.01 ng/ml

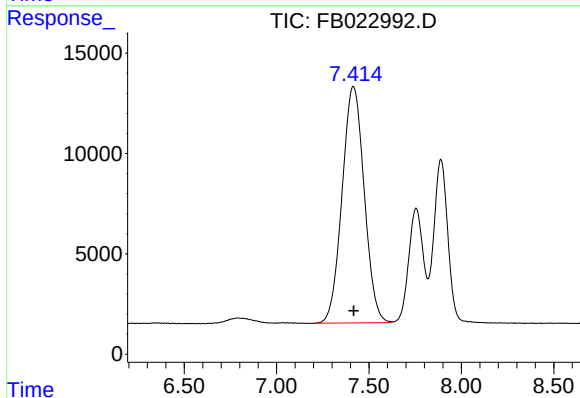


#2 2,2,4-Trimethylpentane

R.T.: 7.415 min
Delta R.T.: -0.003 min
Response: 981696
Conc: 27.81 ng/ml

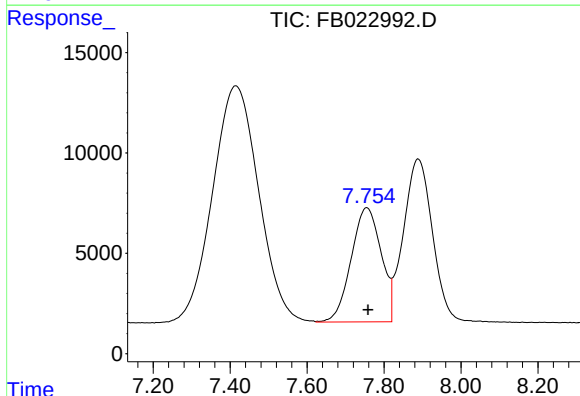


#3 n-Heptane

R.T.: 7.755 min
Delta R.T.: -0.003 min
Response: 307924
Conc: 8.85 ng/ml

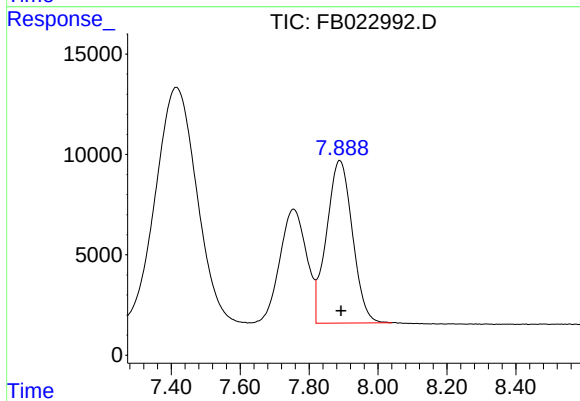


#4 Benzene

R.T.: 7.889 min
Delta R.T.: -0.004 min
Response: 422270
Conc: 9.75 ng/ml

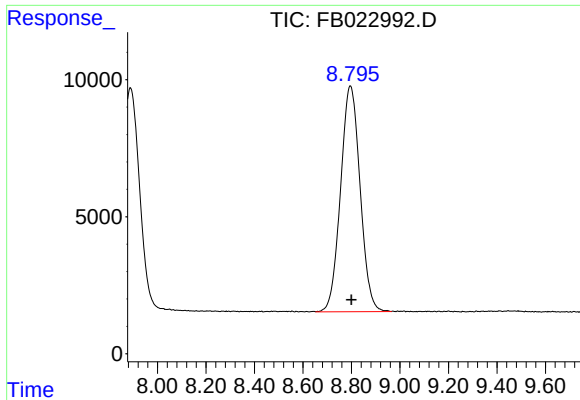


#5 AAA-TFT

R.T.: 8.796 min
Delta R.T.: -0.003 min
Response: 460137
Conc: 20.44 ng/ml

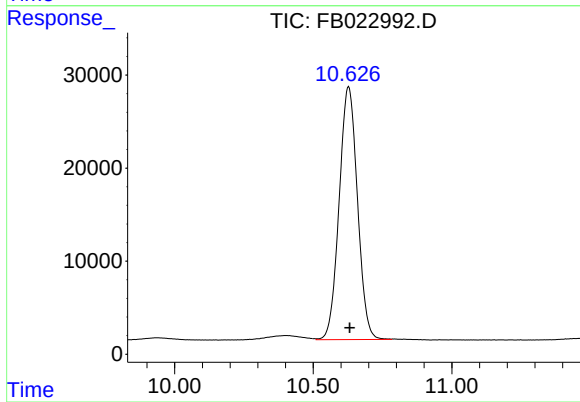


#6 Toluene

R.T.: 10.628 min
Delta R.T.: -0.004 min
Response: 1248465
Conc: 28.96 ng/ml

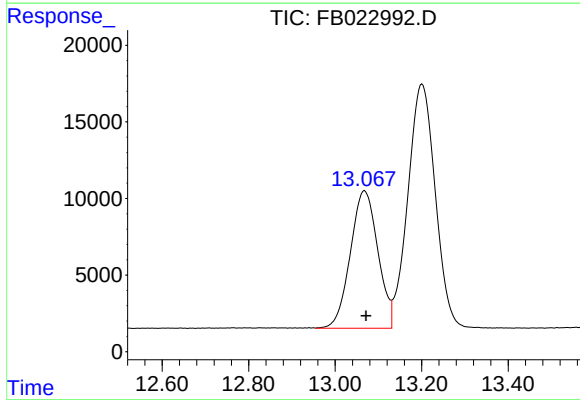


#7 Ethylbenzene

R.T.: 13.068 min
Delta R.T.: -0.004 min
Response: 395764
Conc: 9.91 ng/ml

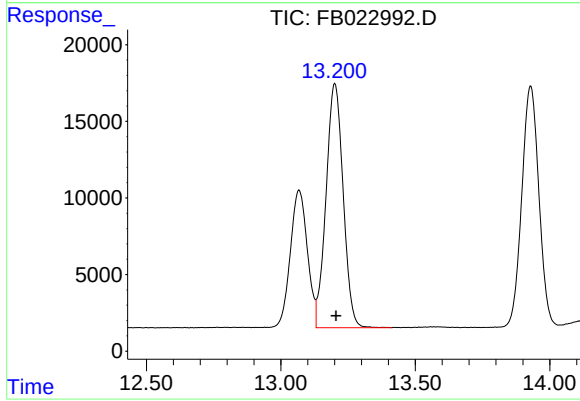


#8 m-Xylene

R.T.: 13.201 min
Delta R.T.: -0.004 min
Response: 704551
Conc: 18.66 ng/ml

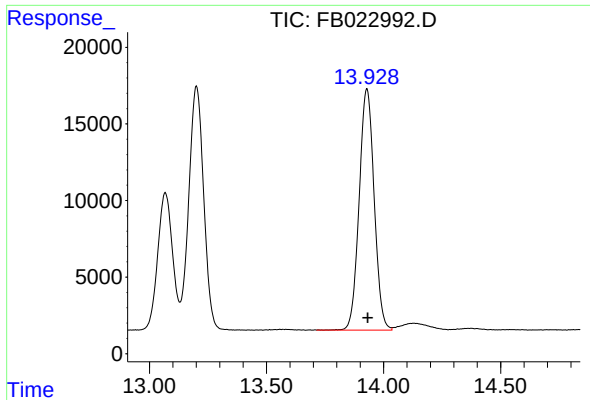

#9 O-Xylene

R.T.: 13.929 min
Delta R.T.: -0.003 min
Response: 700582
Conc: 19.66 ng/ml

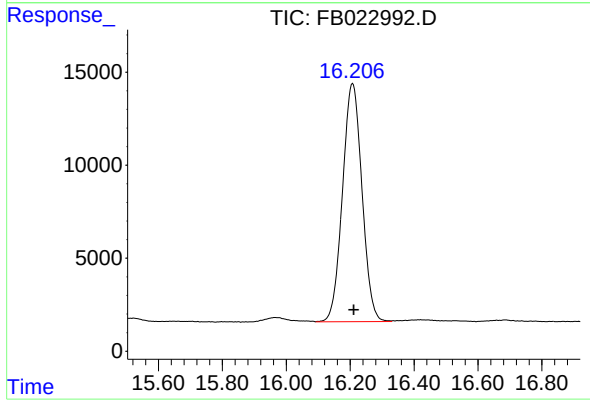

#10 1,2,4-Trimethylbenzene

R.T.: 16.208 min
Delta R.T.: -0.003 min
Response: 542849
Conc: 19.14 ng/ml