

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111419\
 Data File : FB022995.D
 Signal(s) : FID2B.CH
 Acq On : 14 Nov 2019 18:11
 Operator : DD/AJ
 Sample : IDOC-WATER-02
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Nov 15 00:45:28 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB103119.M
 Quant Title :
 QLast Update : Thu Oct 31 14:57:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.796	485065	21.547 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.688	937272	29.137 ng/ml
2) t	2,2,4-Trimethylpentane	7.416	1084913	30.734 ng/ml
3) t	n-Heptane	7.756	348756	10.026 ng/ml
4) t	Benzene	7.890	441838	10.201 ng/ml
6) t	Toluene	10.627	1311432	30.420 ng/ml
7) t	Ethylbenzene	13.067	403440	10.106 ng/ml
8) t	m-Xylene	13.201	755922	20.015 ng/ml
9) t	O-Xylene	13.928	715821	20.084 ng/ml
10) t	1,2,4-Trimethylbenzene	16.207	599071	21.125 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111419\
Data File : FB022995.D
Signal(s) : FID2B.CH
Acq On : 14 Nov 2019 18:11
Operator : DD/AJ
Sample : IDOC-WATER-02
Misc :
ALS Vial : 12 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Nov 15 00:45:28 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB103119.M
Quant Title :
QLast Update : Thu Oct 31 14:57:42 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

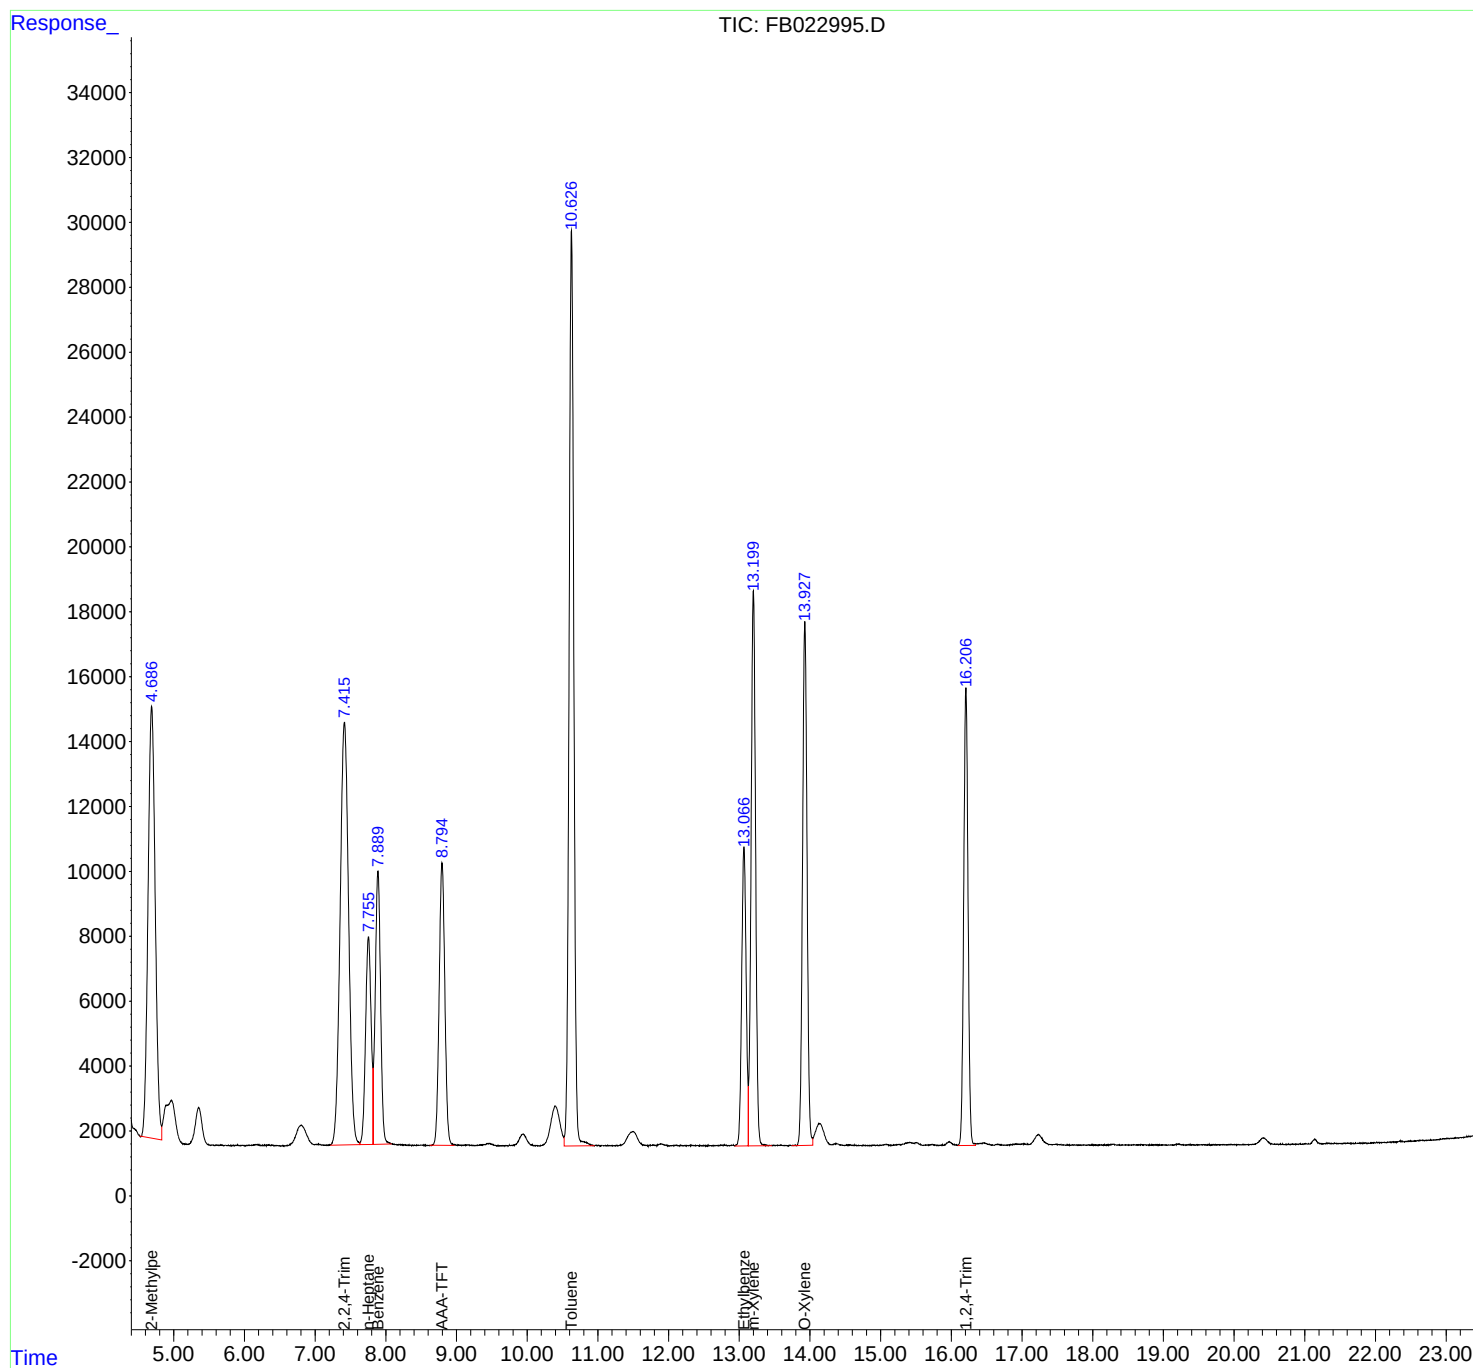

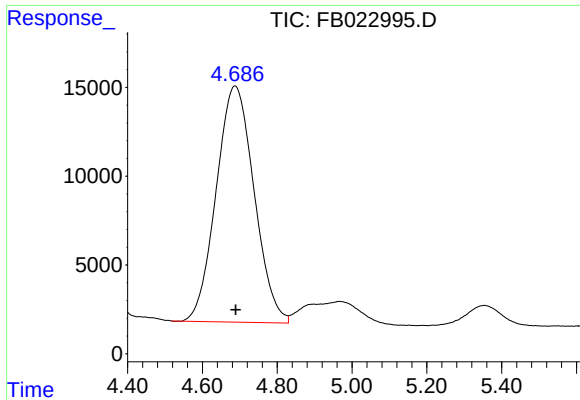


#1 2-Methylpentane

R.T.: 4.688 min
Delta R.T.: -0.001 min
Response: 937272
Conc: 29.14 ng/ml

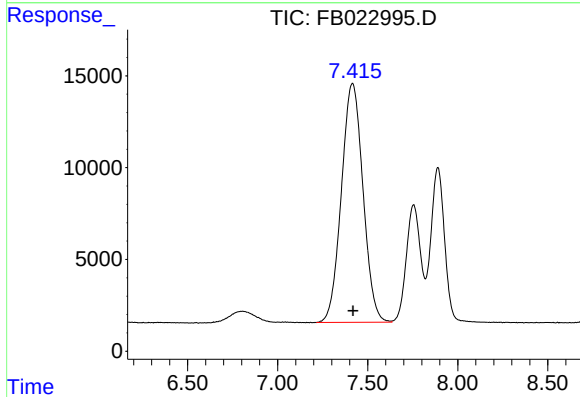


#2 2,2,4-Trimethylpentane

R.T.: 7.416 min
Delta R.T.: -0.002 min
Response: 1084913
Conc: 30.73 ng/ml

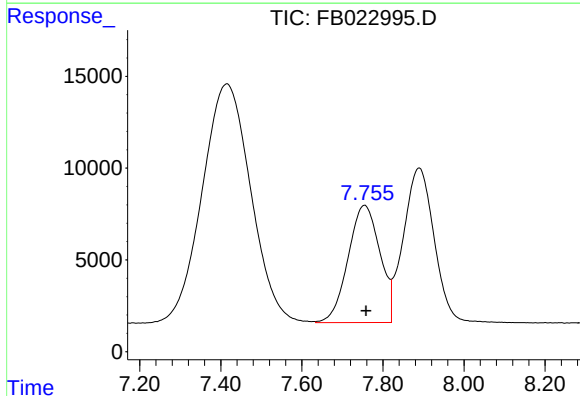


#3 n-Heptane

R.T.: 7.756 min
Delta R.T.: -0.003 min
Response: 348756
Conc: 10.03 ng/ml

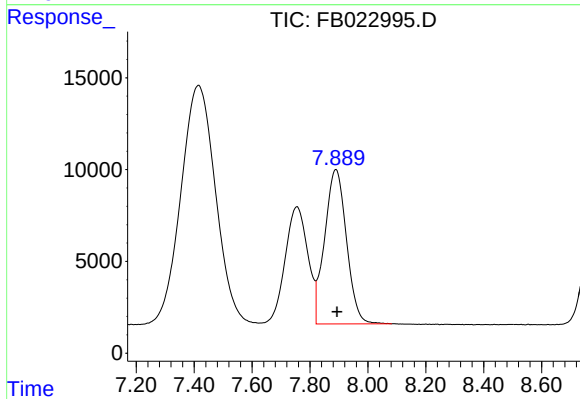


#4 Benzene

R.T.: 7.890 min
Delta R.T.: -0.003 min
Response: 441838
Conc: 10.20 ng/ml

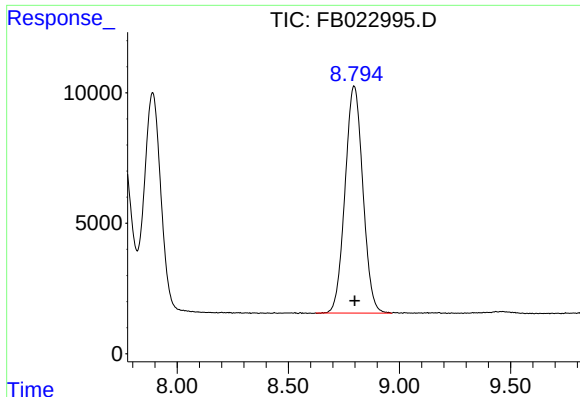


#5 AAA-TFT

R.T.: 8.796 min
Delta R.T.: -0.003 min
Response: 485065
Conc: 21.55 ng/ml

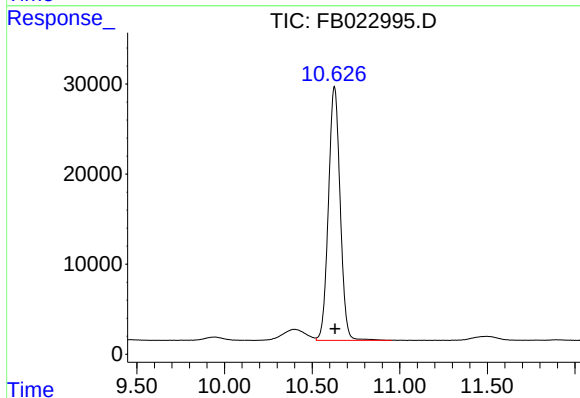


#6 Toluene

R.T.: 10.627 min
Delta R.T.: -0.004 min
Response: 1311432
Conc: 30.42 ng/ml

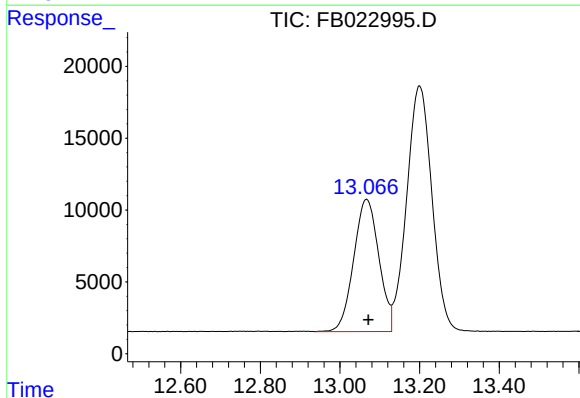


#7 Ethylbenzene

R.T.: 13.067 min
Delta R.T.: -0.004 min
Response: 403440
Conc: 10.11 ng/ml

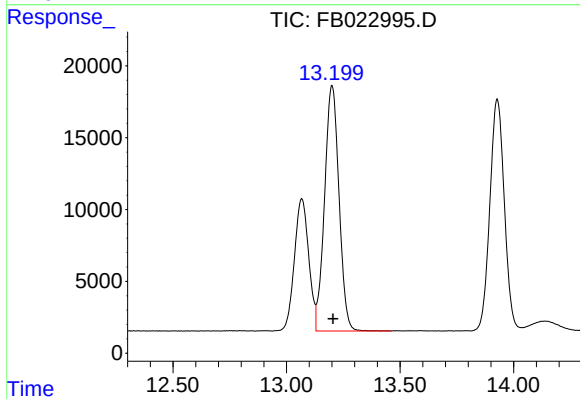


#8 m-Xylene

R.T.: 13.201 min
Delta R.T.: -0.004 min
Response: 755922
Conc: 20.02 ng/ml

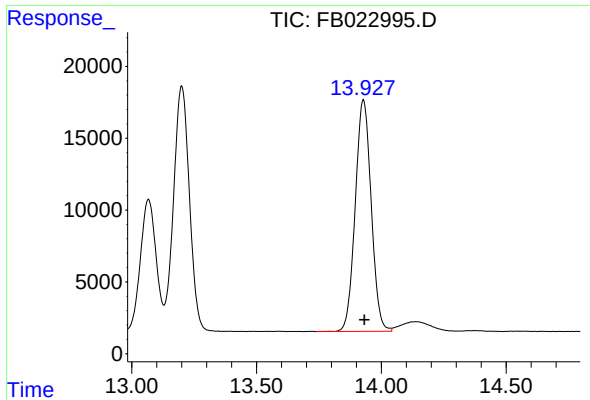

#9 O-Xylene

R.T.: 13.928 min
Delta R.T.: -0.004 min
Response: 715821
Conc: 20.08 ng/ml

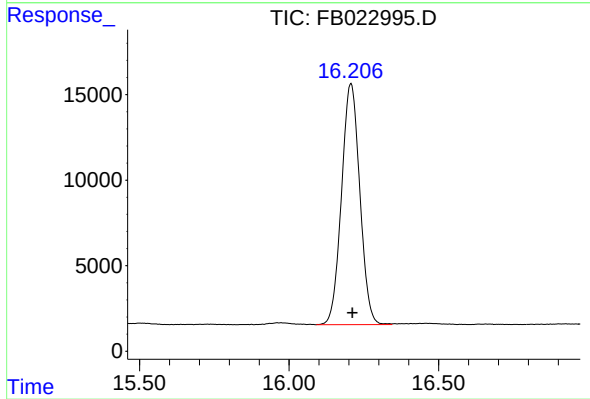

#10 1,2,4-Trimethylbenzene

R.T.: 16.207 min
Delta R.T.: -0.004 min
Response: 599071
Conc: 21.12 ng/ml