

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111419\
 Data File : FB022997.D
 Signal(s) : FID2B.CH
 Acq On : 14 Nov 2019 19:11
 Operator : DD/AJ
 Sample : IDOC-WATER-04
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Nov 15 00:45:49 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB103119.M
 Quant Title :
 QLast Update : Thu Oct 31 14:57:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.796	444231	19.733 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.686	821621	25.542 ng/ml
2) t 2,2,4-Trimethylpentane	7.414	956708	27.102 ng/ml
3) t n-Heptane	7.754	303729	8.732 ng/ml
4) t Benzene	7.889	401969	9.280 ng/ml
6) t Toluene	10.627	1209402	28.054 ng/ml
7) t Ethylbenzene	13.067	384312	9.626 ng/ml
8) t m-Xylene	13.200	735120	19.464 ng/ml
9) t O-Xylene	13.928	704338	19.762 ng/ml
10) t 1,2,4-Trimethylbenzene	16.207	590374	20.818 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111419\
Data File : FB022997.D
Signal(s) : FID2B.CH
Acq On : 14 Nov 2019 19:11
Operator : DD/AJ
Sample : IDOC-WATER-04
Misc :
ALS Vial : 14 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Nov 15 00:45:49 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB103119.M
Quant Title :
QLast Update : Thu Oct 31 14:57:42 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

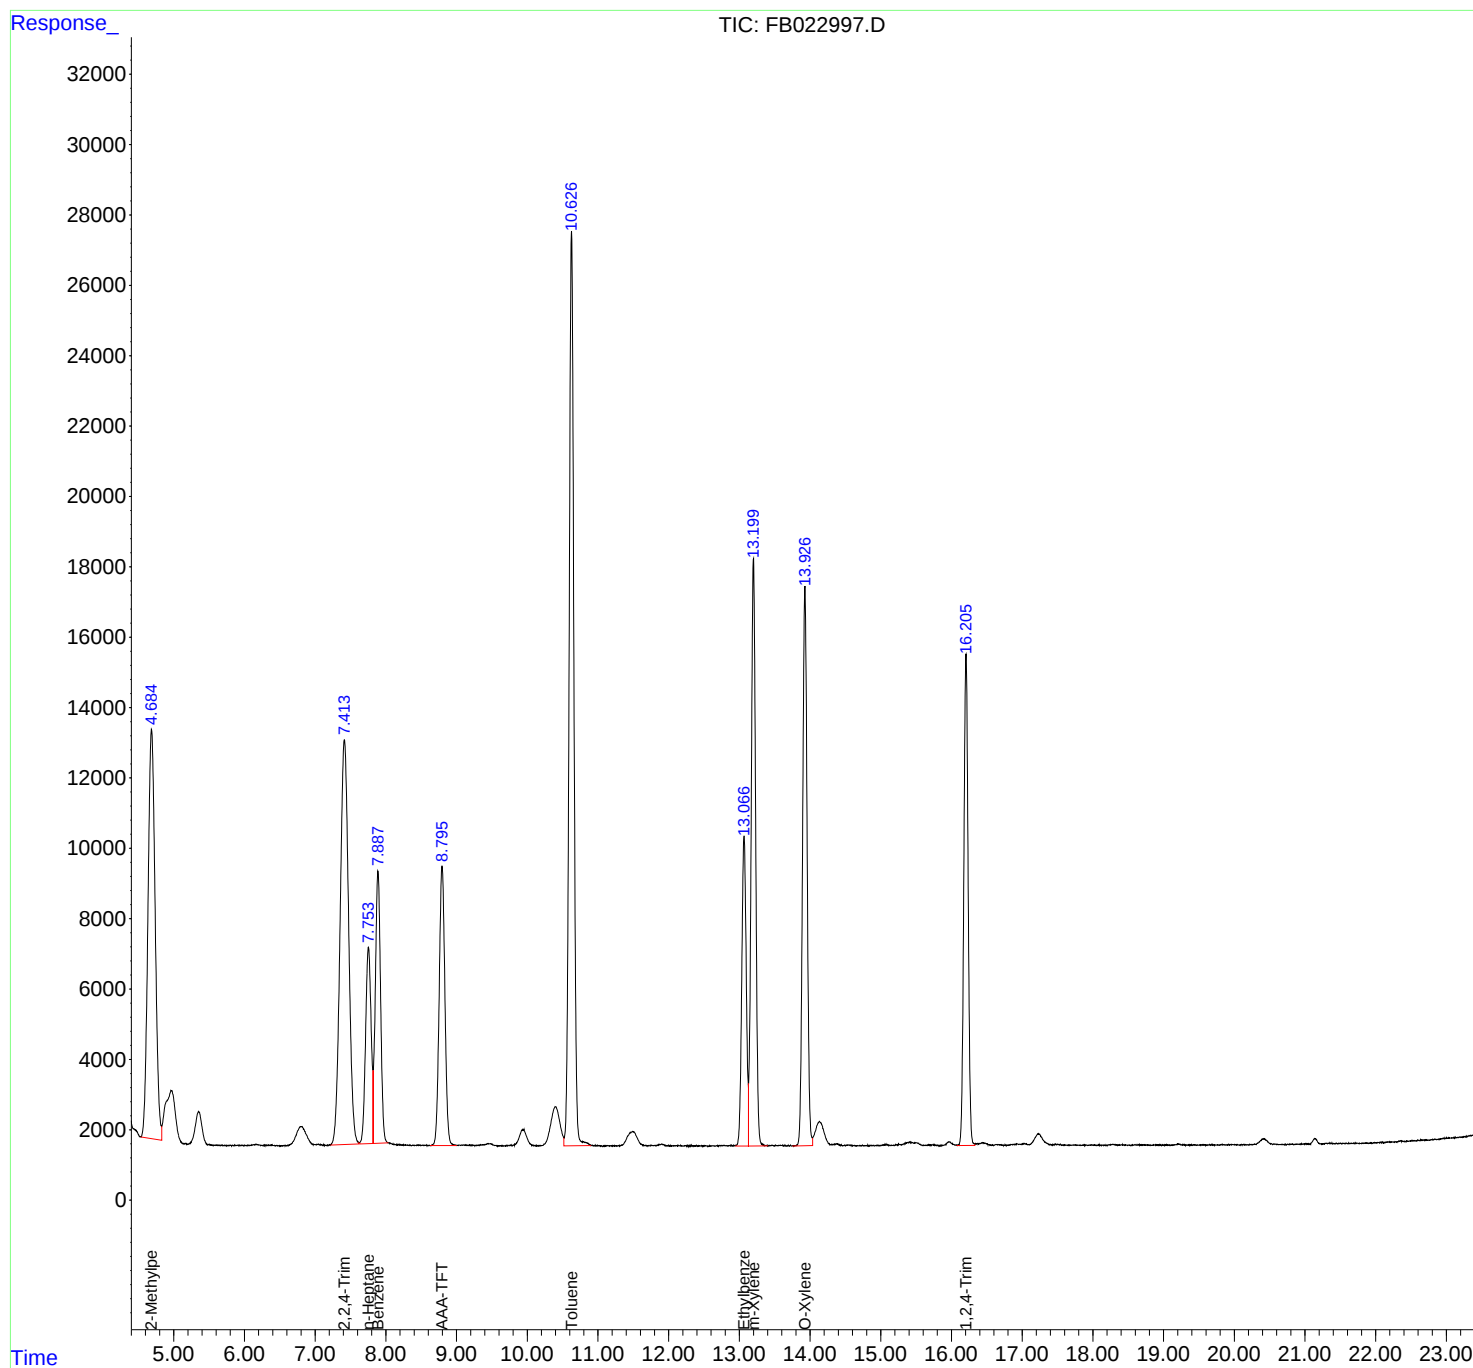

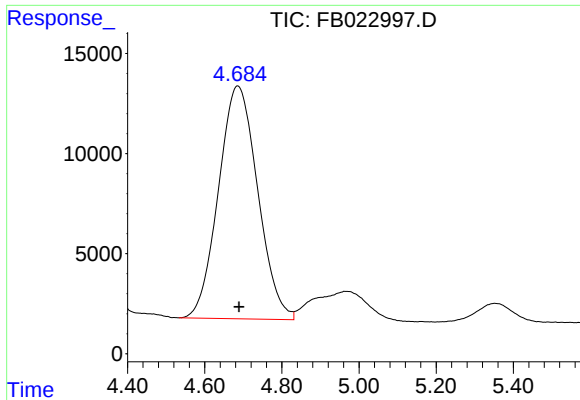


#1 2-Methylpentane

R.T.: 4.686 min
Delta R.T.: -0.003 min
Response: 821621
Conc: 25.54 ng/ml

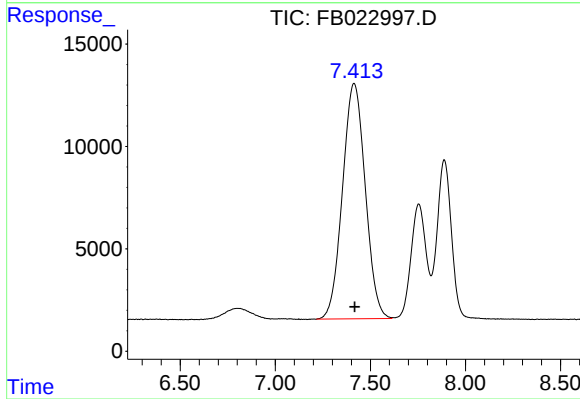


#2 2,2,4-Trimethylpentane

R.T.: 7.414 min
Delta R.T.: -0.004 min
Response: 956708
Conc: 27.10 ng/ml

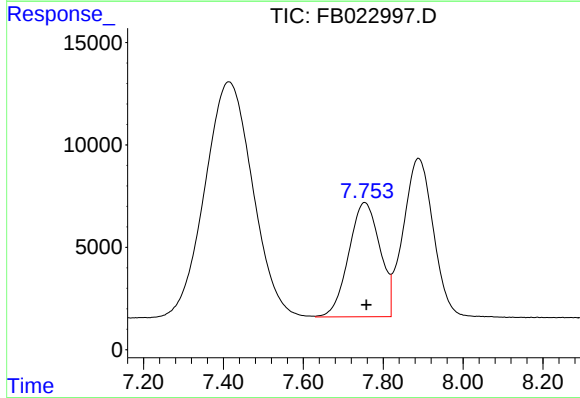


#3 n-Heptane

R.T.: 7.754 min
Delta R.T.: -0.004 min
Response: 303729
Conc: 8.73 ng/ml

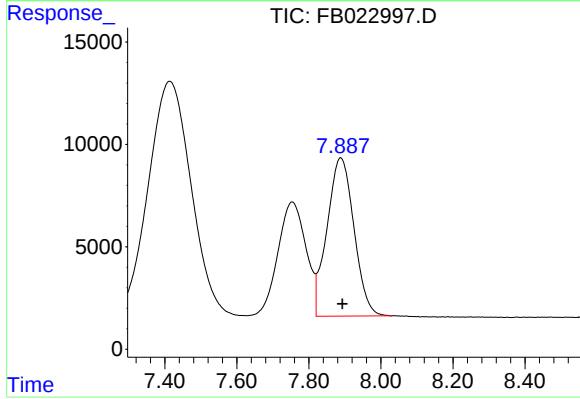


#4 Benzene

R.T.: 7.889 min
Delta R.T.: -0.004 min
Response: 401969
Conc: 9.28 ng/ml

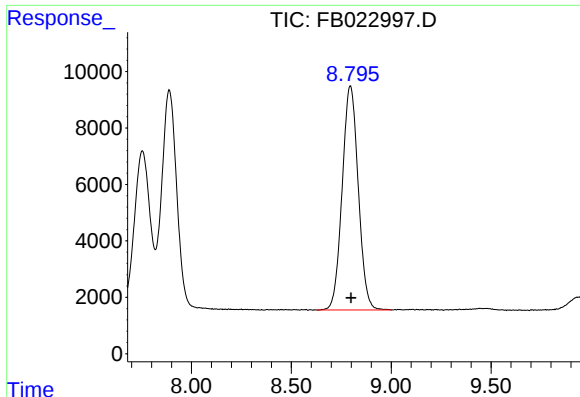


#5 AAA-TFT

R.T.: 8.796 min
Delta R.T.: -0.004 min
Response: 444231
Conc: 19.73 ng/ml

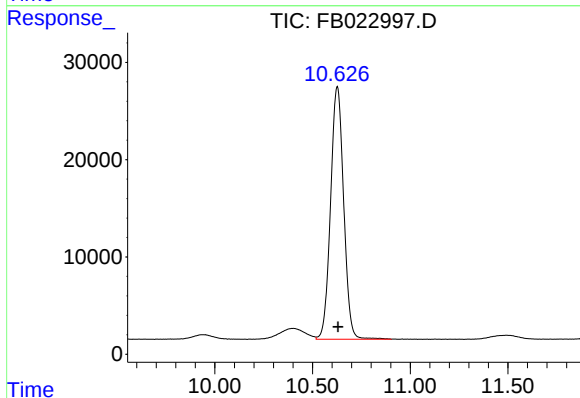


#6 Toluene

R.T.: 10.627 min
Delta R.T.: -0.005 min
Response: 1209402
Conc: 28.05 ng/ml

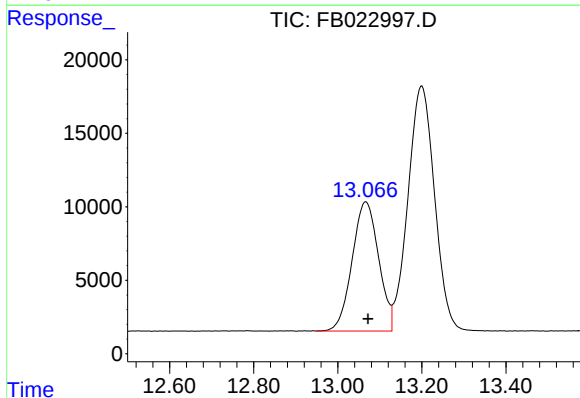


#7 Ethylbenzene

R.T.: 13.067 min
Delta R.T.: -0.005 min
Response: 384312
Conc: 9.63 ng/ml

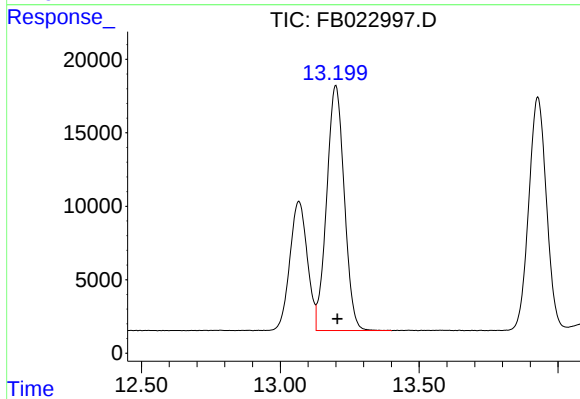


#8 m-Xylene

R.T.: 13.200 min
Delta R.T.: -0.005 min
Response: 735120
Conc: 19.46 ng/ml

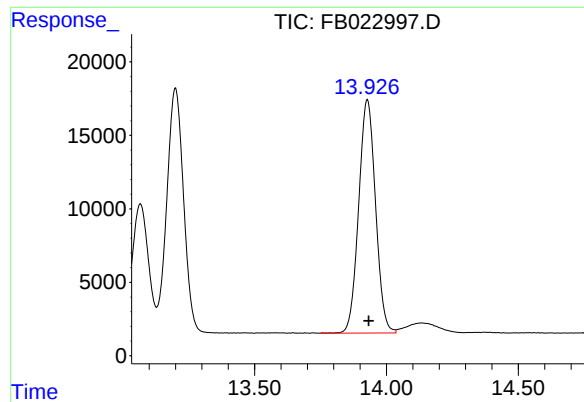

#9 O-Xylene

R.T.: 13.928 min
Delta R.T.: -0.005 min
Response: 704338
Conc: 19.76 ng/ml

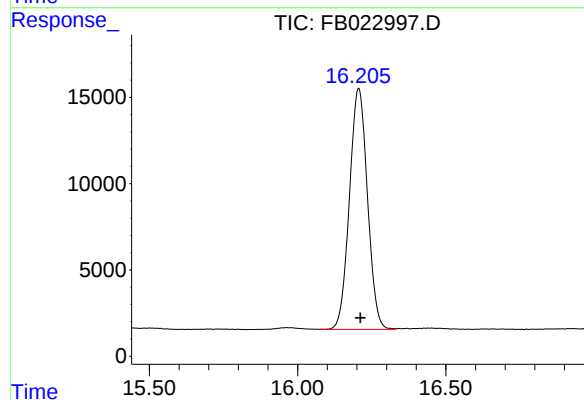

#10 1,2,4-Trimethylbenzene

R.T.: 16.207 min
Delta R.T.: -0.005 min
Response: 590374
Conc: 20.82 ng/ml