

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111422\
 Data File : FB028989.D
 Signal(s) : FID2B.CH
 Acq On : 14 Nov 2022 12:16
 Operator : AJ/MA
 Sample : BSF1114S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF1114S1

Integration File: Calibration.e
 Quant Time: Nov 15 05:56:50 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110122.M
 Quant Title :
 QLast Update : Tue Nov 01 12:44:12 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.785	217120	17.086 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.702	407856	25.022 ng/ml
2) t 2,2,4-Trimethylpentane	7.409	440032	25.043 ng/ml
3) t n-Heptane	7.746	143388	8.155 ng/ml
4) t Benzene	7.880	175935	8.580 ng/ml
6) t Toluene	10.612	519050	25.807 ng/ml
7) t Ethylbenzene	13.049	164774	8.688 ng/ml
8) t m-Xylene	13.181	331739	17.634 ng/ml
9) t O-Xylene	13.908	323705	17.645 ng/ml
10) t 1,2,4-Trimethylbenzene	16.183	347591	18.868 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111422\
Data File : FB028989.D
Signal(s) : FID2B.CH
Acq On : 14 Nov 2022 12:16
Operator : AJ/MA
Sample : BSF1114S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF1114S1

Integration File: Calibration.e
Quant Time: Nov 15 05:56:50 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110122.M
Quant Title :
QLast Update : Tue Nov 01 12:44:12 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

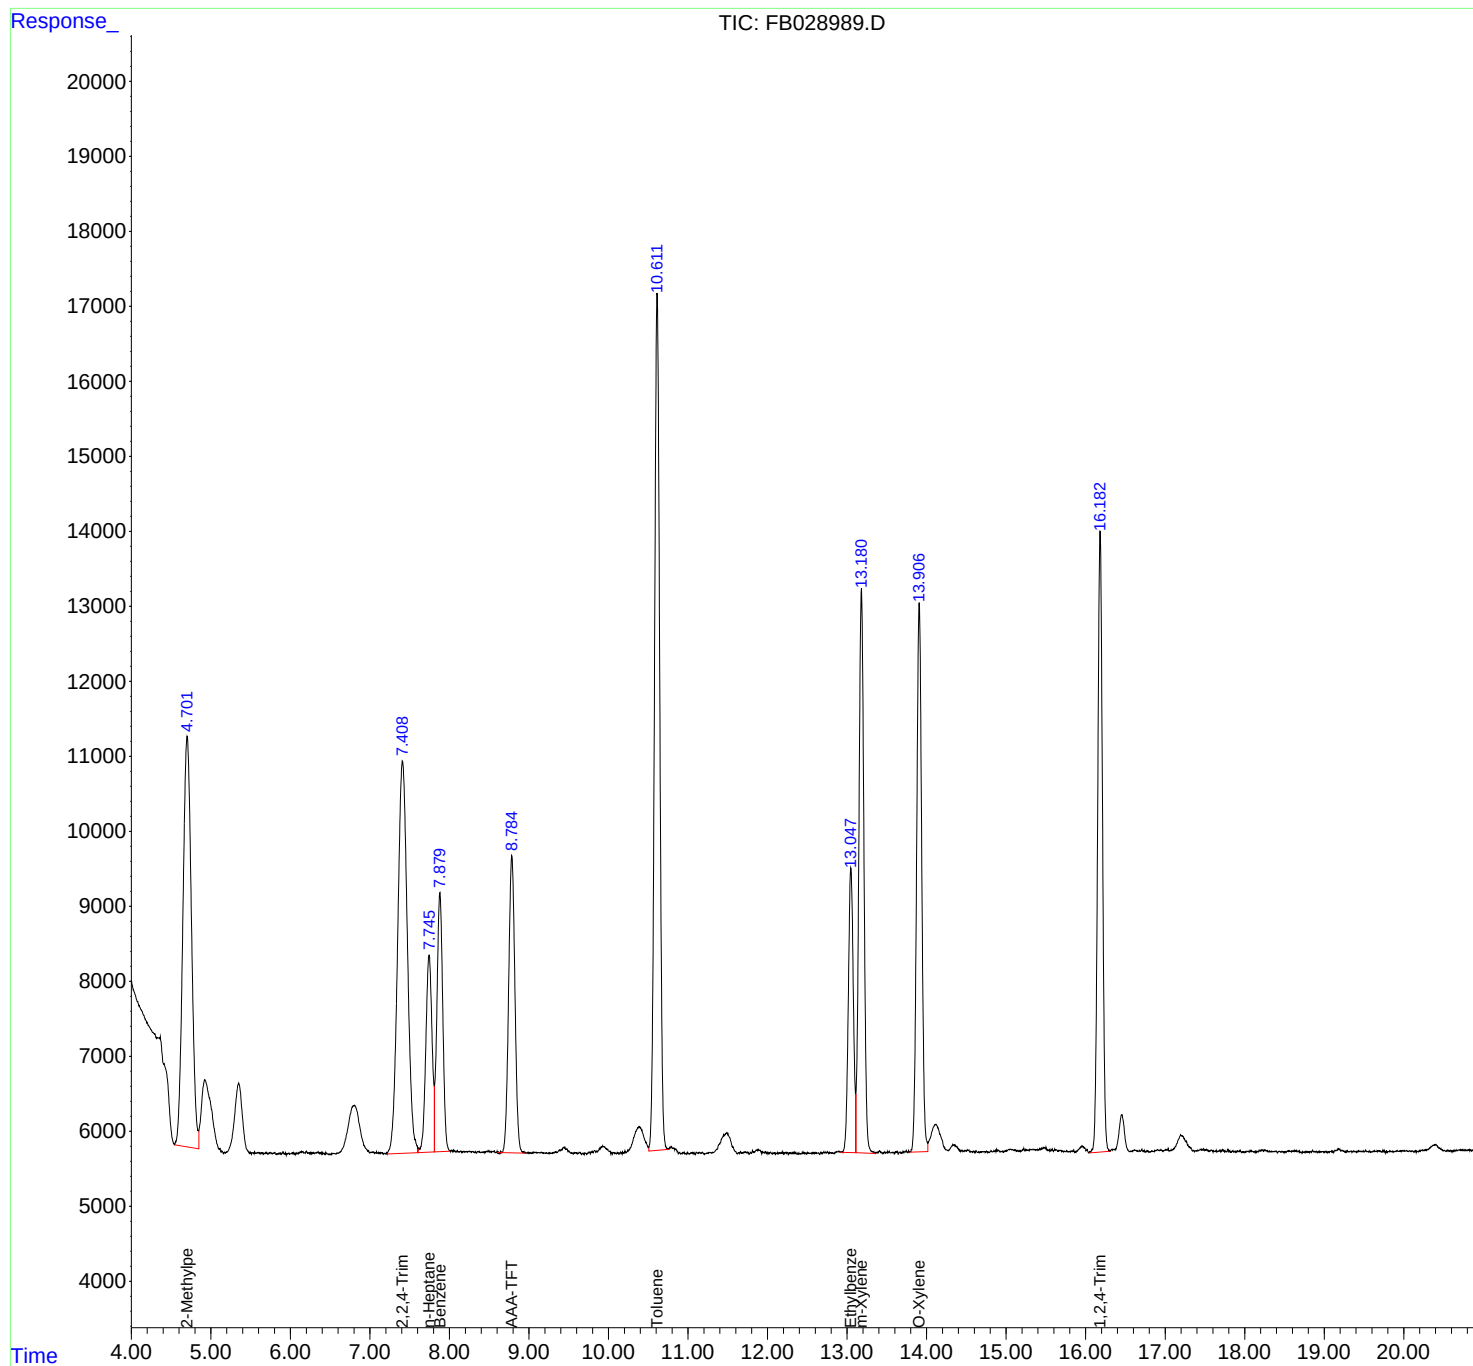


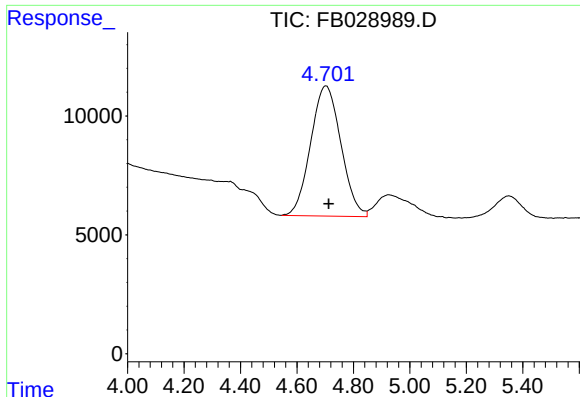

#1 2-Methylpentane


R.T.: 4.702 min
Delta R.T.: -0.010 min
Response: 407856
Conc: 25.02 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1114S1

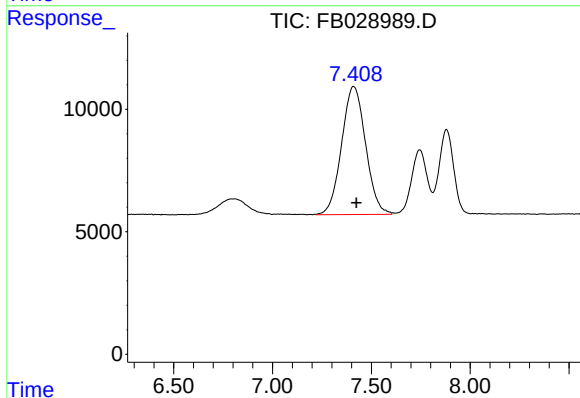


#2 2,2,4-Trimethylpentane

R.T.: 7.409 min
Delta R.T.: -0.015 min
Response: 440032
Conc: 25.04 ng/ml

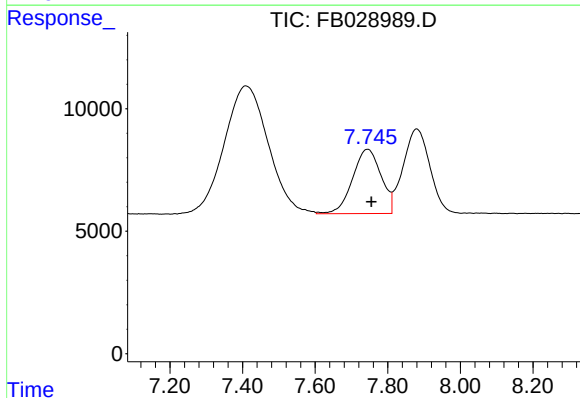


#3 n-Heptane

R.T.: 7.746 min
Delta R.T.: -0.009 min
Response: 143388
Conc: 8.16 ng/ml

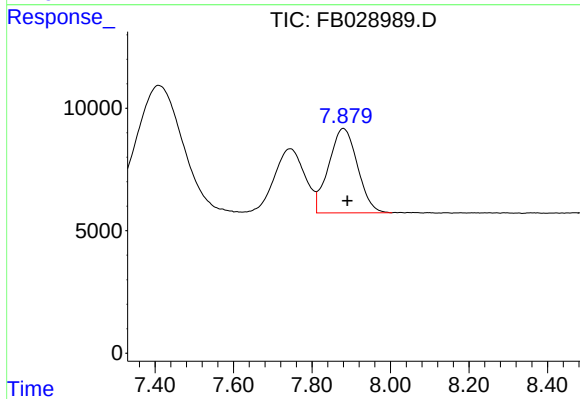

#4 Benzene


R.T.: 7.880 min
Delta R.T.: -0.010 min
Response: 175935
Conc: 8.58 ng/ml

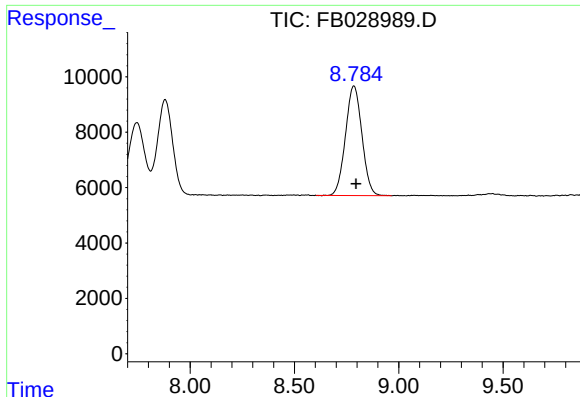

#5 AAA-TFT


R.T.: 8.785 min
Delta R.T.: -0.010 min
Response: 217120
Conc: 17.09 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1114S1

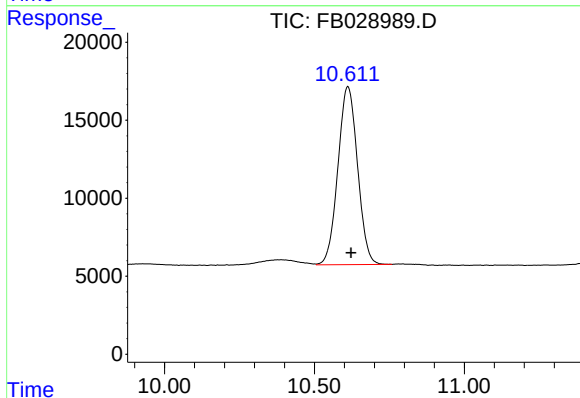


#6 Toluene

R.T.: 10.612 min
Delta R.T.: -0.011 min
Response: 519050
Conc: 25.81 ng/ml

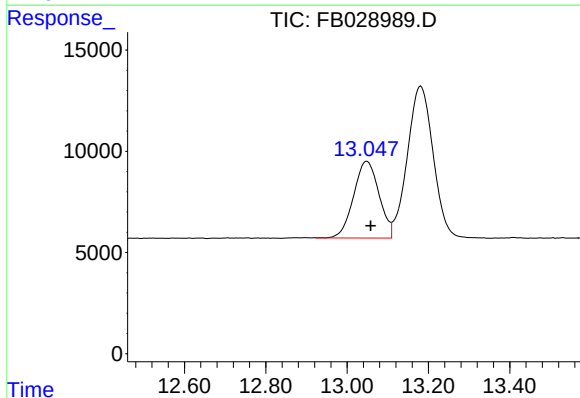


#7 Ethylbenzene

R.T.: 13.049 min
Delta R.T.: -0.010 min
Response: 164774
Conc: 8.69 ng/ml

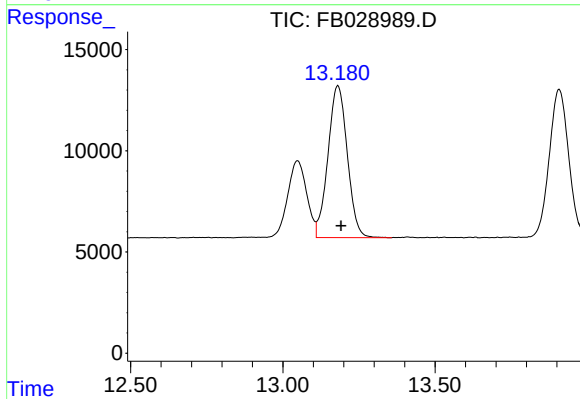

#8 m-Xylene


R.T.: 13.181 min
Delta R.T.: -0.010 min
Response: 331739
Conc: 17.63 ng/ml

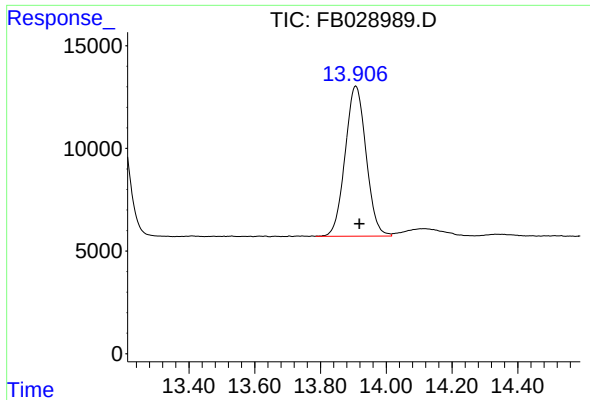

#9 O-Xylene

R.T.: 13.908 min
Delta R.T.: -0.010 min
Response: 323705
Conc: 17.65 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1114S1

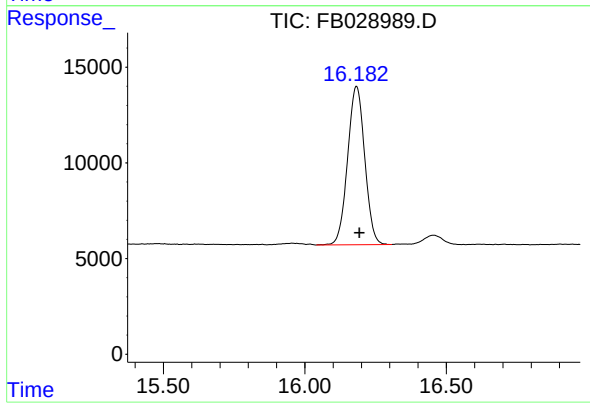

#10 1,2,4-Trimethylbenzene

R.T.: 16.183 min
Delta R.T.: -0.010 min
Response: 347591
Conc: 18.87 ng/ml