

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111422\
 Data File : FB028991.D
 Signal(s) : FID2B.CH
 Acq On : 14 Nov 2022 13:30
 Operator : AJ/MA
 Sample : BSF1114W2
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF1114W2

Integration File: Calibration.e
 Quant Time: Nov 15 05:57:02 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110122.M
 Quant Title :
 QLast Update : Tue Nov 01 12:44:12 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.787	244291	19.224 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.704	391128	23.996 ng/ml
2) t 2,2,4-Trimethylpentane	7.415	431616	24.564 ng/ml
3) t n-Heptane	7.746	140919	8.015 ng/ml
4) t Benzene	7.883	173059	8.439 ng/ml
6) t Toluene	10.615	494883	24.605 ng/ml
7) t Ethylbenzene	13.051	156934	8.275 ng/ml
8) t m-Xylene	13.184	315764	16.784 ng/ml
9) t O-Xylene	13.911	304893	16.620 ng/ml
10) t 1,2,4-Trimethylbenzene	16.186	314674	17.081 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111422\
Data File : FB028991.D
Signal(s) : FID2B.CH
Acq On : 14 Nov 2022 13:30
Operator : AJ/MA
Sample : BSF1114W2
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF1114W2

Integration File: Calibration.e
Quant Time: Nov 15 05:57:02 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110122.M
Quant Title :
QLast Update : Tue Nov 01 12:44:12 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

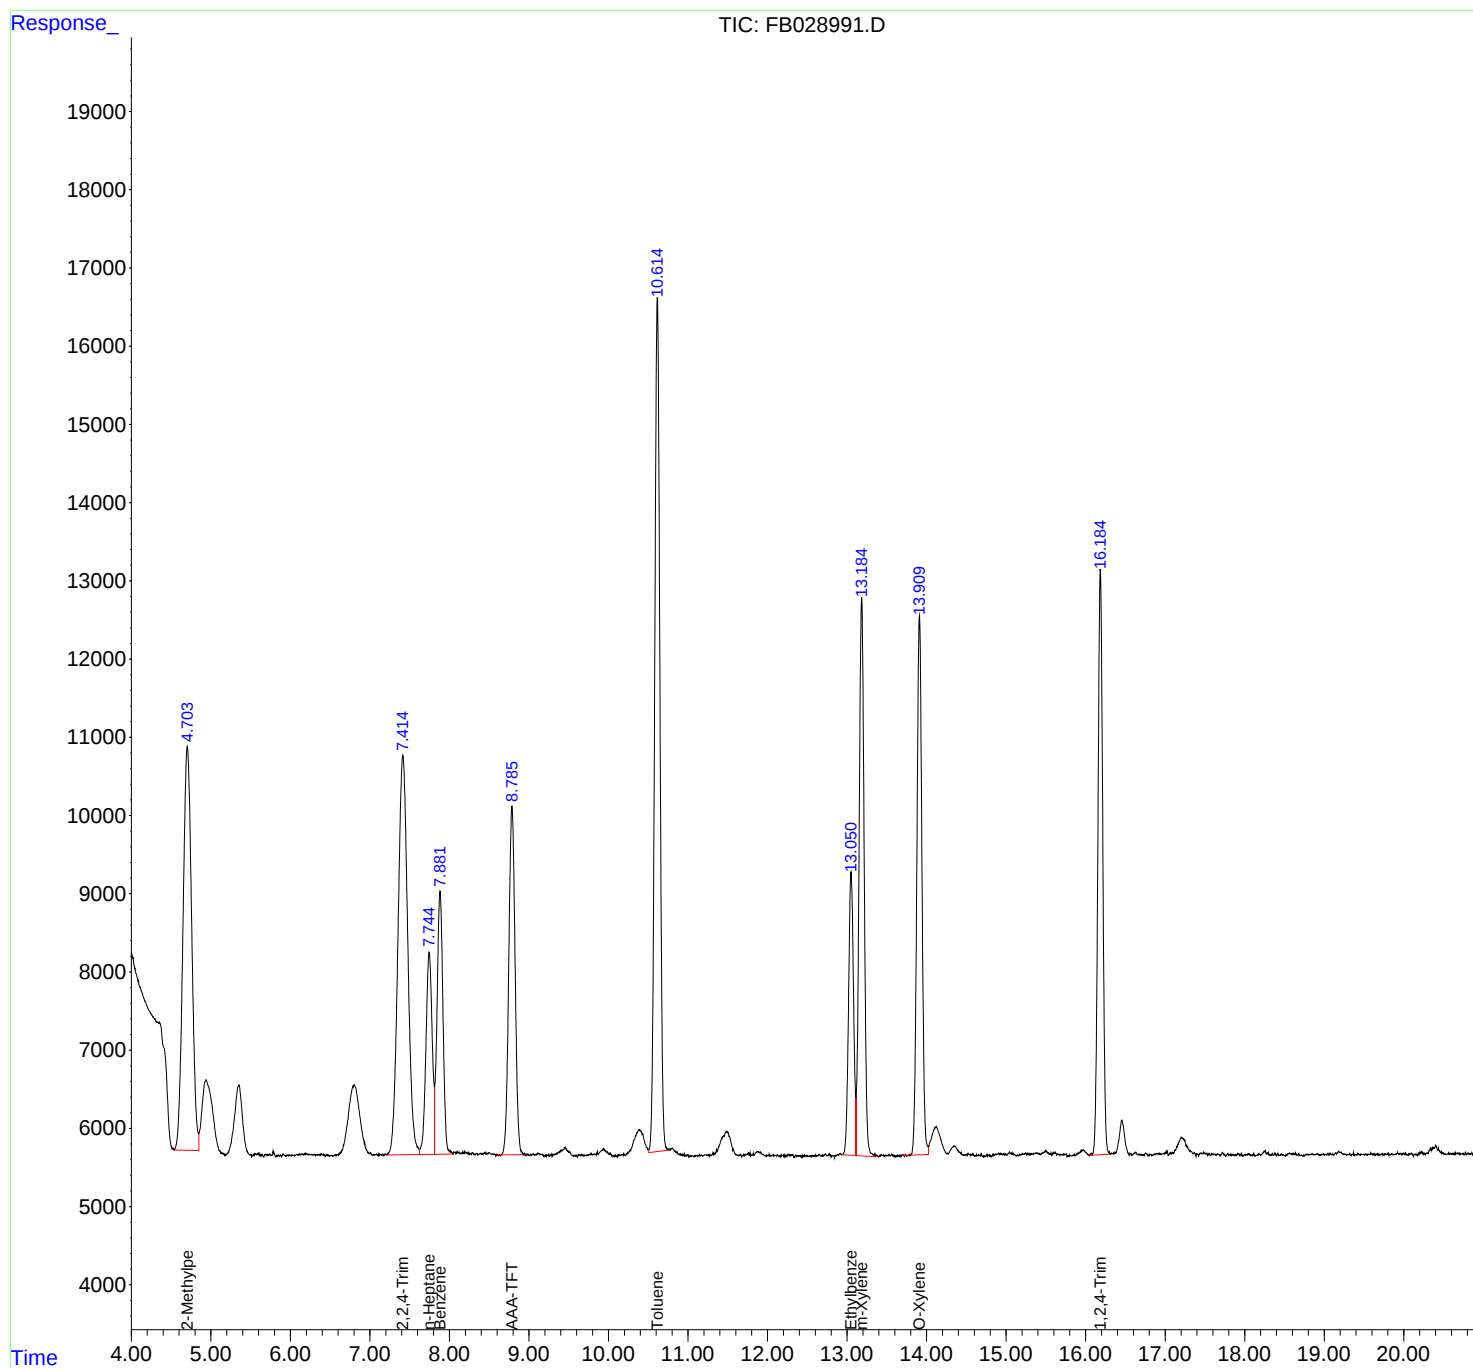


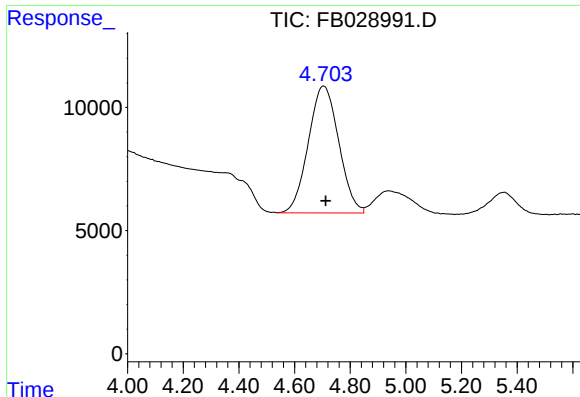

#1 2-Methylpentane


R.T.: 4.704 min
Delta R.T.: -0.008 min
Response: 391128
Conc: 24.00 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1114W2

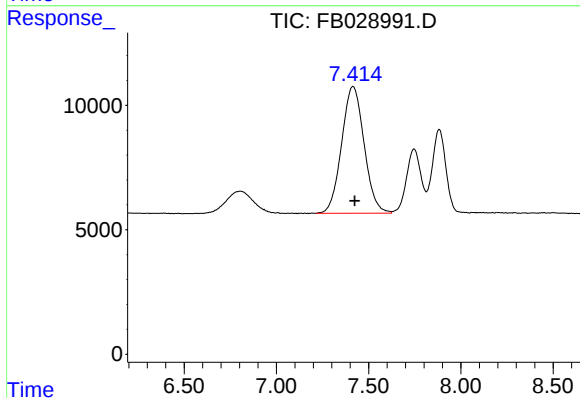


#2 2,2,4-Trimethylpentane

R.T.: 7.415 min
Delta R.T.: -0.009 min
Response: 431616
Conc: 24.56 ng/ml

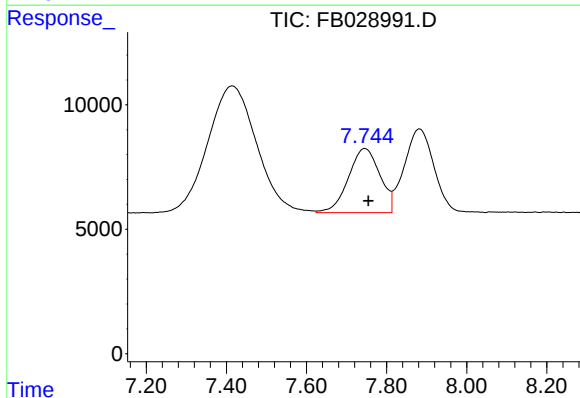


#3 n-Heptane

R.T.: 7.746 min
Delta R.T.: -0.009 min
Response: 140919
Conc: 8.01 ng/ml

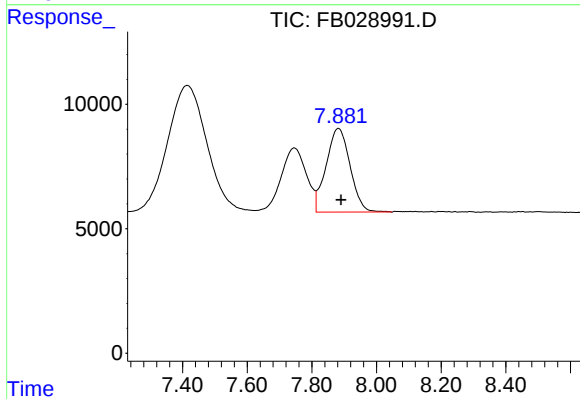

#4 Benzene


R.T.: 7.883 min
Delta R.T.: -0.008 min
Response: 173059
Conc: 8.44 ng/ml

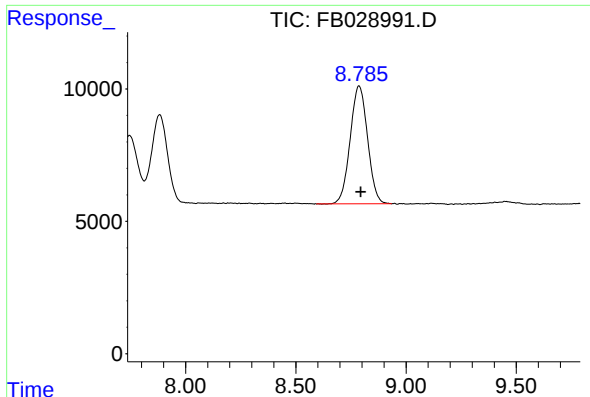

#5 AAA-TFT


R.T.: 8.787 min
Delta R.T.: -0.008 min
Response: 244291
Conc: 19.22 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1114W2

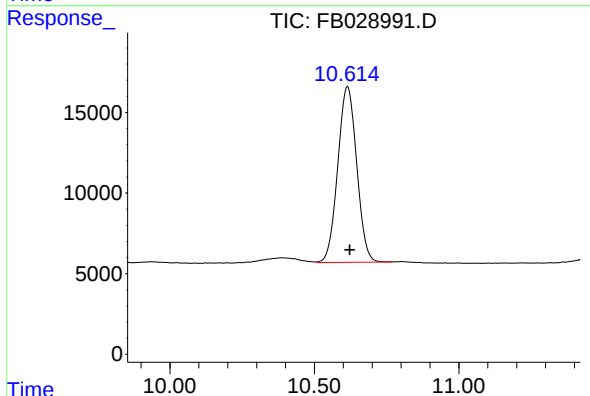


#6 Toluene

R.T.: 10.615 min
Delta R.T.: -0.008 min
Response: 494883
Conc: 24.60 ng/ml

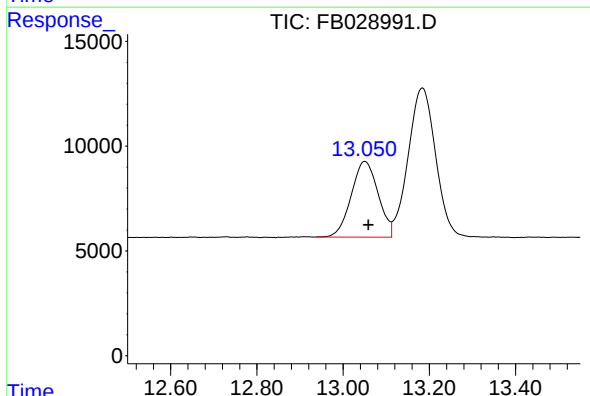


#7 Ethylbenzene

R.T.: 13.051 min
Delta R.T.: -0.008 min
Response: 156934
Conc: 8.27 ng/ml

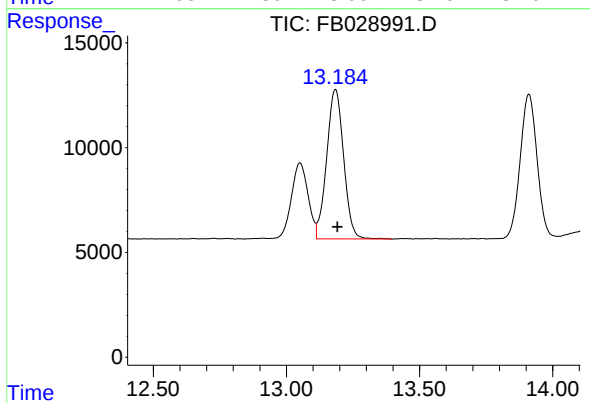

#8 m-Xylene


R.T.: 13.184 min
Delta R.T.: -0.007 min
Response: 315764
Conc: 16.78 ng/ml

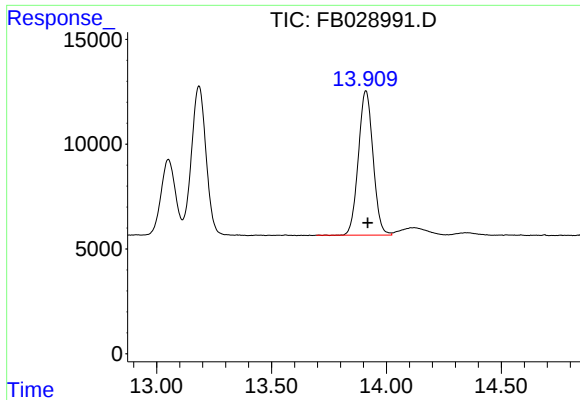

#9 O-Xylene

R.T.: 13.911 min
Delta R.T.: -0.007 min
Response: 304893
Conc: 16.62 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1114W2

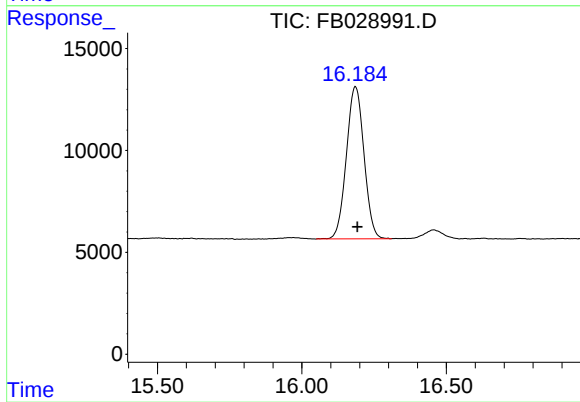

#10 1,2,4-Trimethylbenzene

R.T.: 16.186 min
Delta R.T.: -0.007 min
Response: 314674
Conc: 17.08 ng/ml