

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111422\
 Data File : FB028995.D
 Signal(s) : FID2B.CH
 Acq On : 14 Nov 2022 16:15
 Operator : AJ/MA
 Sample : 20 PPB GRO STD
 Misc : 1.31G/5.00 ML DI WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 20 PPB GRO STD

Integration File: Calibration.e
 Quant Time: Nov 15 05:57:26 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110122.M
 Quant Title :
 QLast Update : Tue Nov 01 12:44:12 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.789	263467	20.734 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.709	438090	26.877 ng/ml
2) t 2,2,4-Trimethylpentane	7.418	502117	28.576 ng/ml
3) t n-Heptane	7.747	157857	8.978 ng/ml
4) t Benzene	7.884	199072	9.708 ng/ml
6) t Toluene	10.616	574501	28.563 ng/ml
7) t Ethylbenzene	13.053	183808	9.692 ng/ml
8) t m-Xylene	13.186	365715	19.440 ng/ml
9) t O-Xylene	13.912	354496	19.324 ng/ml
10) t 1,2,4-Trimethylbenzene	16.188	352620	19.141 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111422\
Data File : FB028995.D
Signal(s) : FID2B.CH
Acq On : 14 Nov 2022 16:15
Operator : AJ/MA
Sample : 20 PPB GRO STD
Misc : 1.31G/5.00 ML DI WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
20 PPB GRO STD

Integration File: Calibration.e
Quant Time: Nov 15 05:57:26 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110122.M
Quant Title :
QLast Update : Tue Nov 01 12:44:12 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

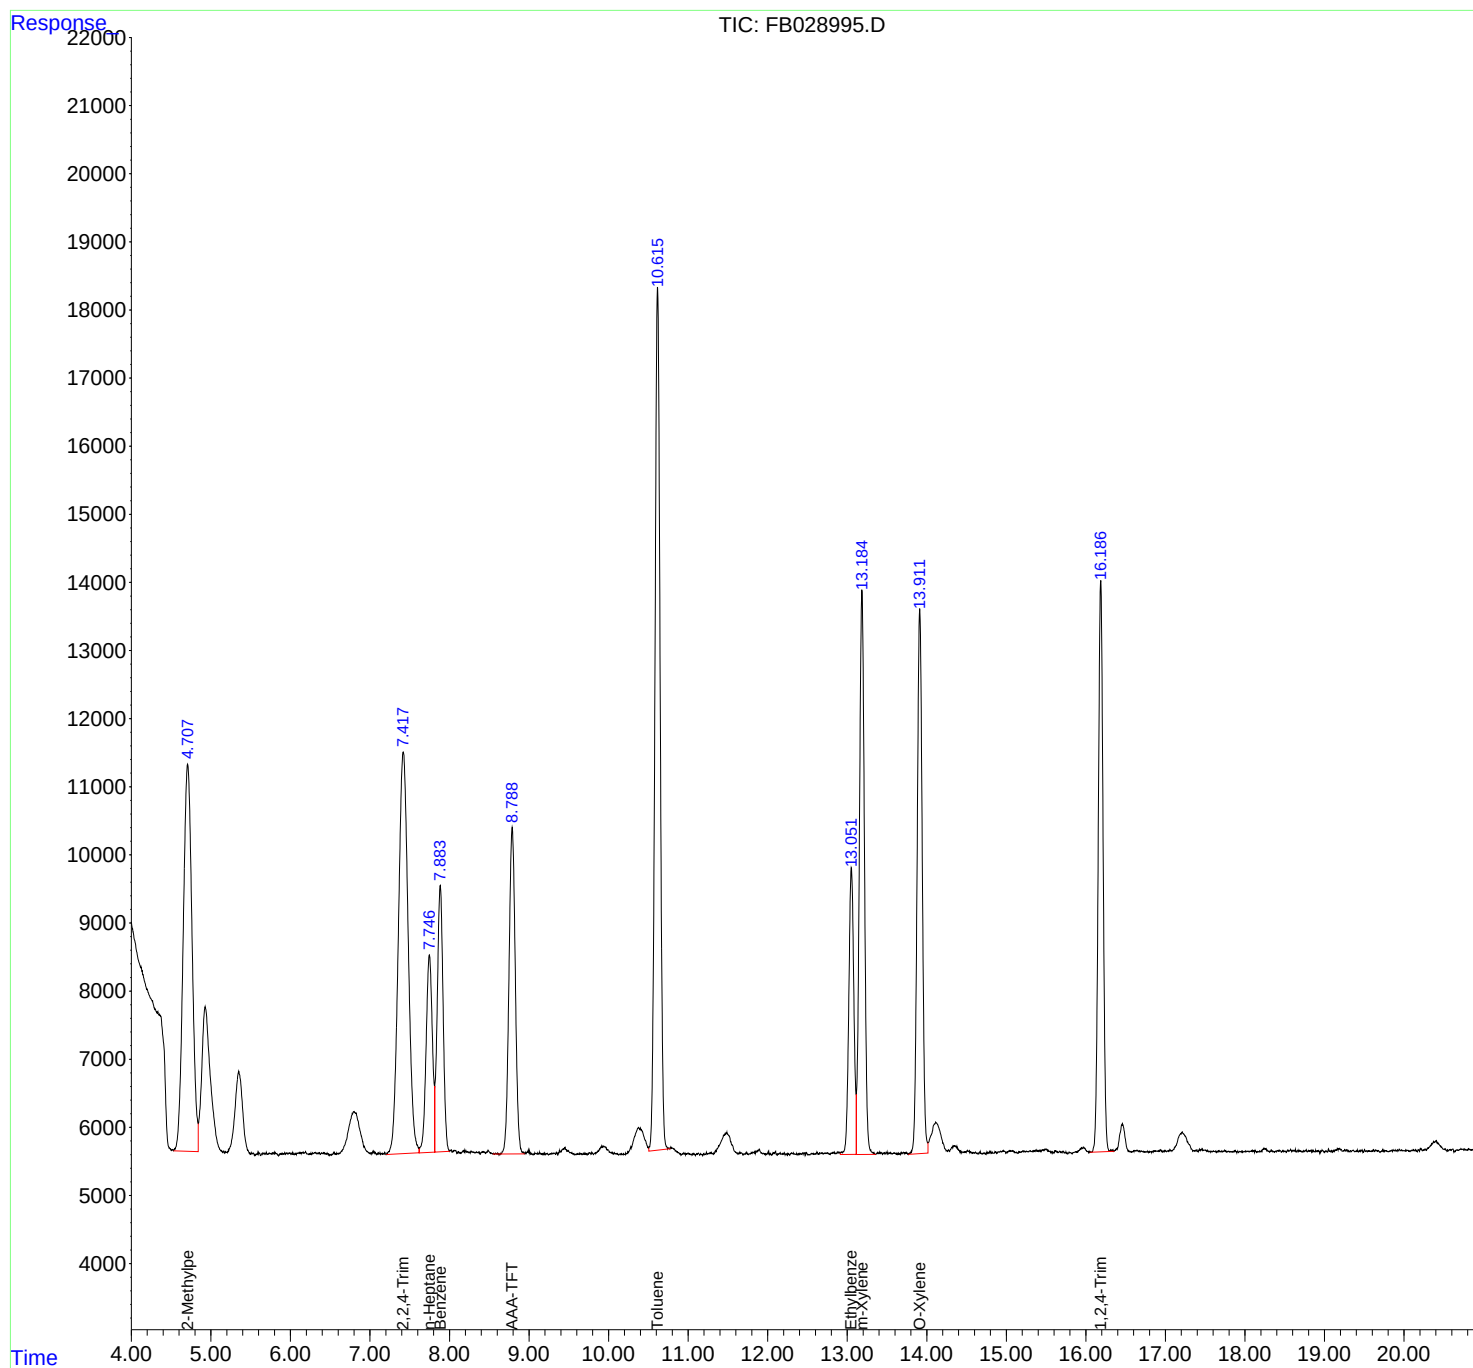


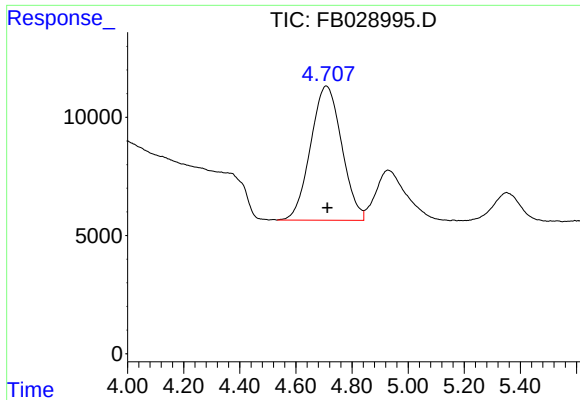

#1 2-Methylpentane


R.T.: 4.709 min
Delta R.T.: -0.003 min
Response: 438090
Conc: 26.88 ng/ml

Instrument :
FID_B
ClientSampleId :
20 PPB GRO STD

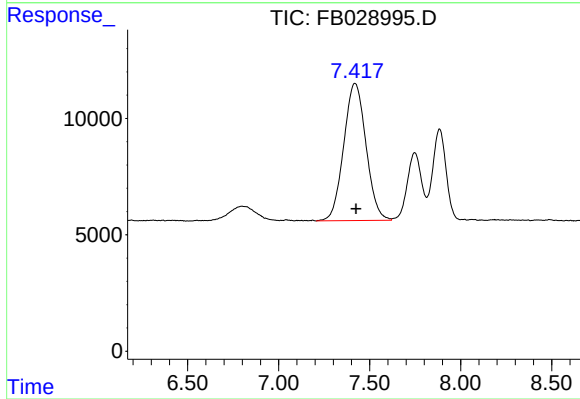


#2 2,2,4-Trimethylpentane

R.T.: 7.418 min
Delta R.T.: -0.006 min
Response: 502117
Conc: 28.58 ng/ml

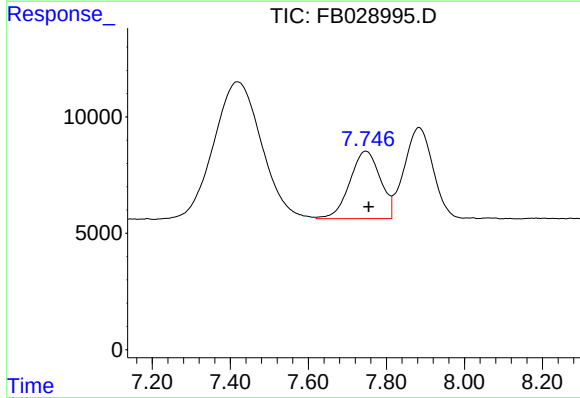


#3 n-Heptane

R.T.: 7.747 min
Delta R.T.: -0.007 min
Response: 157857
Conc: 8.98 ng/ml

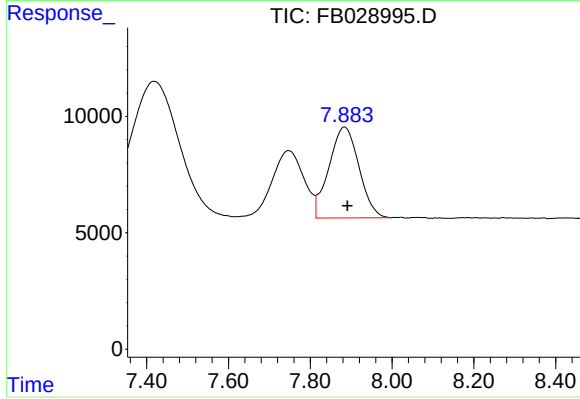

#4 Benzene


R.T.: 7.884 min
Delta R.T.: -0.006 min
Response: 199072
Conc: 9.71 ng/ml

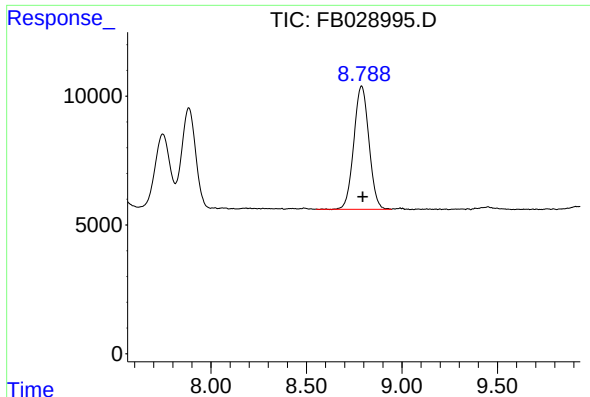

#5 AAA-TFT


R.T.: 8.789 min
Delta R.T.: -0.006 min
Response: 263467
Conc: 20.73 ng/ml

Instrument :
FID_B
ClientSampleId :
20 PPB GRO STD

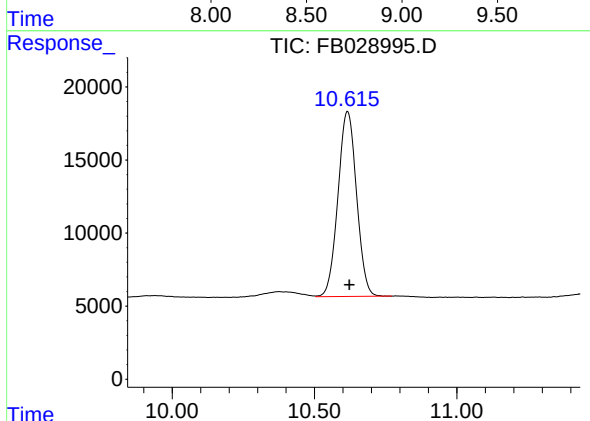


#6 Toluene

R.T.: 10.616 min
Delta R.T.: -0.006 min
Response: 574501
Conc: 28.56 ng/ml

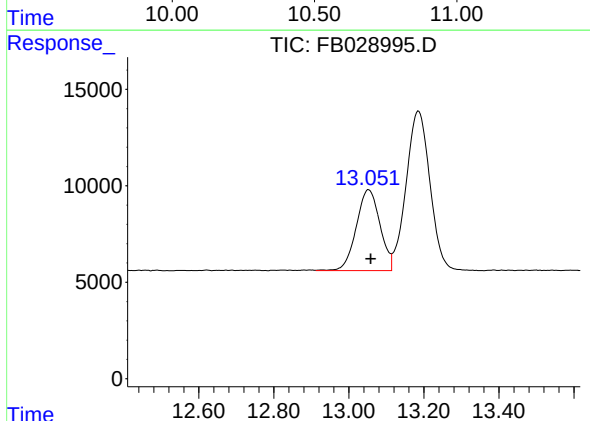


#7 Ethylbenzene

R.T.: 13.053 min
Delta R.T.: -0.006 min
Response: 183808
Conc: 9.69 ng/ml

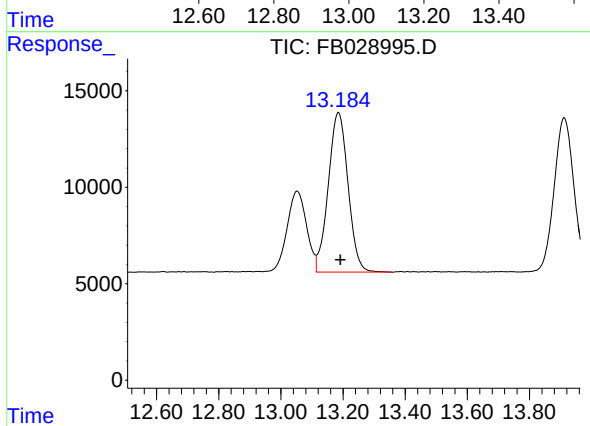

#8 m-Xylene


R.T.: 13.186 min
Delta R.T.: -0.006 min
Response: 365715
Conc: 19.44 ng/ml

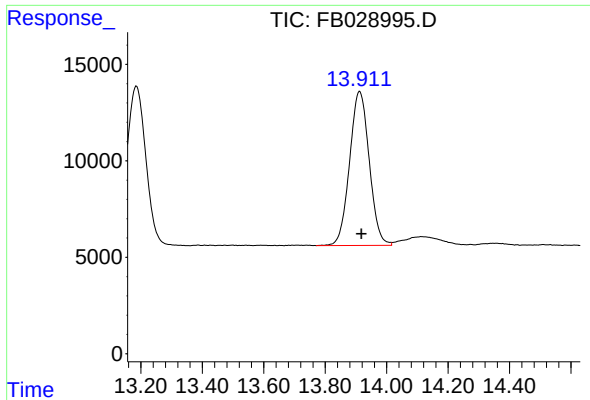

#9 O-Xylene

R.T.: 13.912 min
Delta R.T.: -0.006 min
Response: 354496
Conc: 19.32 ng/ml

Instrument :
FID_B
ClientSampleId :
20 PPB GRO STD

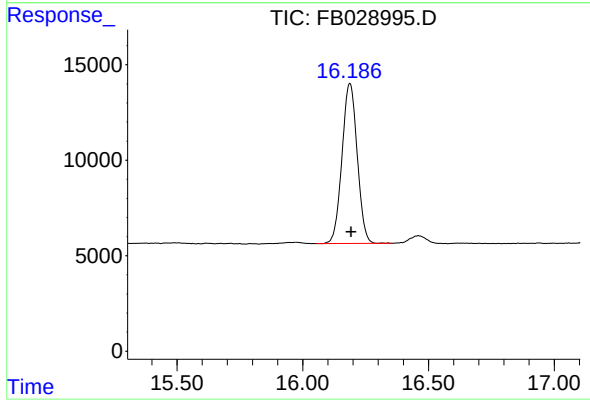

#10 1,2,4-Trimethylbenzene

R.T.: 16.188 min
Delta R.T.: -0.005 min
Response: 352620
Conc: 19.14 ng/ml