

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111422\
 Data File : FB029005.D
 Signal(s) : FID2B.CH
 Acq On : 14 Nov 2022 22:24
 Operator : AJ/MA
 Sample : BSF1114S2
 Misc : 1.31G/5.00 ML DI WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF1114S2

Integration File: Calibration.e
 Quant Time: Nov 15 05:58:25 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110122.M
 Quant Title :
 QLast Update : Tue Nov 01 12:44:12 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.786	207816	16.354 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.703	430439	26.408 ng/ml
2) t 2,2,4-Trimethylpentane	7.412	479031	27.262 ng/ml
3) t n-Heptane	7.745	153958	8.756 ng/ml
4) t Benzene	7.881	192166	9.371 ng/ml
6) t Toluene	10.614	551694	27.430 ng/ml
7) t Ethylbenzene	13.050	175743	9.266 ng/ml
8) t m-Xylene	13.183	350688	18.641 ng/ml
9) t O-Xylene	13.910	345255	18.820 ng/ml
10) t 1,2,4-Trimethylbenzene	16.185	353555	19.192 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111422\
Data File : FB029005.D
Signal(s) : FID2B.CH
Acq On : 14 Nov 2022 22:24
Operator : AJ/MA
Sample : BSF1114S2
Misc : 1.31G/5.00 ML DI WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF1114S2

Integration File: Calibration.e
Quant Time: Nov 15 05:58:25 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110122.M
Quant Title :
QLast Update : Tue Nov 01 12:44:12 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

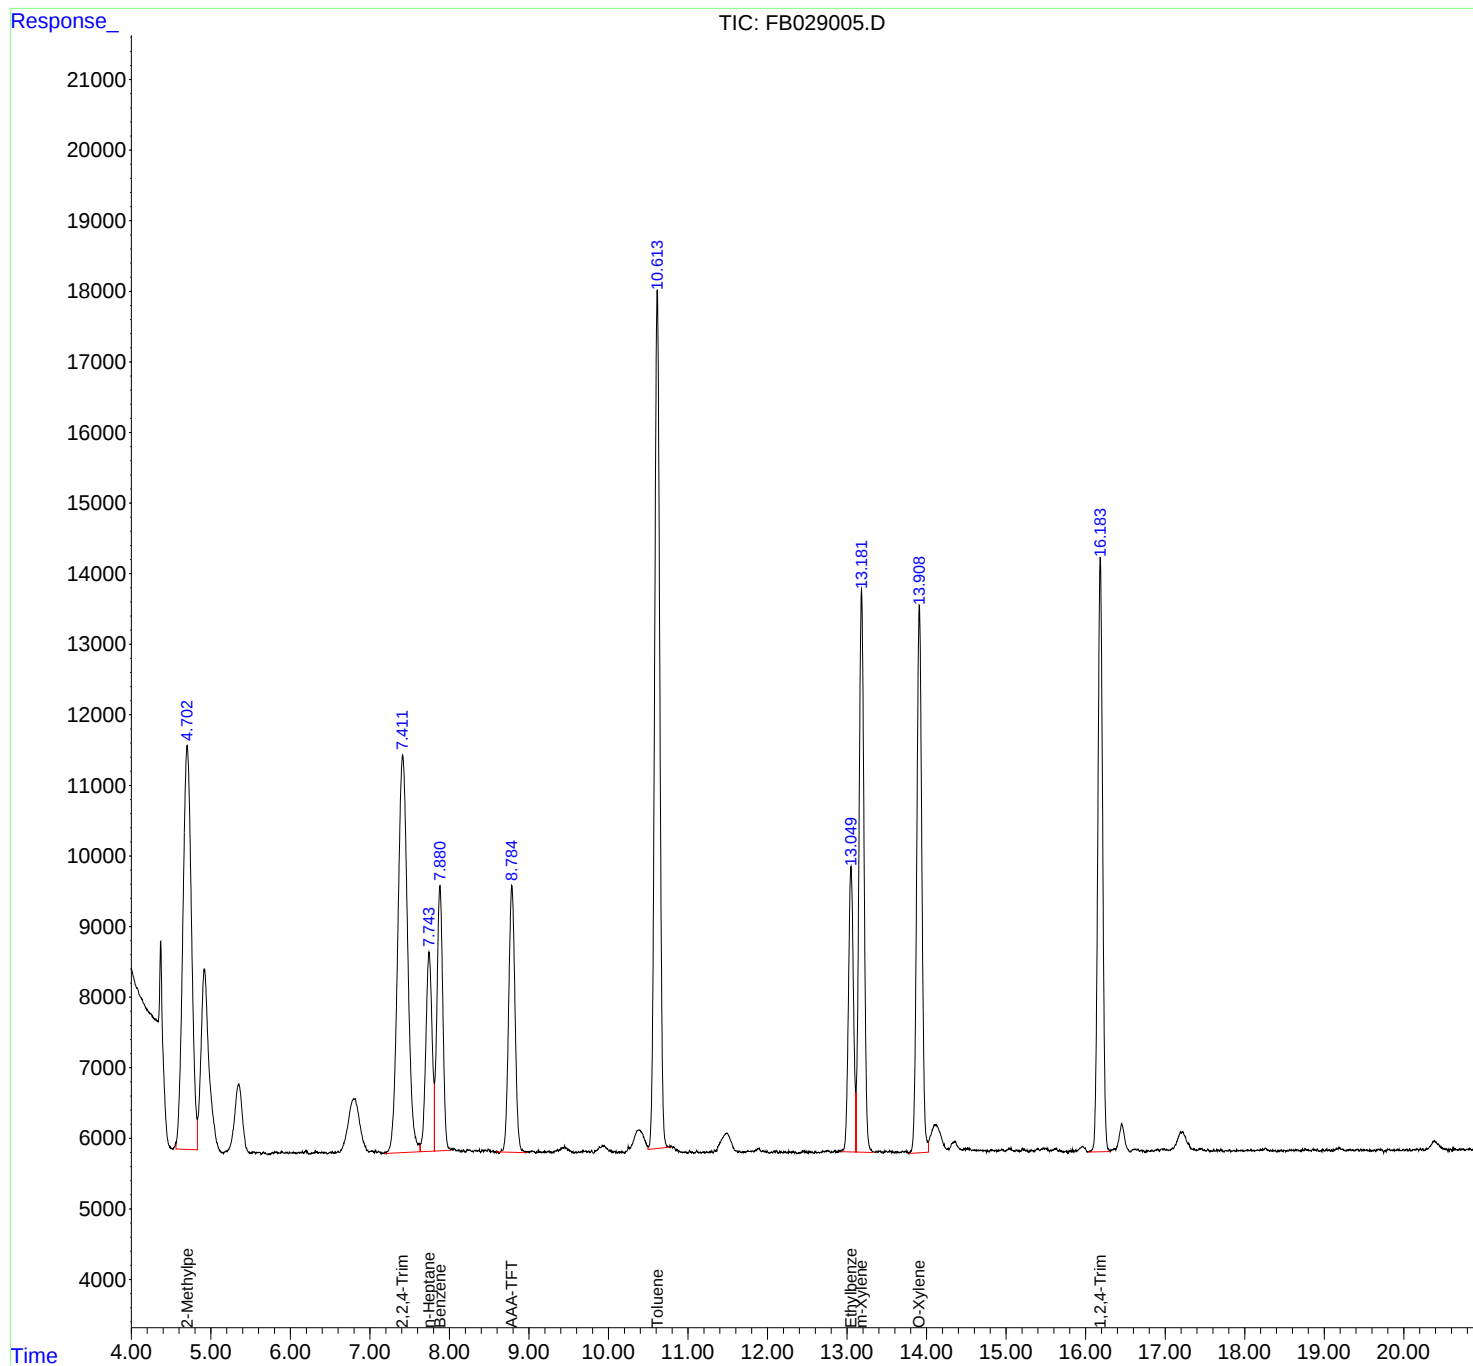


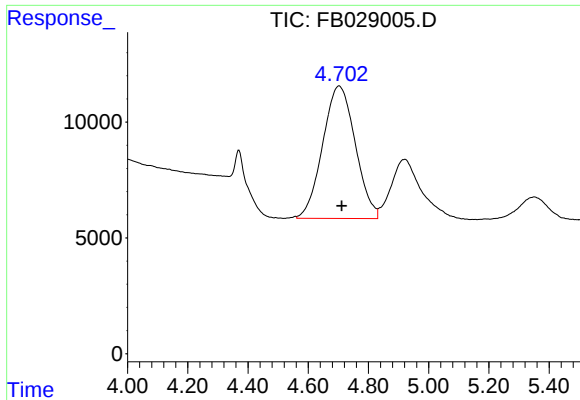

#1 2-Methylpentane


R.T.: 4.703 min
Delta R.T.: -0.009 min
Response: 430439
Conc: 26.41 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1114S2

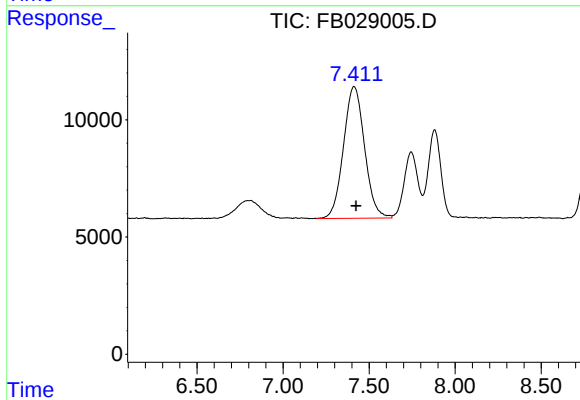


#2 2,2,4-Trimethylpentane

R.T.: 7.412 min
Delta R.T.: -0.012 min
Response: 479031
Conc: 27.26 ng/ml

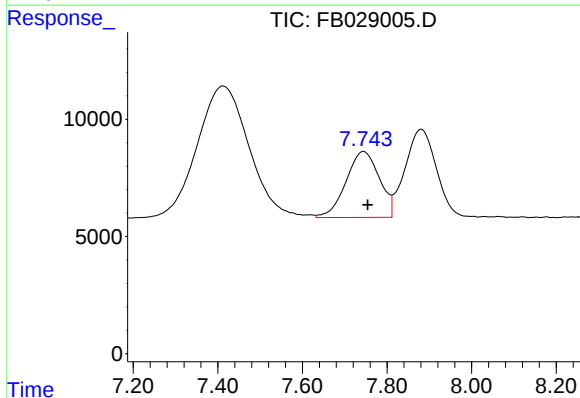


#3 n-Heptane

R.T.: 7.745 min
Delta R.T.: -0.010 min
Response: 153958
Conc: 8.76 ng/ml

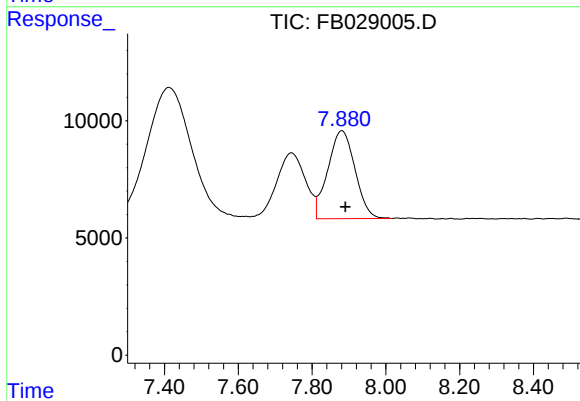

#4 Benzene


R.T.: 7.881 min
Delta R.T.: -0.009 min
Response: 192166
Conc: 9.37 ng/ml

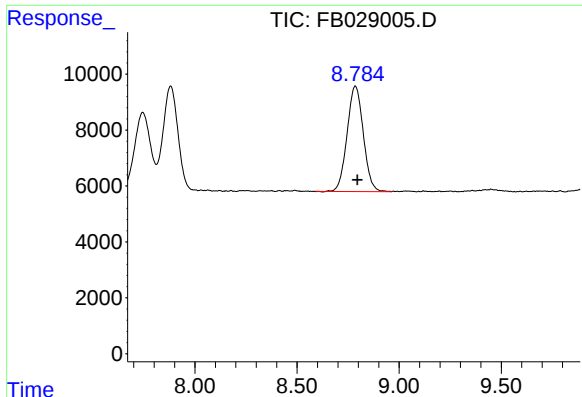

#5 AAA-TFT


R.T.: 8.786 min
Delta R.T.: -0.009 min
Response: 207816
Conc: 16.35 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1114S2

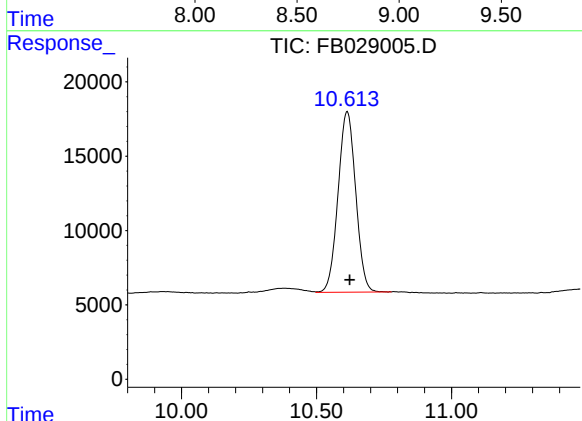


#6 Toluene

R.T.: 10.614 min
Delta R.T.: -0.009 min
Response: 551694
Conc: 27.43 ng/ml

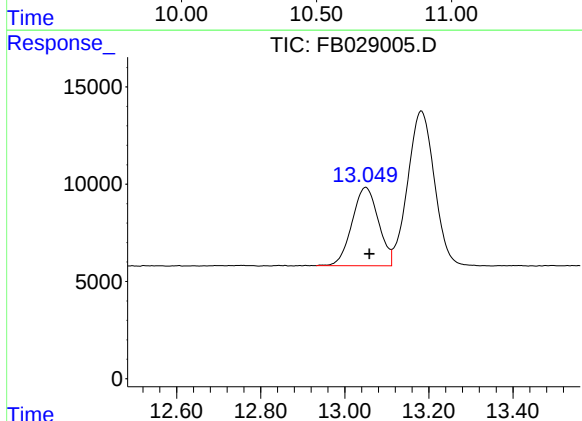


#7 Ethylbenzene

R.T.: 13.050 min
Delta R.T.: -0.008 min
Response: 175743
Conc: 9.27 ng/ml

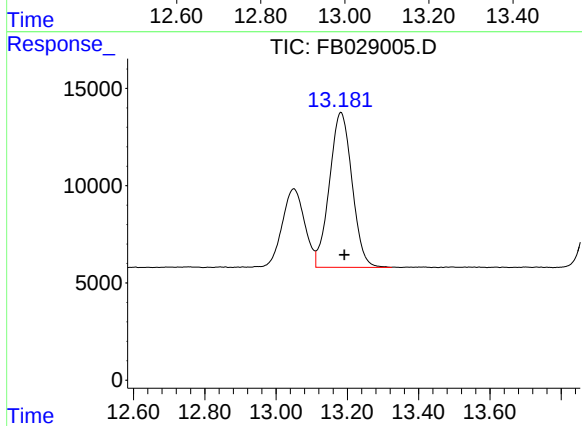

#8 m-Xylene


R.T.: 13.183 min
Delta R.T.: -0.009 min
Response: 350688
Conc: 18.64 ng/ml

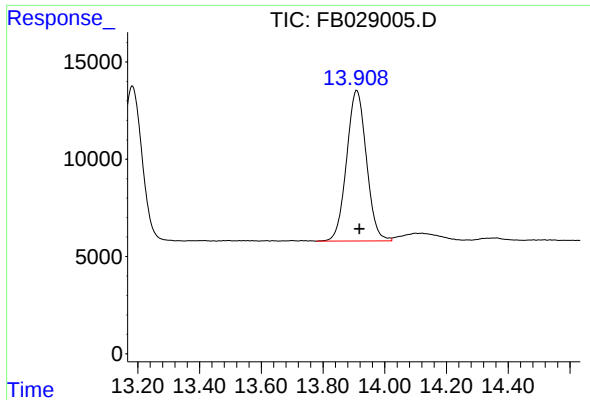

#9 O-Xylene

R.T.: 13.910 min
Delta R.T.: -0.009 min
Response: 345255
Conc: 18.82 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1114S2

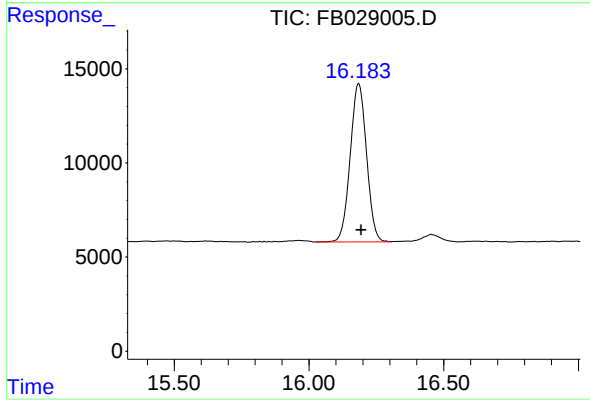

#10 1,2,4-Trimethylbenzene

R.T.: 16.185 min
Delta R.T.: -0.008 min
Response: 353555
Conc: 19.19 ng/ml