

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111422\
 Data File : FB029010.D
 Signal(s) : FID2B.CH
 Acq On : 15 Nov 2022 2:03
 Operator : AJ/MA
 Sample : N5607-12MS
 Misc : 1.06G/5.00 ML DI WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 WC-40MS

Integration File: Calibration.e
 Quant Time: Nov 15 05:58:55 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110122.M
 Quant Title :
 QLast Update : Tue Nov 01 12:44:12 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.782	220239	17.332 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.694	387595	23.779 ng/ml
2) t 2,2,4-Trimethylpentane	7.409	452412	25.747 ng/ml
3) t n-Heptane	7.740	146930	8.357 ng/ml
4) t Benzene	7.876	190322	9.281 ng/ml
6) t Toluene	10.610	551972	27.443 ng/ml
7) t Ethylbenzene	13.047	173104	9.127 ng/ml
8) t m-Xylene	13.180	340866	18.119 ng/ml
9) t O-Xylene	13.907	322780	17.595 ng/ml
10) t 1,2,4-Trimethylbenzene	16.182	323484	17.560 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111422\
Data File : FB029010.D
Signal(s) : FID2B.CH
Acq On : 15 Nov 2022 2:03
Operator : AJ/MA
Sample : N5607-12MS
Misc : 1.06G/5.00 ML DI WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
WC-40MS

Integration File: Calibration.e
Quant Time: Nov 15 05:58:55 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110122.M
Quant Title :
QLast Update : Tue Nov 01 12:44:12 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

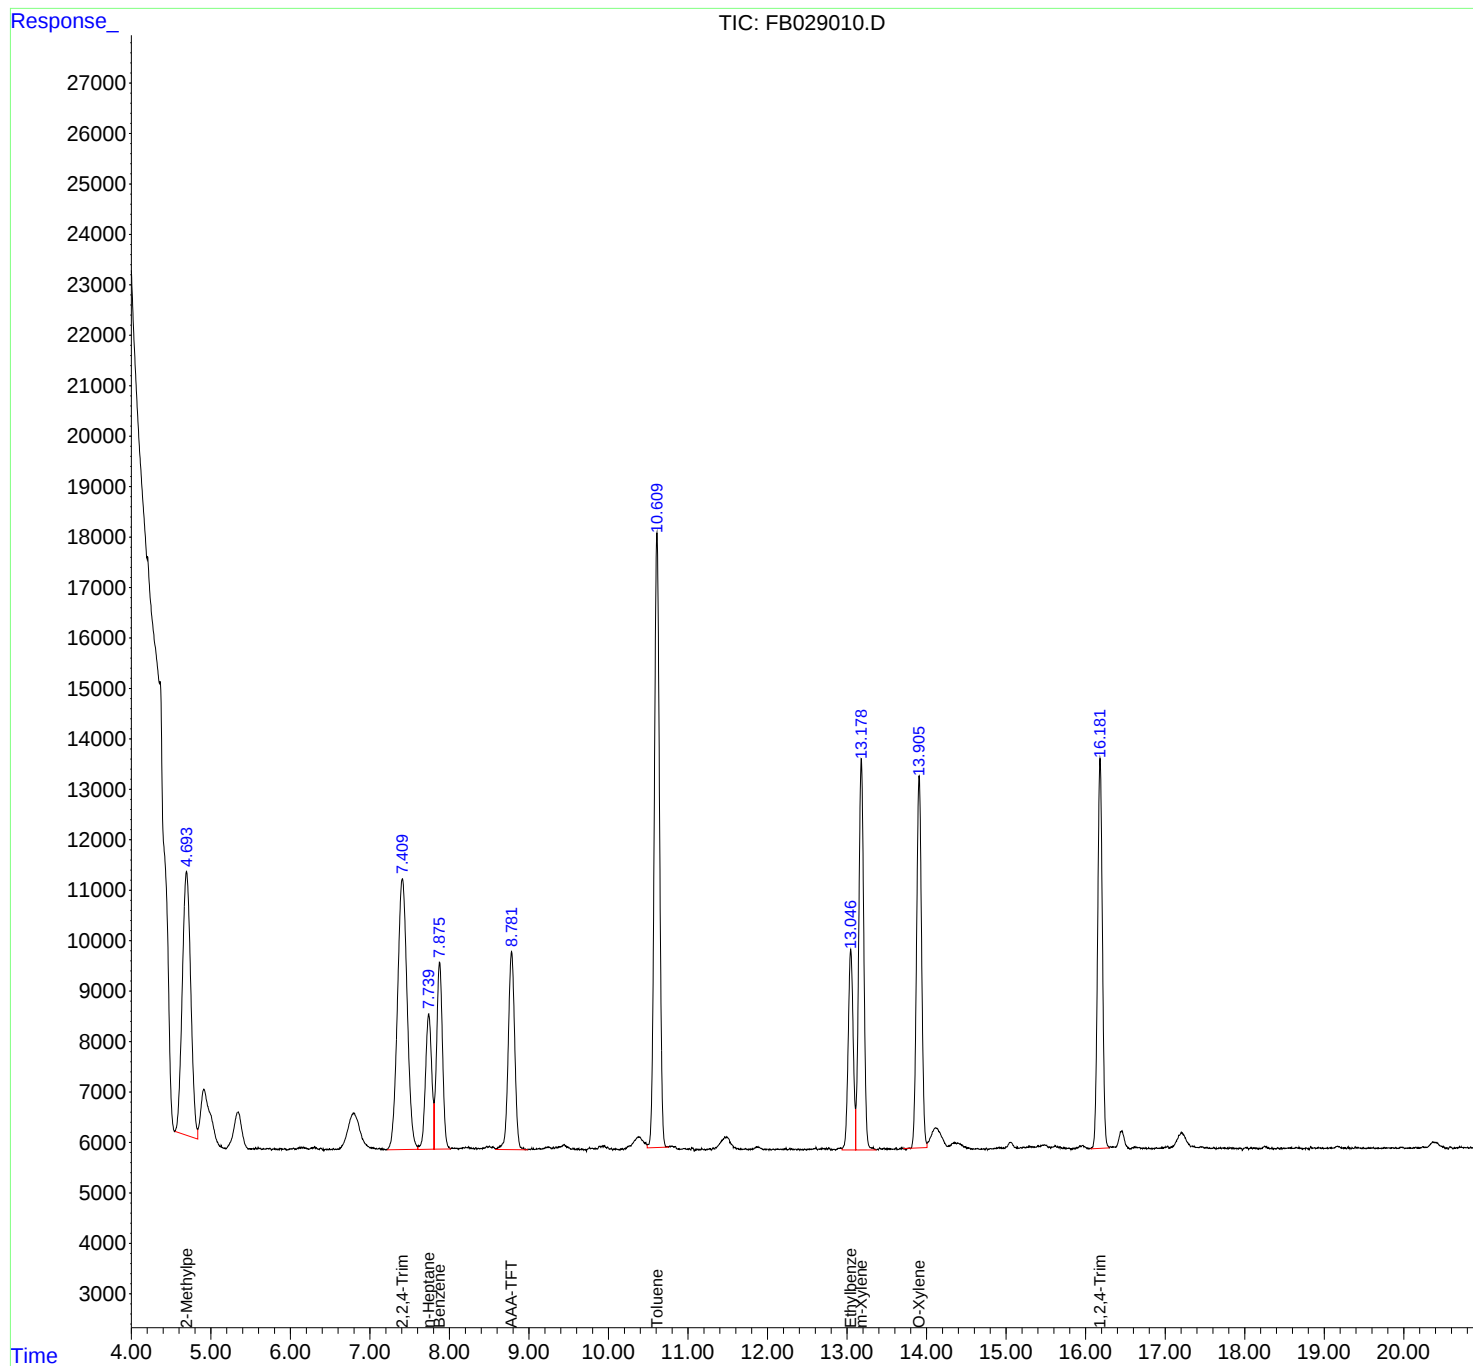


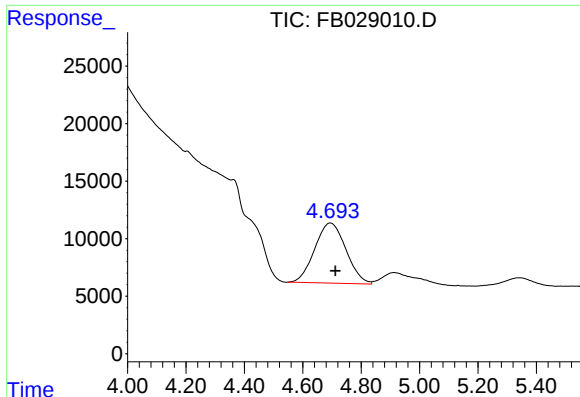

#1 2-Methylpentane


R.T.: 4.694 min
Delta R.T.: -0.018 min
Response: 387595
Conc: 23.78 ng/ml

Instrument :
FID_B
ClientSampleId :
WC-40MS

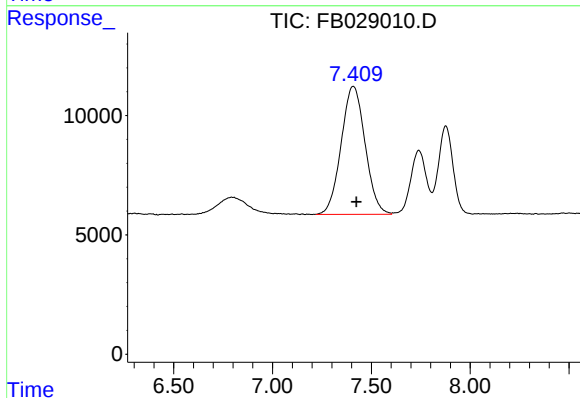


#2 2,2,4-Trimethylpentane

R.T.: 7.409 min
Delta R.T.: -0.015 min
Response: 452412
Conc: 25.75 ng/ml

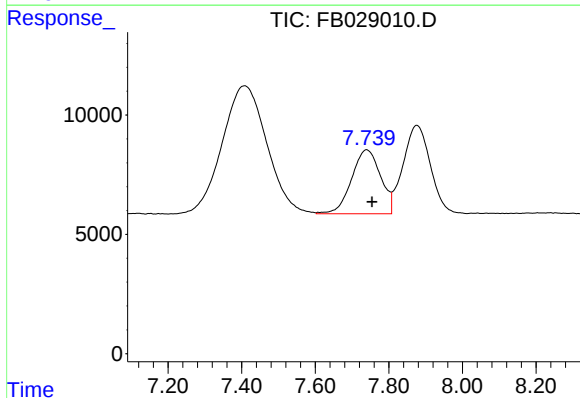


#3 n-Heptane

R.T.: 7.740 min
Delta R.T.: -0.015 min
Response: 146930
Conc: 8.36 ng/ml

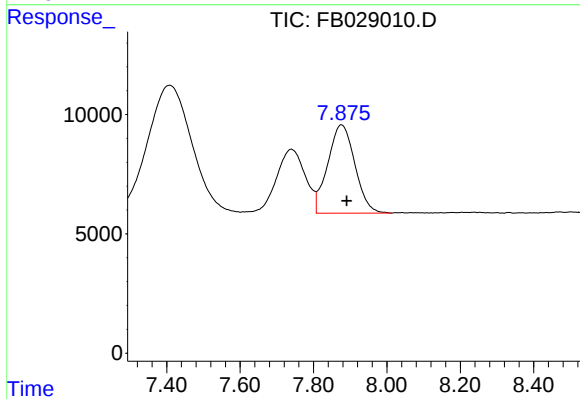

#4 Benzene


R.T.: 7.876 min
Delta R.T.: -0.014 min
Response: 190322
Conc: 9.28 ng/ml

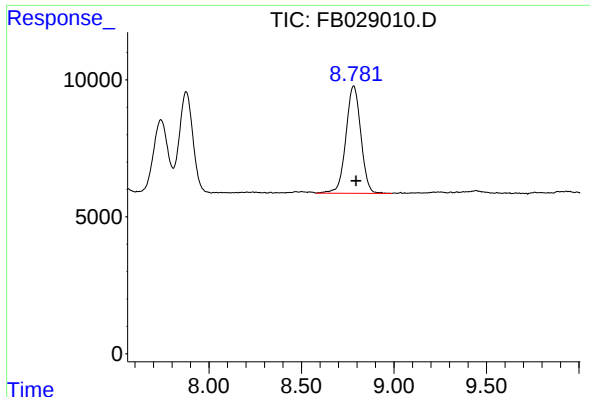

#5 AAA-TFT


R.T.: 8.782 min
Delta R.T.: -0.012 min
Response: 220239
Conc: 17.33 ng/ml

Instrument :
FID_B
ClientSampleId :
WC-40MS

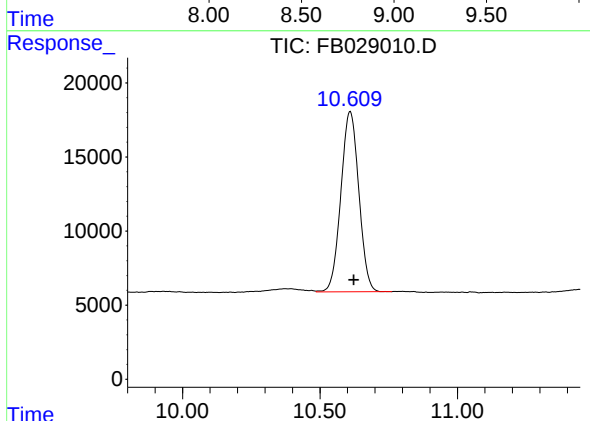


#6 Toluene

R.T.: 10.610 min
Delta R.T.: -0.013 min
Response: 551972
Conc: 27.44 ng/ml

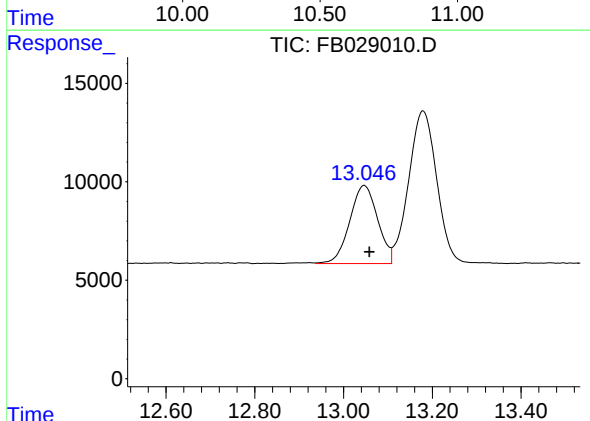


#7 Ethylbenzene

R.T.: 13.047 min
Delta R.T.: -0.011 min
Response: 173104
Conc: 9.13 ng/ml

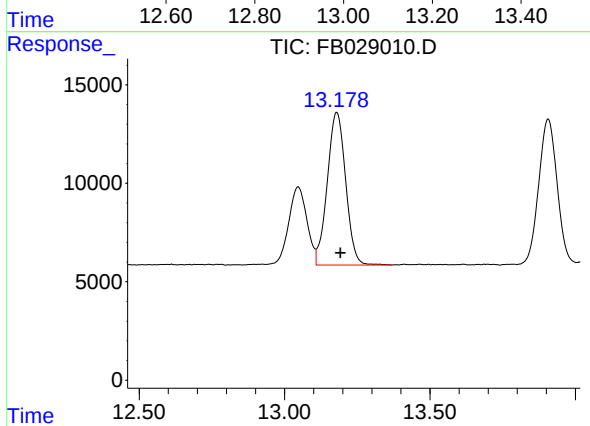

#8 m-Xylene


R.T.: 13.180 min
Delta R.T.: -0.012 min
Response: 340866
Conc: 18.12 ng/ml

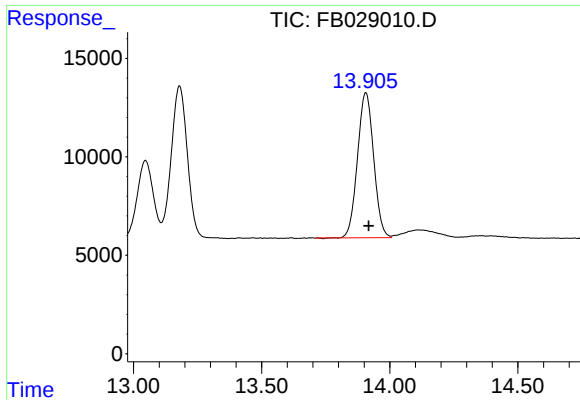

#9 O-Xylene

R.T.: 13.907 min
Delta R.T.: -0.011 min
Response: 322780
Conc: 17.59 ng/ml

Instrument :
FID_B
ClientSampleId :
WC-40MS

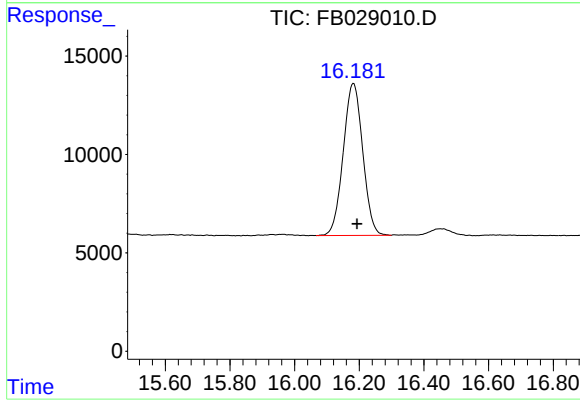

#10 1,2,4-Trimethylbenzene

R.T.: 16.182 min
Delta R.T.: -0.011 min
Response: 323484
Conc: 17.56 ng/ml