

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111422\
 Data File : FB029011.D
 Signal(s) : FID2B.CH
 Acq On : 15 Nov 2022 2:40
 Operator : AJ/MA
 Sample : N5607-12MSD
 Misc : 1.95G/5.00 ML DI WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 WC-40MSD

Integration File: Calibration.e
 Quant Time: Nov 15 05:59:01 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110122.M
 Quant Title :
 QLast Update : Tue Nov 01 12:44:12 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.782	232988	18.335 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.694	366038	22.457 ng/ml
2) t 2,2,4-Trimethylpentane	7.408	455057	25.898 ng/ml
3) t n-Heptane	7.740	147695	8.400 ng/ml
4) t Benzene	7.876	197010	9.607 ng/ml
6) t Toluene	10.610	562595	27.972 ng/ml
7) t Ethylbenzene	13.047	174825	9.218 ng/ml
8) t m-Xylene	13.179	345760	18.379 ng/ml
9) t O-Xylene	13.906	334599	18.239 ng/ml
10) t 1,2,4-Trimethylbenzene	16.181	321607	17.458 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111422\
Data File : FB029011.D
Signal(s) : FID2B.CH
Acq On : 15 Nov 2022 2:40
Operator : AJ/MA
Sample : N5607-12MSD
Misc : 1.95G/5.00 ML DI WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
WC-40MSD

Integration File: Calibration.e
Quant Time: Nov 15 05:59:01 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110122.M
Quant Title :
QLast Update : Tue Nov 01 12:44:12 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

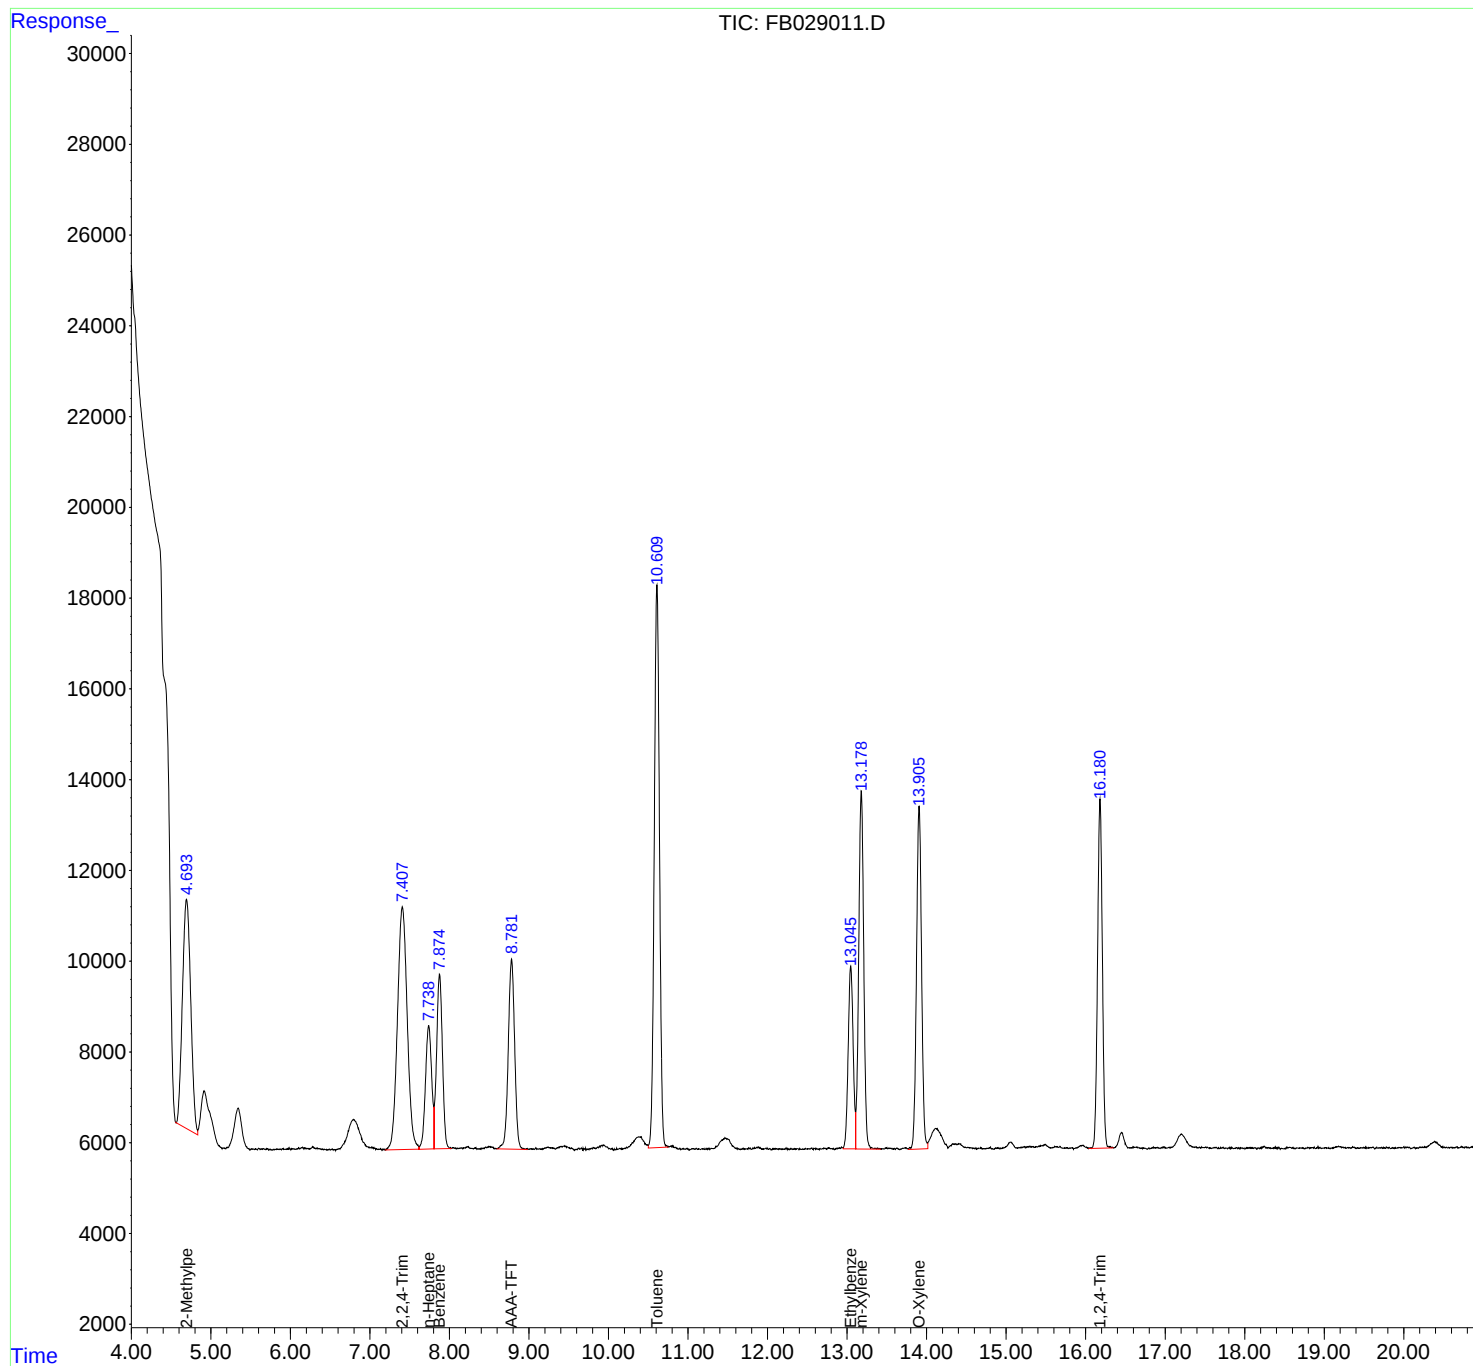


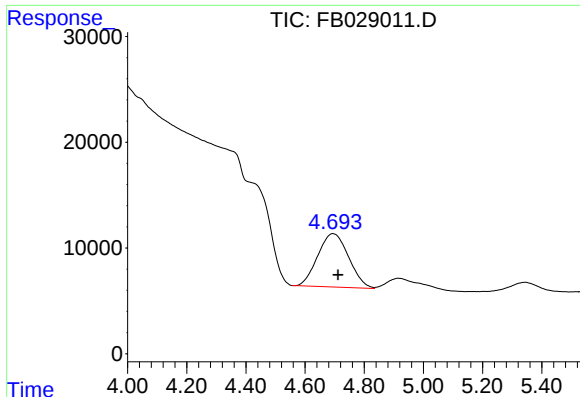

#1 2-Methylpentane


R.T.: 4.694 min
Delta R.T.: -0.018 min
Response: 366038
Conc: 22.46 ng/ml

Instrument :
FID_B
ClientSampleId :
WC-40MSD

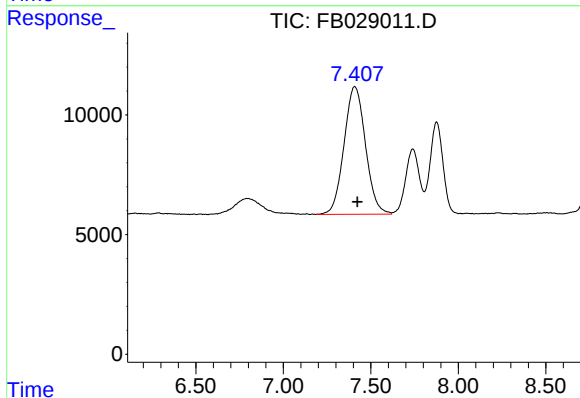


#2 2,2,4-Trimethylpentane

R.T.: 7.408 min
Delta R.T.: -0.016 min
Response: 455057
Conc: 25.90 ng/ml

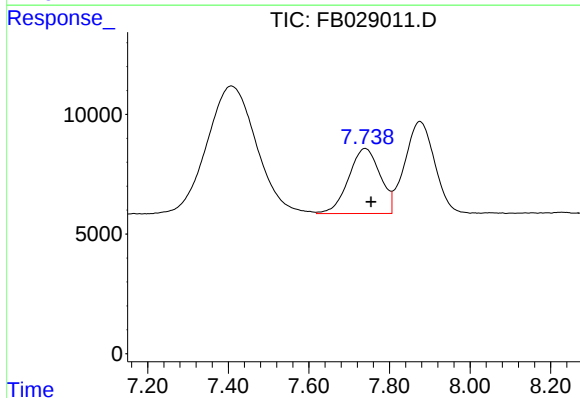


#3 n-Heptane

R.T.: 7.740 min
Delta R.T.: -0.015 min
Response: 147695
Conc: 8.40 ng/ml

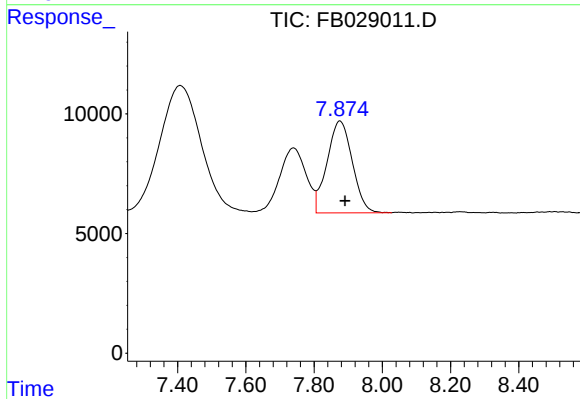

#4 Benzene


R.T.: 7.876 min
Delta R.T.: -0.015 min
Response: 197010
Conc: 9.61 ng/ml

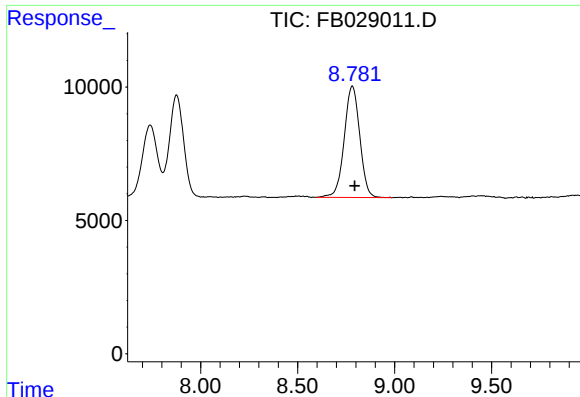

#5 AAA-TFT


R.T.: 8.782 min
Delta R.T.: -0.012 min
Response: 232988
Conc: 18.33 ng/ml

Instrument :
FID_B
ClientSampleId :
WC-40MSD

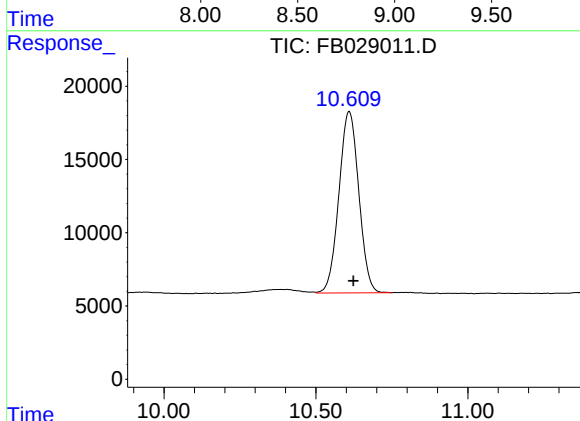


#6 Toluene

R.T.: 10.610 min
Delta R.T.: -0.013 min
Response: 562595
Conc: 27.97 ng/ml

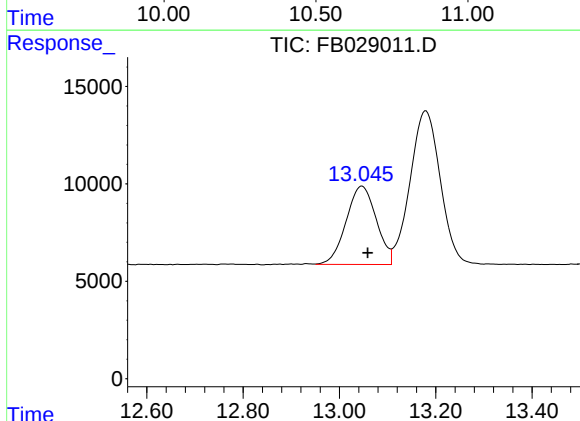


#7 Ethylbenzene

R.T.: 13.047 min
Delta R.T.: -0.012 min
Response: 174825
Conc: 9.22 ng/ml

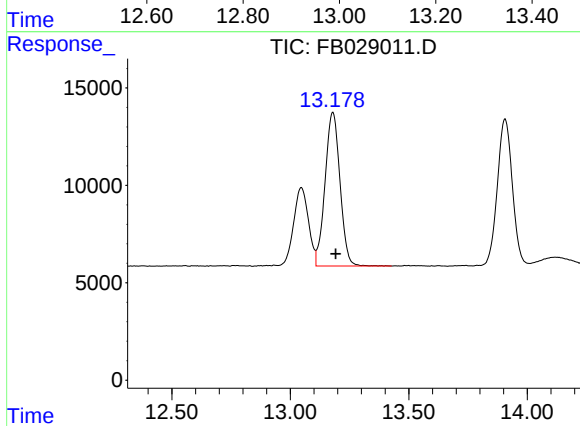

#8 m-Xylene


R.T.: 13.179 min
Delta R.T.: -0.012 min
Response: 345760
Conc: 18.38 ng/ml

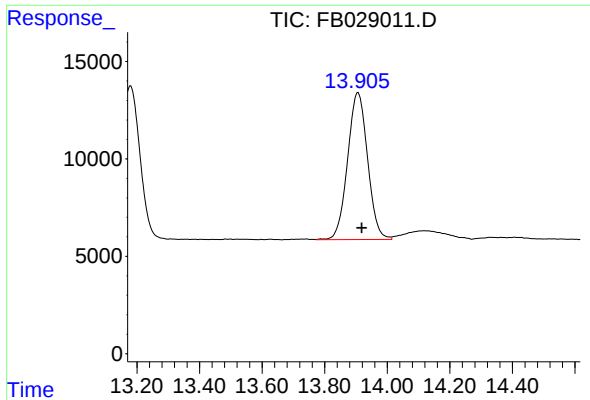

#9 O-Xylene

R.T.: 13.906 min
Delta R.T.: -0.012 min
Response: 334599
Conc: 18.24 ng/ml

Instrument :
FID_B
ClientSampleId :
WC-40MSD

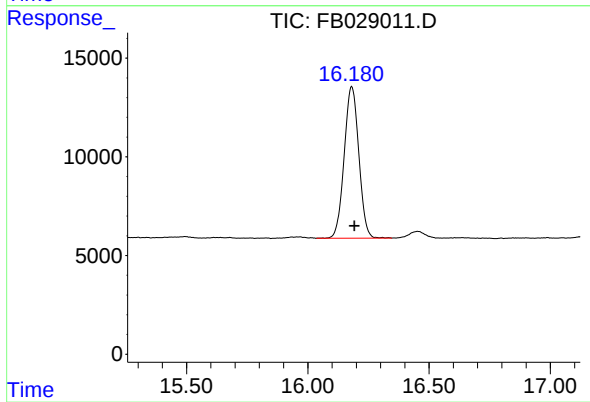

#10 1,2,4-Trimethylbenzene

R.T.: 16.181 min
Delta R.T.: -0.011 min
Response: 321607
Conc: 17.46 ng/ml