

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111424\
Data File : FB031170.D
Signal(s) : FID2B.CH
Acq On : 14 Nov 2024 14:44
Operator : YP/AJ
Sample : VBF1114S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Nov 15 03:09:03 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB102824.M
Quant Title :
QLast Update : Mon Oct 28 12:19:57 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.787	521788	18.903 ng/ml
Target Compounds			
6) t Toluene	10.612	7268	0.146 ng/ml
8) t m-Xylene	13.187	8507	0.175 ng/ml
9) t O-Xylene	13.914	8906	0.195 ng/ml
10) t 1,2,4-Trimethylbenzene	16.191	20175	0.542 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111424\
Data File : FB031170.D
Signal(s) : FID2B.CH
Acq On : 14 Nov 2024 14:44
Operator : YP/AJ
Sample : VBF1114S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Nov 15 03:09:03 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB102824.M
Quant Title :
QLast Update : Mon Oct 28 12:19:57 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

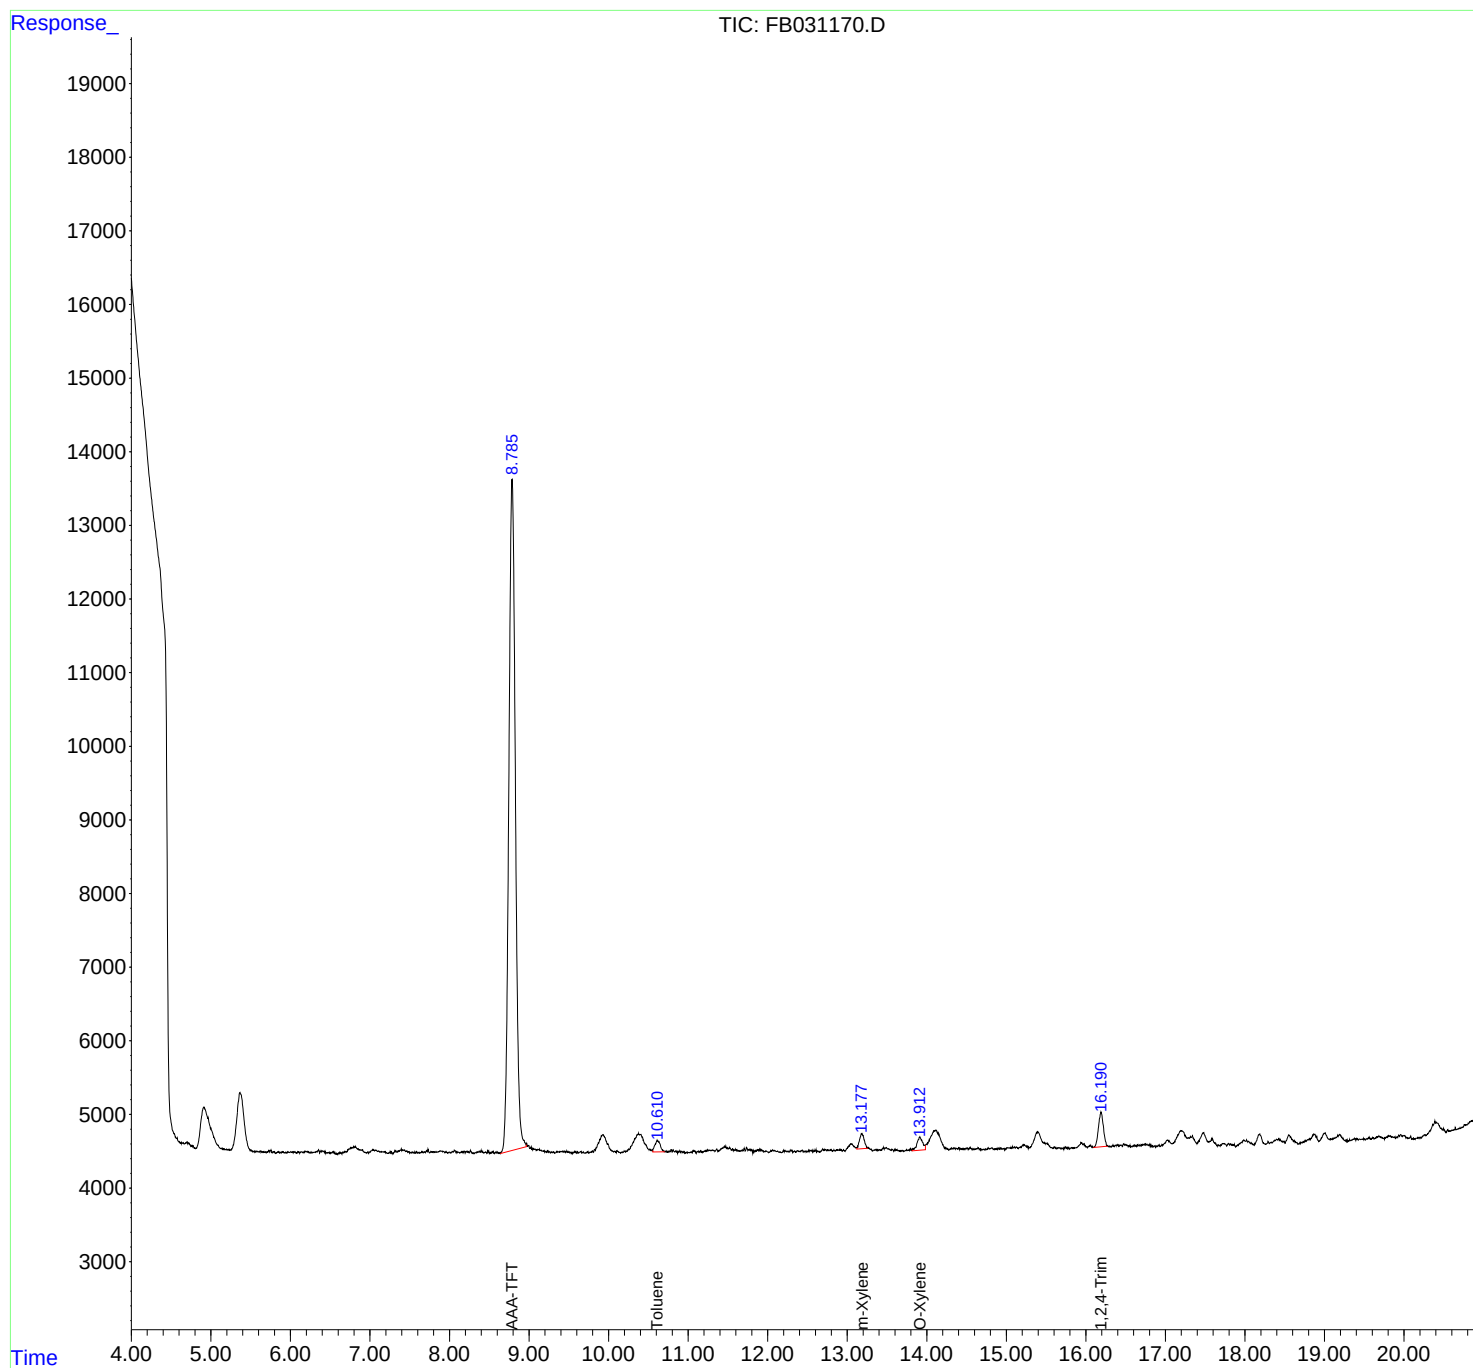


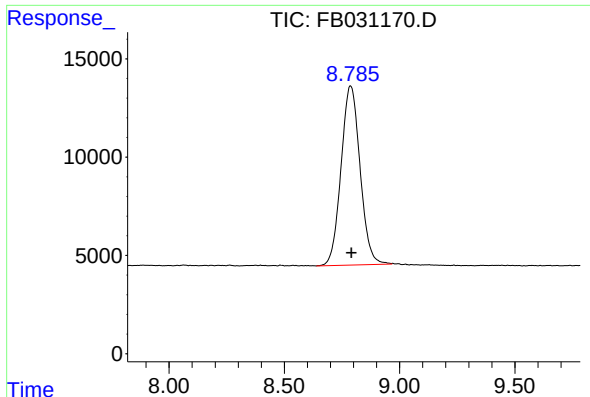

#5 AAA-TFT


R.T.: 8.787 min
Delta R.T.: -0.004 min
Response: 521788
Conc: 18.90 ng/ml

Instrument :
FID_B
ClientSampleId :

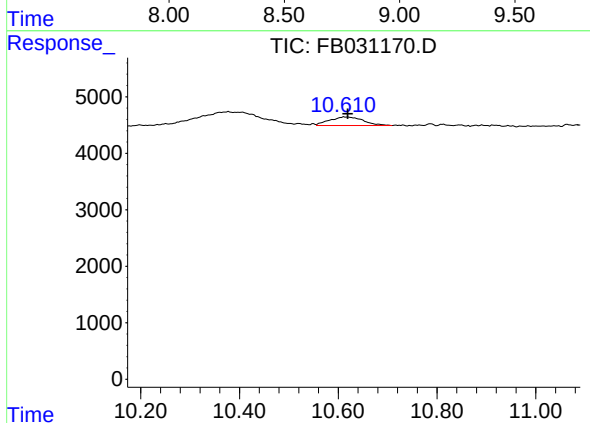


#6 Toluene

R.T.: 10.612 min
Delta R.T.: -0.007 min
Response: 7268
Conc: 0.15 ng/ml

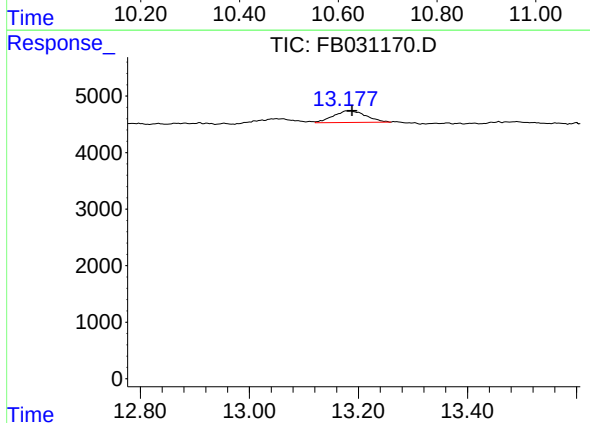


#8 m-Xylene

R.T.: 13.187 min
Delta R.T.: -0.001 min
Response: 8507
Conc: 0.17 ng/ml

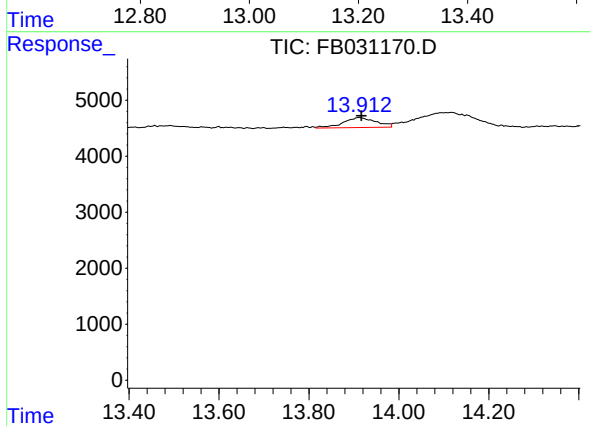

#9 O-Xylene

R.T.: 13.914 min
Delta R.T.: -0.003 min
Response: 8906
Conc: 0.20 ng/ml

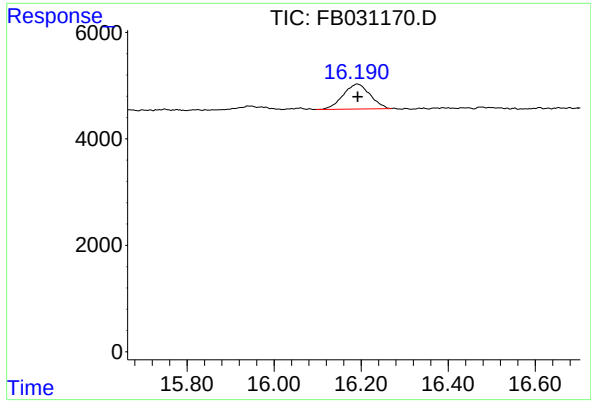

#10 1,2,4-Trimethylbenzene

R.T.: 16.191 min
Delta R.T.: 0.000 min
Response: 20175
Conc: 0.54 ng/ml

Instrument :
FID_B
ClientSampleId :