

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111424\
 Data File : FB031174.D
 Signal(s) : FID2B.CH
 Acq On : 14 Nov 2024 16:46
 Operator : YP/AJ
 Sample : P4839-02 50X
 Misc : 8.52G/5.00 ML MEOH
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Nov 15 03:09:30 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB102824.M
 Quant Title :
 QLast Update : Mon Oct 28 12:19:57 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.851	14639638	530.366 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.716	32392861	824.780 ng/ml
2) t 2,2,4-Trimethylpentane	7.431	38628368	824.753 ng/ml
3) t n-Heptane	7.740	9761396	215.387 ng/ml
6) t Toluene	10.680	1363433	27.303 ng/ml
7) t Ethylbenzene	13.010	2669679	59.641 ng/ml
8) t m-Xylene	13.181	554431	11.399 ng/ml
9) t O-Xylene	13.922	356332	7.817 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111424\
Data File : FB031174.D
Signal(s) : FID2B.CH
Acq On : 14 Nov 2024 16:46
Operator : YP/AJ
Sample : P4839-02 50X
Misc : 8.52G/5.00 ML MEOH
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Nov 15 03:09:30 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB102824.M
Quant Title :
QLast Update : Mon Oct 28 12:19:57 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

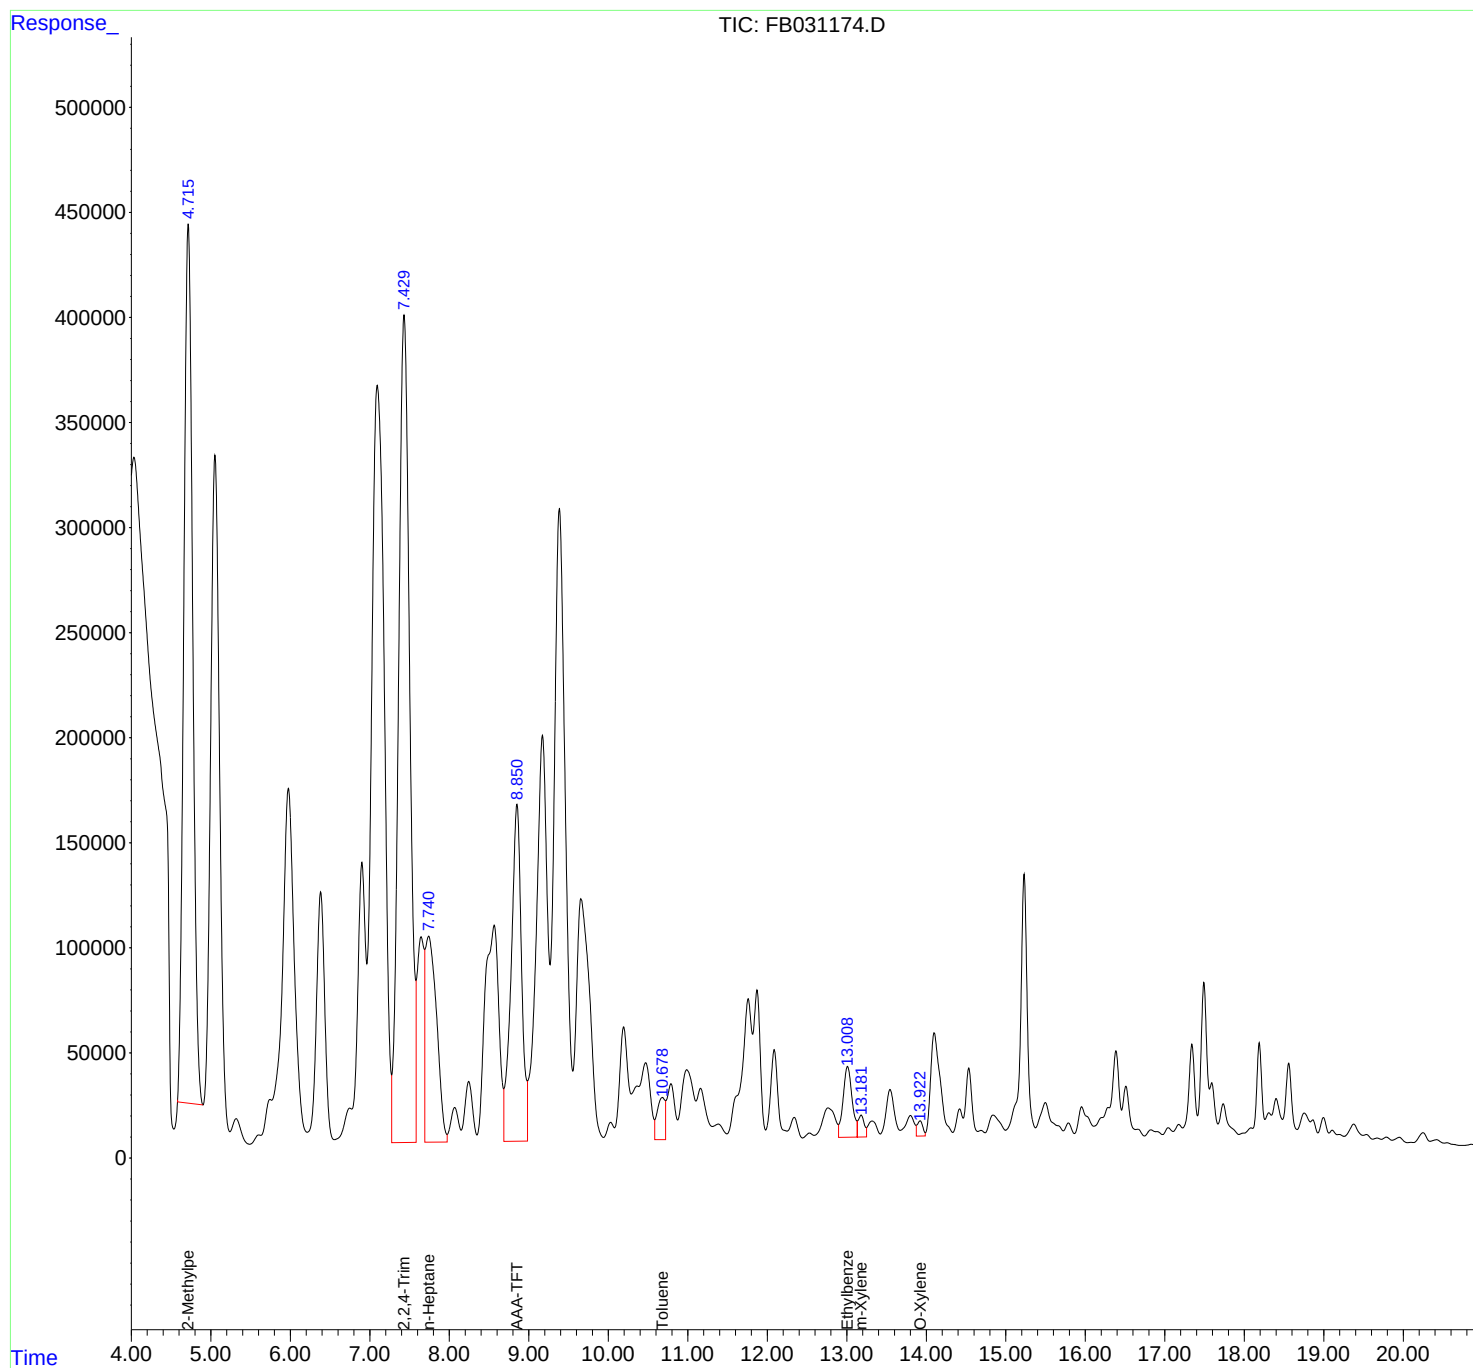


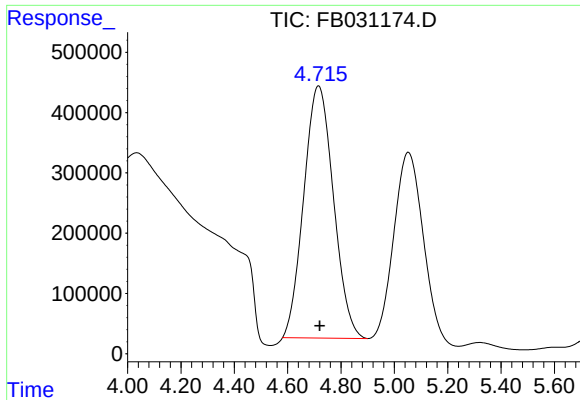

#1 2-Methylpentane


R.T.: 4.716 min
Delta R.T.: -0.004 min
Response: 32392861
Conc: 824.78 ng/ml

Instrument :
FID_B
ClientSampleId :

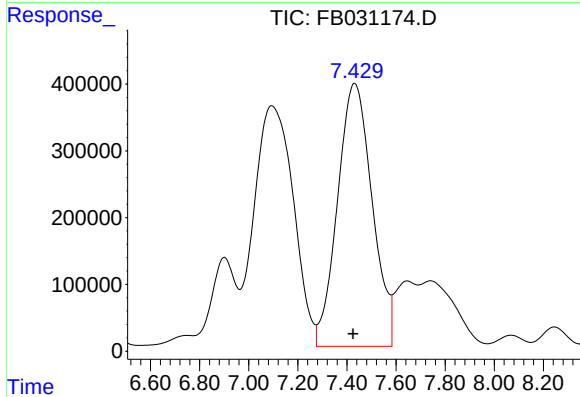


#2 2,2,4-Trimethylpentane

R.T.: 7.431 min
Delta R.T.: 0.007 min
Response: 38628368
Conc: 824.75 ng/ml

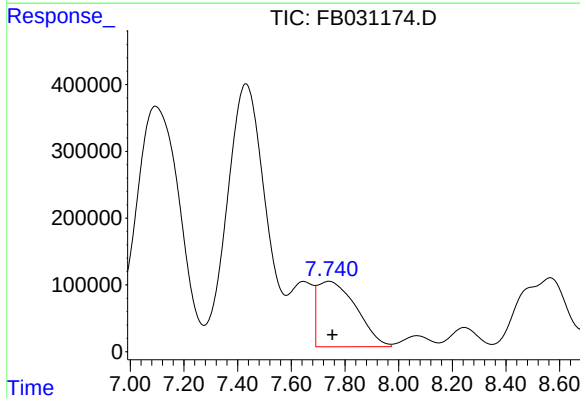


#3 n-Heptane

R.T.: 7.740 min
Delta R.T.: -0.012 min
Response: 9761396
Conc: 215.39 ng/ml

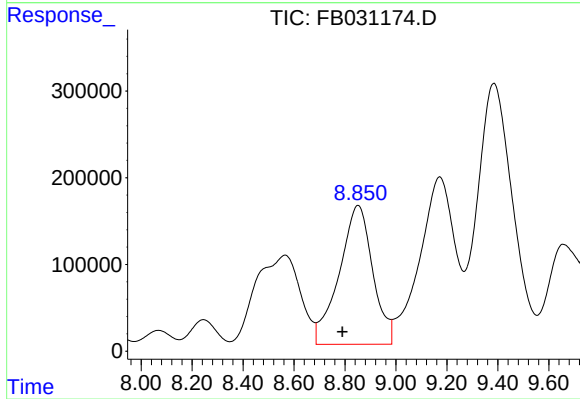

#5 AAA-TFT


R.T.: 8.851 min
Delta R.T.: 0.061 min
Response: 14639638
Conc: 530.37 ng/ml

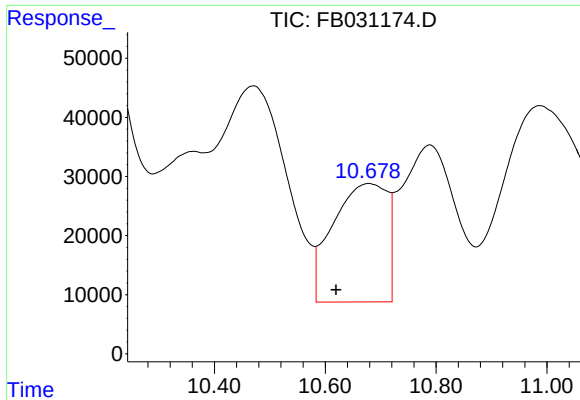

#6 Toluene


R.T.: 10.680 min
Delta R.T.: 0.060 min
Response: 1363433
Conc: 27.30 ng/ml

Instrument :
FID_B
ClientSampleId :

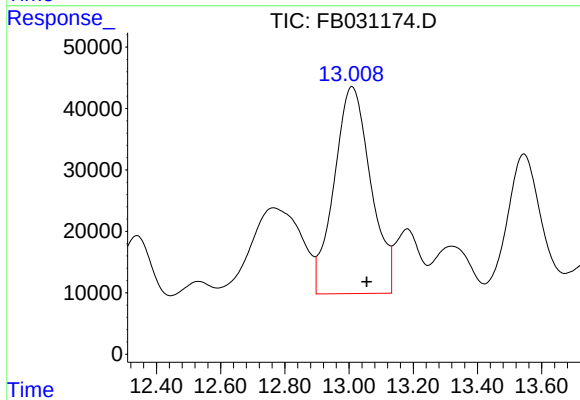


#7 Ethylbenzene

R.T.: 13.010 min
Delta R.T.: -0.045 min
Response: 2669679
Conc: 59.64 ng/ml

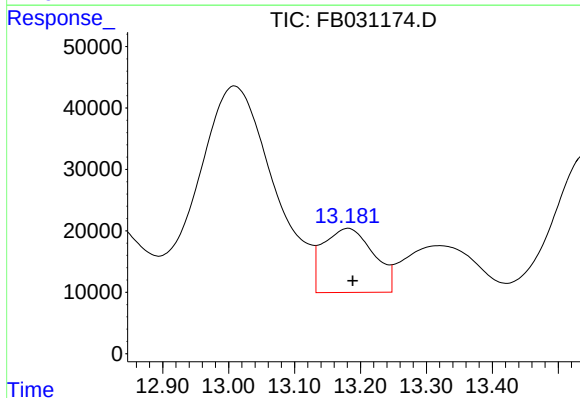

#8 m-Xylene

R.T.: 13.181 min
Delta R.T.: -0.008 min
Response: 554431
Conc: 11.40 ng/ml

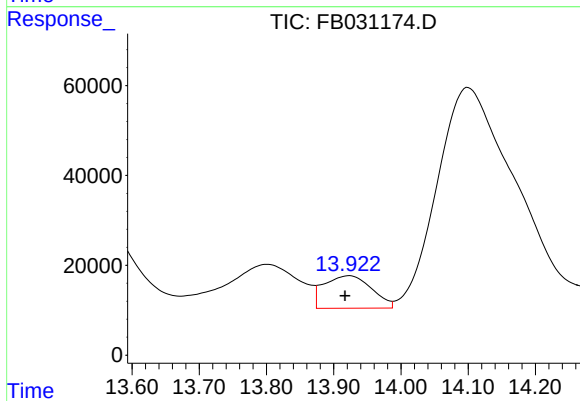

#9 O-Xylene

R.T.: 13.922 min
Delta R.T.: 0.005 min
Response: 356332
Conc: 7.82 ng/ml