

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111424\
 Data File : FB031175.D
 Signal(s) : FID2B.CH
 Acq On : 14 Nov 2024 17:13
 Operator : YP/AJ
 Sample : P4839-03 50X
 Misc : 7.49G/5.00 ML MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Nov 15 03:09:38 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB102824.M
 Quant Title :
 QLast Update : Mon Oct 28 12:19:57 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.838	3376615	122.328 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.716	6893759	175.527 ng/ml
2) t 2,2,4-Trimethylpentane	7.431	7945286	169.639 ng/ml
3) t n-Heptane	7.737	1936478	42.729 ng/ml
6) t Toluene	10.687	449511	9.002 ng/ml
7) t Ethylbenzene	13.047	1031091	23.035 ng/ml
8) t m-Xylene	13.182	421971	8.676 ng/ml
9) t O-Xylene	13.920	53228	1.168 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111424\
Data File : FB031175.D
Signal(s) : FID2B.CH
Acq On : 14 Nov 2024 17:13
Operator : YP/AJ
Sample : P4839-03 50X
Misc : 7.49G/5.00 ML MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Nov 15 03:09:38 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB102824.M
Quant Title :
QLast Update : Mon Oct 28 12:19:57 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

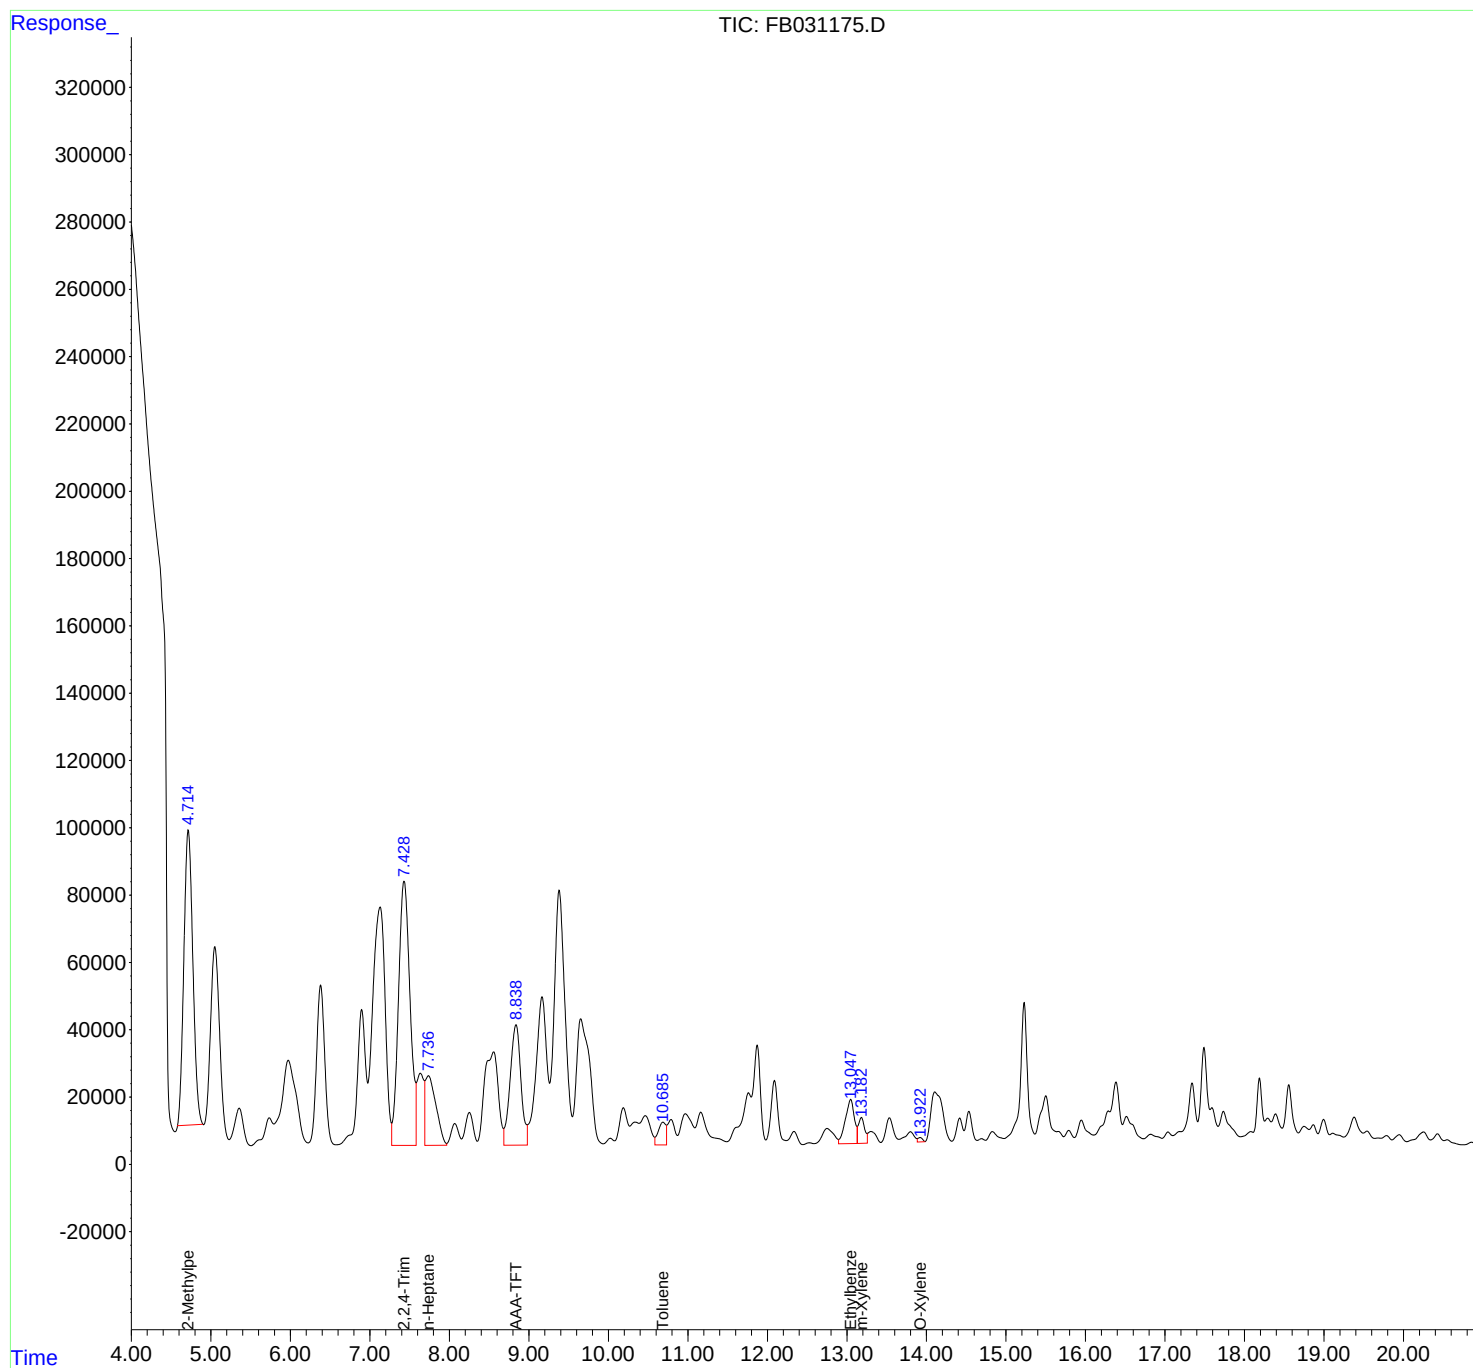


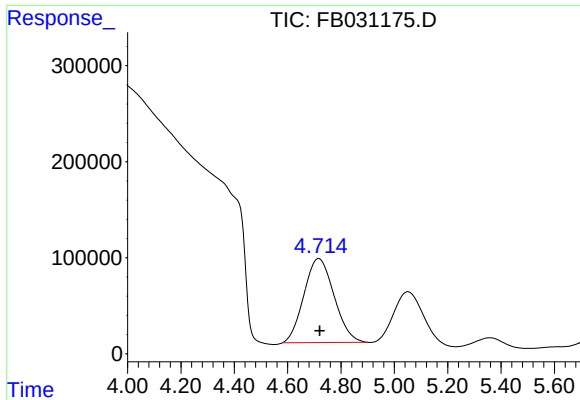

#1 2-Methylpentane


R.T.: 4.716 min
Delta R.T.: -0.004 min
Response: 6893759
Conc: 175.53 ng/ml

Instrument :
FID_B
ClientSampleId :

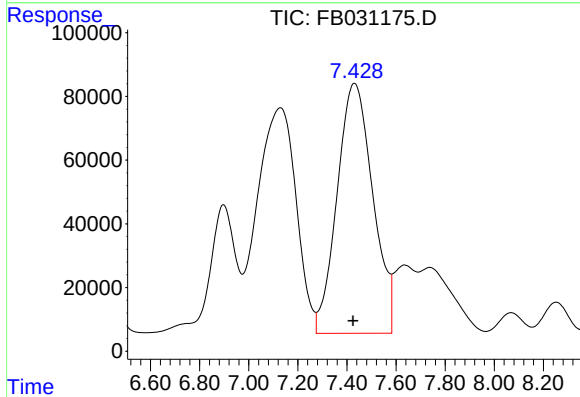


#2 2,2,4-Trimethylpentane

R.T.: 7.431 min
Delta R.T.: 0.006 min
Response: 7945286
Conc: 169.64 ng/ml

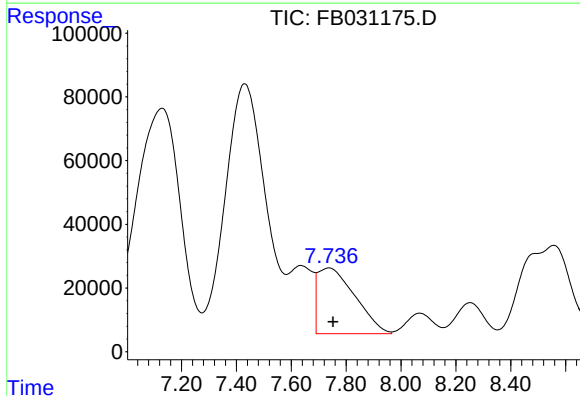


#3 n-Heptane

R.T.: 7.737 min
Delta R.T.: -0.015 min
Response: 1936478
Conc: 42.73 ng/ml

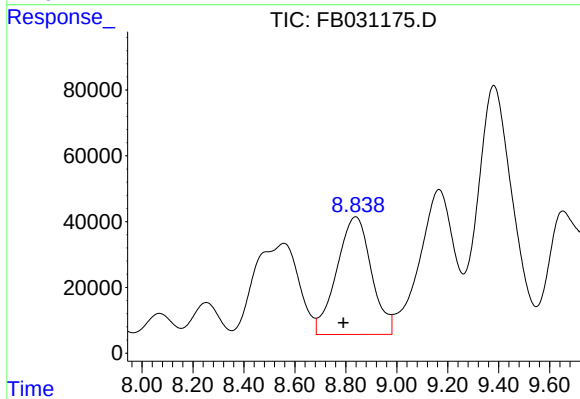

#5 AAA-TFT


R.T.: 8.838 min
Delta R.T.: 0.048 min
Response: 3376615
Conc: 122.33 ng/ml

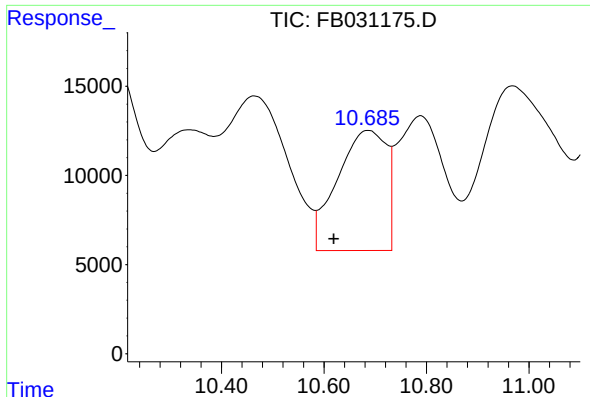

#6 Toluene


R.T.: 10.687 min
Delta R.T.: 0.068 min
Response: 449511
Conc: 9.00 ng/ml

Instrument :
FID_B
ClientSampleId :

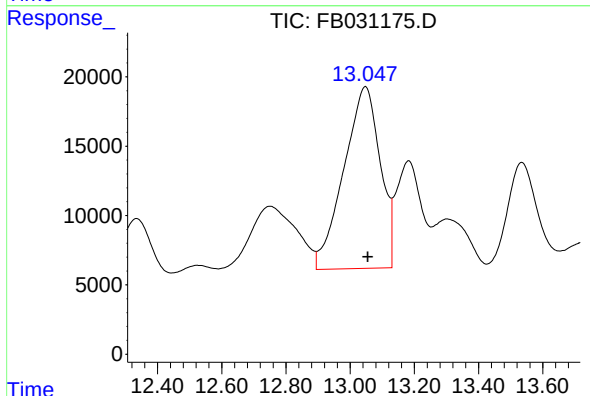


#7 Ethylbenzene

R.T.: 13.047 min
Delta R.T.: -0.008 min
Response: 1031091
Conc: 23.03 ng/ml

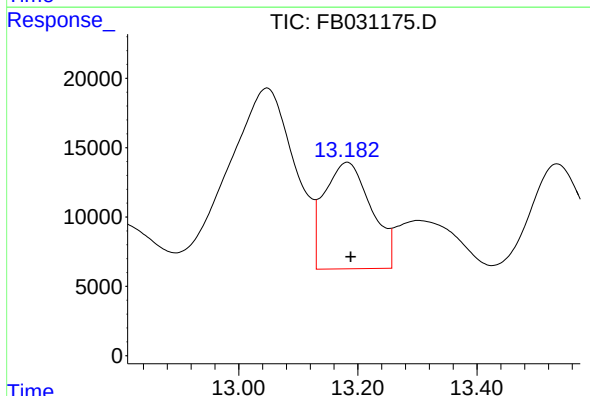

#8 m-Xylene

R.T.: 13.182 min
Delta R.T.: -0.006 min
Response: 421971
Conc: 8.68 ng/ml

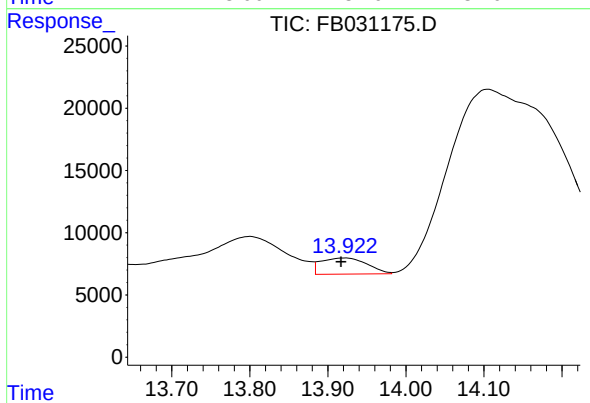

#9 O-Xylene

R.T.: 13.920 min
Delta R.T.: 0.004 min
Response: 53228
Conc: 1.17 ng/ml