

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111424\
 Data File : FB031172.D
 Signal(s) : FID2B.CH
 Acq On : 14 Nov 2024 15:37
 Operator : YP/AJ
 Sample : BSF1114S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF1114S1

Integration File: Calibration.e
 Quant Time: Nov 15 03:09:16 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB102824.M
 Quant Title :
 QLast Update : Mon Oct 28 12:19:57 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.790	504358	18.272 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.717	1129273	28.753 ng/ml
2) t 2,2,4-Trimethylpentane	7.420	1386273	29.598 ng/ml
3) t n-Heptane	7.751	415005	9.157 ng/ml
4) t Benzene	7.890	512787	9.593 ng/ml
6) t Toluene	10.618	1466263	29.362 ng/ml
7) t Ethylbenzene	13.055	428075	9.563 ng/ml
8) t m-Xylene	13.188	912613	18.763 ng/ml
9) t O-Xylene	13.916	848626	18.617 ng/ml
10) t 1,2,4-Trimethylbenzene	16.193	682043	18.330 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111424\
Data File : FB031172.D
Signal(s) : FID2B.CH
Acq On : 14 Nov 2024 15:37
Operator : YP/AJ
Sample : BSF1114S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF1114S1

Integration File: Calibration.e
Quant Time: Nov 15 03:09:16 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB102824.M
Quant Title :
QLast Update : Mon Oct 28 12:19:57 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

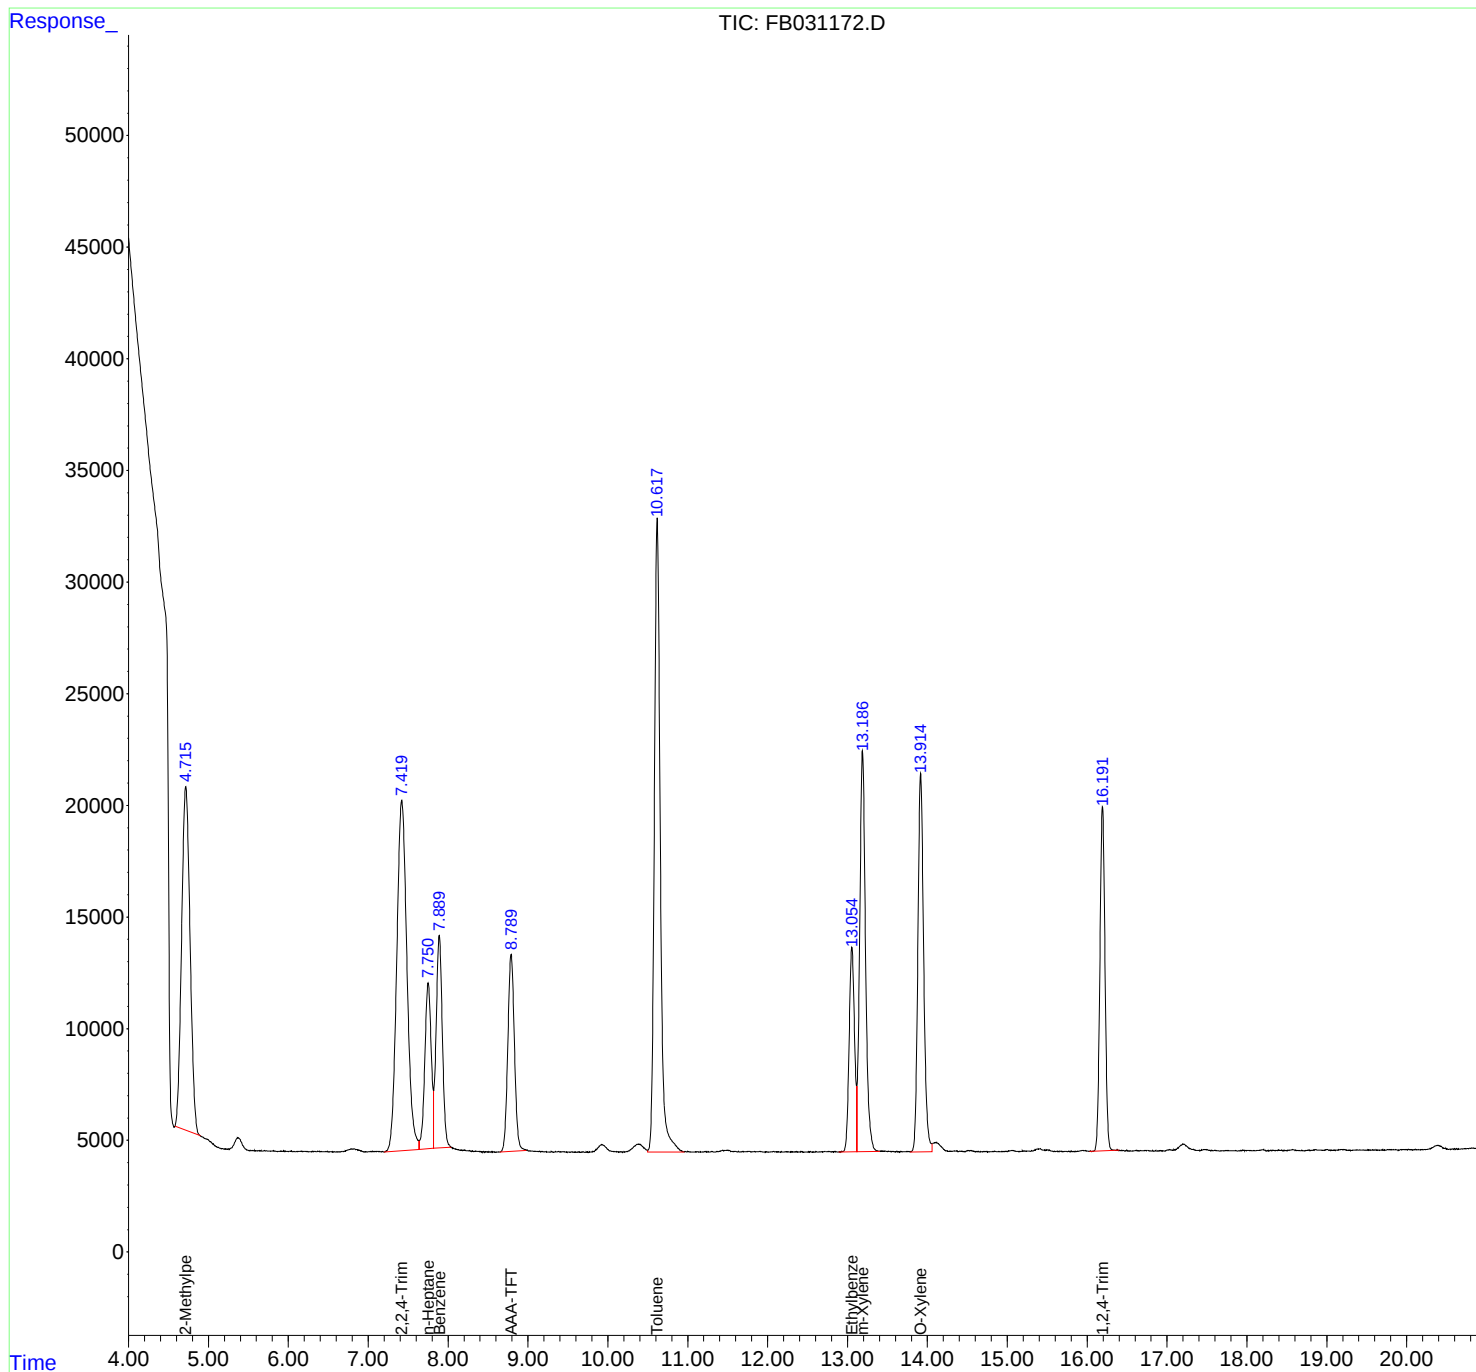


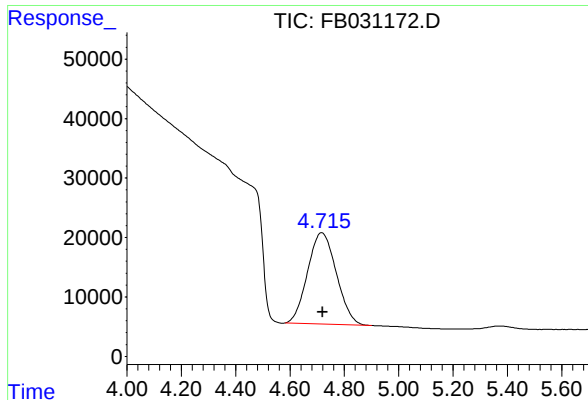

#1 2-Methylpentane


R.T.: 4.717 min
Delta R.T.: -0.003 min
Response: 1129273
Conc: 28.75 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1114S1

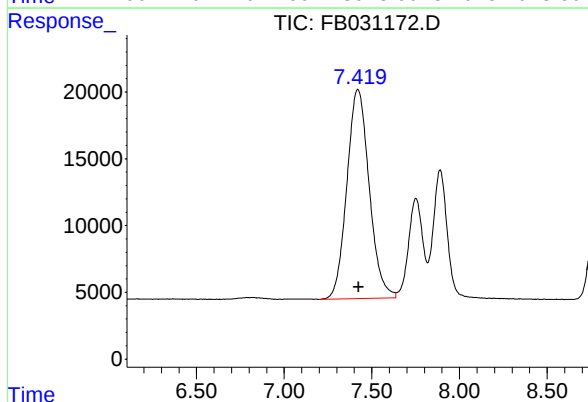


#2 2,2,4-Trimethylpentane

R.T.: 7.420 min
Delta R.T.: -0.004 min
Response: 1386273
Conc: 29.60 ng/ml

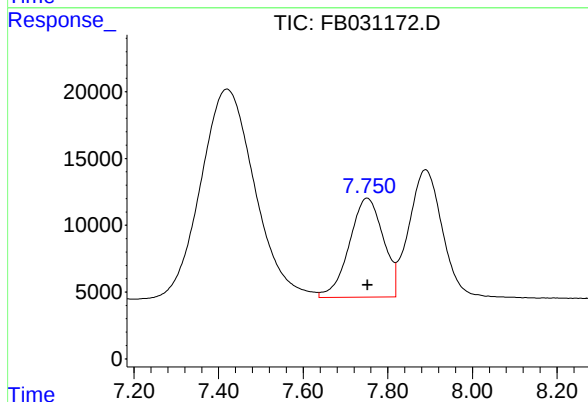


#3 n-Heptane

R.T.: 7.751 min
Delta R.T.: -0.001 min
Response: 415005
Conc: 9.16 ng/ml

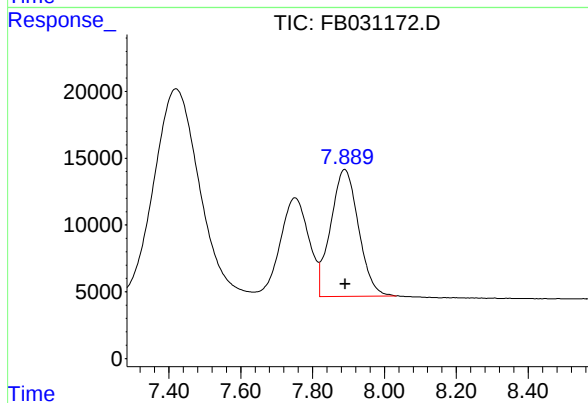

#4 Benzene


R.T.: 7.890 min
Delta R.T.: -0.001 min
Response: 512787
Conc: 9.59 ng/ml

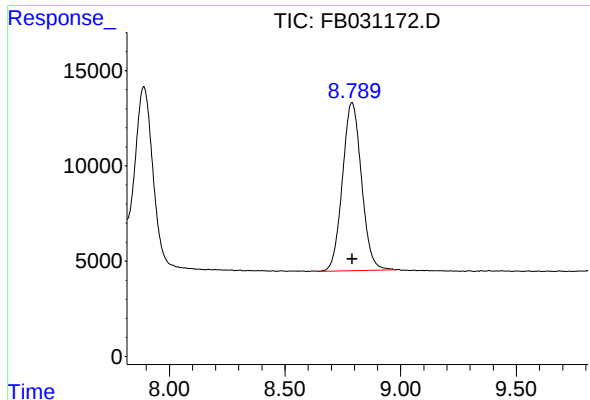

#5 AAA-TFT


R.T.: 8.790 min
Delta R.T.: 0.000 min
Response: 504358
Conc: 18.27 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1114S1

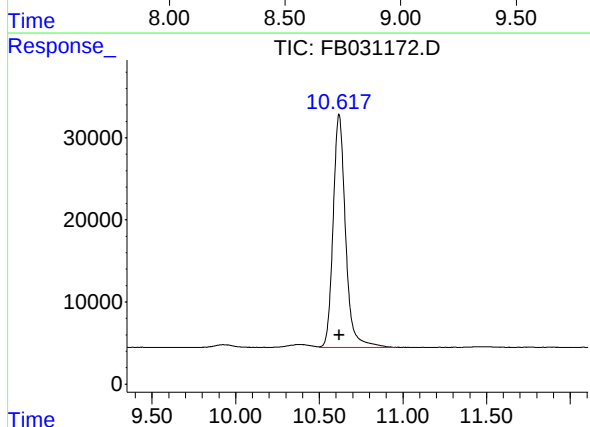


#6 Toluene

R.T.: 10.618 min
Delta R.T.: 0.000 min
Response: 1466263
Conc: 29.36 ng/ml

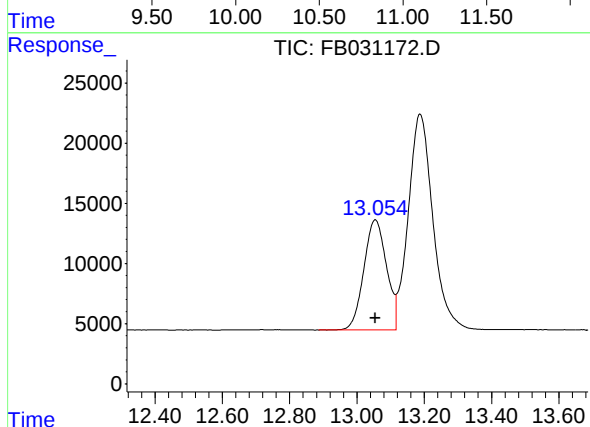


#7 Ethylbenzene

R.T.: 13.055 min
Delta R.T.: 0.000 min
Response: 428075
Conc: 9.56 ng/ml

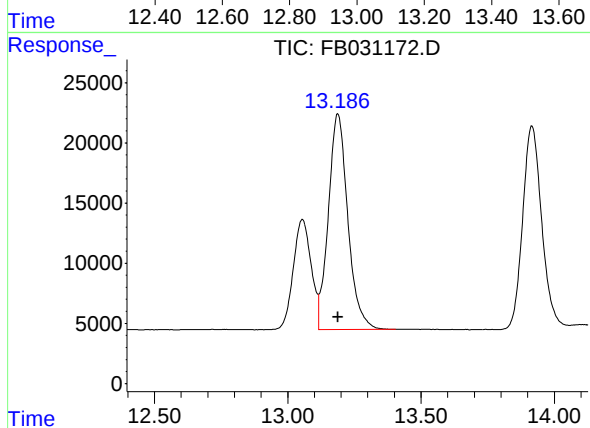

#8 m-Xylene


R.T.: 13.188 min
Delta R.T.: 0.000 min
Response: 912613
Conc: 18.76 ng/ml

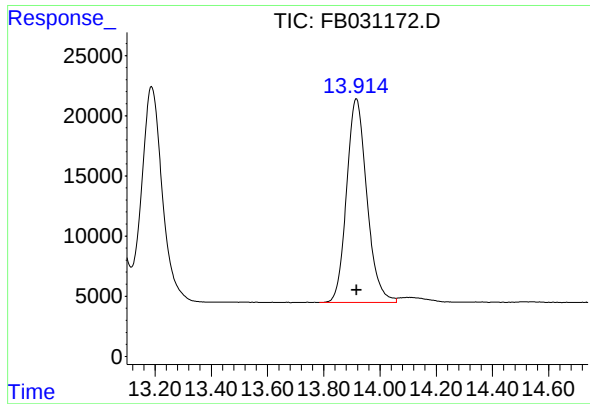

#9 O-Xylene

R.T.: 13.916 min
Delta R.T.: 0.000 min
Response: 848626
Conc: 18.62 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1114S1

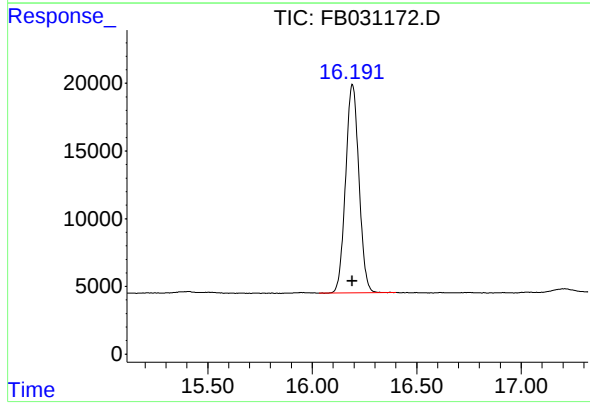

#10 1,2,4-Trimethylbenzene

R.T.: 16.193 min
Delta R.T.: 0.000 min
Response: 682043
Conc: 18.33 ng/ml