

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111424\
 Data File : FB031179.D
 Signal(s) : FID2B.CH
 Acq On : 14 Nov 2024 19:00
 Operator : YP/AJ
 Sample : BSF1114S2
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF1114S2

Integration File: Calibration.e
 Quant Time: Nov 15 03:10:04 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB102824.M
 Quant Title :
 QLast Update : Mon Oct 28 12:19:57 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.791	514468	18.638 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.717	1038585	26.444 ng/ml
2) t 2,2,4-Trimethylpentane	7.421	1299927	27.755 ng/ml
3) t n-Heptane	7.752	395772	8.733 ng/ml
4) t Benzene	7.890	496374	9.286 ng/ml
6) t Toluene	10.619	1368948	27.414 ng/ml
7) t Ethylbenzene	13.056	405536	9.060 ng/ml
8) t m-Xylene	13.190	858628	17.653 ng/ml
9) t O-Xylene	13.918	784639	17.213 ng/ml
10) t 1,2,4-Trimethylbenzene	16.194	670117	18.010 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111424\
Data File : FB031179.D
Signal(s) : FID2B.CH
Acq On : 14 Nov 2024 19:00
Operator : YP/AJ
Sample : BSF1114S2
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF1114S2

Integration File: Calibration.e
Quant Time: Nov 15 03:10:04 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB102824.M
Quant Title :
QLast Update : Mon Oct 28 12:19:57 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

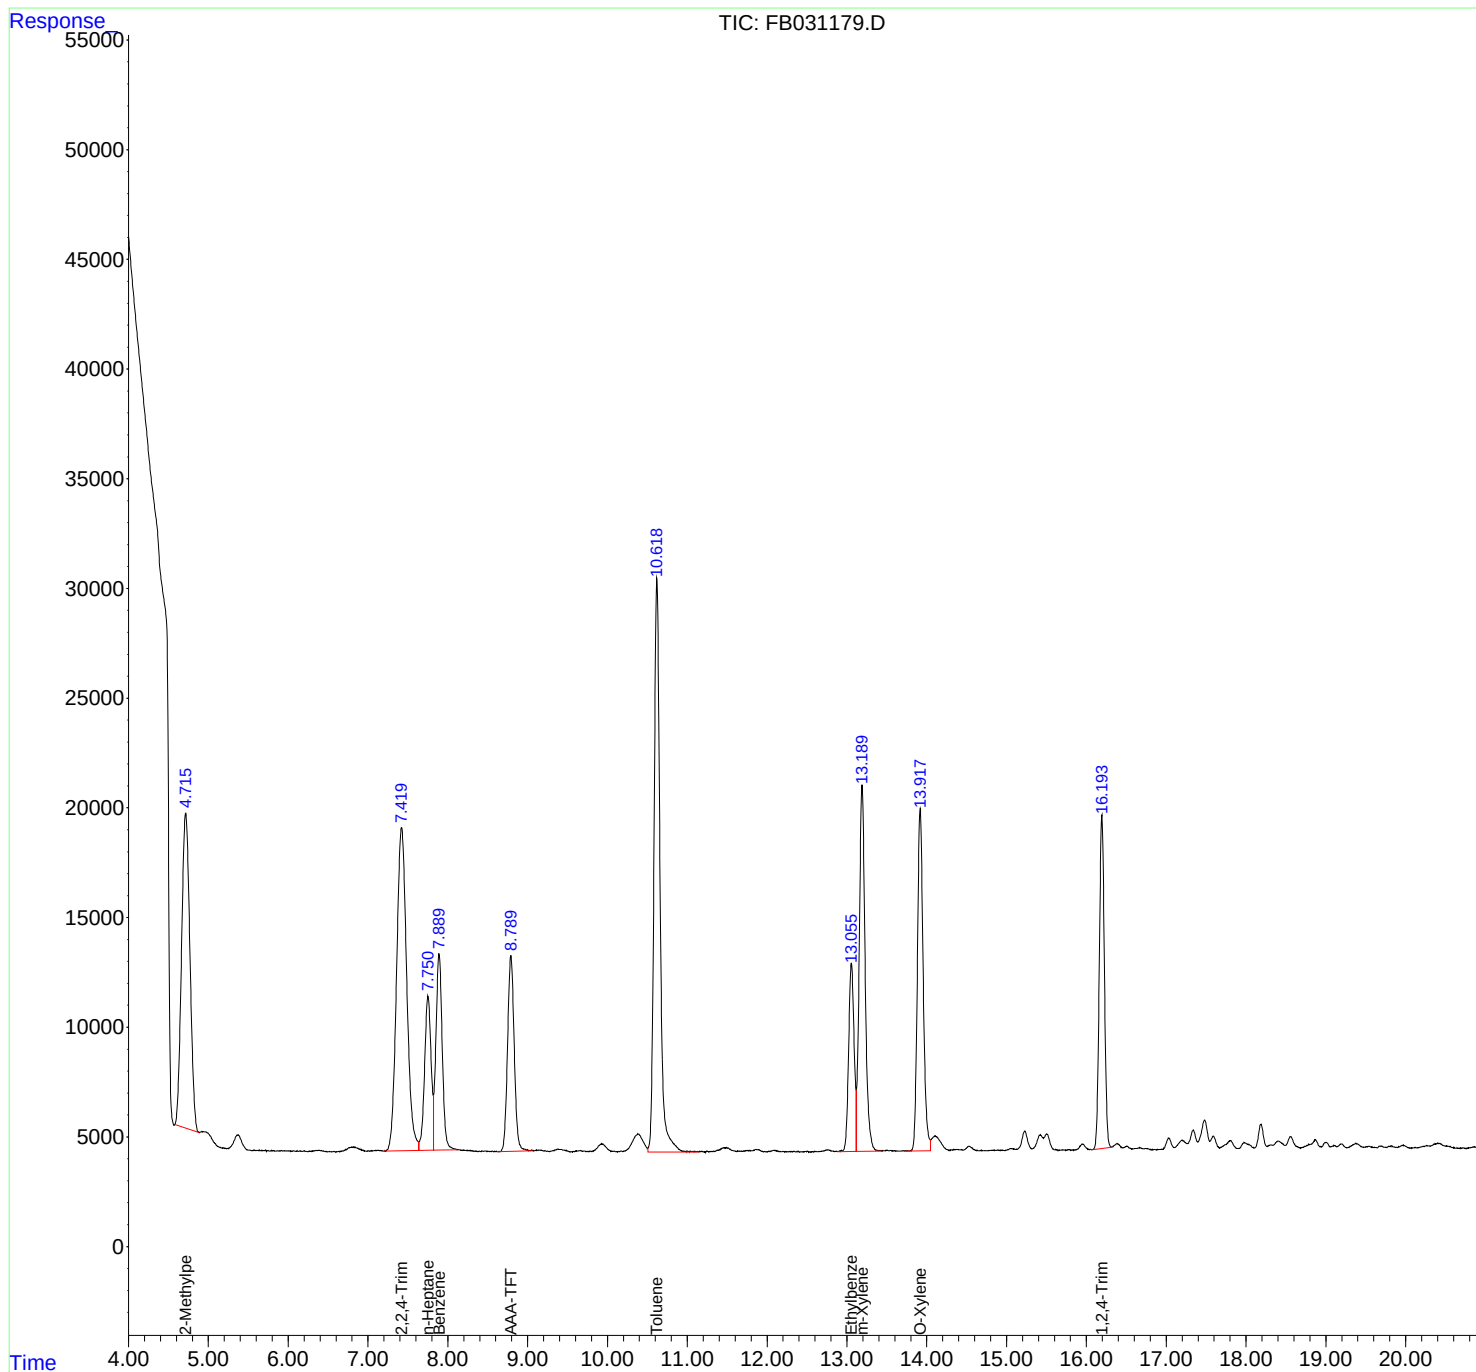


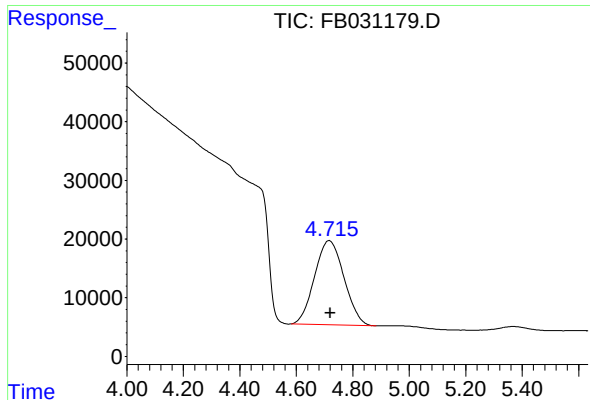

#1 2-Methylpentane


R.T.: 4.717 min
Delta R.T.: -0.003 min
Response: 1038585
Conc: 26.44 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1114S2

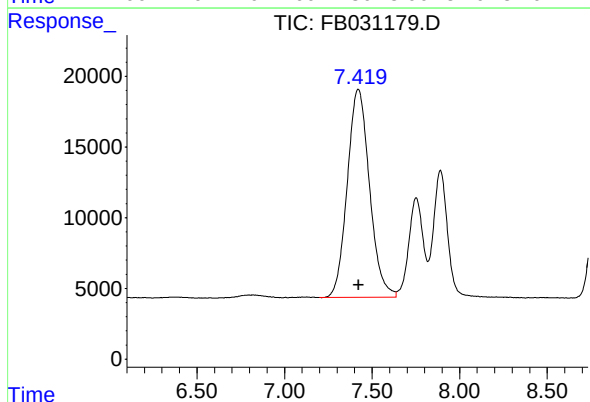


#2 2,2,4-Trimethylpentane

R.T.: 7.421 min
Delta R.T.: -0.004 min
Response: 1299927
Conc: 27.75 ng/ml

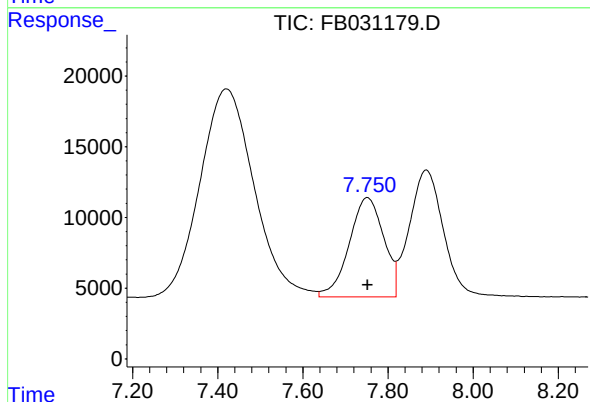


#3 n-Heptane

R.T.: 7.752 min
Delta R.T.: 0.000 min
Response: 395772
Conc: 8.73 ng/ml

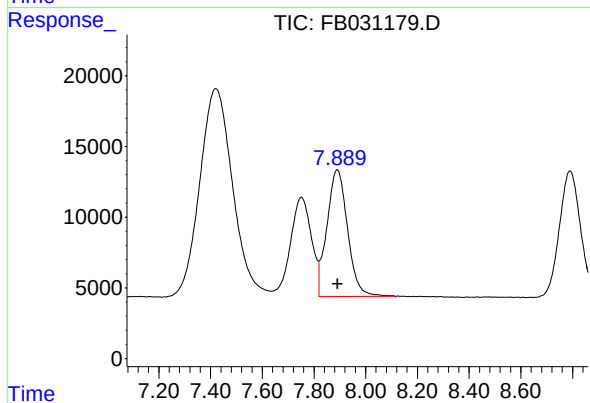

#4 Benzene


R.T.: 7.890 min
Delta R.T.: -0.001 min
Response: 496374
Conc: 9.29 ng/ml

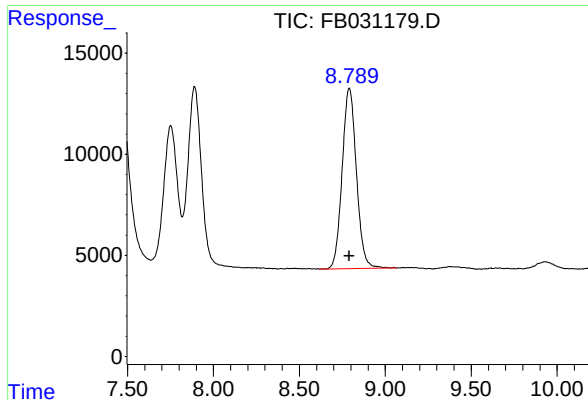

#5 AAA-TFT


R.T.: 8.791 min
Delta R.T.: 0.000 min
Response: 514468
Conc: 18.64 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1114S2

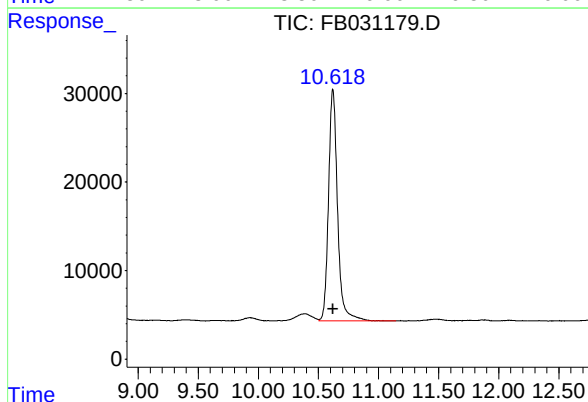


#6 Toluene

R.T.: 10.619 min
Delta R.T.: 0.000 min
Response: 1368948
Conc: 27.41 ng/ml

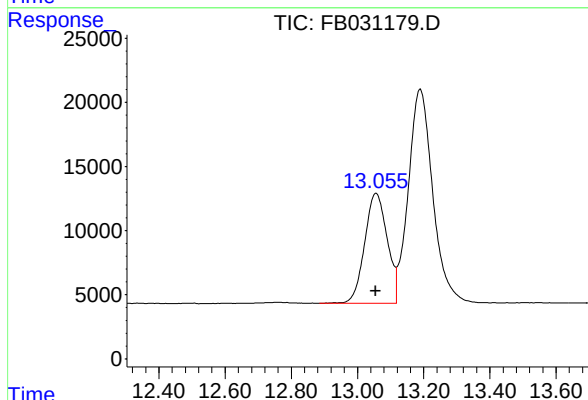


#7 Ethylbenzene

R.T.: 13.056 min
Delta R.T.: 0.001 min
Response: 405536
Conc: 9.06 ng/ml

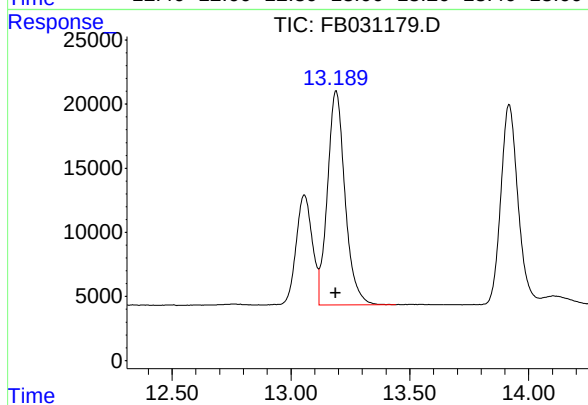

#8 m-Xylene


R.T.: 13.190 min
Delta R.T.: 0.002 min
Response: 858628
Conc: 17.65 ng/ml

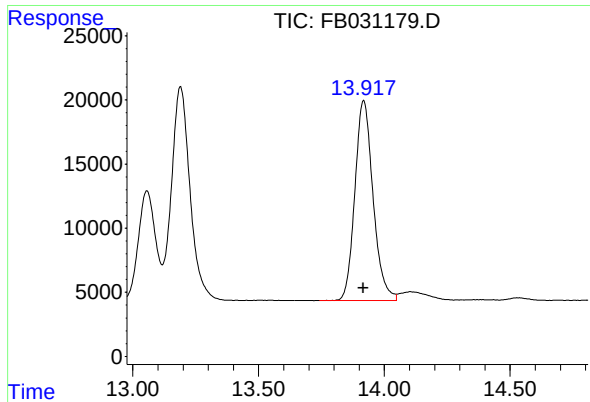

#9 O-Xylene

R.T.: 13.918 min
Delta R.T.: 0.001 min
Response: 784639
Conc: 17.21 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1114S2

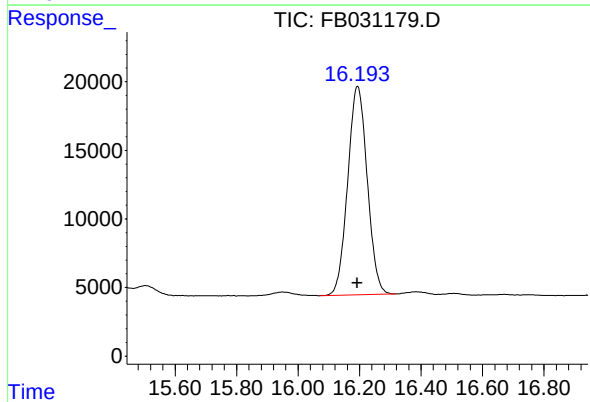

#10 1,2,4-Trimethylbenzene

R.T.: 16.194 min
Delta R.T.: 0.002 min
Response: 670117
Conc: 18.01 ng/ml