

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111518\
 Data File : FB018793.D
 Signal(s) : FID2B.CH
 Acq On : 15 Nov 2018 9:07
 Operator : MJ/SJ
 Sample : BSF1115S1
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Nov 16 05:55:15 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110918.M
 Quant Title :
 QLast Update : Fri Nov 09 10:53:13 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.105	157591	18.270 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.958	409900	28.026 ng/ml
2) t 2,2,4-Trimethylpentane	7.720	447554	30.511 ng/ml
3) t n-Heptane	8.060	141859	9.834 ng/ml
4) t Benzene	8.200	180484	9.962 ng/ml
6) t Toluene	10.953	450623	29.799 ng/ml
7) t Ethylbenzene	13.403	155845	9.993 ng/ml
8) t m-Xylene	13.536	328043	19.746 ng/ml
9) t O-Xylene	14.267	342874	19.985 ng/ml
10) t 1,2,4-Trimethylbenzene	16.550	404203	20.376 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111518\
Data File : FB018793.D
Signal(s) : FID2B.CH
Acq On : 15 Nov 2018 9:07
Operator : MJ/SJ
Sample : BSF1115S1
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Nov 16 05:55:15 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110918.M
Quant Title :
QLast Update : Fri Nov 09 10:53:13 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

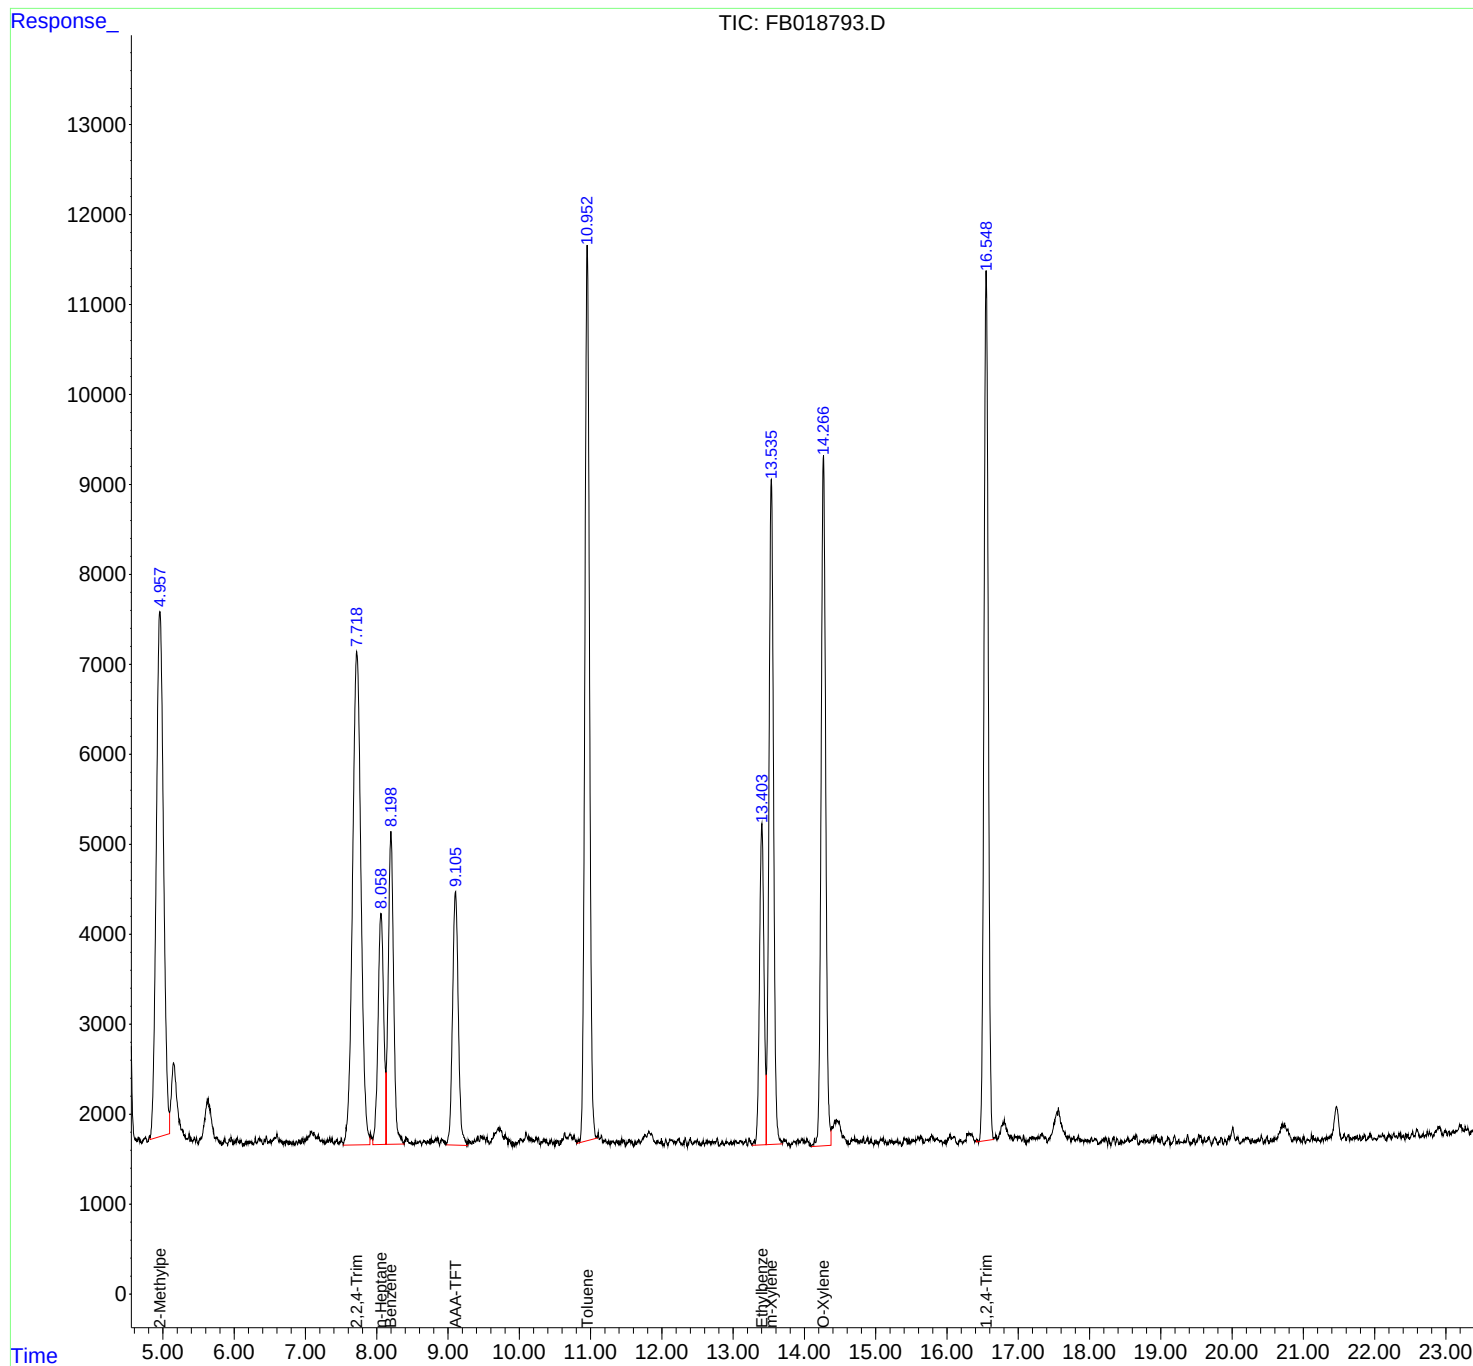

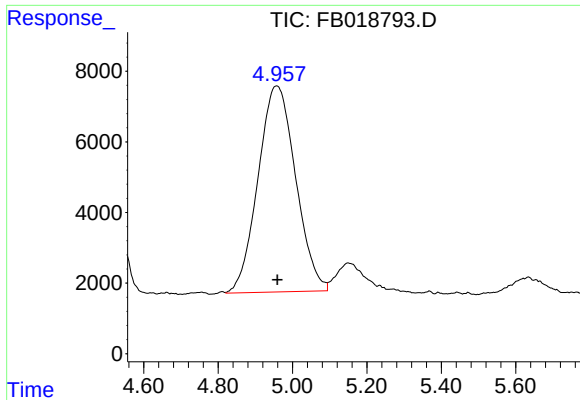


#1 2-Methylpentane

R.T.: 4.958 min
Delta R.T.: -0.002 min
Response: 409900
Conc: 28.03 ng/ml

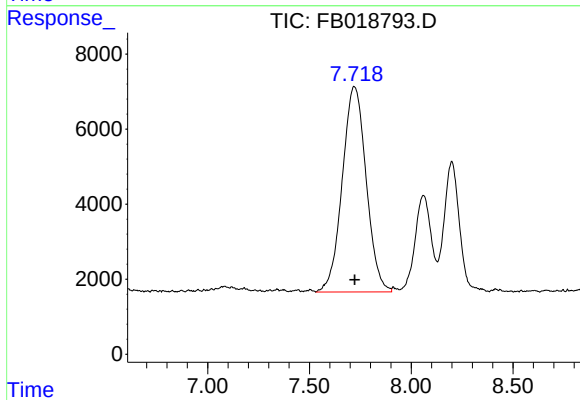


#2 2,2,4-Trimethylpentane

R.T.: 7.720 min
Delta R.T.: -0.004 min
Response: 447554
Conc: 30.51 ng/ml

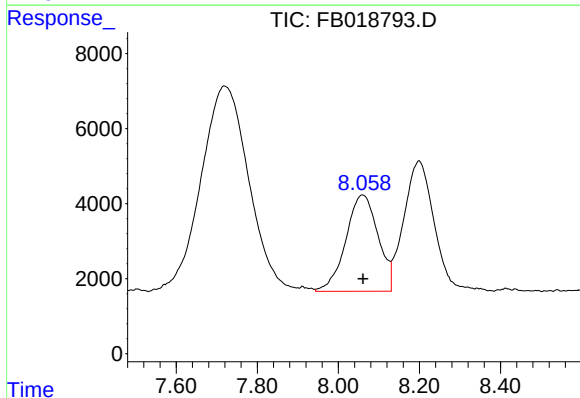


#3 n-Heptane

R.T.: 8.060 min
Delta R.T.: 0.000 min
Response: 141859
Conc: 9.83 ng/ml

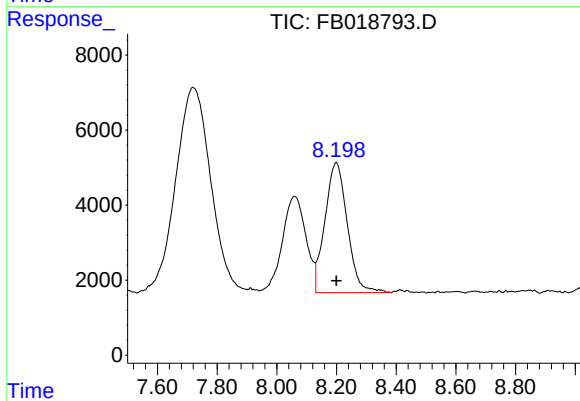


#4 Benzene

R.T.: 8.200 min
Delta R.T.: 0.000 min
Response: 180484
Conc: 9.96 ng/ml

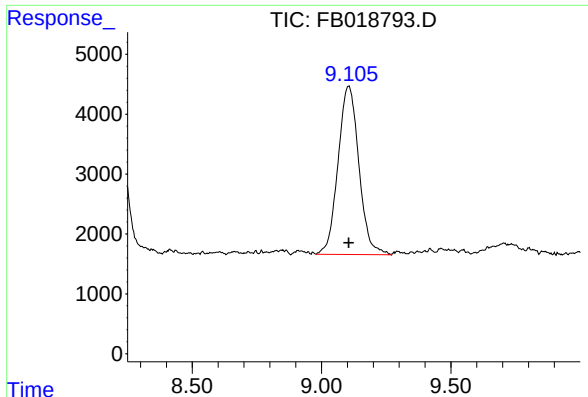


#5 AAA-TFT

R.T.: 9.105 min
Delta R.T.: 0.000 min
Response: 157591
Conc: 18.27 ng/ml

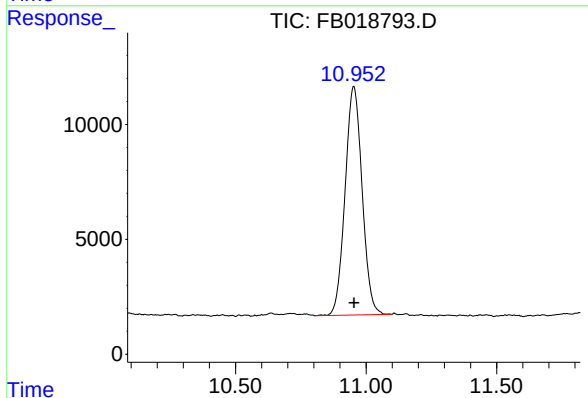


#6 Toluene

R.T.: 10.953 min
Delta R.T.: -0.001 min
Response: 450623
Conc: 29.80 ng/ml

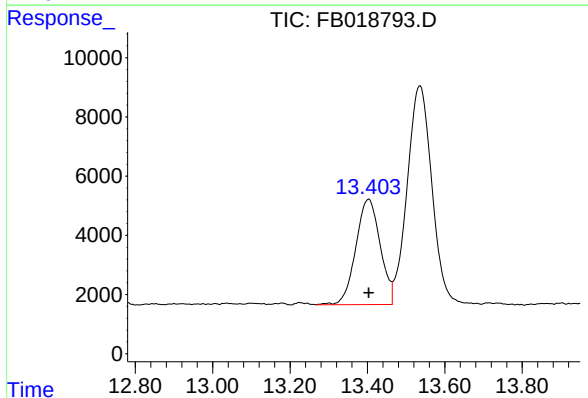


#7 Ethylbenzene

R.T.: 13.403 min
Delta R.T.: 0.000 min
Response: 155845
Conc: 9.99 ng/ml

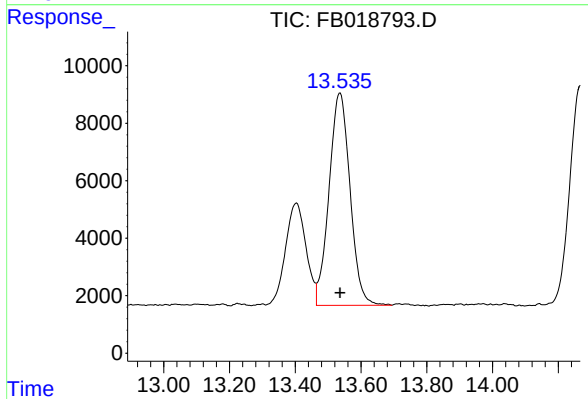


#8 m-Xylene

R.T.: 13.536 min
Delta R.T.: 0.000 min
Response: 328043
Conc: 19.75 ng/ml

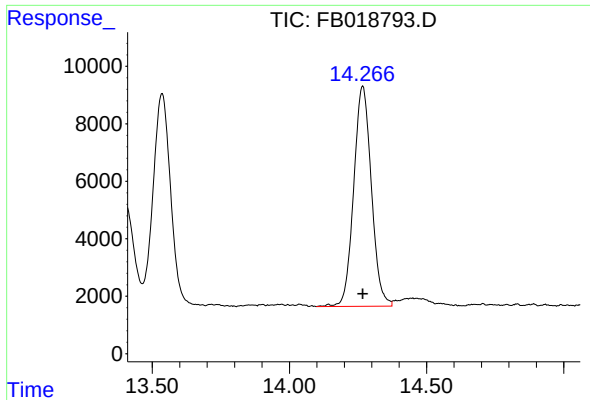

#9 O-Xylene

R.T.: 14.267 min
Delta R.T.: 0.000 min
Response: 342874
Conc: 19.98 ng/ml

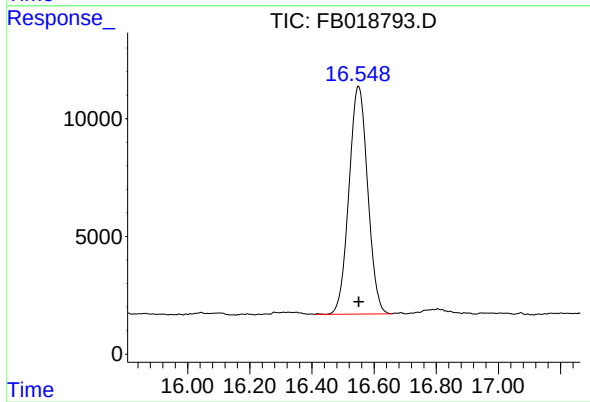

#10 1,2,4-Trimethylbenzene

R.T.: 16.550 min
Delta R.T.: 0.000 min
Response: 404203
Conc: 20.38 ng/ml